

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 23:36
 Operator : YP\AJ
 Sample : N4698-08 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-33A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:03:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.432	3.685	2690340	2249232	1.514	1.489
2)	SA Decachlor...	10.255	8.788	2540960	1981288	1.644	1.654
Target Compounds							
3)	L1 AR-1016-1	0.000	4.800	0	258791	N.D.	5.193 #
4)	L1 AR-1016-2	0.000	4.800	0	258791	N.D.	3.625 #
12)	L3 AR-1232-2	0.000	4.800	0	258791	N.D.	8.373 #
16)	L4 AR-1242-1	0.000	4.800	0	258791	N.D.	5.984 #
17)	L4 AR-1242-2	0.000	4.800	0	258791	N.D.	4.286 #
20)	L4 AR-1242-5	6.504f	5.612	155485	188095	4.361	4.953
21)	L5 AR-1248-1	0.000	4.800	0	258791	N.D.	8.004 #
24)	L5 AR-1248-4	6.504	0.000	155485	0	2.564	N.D. #
25)	L5 AR-1248-5	6.504f	0.000	155485	0	2.491	N.D. #
26)	L6 AR-1254-1	6.476	5.612	377434	188095	6.075	2.316 #
27)	L6 AR-1254-2	6.689	0.000	669215	0	5.797	N.D. #
28)	L6 AR-1254-3	7.056	0.000	489121	0	4.018	N.D. #
30)	L6 AR-1254-5	7.790f	0.000	270697	0	3.038	N.D. #
31)	L7 AR-1260-1	7.220	0.000	346949	0	3.716	N.D. #
32)	L7 AR-1260-2	0.000	6.470f	0	284360	N.D.	3.216 #
33)	L7 AR-1260-3	0.000	6.647	0	525430	N.D.	6.195 #
38)	L8 AR-1262-3	0.000	7.645	0	809858	N.D.	12.490 #
41)	L9 AR-1268-1	0.000	7.645	0	809858	N.D.	4.296 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 23:36
Operator : YP\AJ
Sample : N4698-08 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:03:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

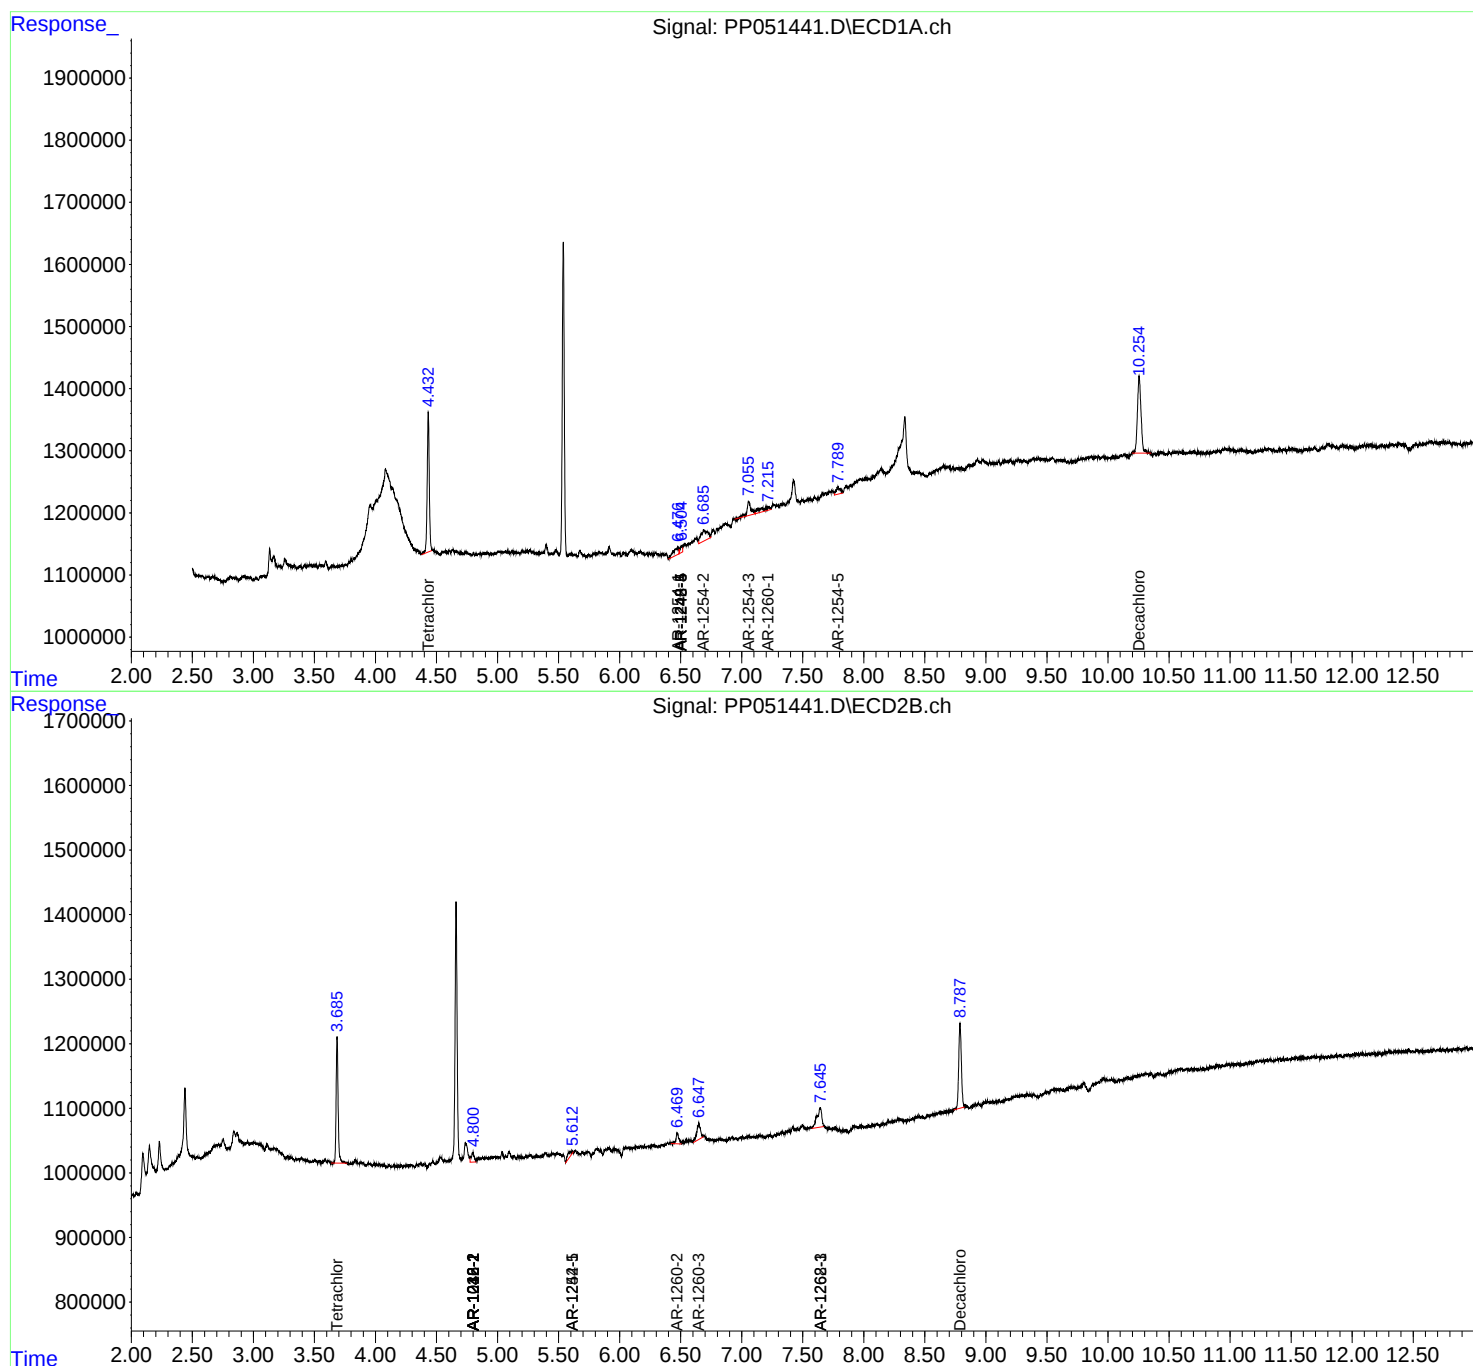


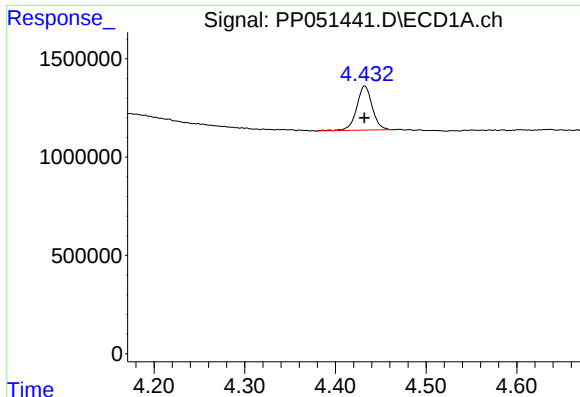

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: 0.000 min
Response: 2690340
Conc: 1.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

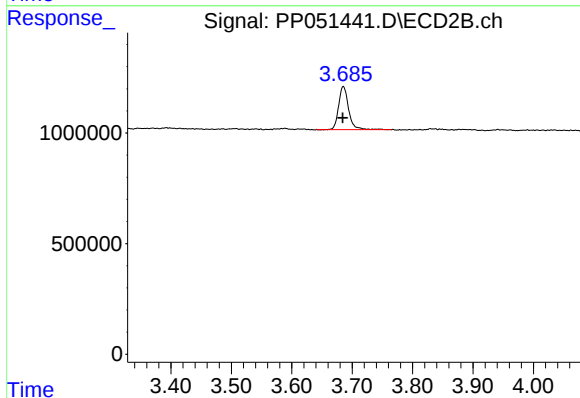


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 2249232
Conc: 1.49 ng/ml

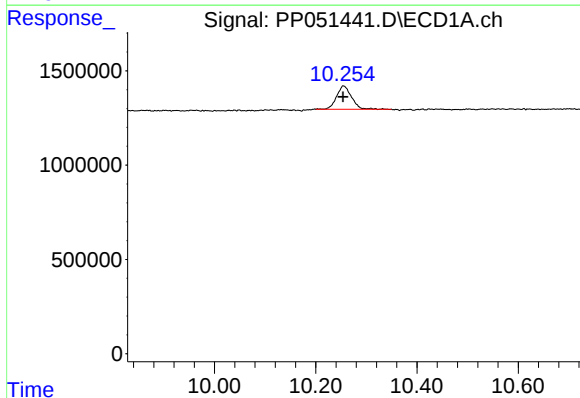


#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: 0.002 min
Response: 2540960
Conc: 1.64 ng/ml

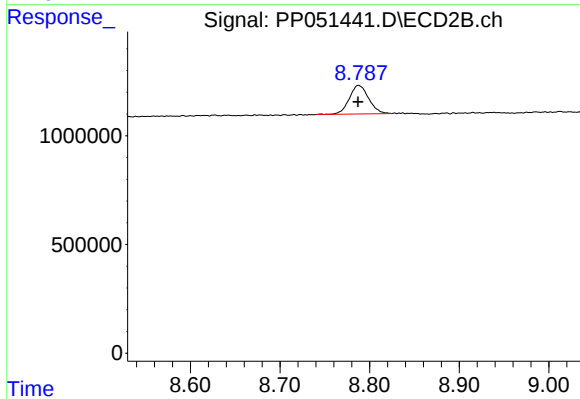

#2 Decachlorobiphenyl


R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 1981288
Conc: 1.65 ng/ml

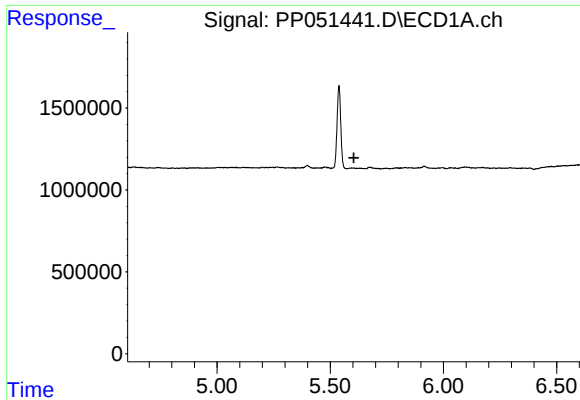

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

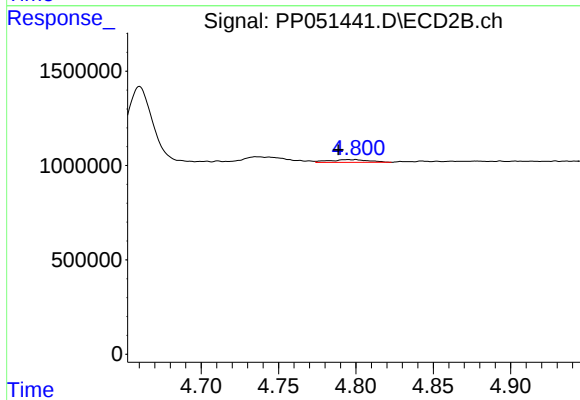


#3 AR-1016-1

R.T.: 4.800 min
Delta R.T.: 0.011 min
Response: 258791
Conc: 5.19 ng/ml

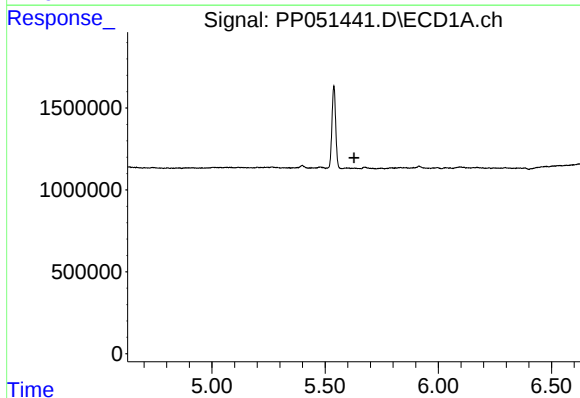


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.627 min
Response: 0
Conc: N.D.

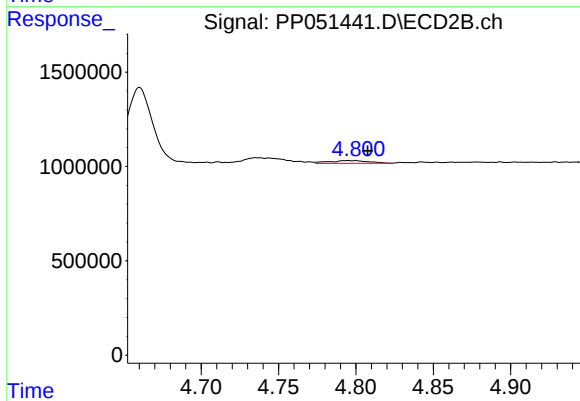

#4 AR-1016-2


R.T.: 4.800 min
Delta R.T.: -0.008 min
Response: 258791
Conc: 3.63 ng/ml

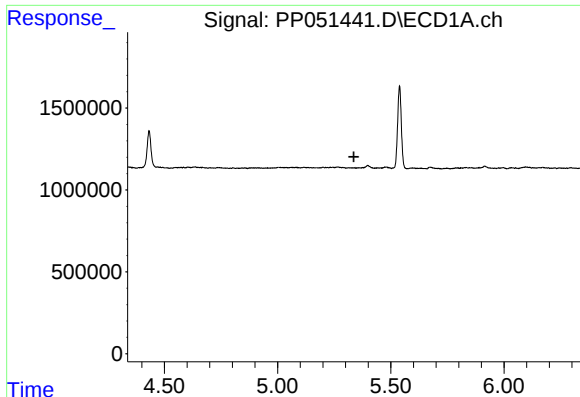

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

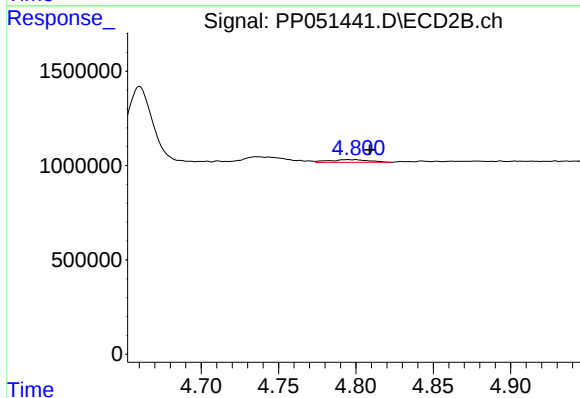


#12 AR-1232-2

R.T.: 4.800 min
Delta R.T.: -0.009 min
Response: 258791
Conc: 8.37 ng/ml

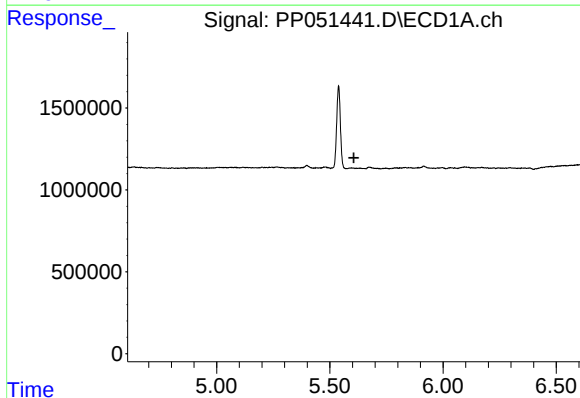


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 5.606 min
Response: 0
Conc: N.D.

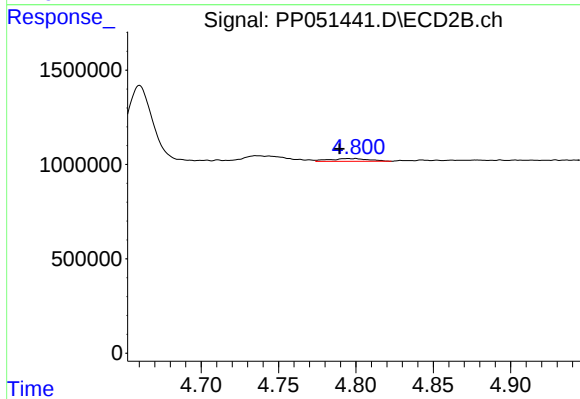

#16 AR-1242-1


R.T.: 4.800 min
Delta R.T.: 0.010 min
Response: 258791
Conc: 5.98 ng/ml

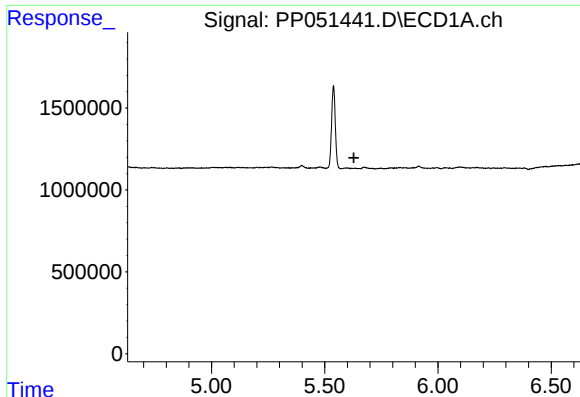

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.629 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

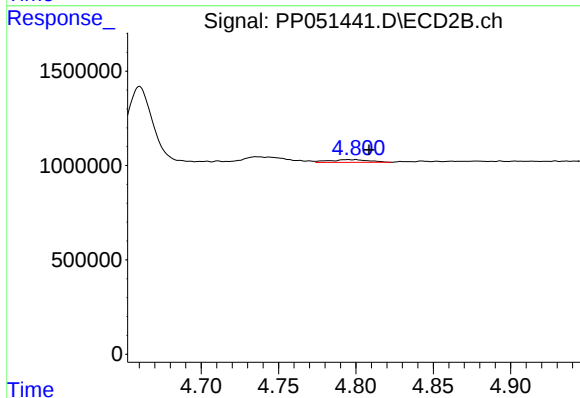


#17 AR-1242-2

R.T.: 4.800 min
Delta R.T.: -0.009 min
Response: 258791
Conc: 4.29 ng/ml

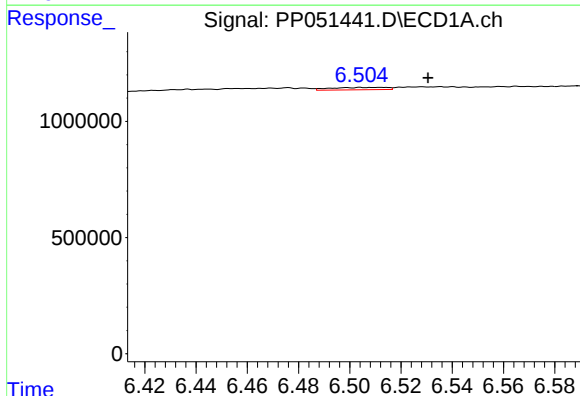


#20 AR-1242-5

R.T.: 6.504 min
Delta R.T.: -0.026 min
Response: 155485
Conc: 4.36 ng/ml

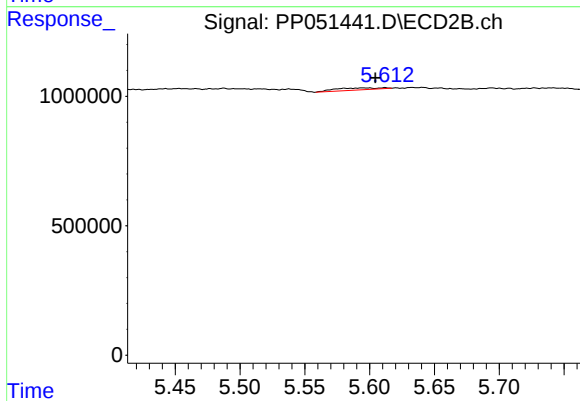

#20 AR-1242-5


R.T.: 5.612 min
Delta R.T.: 0.007 min
Response: 188095
Conc: 4.95 ng/ml

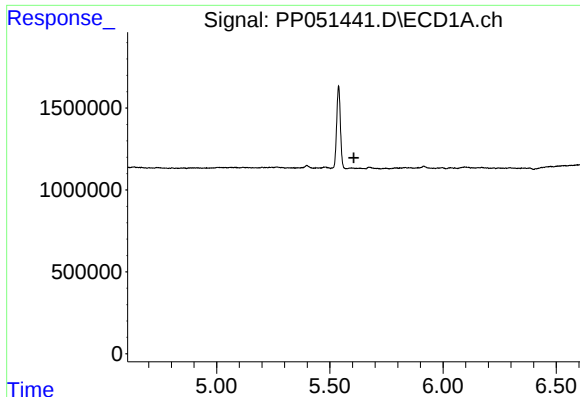

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

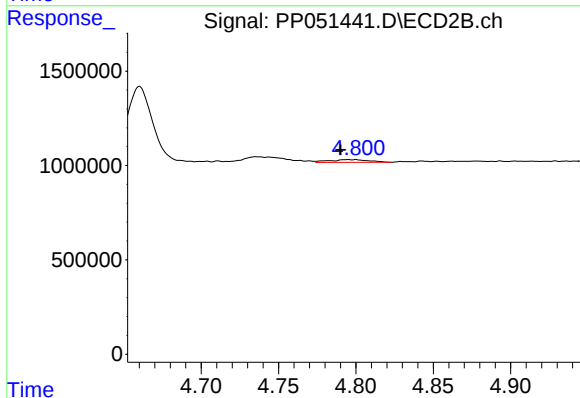


#21 AR-1248-1

R.T.: 4.800 min
Delta R.T.: 0.010 min
Response: 258791
Conc: 8.00 ng/ml

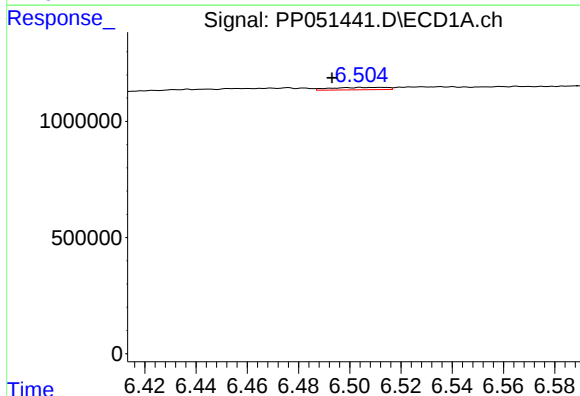


#24 AR-1248-4

R.T.: 6.504 min
Delta R.T.: 0.011 min
Response: 155485
Conc: 2.56 ng/ml

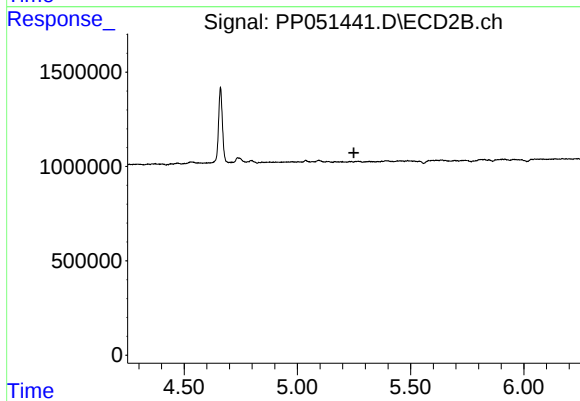

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.249 min
Response: 0
Conc: N.D.

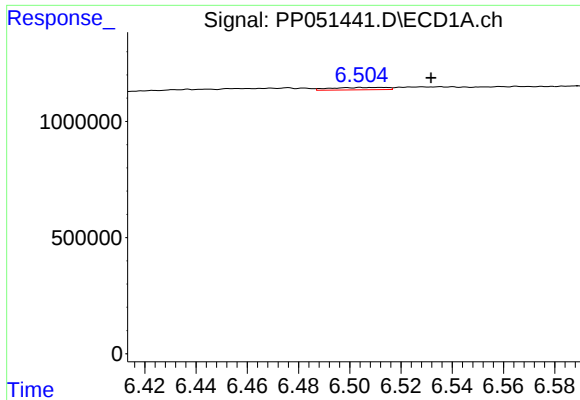

#25 AR-1248-5


R.T.: 6.504 min
Delta R.T.: -0.027 min
Response: 155485
Conc: 2.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

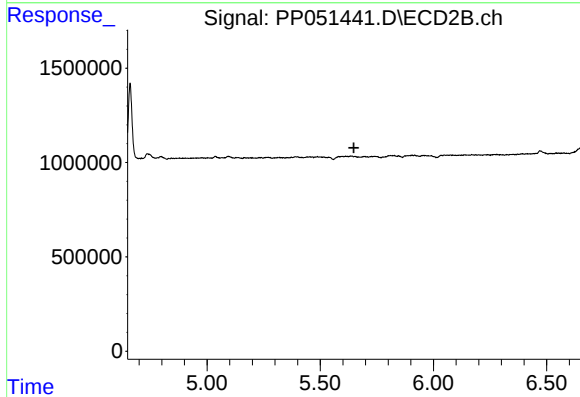


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.648 min
Response: 0
Conc: N.D.

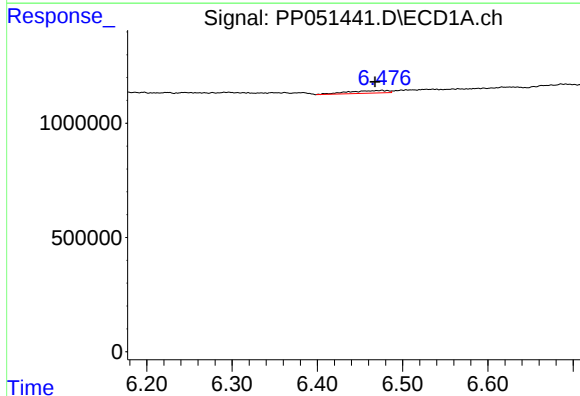


#26 AR-1254-1

R.T.: 6.476 min
Delta R.T.: 0.008 min
Response: 377434
Conc: 6.07 ng/ml

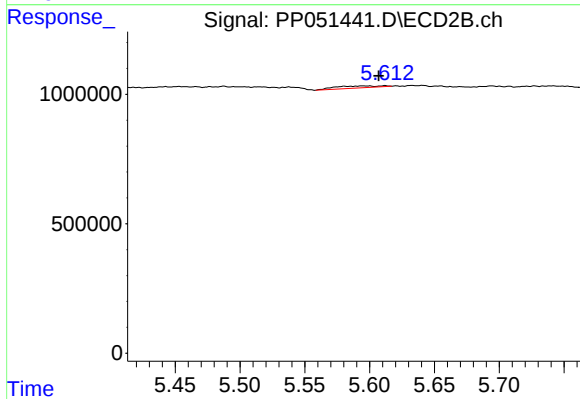

#26 AR-1254-1


R.T.: 5.612 min
Delta R.T.: 0.005 min
Response: 188095
Conc: 2.32 ng/ml

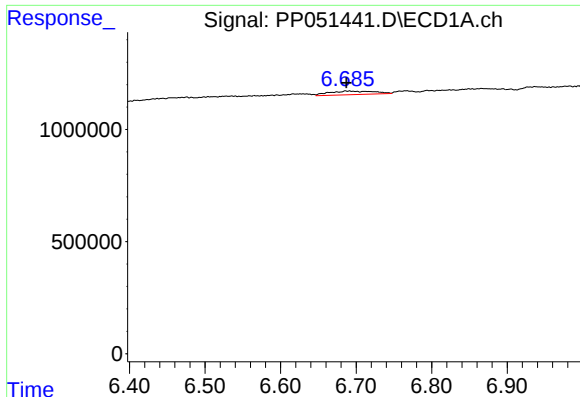

#27 AR-1254-2


R.T.: 6.689 min
Delta R.T.: 0.002 min
Response: 669215
Conc: 5.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

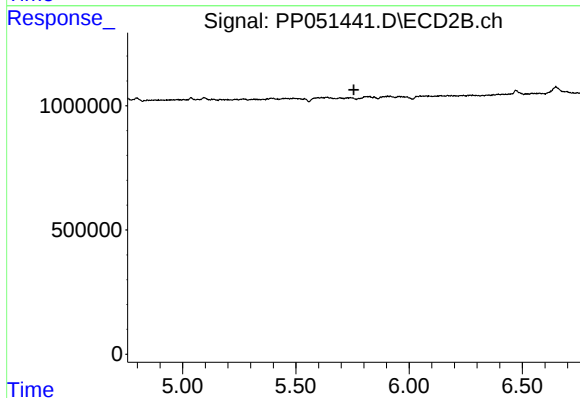


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.756 min
Response: 0
Conc: N.D.

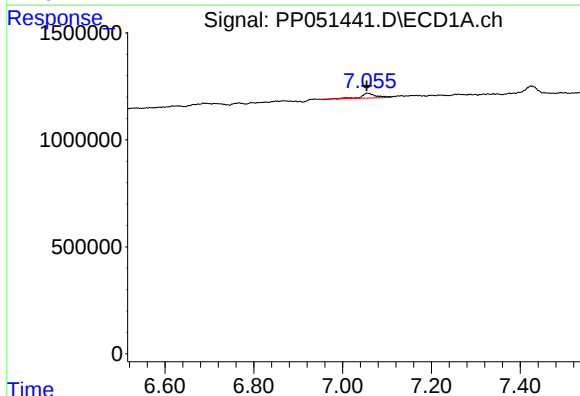


#28 AR-1254-3

R.T.: 7.056 min
Delta R.T.: 0.002 min
Response: 489121
Conc: 4.02 ng/ml

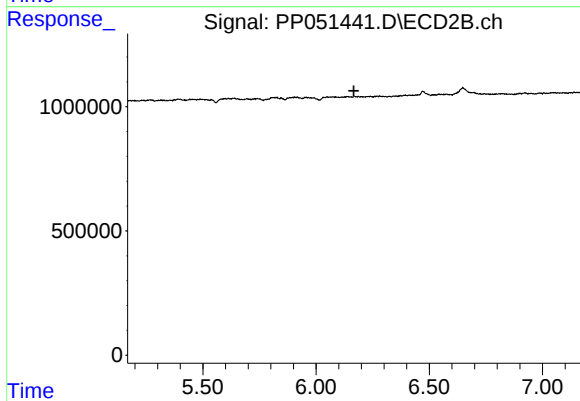

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.167 min
Response: 0
Conc: N.D.

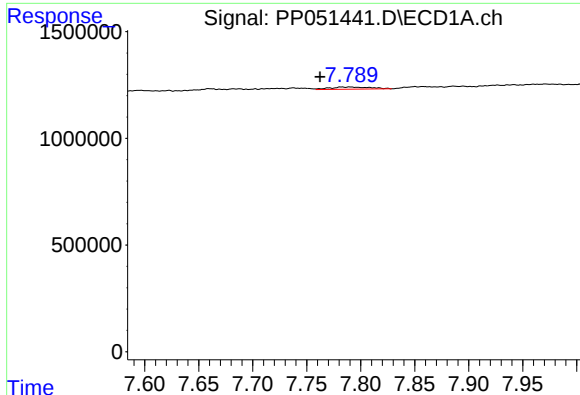

#30 AR-1254-5


R.T.: 7.790 min
Delta R.T.: 0.027 min
Response: 270697
Conc: 3.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

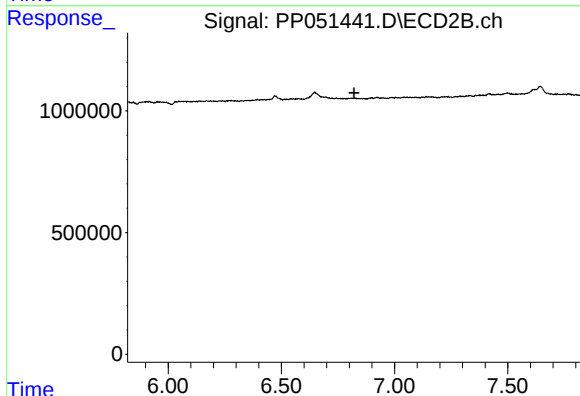


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.821 min
Response: 0
Conc: N.D.

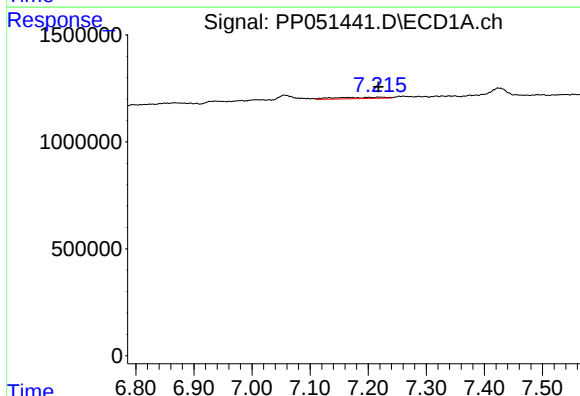


#31 AR-1260-1

R.T.: 7.220 min
Delta R.T.: 0.002 min
Response: 346949
Conc: 3.72 ng/ml

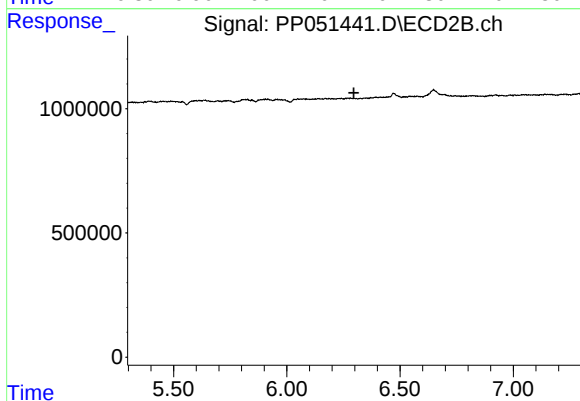

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

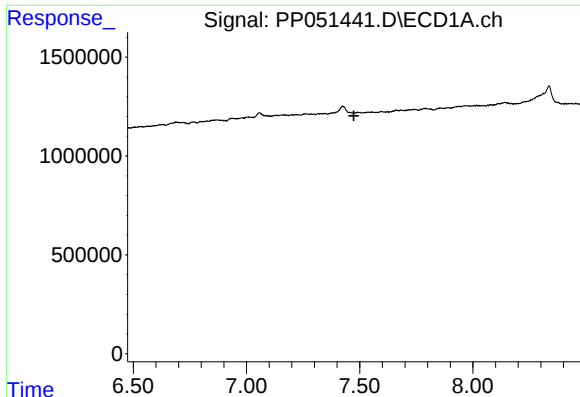

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

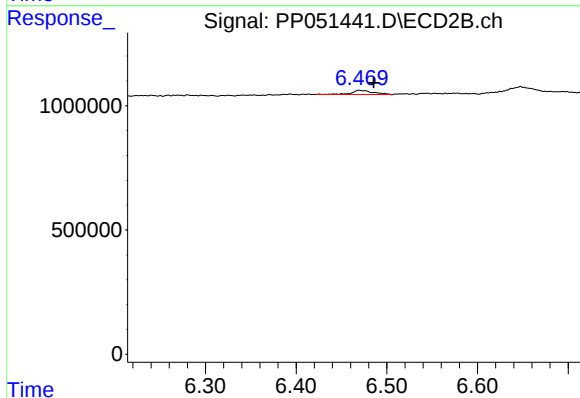


#32 AR-1260-2

R.T.: 6.470 min
Delta R.T.: -0.016 min
Response: 284360
Conc: 3.22 ng/ml

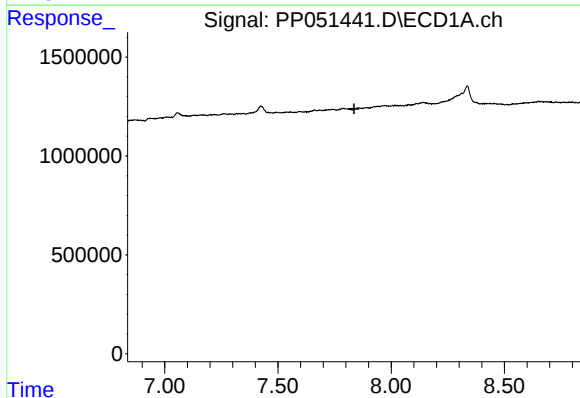


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.836 min
Response: 0
Conc: N.D.

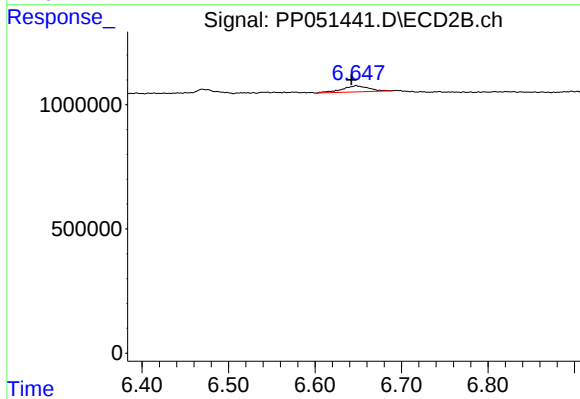

#33 AR-1260-3


R.T.: 6.647 min
Delta R.T.: 0.005 min
Response: 525430
Conc: 6.20 ng/ml

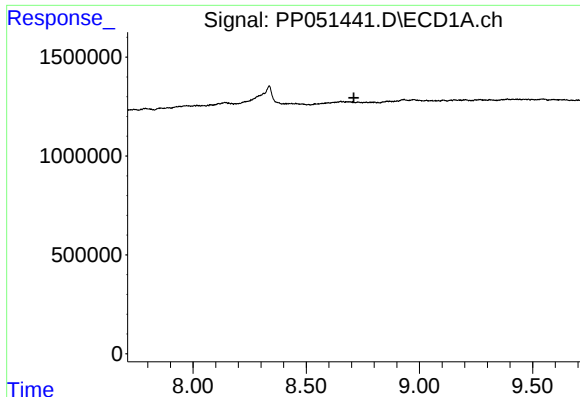

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-33A

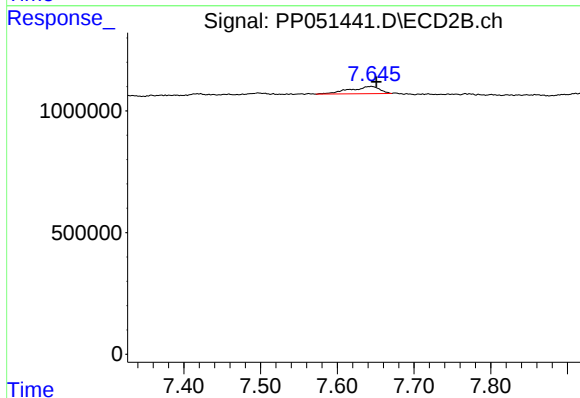


#38 AR-1262-3

R.T.: 7.645 min
Delta R.T.: -0.006 min
Response: 809858
Conc: 12.49 ng/ml

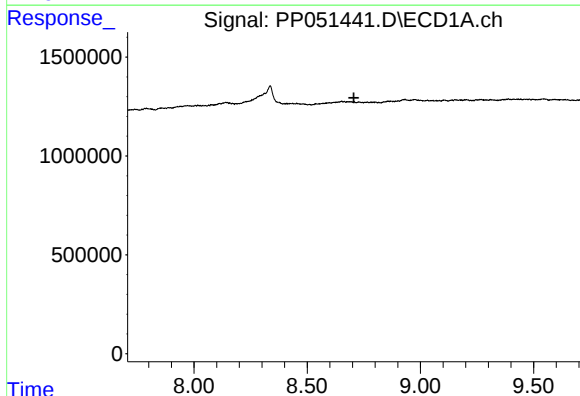

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

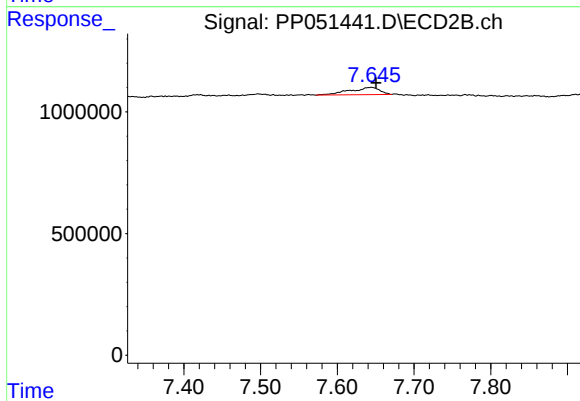

#41 AR-1268-1

R.T.: 7.645 min
Delta R.T.: -0.006 min
Response: 809858
Conc: 4.30 ng/ml