

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 06:11
 Operator : YP\AJ
 Sample : N4698-10 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-34A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 07:03:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.431	3.685	2781027	2215869	1.565	1.467
2)	SA Decachlor...	10.256	8.787	2606097	2084911	1.686	1.740
Target Compounds							
5)	L1 AR-1016-3	5.677	0.000	170044	0	3.108	N.D. #
18)	L4 AR-1242-3	5.677	0.000	170044	0	3.593	N.D. #
20)	L4 AR-1242-5	6.534	0.000	154337	0	4.328	N.D. #
25)	L5 AR-1248-5	6.534	0.000	154337	0	2.473	N.D. #
27)	L6 AR-1254-2	6.693	0.000	64776	0	0.561	N.D. #
28)	L6 AR-1254-3	7.055	0.000	226244	0	1.859	N.D. #
30)	L6 AR-1254-5	7.791f	0.000	235484	0	2.643	N.D. #
33)	L7 AR-1260-3	7.838	6.645	68266	430820	0.884	5.080 #
34)	L7 AR-1260-4	8.045f	0.000	256693	0	2.893	N.D. #
36)	L8 AR-1262-1	7.838	0.000	68266	0	0.666	N.D. #
38)	L8 AR-1262-3	0.000	7.644	0	531859	N.D.	8.203 #
41)	L9 AR-1268-1	0.000	7.644	0	531859	N.D.	2.821 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 06:11
Operator : YP\AJ
Sample : N4698-10 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 07:03:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

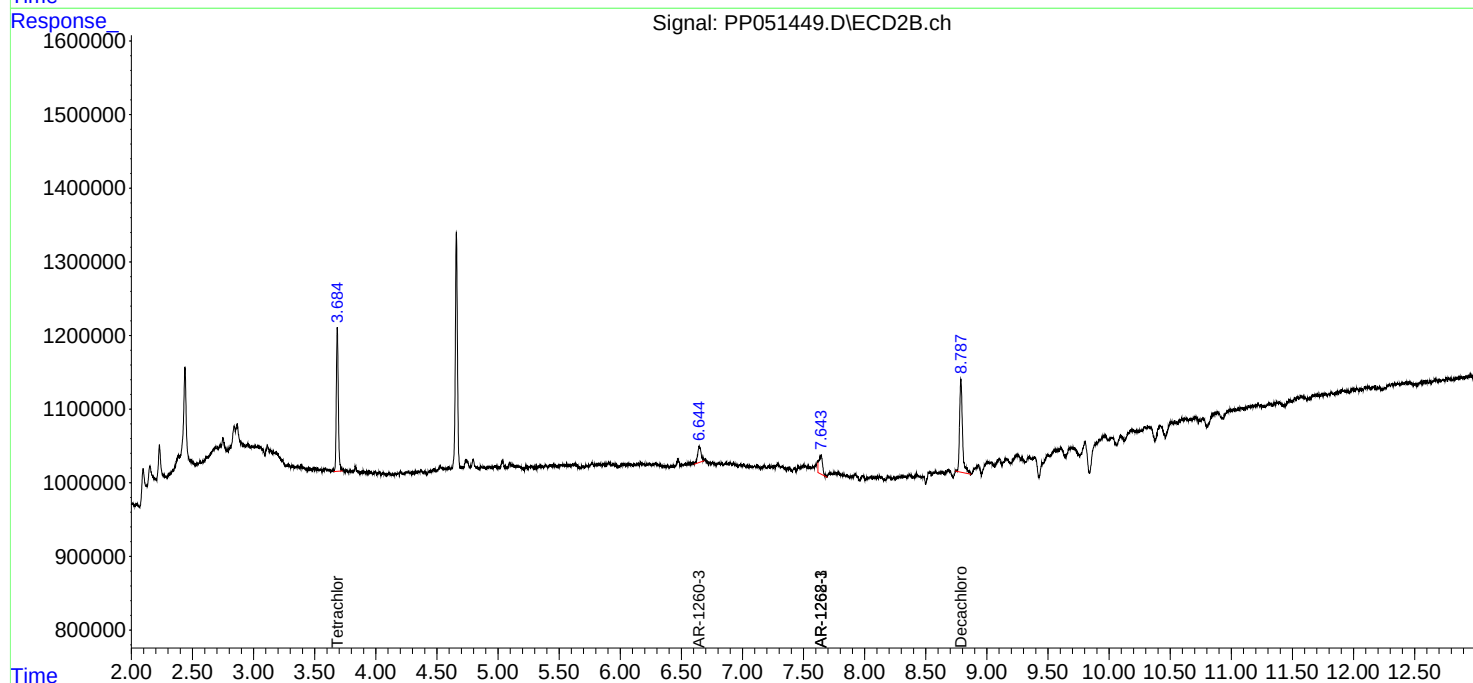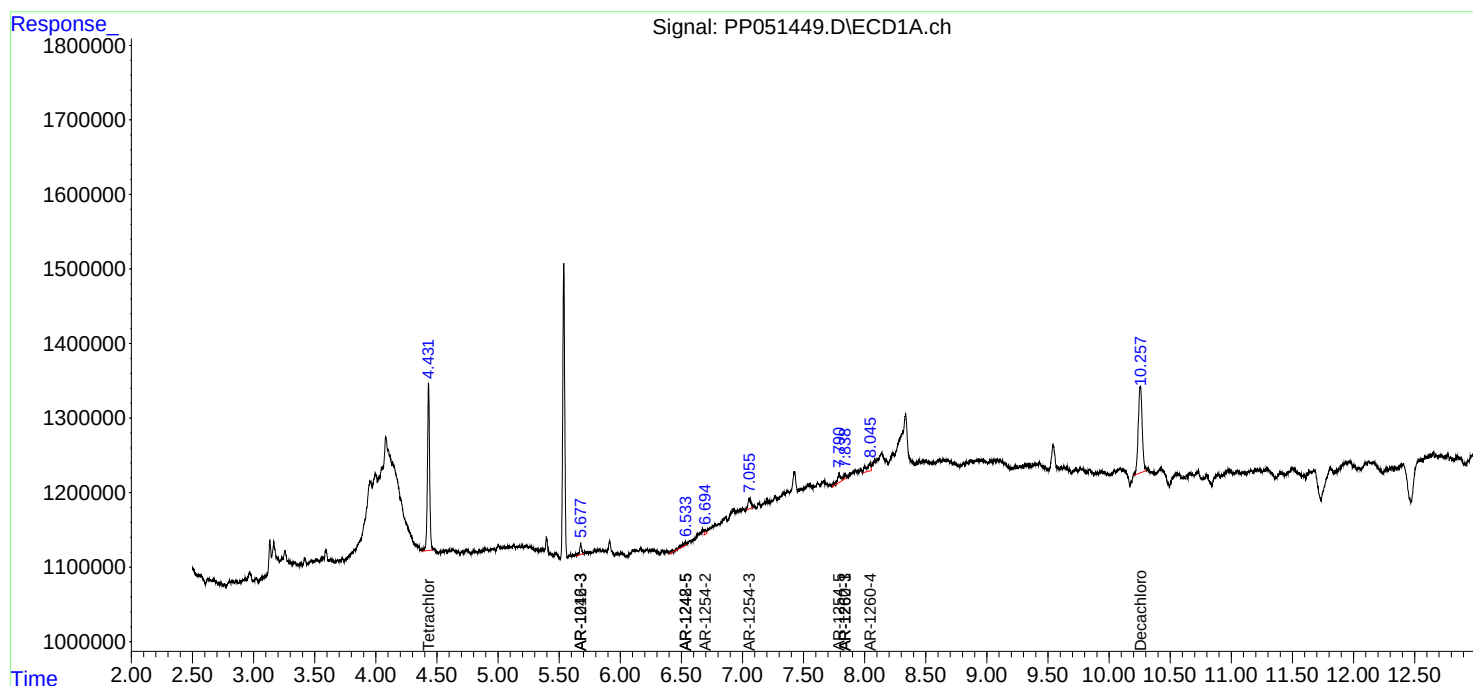


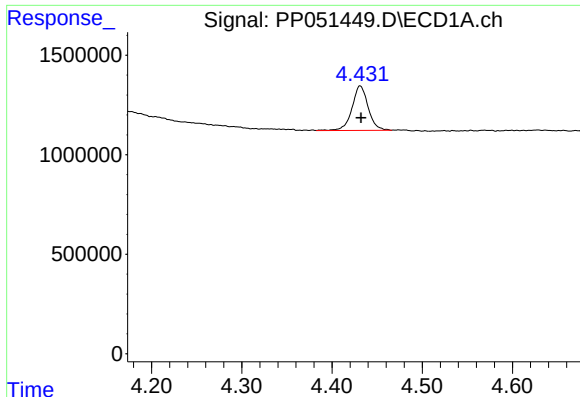

#1 Tetrachloro-m-xylene


R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 2781027
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

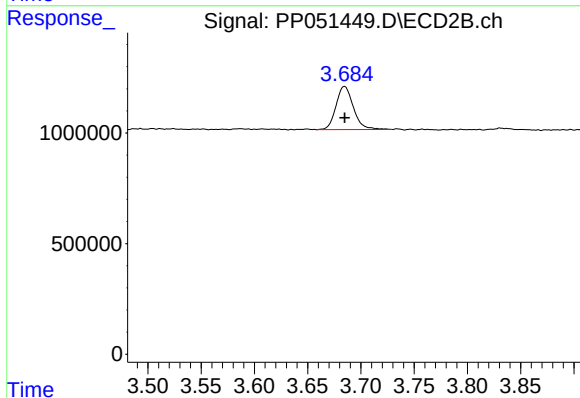


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 2215869
Conc: 1.47 ng/ml

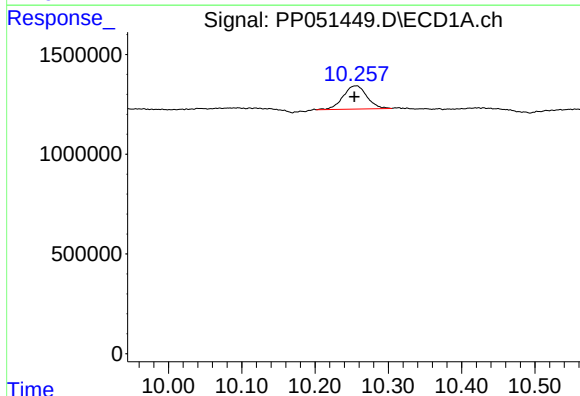


#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.002 min
Response: 2606097
Conc: 1.69 ng/ml

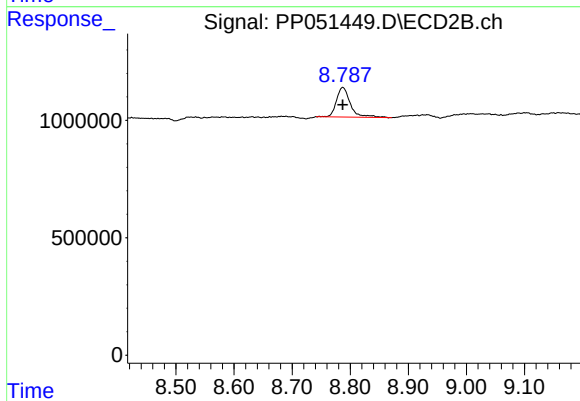

#2 Decachlorobiphenyl


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 2084911
Conc: 1.74 ng/ml

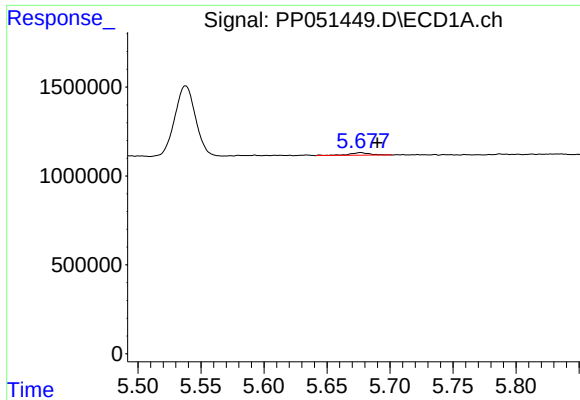

#5 AR-1016-3


R.T.: 5.677 min
Delta R.T.: -0.014 min
Response: 170044
Conc: 3.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

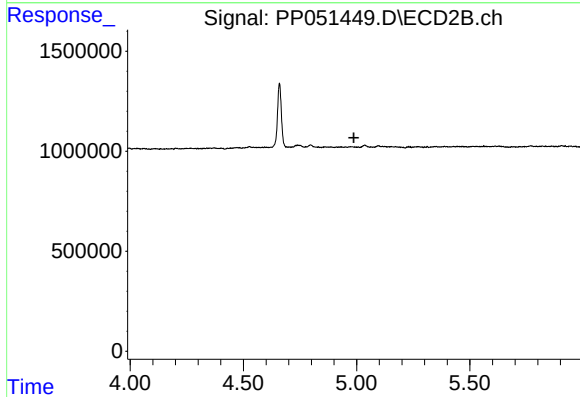


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

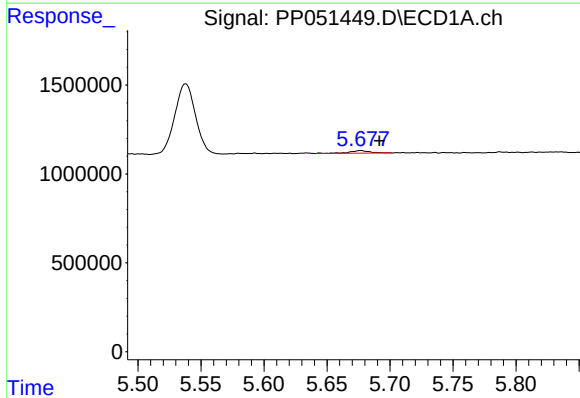


#18 AR-1242-3

R.T.: 5.677 min
Delta R.T.: -0.015 min
Response: 170044
Conc: 3.59 ng/ml

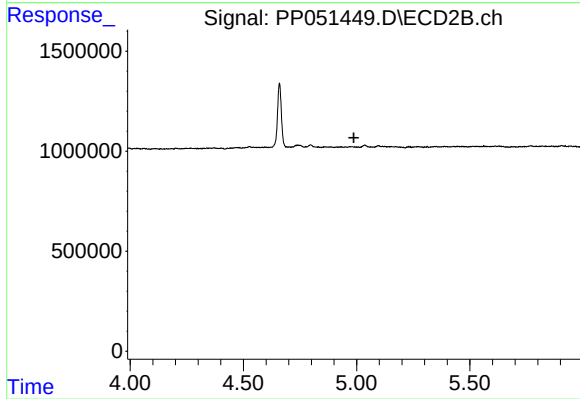

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

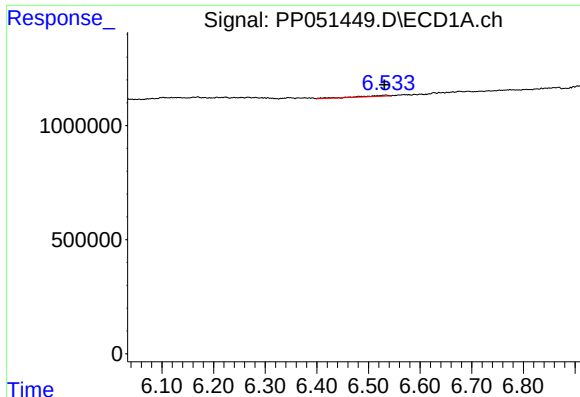

#20 AR-1242-5


R.T.: 6.534 min
Delta R.T.: 0.003 min
Response: 154337
Conc: 4.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

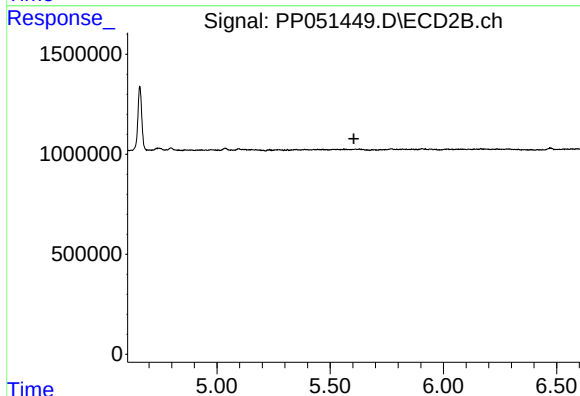


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.604 min
Response: 0
Conc: N.D.

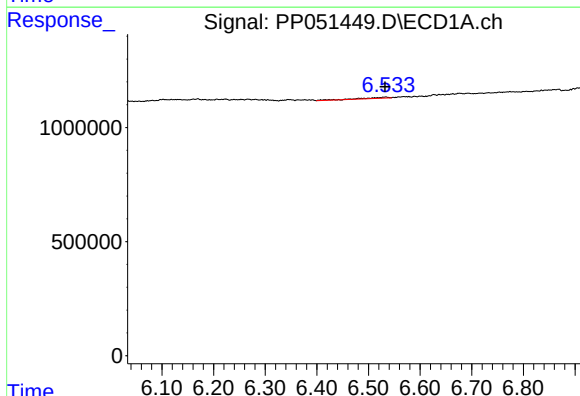


#25 AR-1248-5

R.T.: 6.534 min
Delta R.T.: 0.002 min
Response: 154337
Conc: 2.47 ng/ml

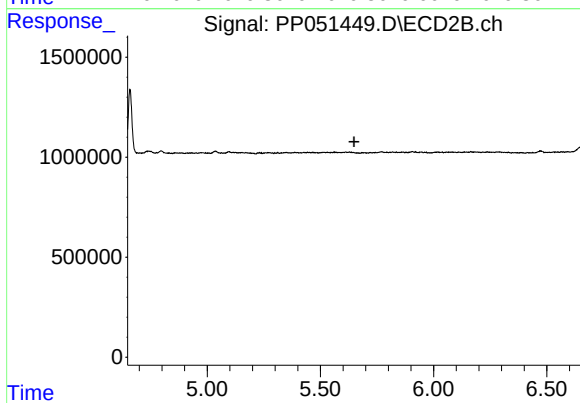

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.648 min
Response: 0
Conc: N.D.

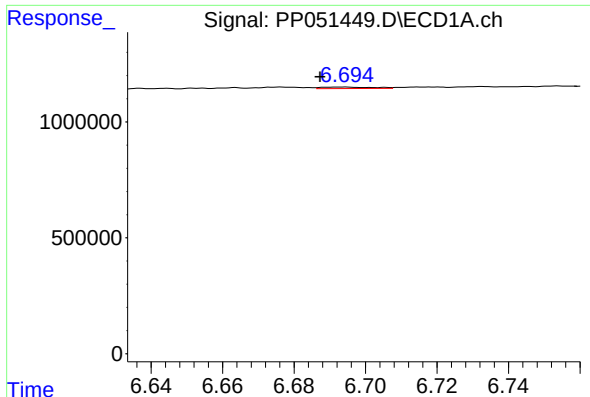

#27 AR-1254-2


R.T.: 6.693 min
Delta R.T.: 0.006 min
Response: 64776
Conc: 0.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

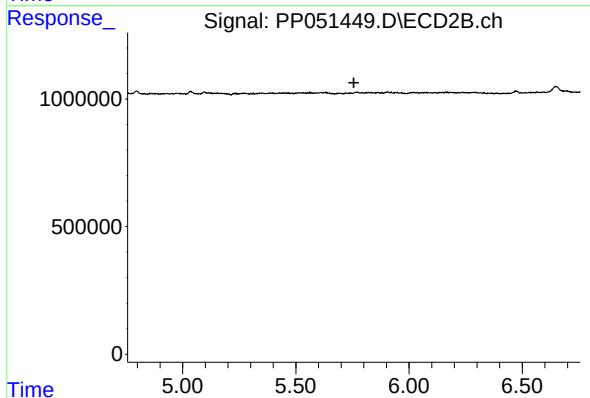


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.756 min
Response: 0
Conc: N.D.

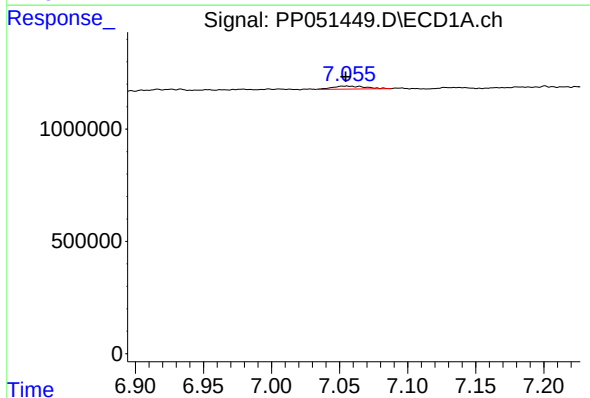


#28 AR-1254-3

R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 226244
Conc: 1.86 ng/ml

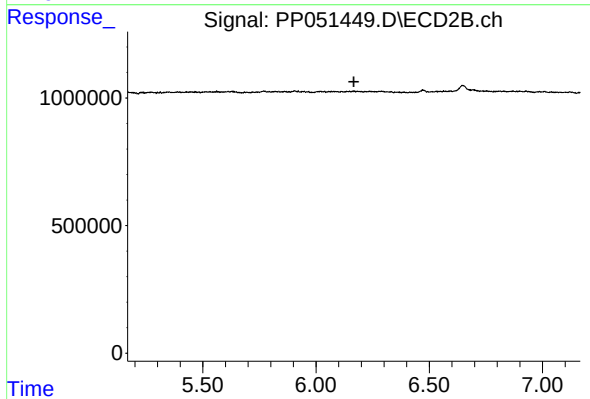

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.167 min
Response: 0
Conc: N.D.

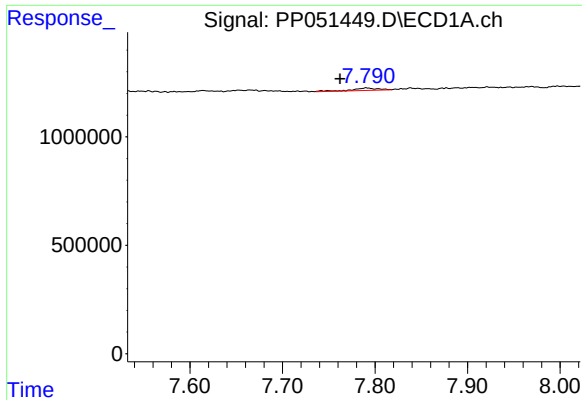

#30 AR-1254-5


R.T.: 7.791 min
Delta R.T.: 0.028 min
Response: 235484
Conc: 2.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

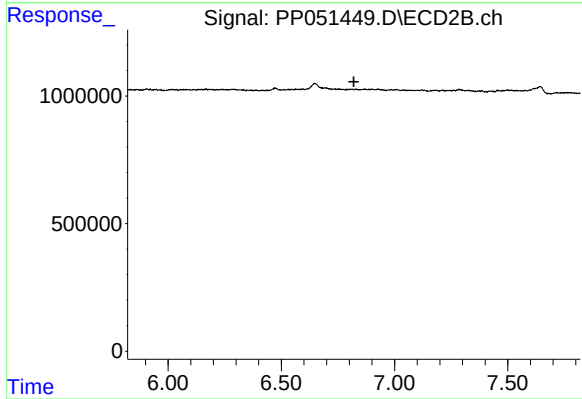


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.821 min
Response: 0
Conc: N.D.

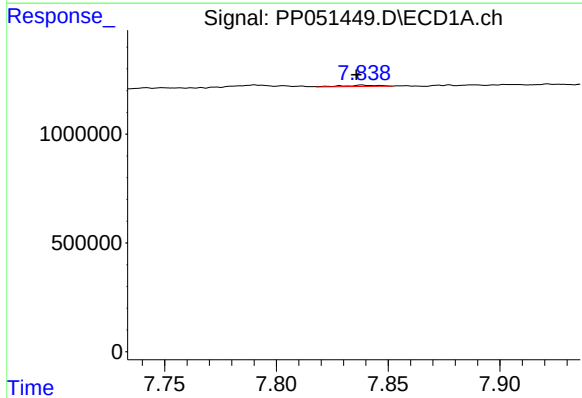


#33 AR-1260-3

R.T.: 7.838 min
Delta R.T.: 0.003 min
Response: 68266
Conc: 0.88 ng/ml

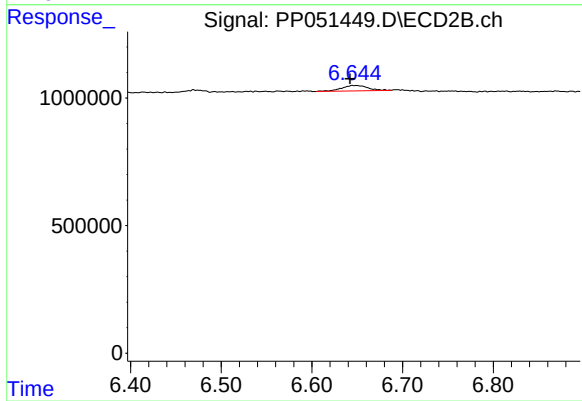

#33 AR-1260-3


R.T.: 6.645 min
Delta R.T.: 0.003 min
Response: 430820
Conc: 5.08 ng/ml

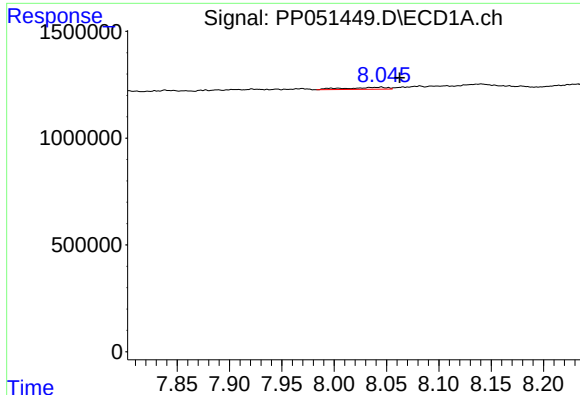

#34 AR-1260-4


R.T.: 8.045 min
Delta R.T.: -0.018 min
Response: 256693
Conc: 2.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

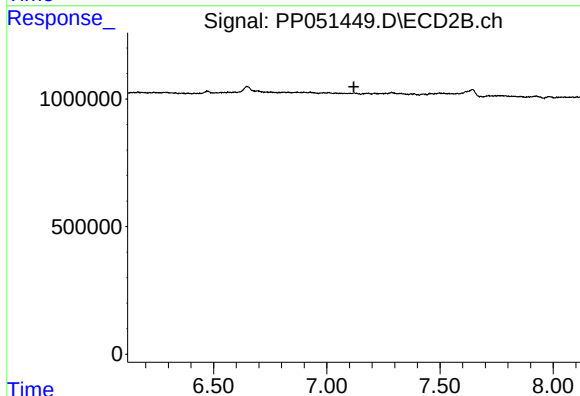


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

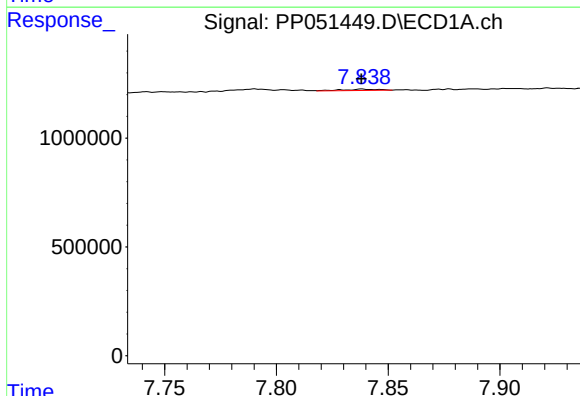


#36 AR-1262-1

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 68266
Conc: 0.67 ng/ml

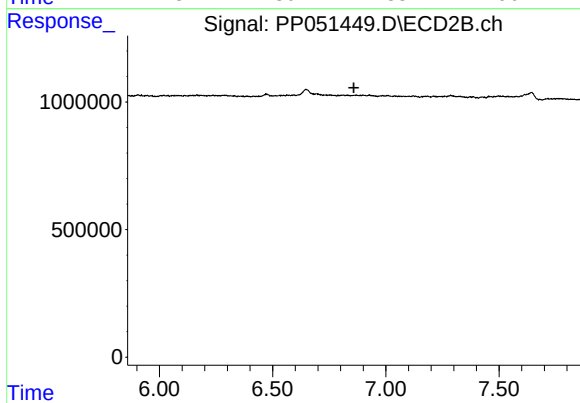

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

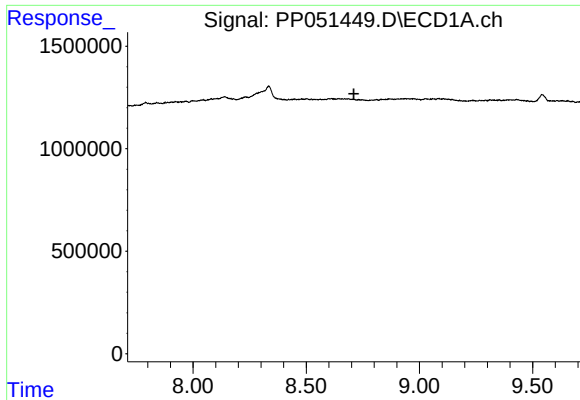

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34A

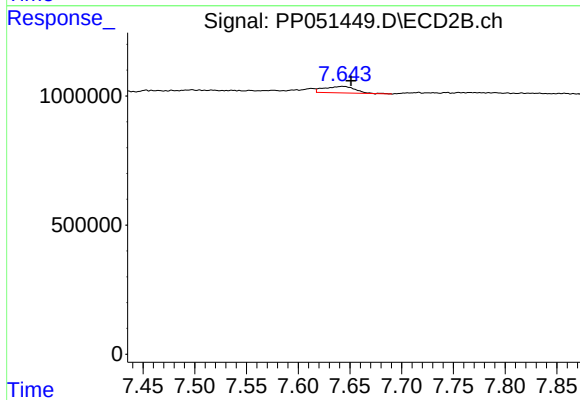


#38 AR-1262-3

R.T.: 7.644 min
Delta R.T.: -0.007 min
Response: 531859
Conc: 8.20 ng/ml

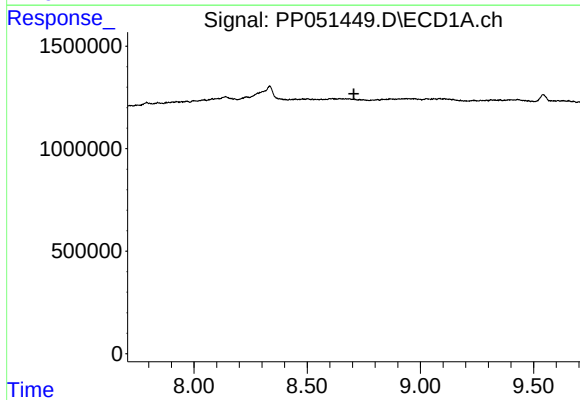

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

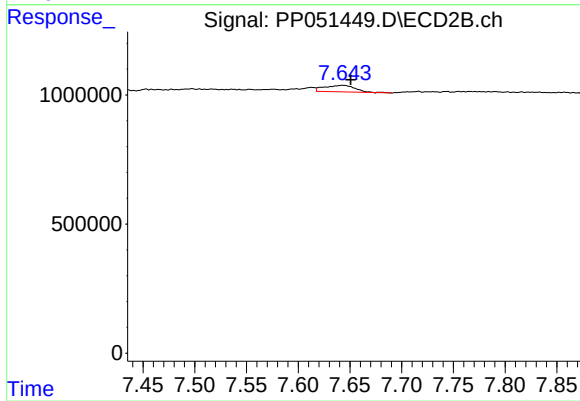

#41 AR-1268-1

R.T.: 7.644 min
Delta R.T.: -0.007 min
Response: 531859
Conc: 2.82 ng/ml