

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 06:27
 Operator : YP\AJ
 Sample : N4698-11 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-34B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 07:03:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.685	3137561	2214922	1.766	1.466
2) SA Decachlor...	10.256	8.787	2413736	2144726	1.562	1.790
Target Compounds						
5) L1 AR-1016-3	5.676	0.000	112019	0	2.047	N.D. #
18) L4 AR-1242-3	5.676f	0.000	112019	0	2.367	N.D. #
27) L6 AR-1254-2	6.690	0.000	41166	0	0.357	N.D. #
28) L6 AR-1254-3	7.056	0.000	365027	0	2.999	N.D. #
30) L6 AR-1254-5	7.772	0.000	84870	0	0.953	N.D. #
31) L7 AR-1260-1	7.192f	0.000	42437	0	0.455	N.D. #
32) L7 AR-1260-2	7.489	0.000	283424	0	2.684	N.D. #
33) L7 AR-1260-3	7.863f	6.648	210805	454508	2.729	5.359 #
36) L8 AR-1262-1	7.863f	0.000	210805	0	2.056	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 06:27
Operator : YP\AJ
Sample : N4698-11 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 07:03:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

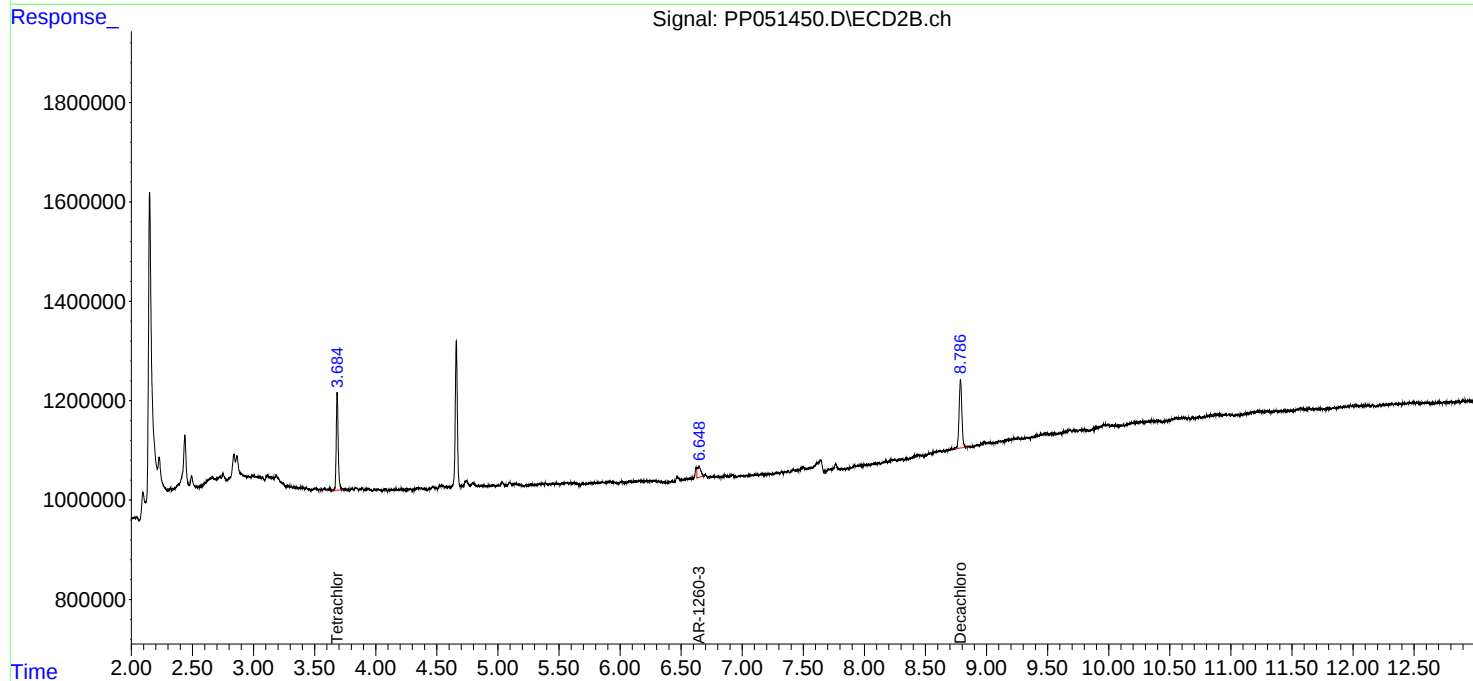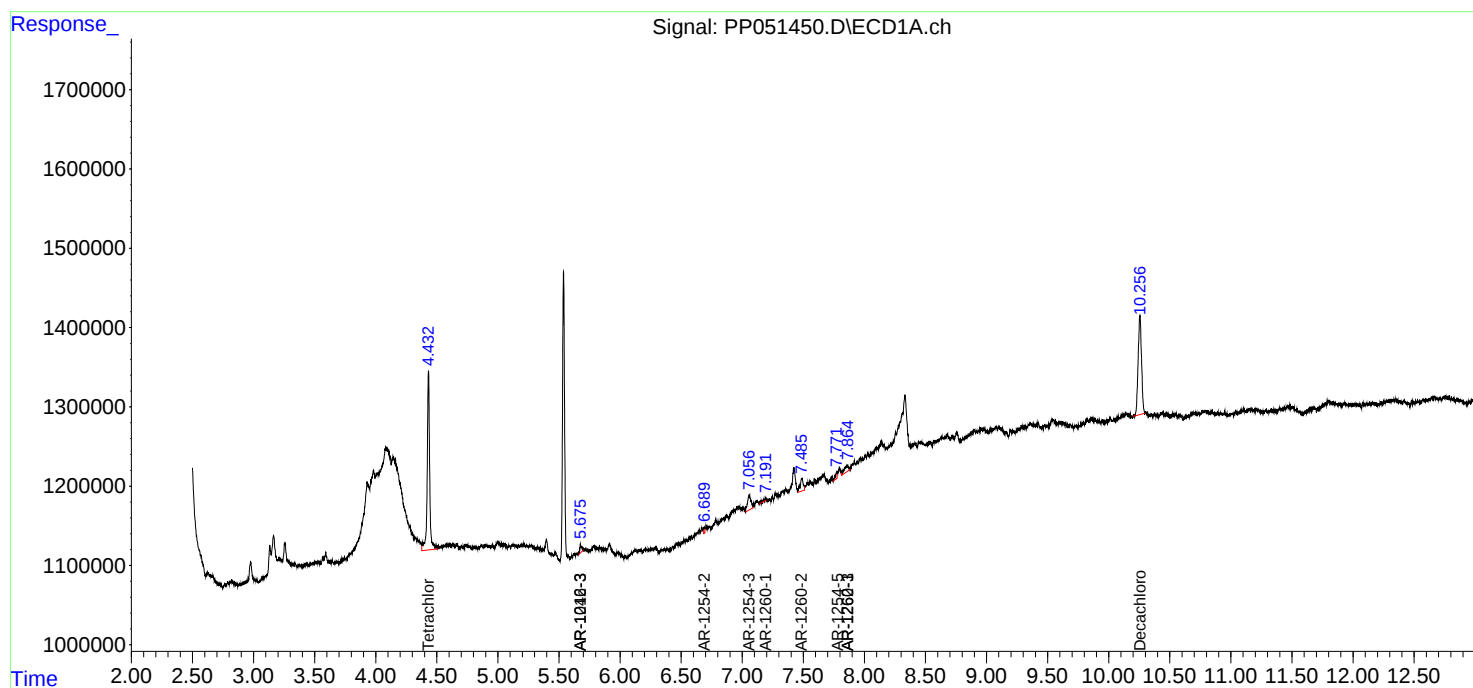


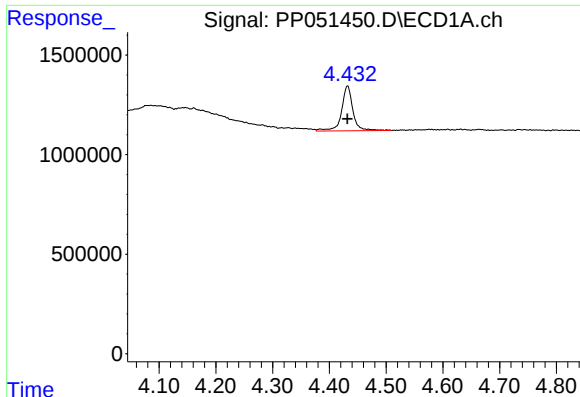

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: 0.000 min
Response: 3137561
Conc: 1.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

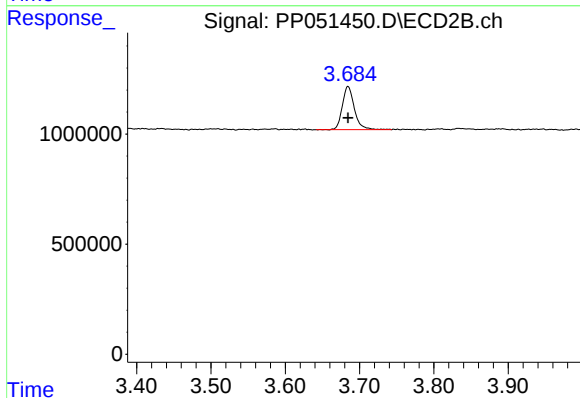


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 2214922
Conc: 1.47 ng/ml

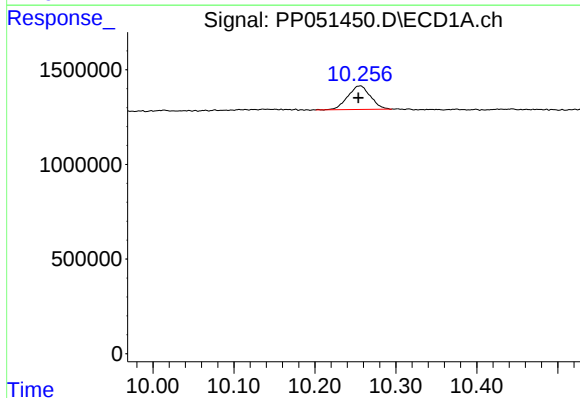


#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.002 min
Response: 2413736
Conc: 1.56 ng/ml

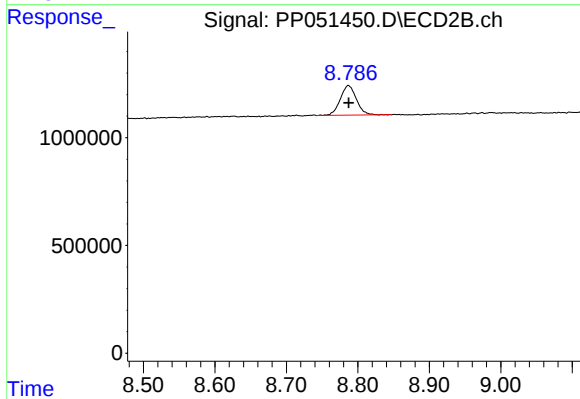

#2 Decachlorobiphenyl


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 2144726
Conc: 1.79 ng/ml

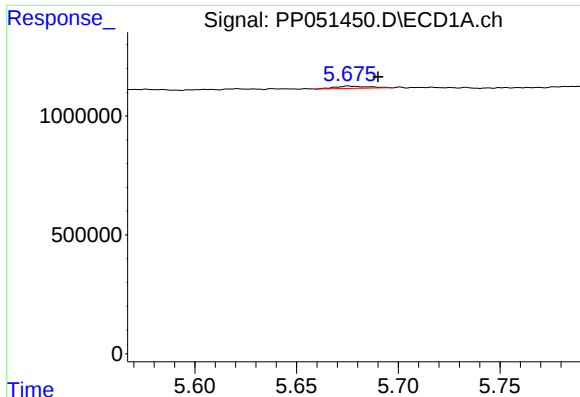

#5 AR-1016-3


R.T.: 5.676 min
Delta R.T.: -0.015 min
Response: 112019
Conc: 2.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

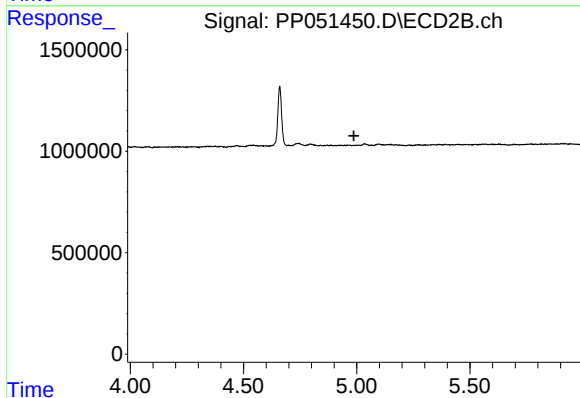


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

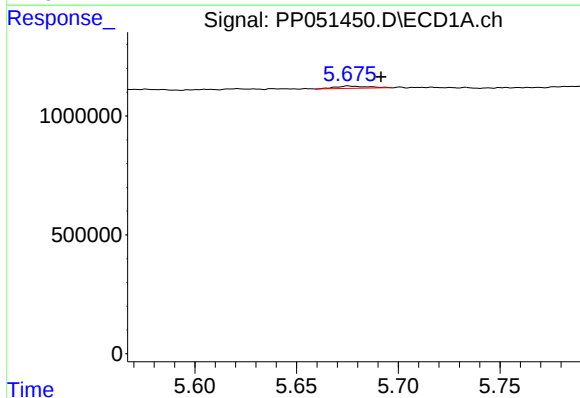


#18 AR-1242-3

R.T.: 5.676 min
Delta R.T.: -0.016 min
Response: 112019
Conc: 2.37 ng/ml

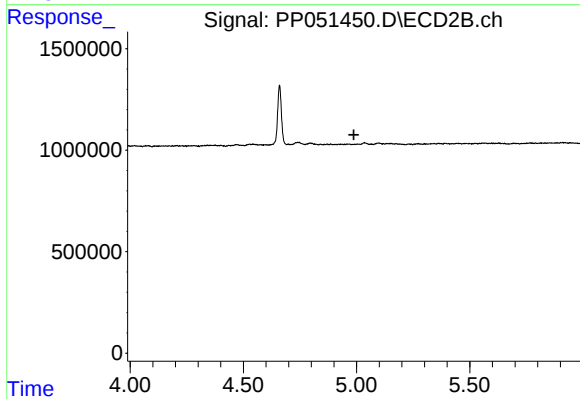

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

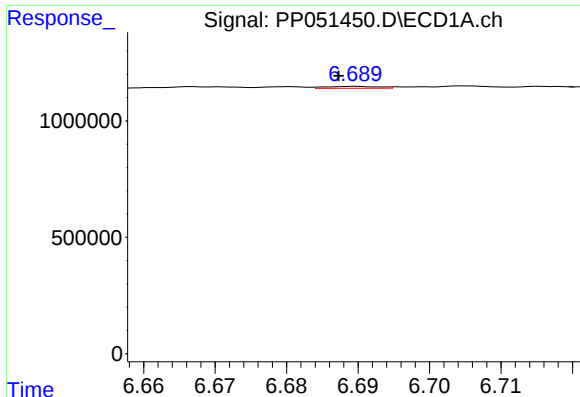

#27 AR-1254-2


R.T.: 6.690 min
Delta R.T.: 0.002 min
Response: 41166
Conc: 0.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

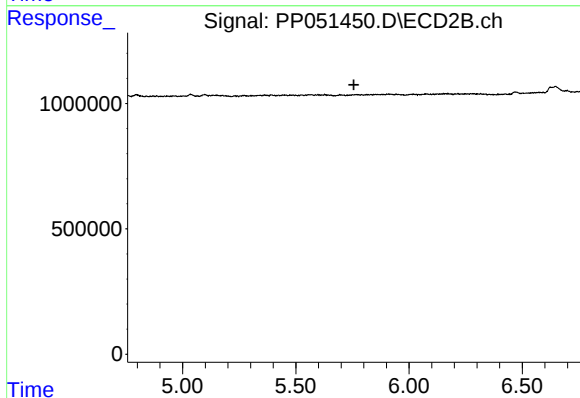


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.756 min
Response: 0
Conc: N.D.

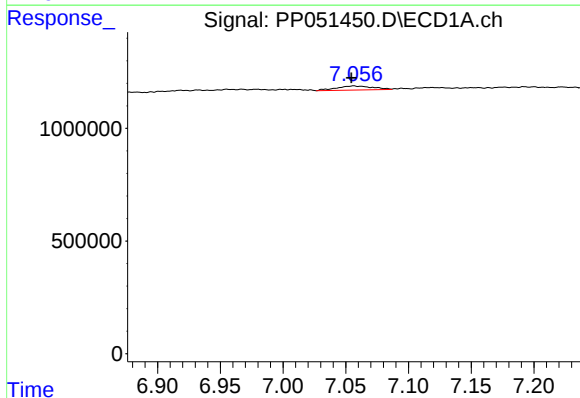


#28 AR-1254-3

R.T.: 7.056 min
Delta R.T.: 0.002 min
Response: 365027
Conc: 3.00 ng/ml

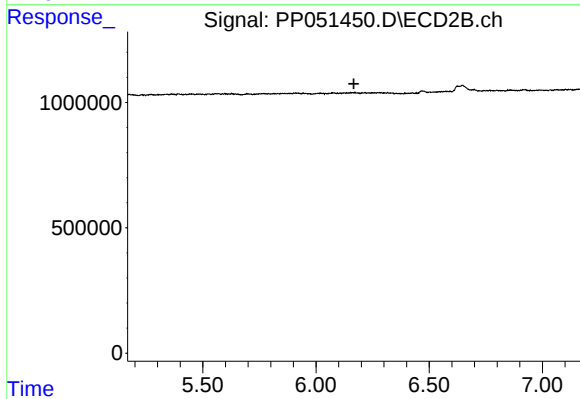

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.167 min
Response: 0
Conc: N.D.

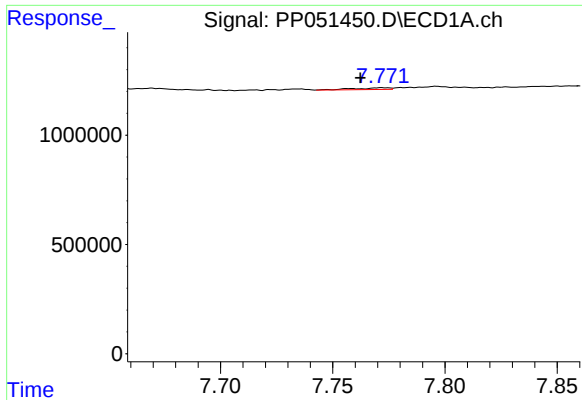

#30 AR-1254-5


R.T.: 7.772 min
Delta R.T.: 0.010 min
Response: 84870
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

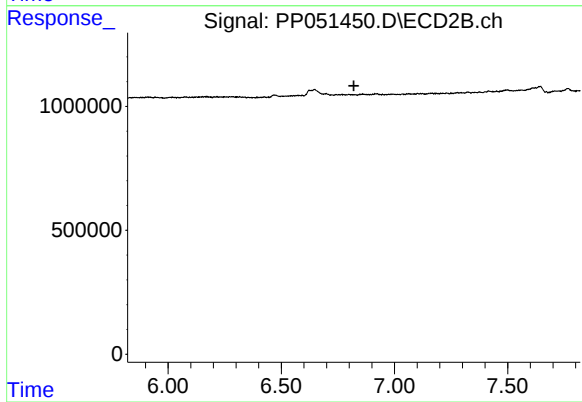


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.821 min
Response: 0
Conc: N.D.

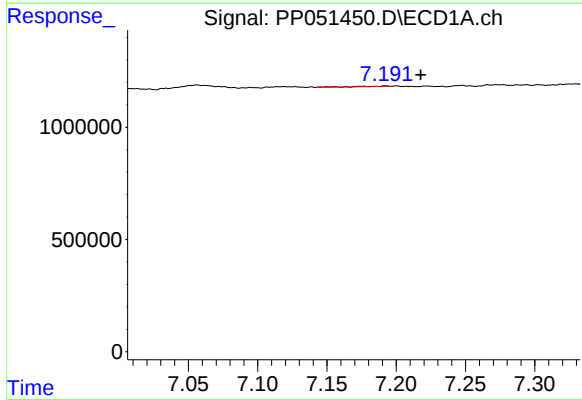


#31 AR-1260-1

R.T.: 7.192 min
Delta R.T.: -0.025 min
Response: 42437
Conc: 0.45 ng/ml

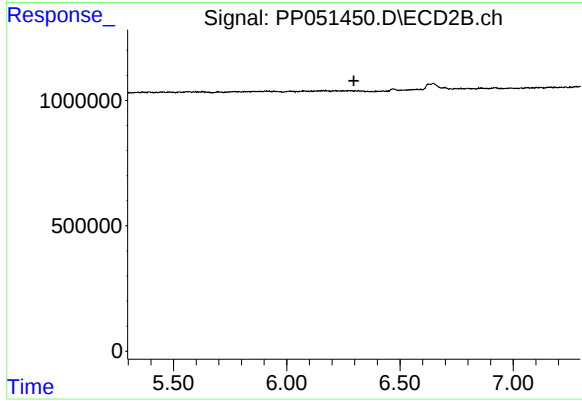

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

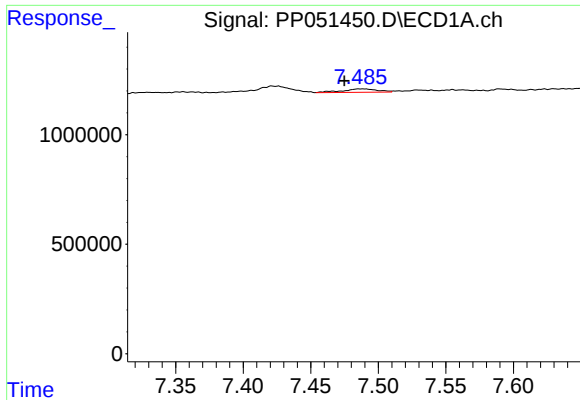

#32 AR-1260-2


R.T.: 7.489 min
Delta R.T.: 0.014 min
Response: 283424
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

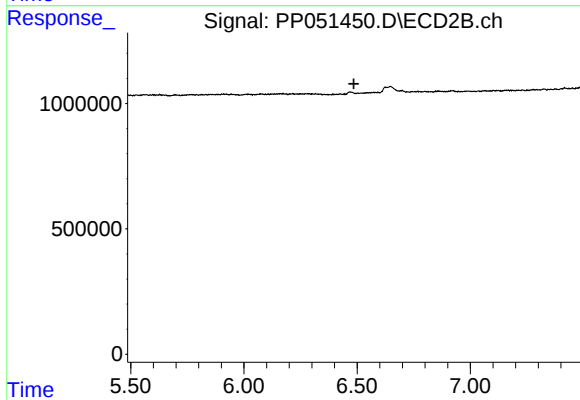


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

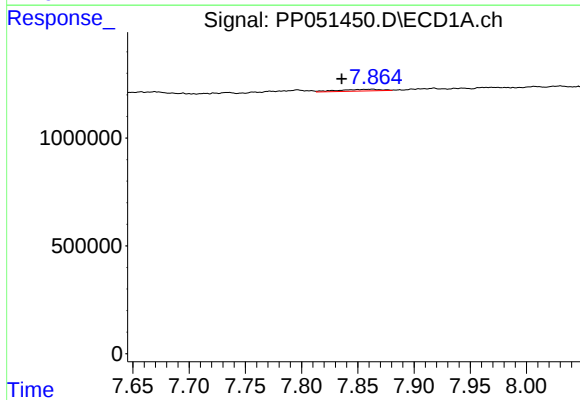


#33 AR-1260-3

R.T.: 7.863 min
Delta R.T.: 0.027 min
Response: 210805
Conc: 2.73 ng/ml

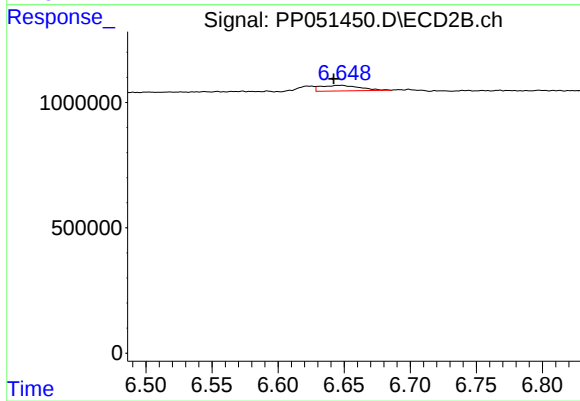

#33 AR-1260-3


R.T.: 6.648 min
Delta R.T.: 0.005 min
Response: 454508
Conc: 5.36 ng/ml

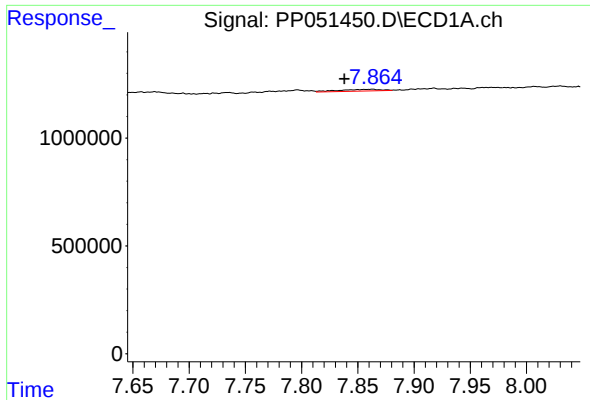

#36 AR-1262-1

R.T.: 7.863 min
Delta R.T.: 0.025 min
Response: 210805
Conc: 2.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-34B

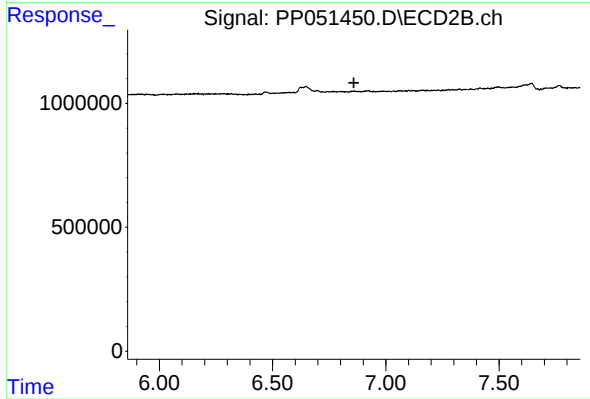

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.