

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 07:17
 Operator : YP\AJ
 Sample : N4699-02 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226538LOZ-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/20/2022
 Supervised By :Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 08:27:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.431	3.685	2770039	2572604	1.559m	1.703
2) SA Decachlor...	10.256	8.787	2581120	2275164	1.670	1.899

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 07:17
Operator : YP\AJ
Sample : N4699-02 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC226538LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2022
Supervised By :Ankita Jodhani 09/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 08:27:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

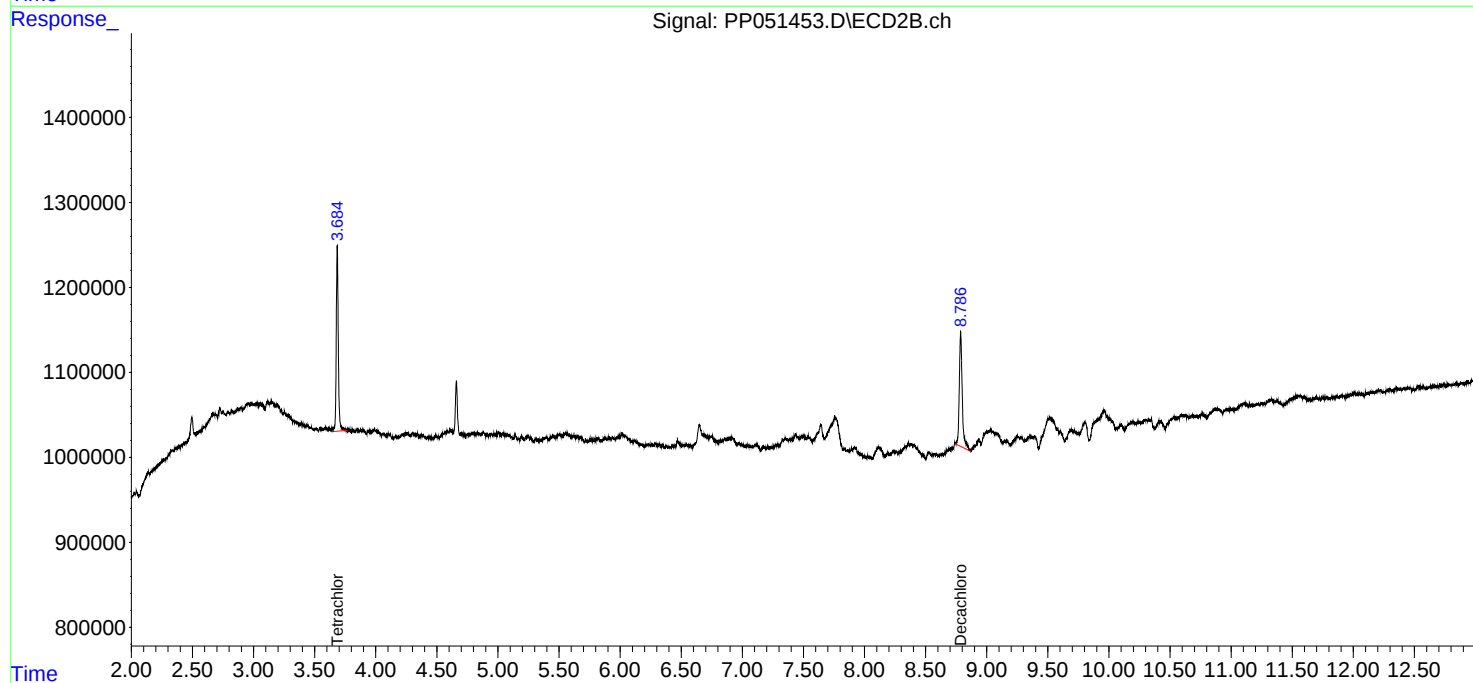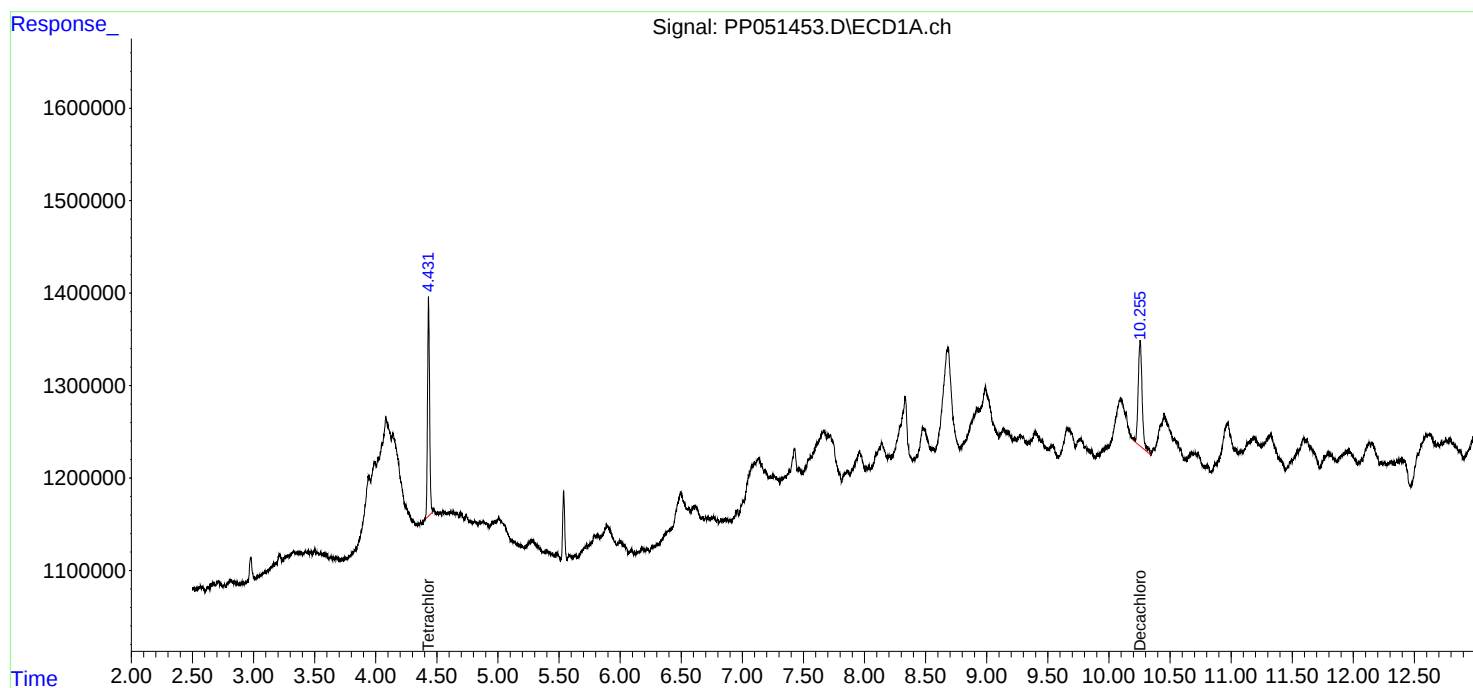

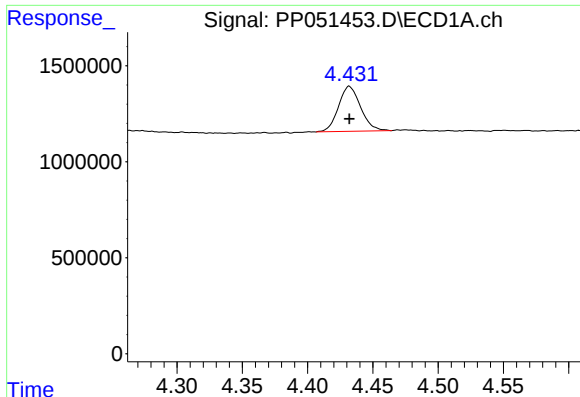


#1 Tetrachloro-m-xylene

R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 2770039
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226538LOZ-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2022
Supervised By :Ankita Jodhani 09/20/2022

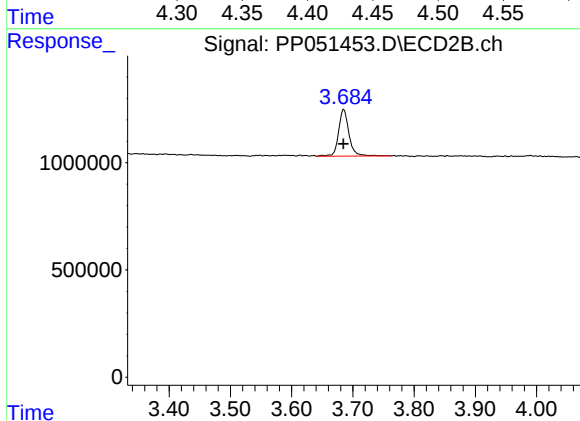


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 2572604
Conc: 1.70 ng/ml

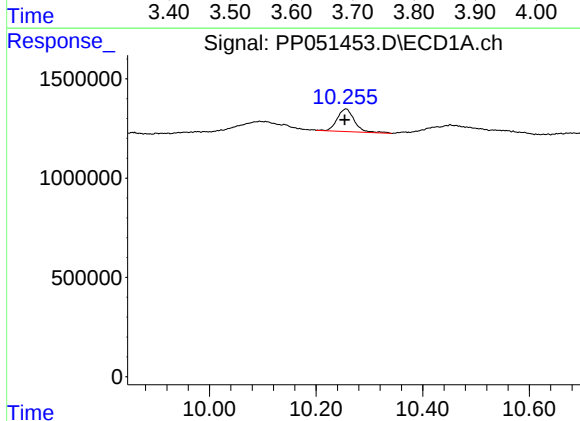

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.002 min
Response: 2581120
Conc: 1.67 ng/ml

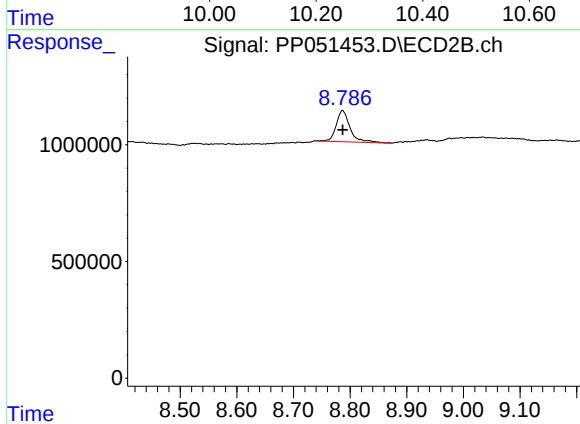

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 2275164
Conc: 1.90 ng/ml