

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
 Data File : PP059968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 21:09
 Operator : YP\AJ
 Sample : 04493-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/20/2023
 Supervised By :Ankita Jodhani 09/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:27:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.659	25062878	67944118	12.048m	41.712 #
2) SA Decachlor...	10.427	8.747	24379275	17619600	15.983m	11.636 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
Data File : PP059968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 21:09
Operator : YP\AJ
Sample : 04493-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:27:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

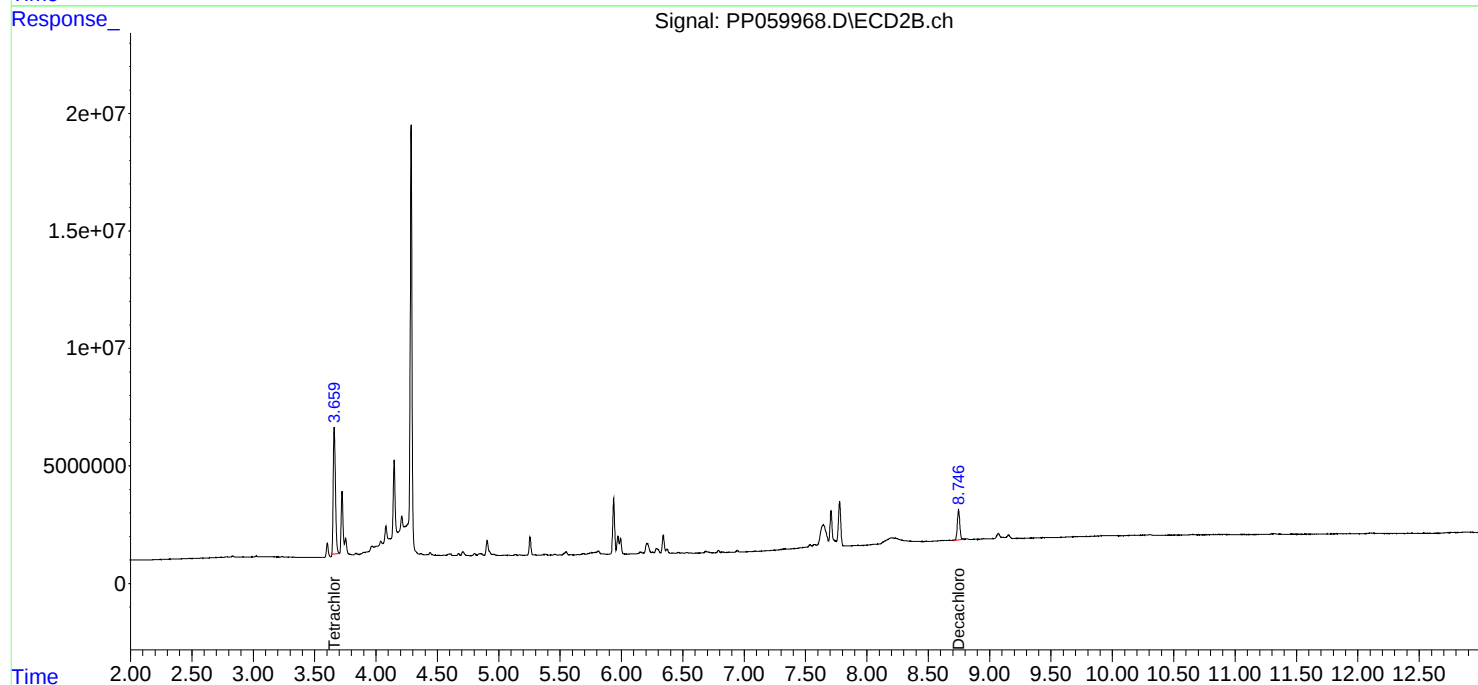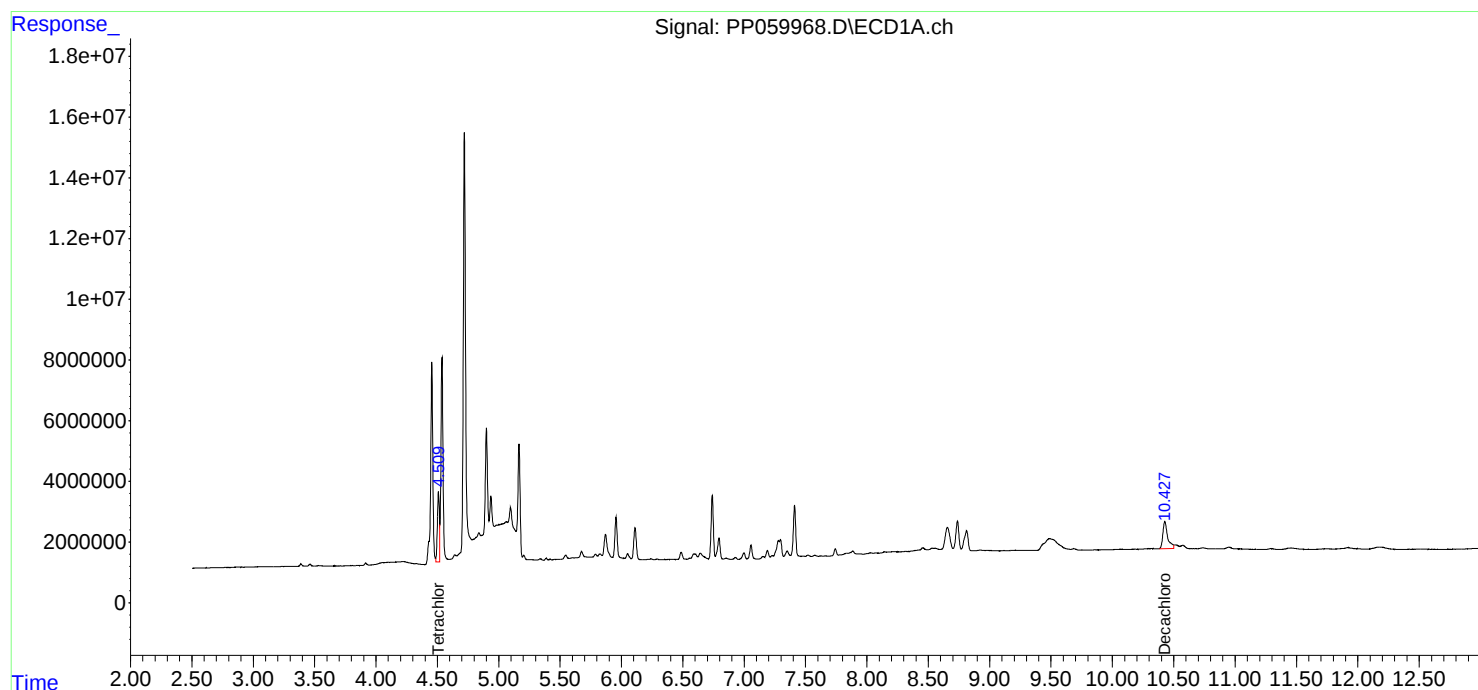

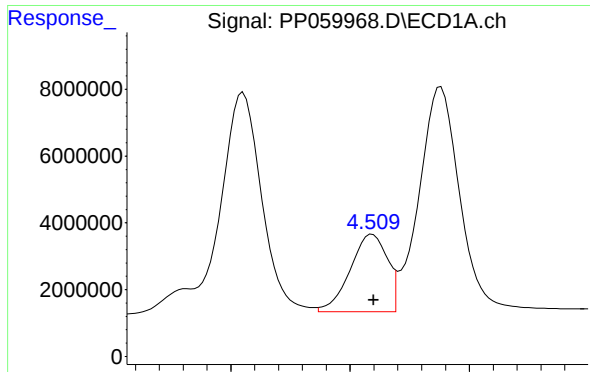


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: -0.001 min
Response: 25062878
Conc: 12.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

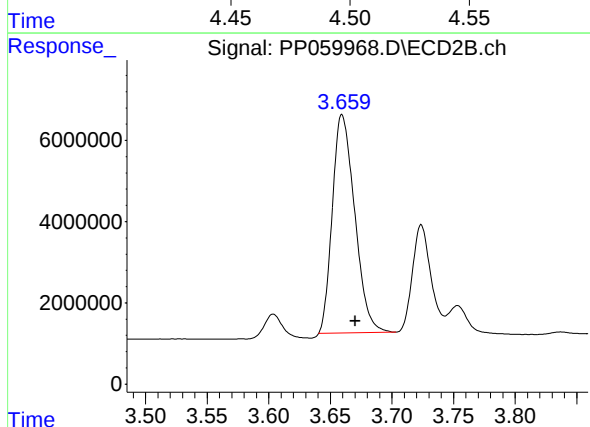


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.011 min
Response: 67944118
Conc: 41.71 ng/ml

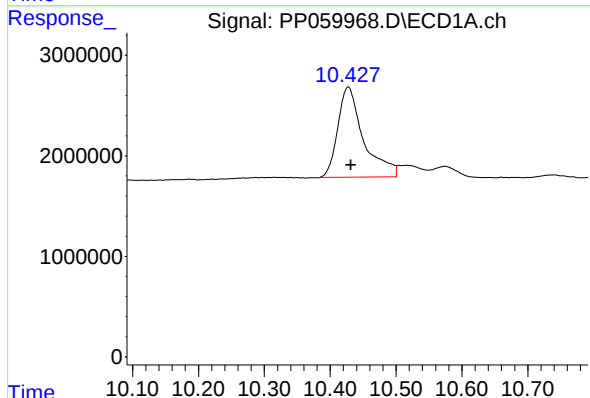

#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.005 min
Response: 24379275
Conc: 15.98 ng/ml m

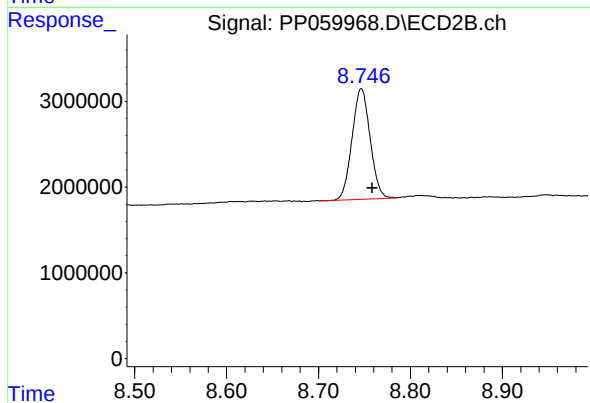

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.012 min
Response: 17619600
Conc: 11.64 ng/ml