

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
 Data File : PP059985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 02:06
 Operator : YP\AJ
 Sample : 04487-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 003

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/20/2023
 Supervised By :Ankita Jodhani 09/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 02:57:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.679	55032317	24331752	26.454	14.938 #
2) SA Decachlor...	10.427	8.744	33825279	28733701	22.176	18.977
Target Compounds						
26) L6 AR-1254-1	6.572	5.592	5364463	6434584	67.193m	64.117m
27) L6 AR-1254-2	6.797	5.743	6815556	3728224	56.904	42.914
28) L6 AR-1254-3	7.163	6.148	4710612	6361964	38.777m	45.313
29) L6 AR-1254-4	7.451	6.376	3460310	3429740	38.910m	40.745
30) L6 AR-1254-5	7.871	6.795	4994185	5383612	51.341m	45.386

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
Data File : PP059985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 02:06
Operator : YP\AJ
Sample : 04487-03
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 02:57:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

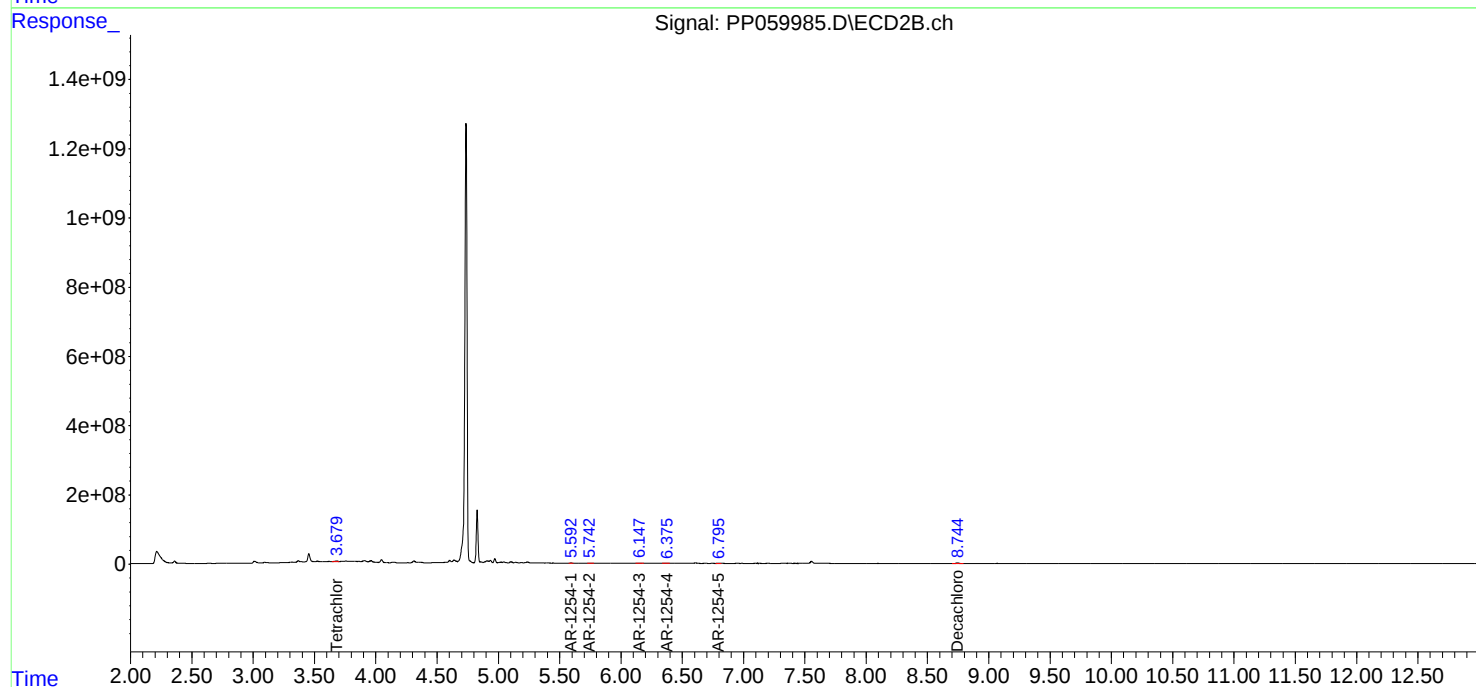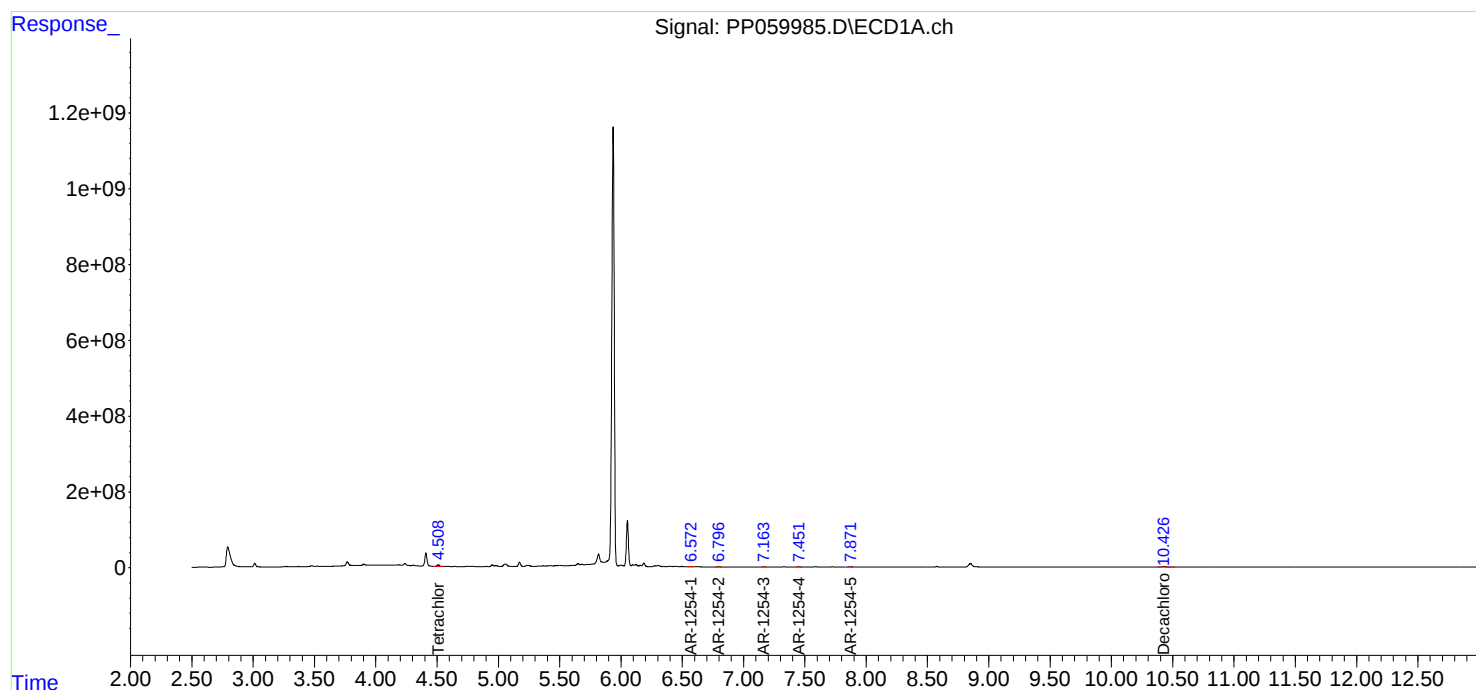

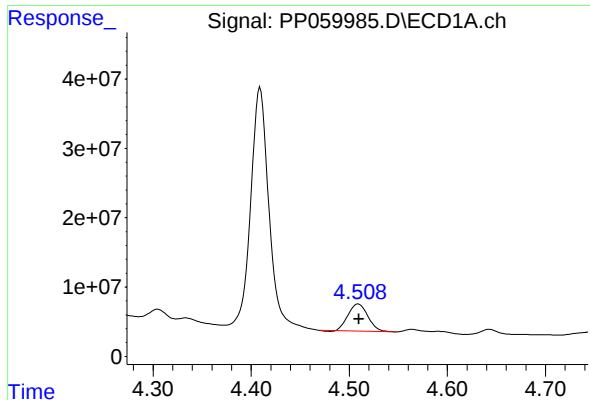


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 55032317
Conc: 26.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

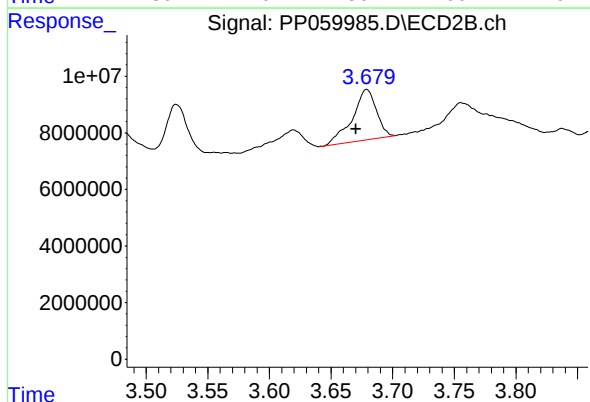


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: 0.009 min
Response: 24331752
Conc: 14.94 ng/ml

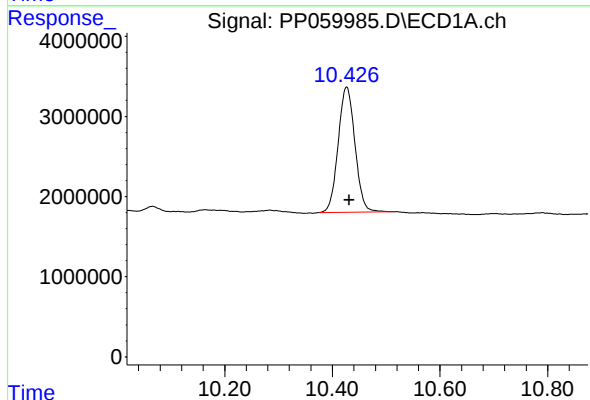


#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.005 min
Response: 33825279
Conc: 22.18 ng/ml

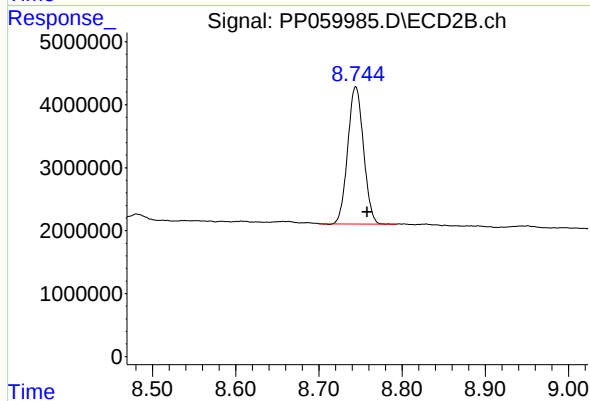

#2 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: -0.014 min
Response: 28733701
Conc: 18.98 ng/ml

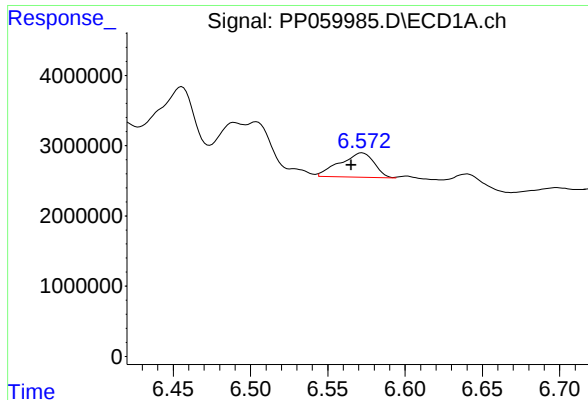


#26 AR-1254-1

R.T.: 6.572 min
Delta R.T.: 0.006 min
Response: 5364463
Conc: 67.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

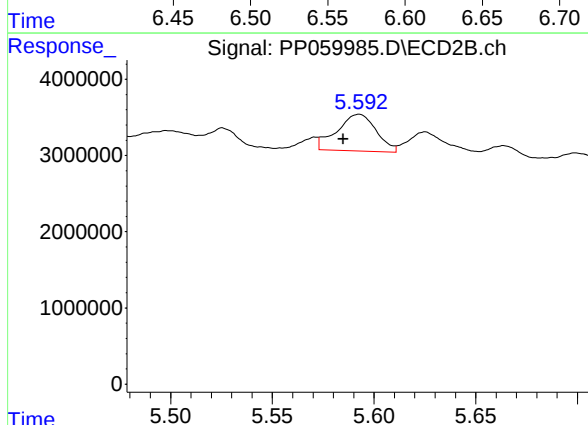


#26 AR-1254-1

R.T.: 5.592 min
Delta R.T.: 0.007 min
Response: 6434584
Conc: 64.12 ng/ml

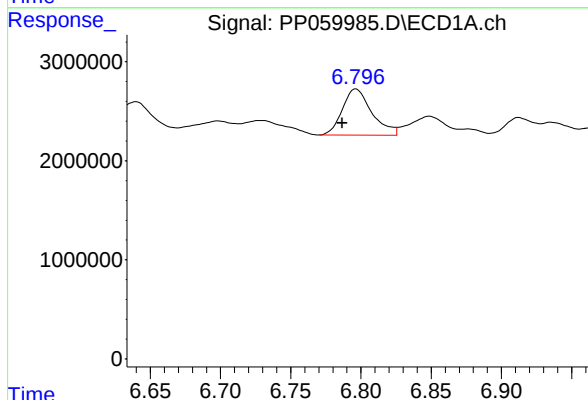


#27 AR-1254-2

R.T.: 6.797 min
Delta R.T.: 0.010 min
Response: 6815556
Conc: 56.90 ng/ml

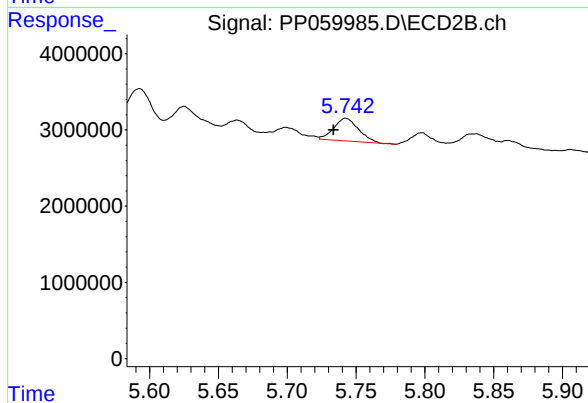

#27 AR-1254-2

R.T.: 5.743 min
Delta R.T.: 0.009 min
Response: 3728224
Conc: 42.91 ng/ml

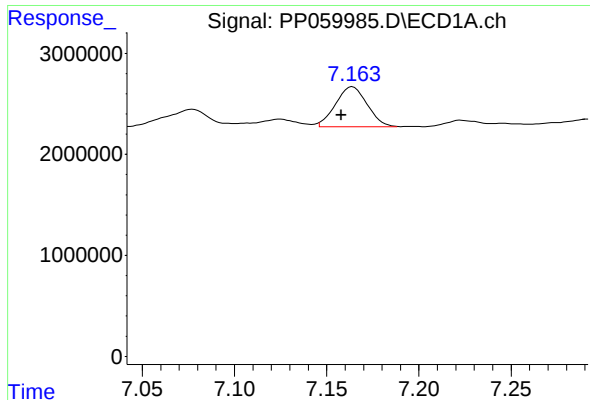


#28 AR-1254-3

R.T.: 7.163 min
Delta R.T.: 0.006 min
Response: 4710612
Conc: 38.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

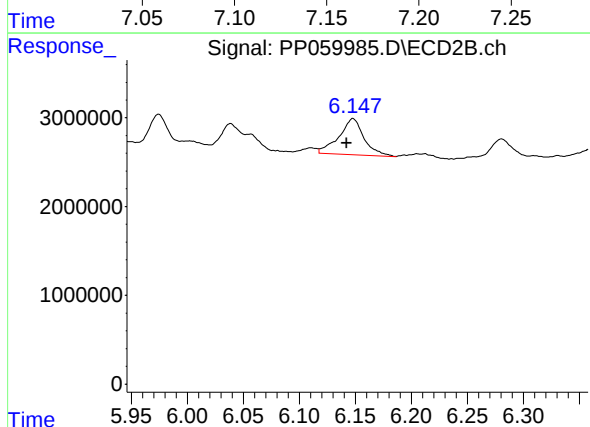


#28 AR-1254-3

R.T.: 6.148 min
Delta R.T.: 0.006 min
Response: 6361964
Conc: 45.31 ng/ml

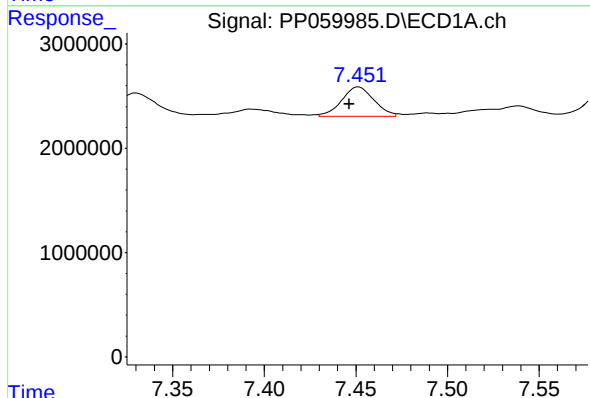


#29 AR-1254-4

R.T.: 7.451 min
Delta R.T.: 0.005 min
Response: 3460310
Conc: 38.91 ng/ml m

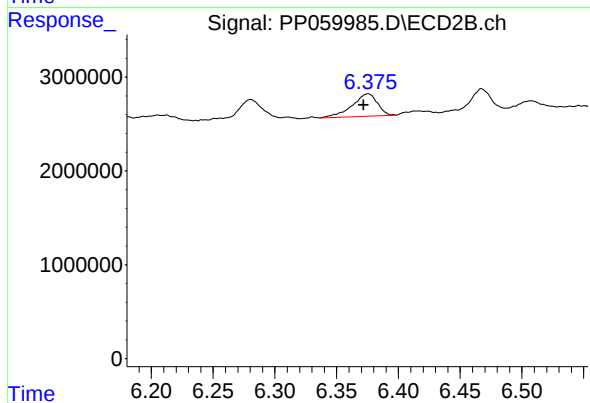

#29 AR-1254-4

R.T.: 6.376 min
Delta R.T.: 0.004 min
Response: 3429740
Conc: 40.75 ng/ml

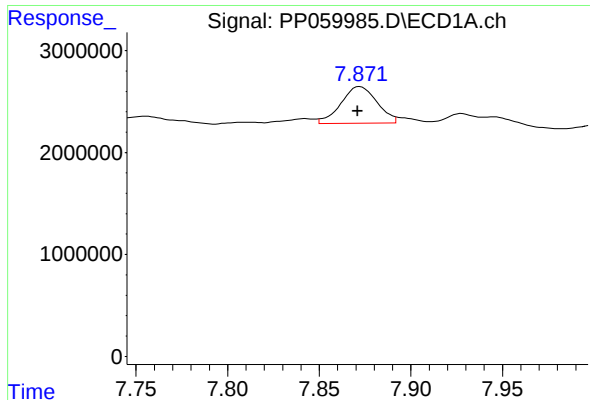


#30 AR-1254-5

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 4994185
Conc: 51.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
003

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/20/2023
Supervised By :Ankita Jodhani 09/20/2023

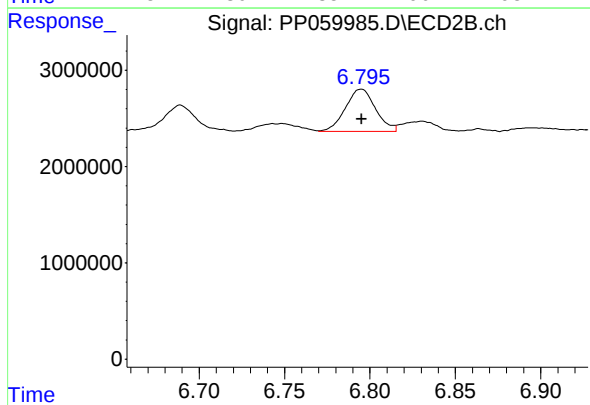

#30 AR-1254-5

R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 5383612
Conc: 45.39 ng/ml