

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP091923\  
 Data File : PP059995.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Sep 2023 05:09  
 Operator : YP\AJ  
 Sample : 04486-02 10X  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FDA711T-END-1-2

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 20 05:47:06 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP091823.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Sep 19 09:22:53 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

|                    |        |       |         |         |       |       |
|--------------------|--------|-------|---------|---------|-------|-------|
| 1) SA Tetrachlo... | 4.508  | 3.666 | 4072291 | 2911313 | 1.958 | 1.787 |
| 2) SA Decachlor... | 10.427 | 8.744 | 4228980 | 3925448 | 2.772 | 2.592 |

#### Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP091923\  
Data File : PP059995.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Sep 2023 05:09  
Operator : YP\AJ  
Sample : 04486-02 10X  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FDA711T-END-1-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 20 05:47:06 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP091823.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Sep 19 09:22:53 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

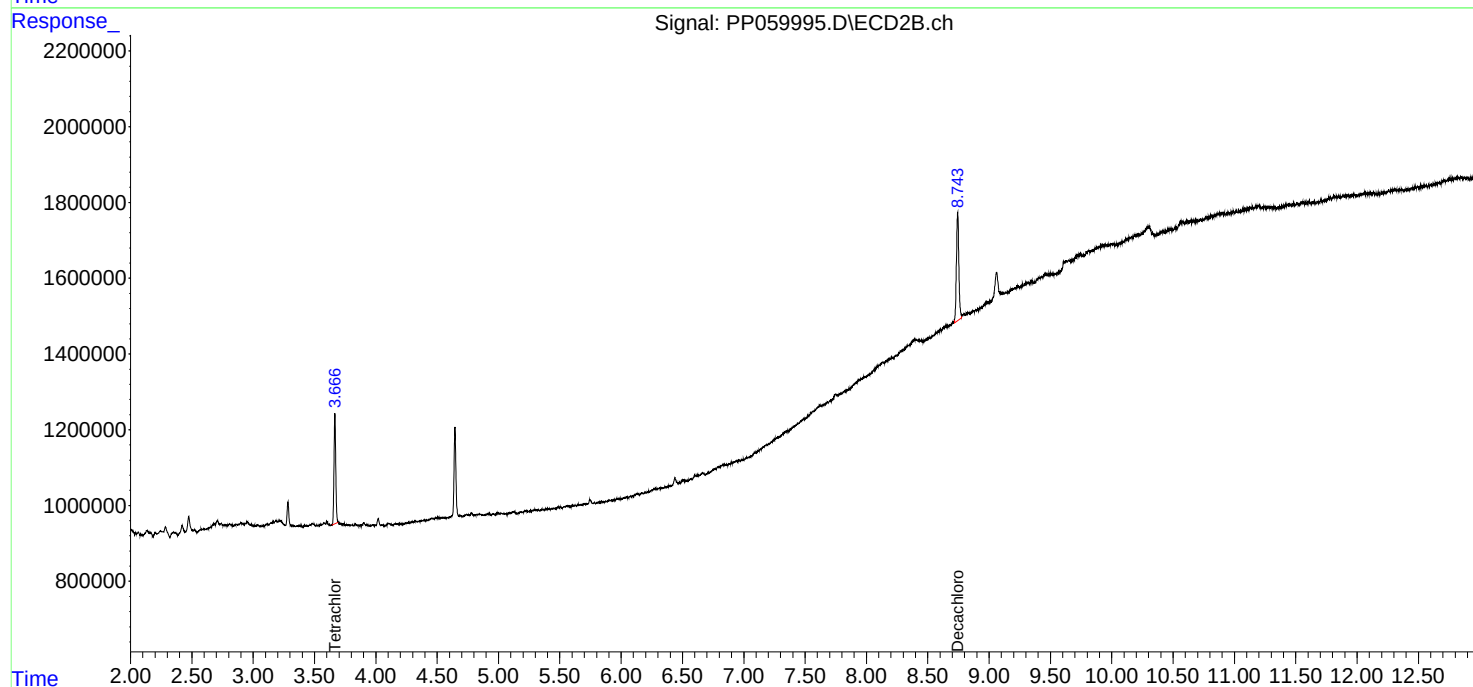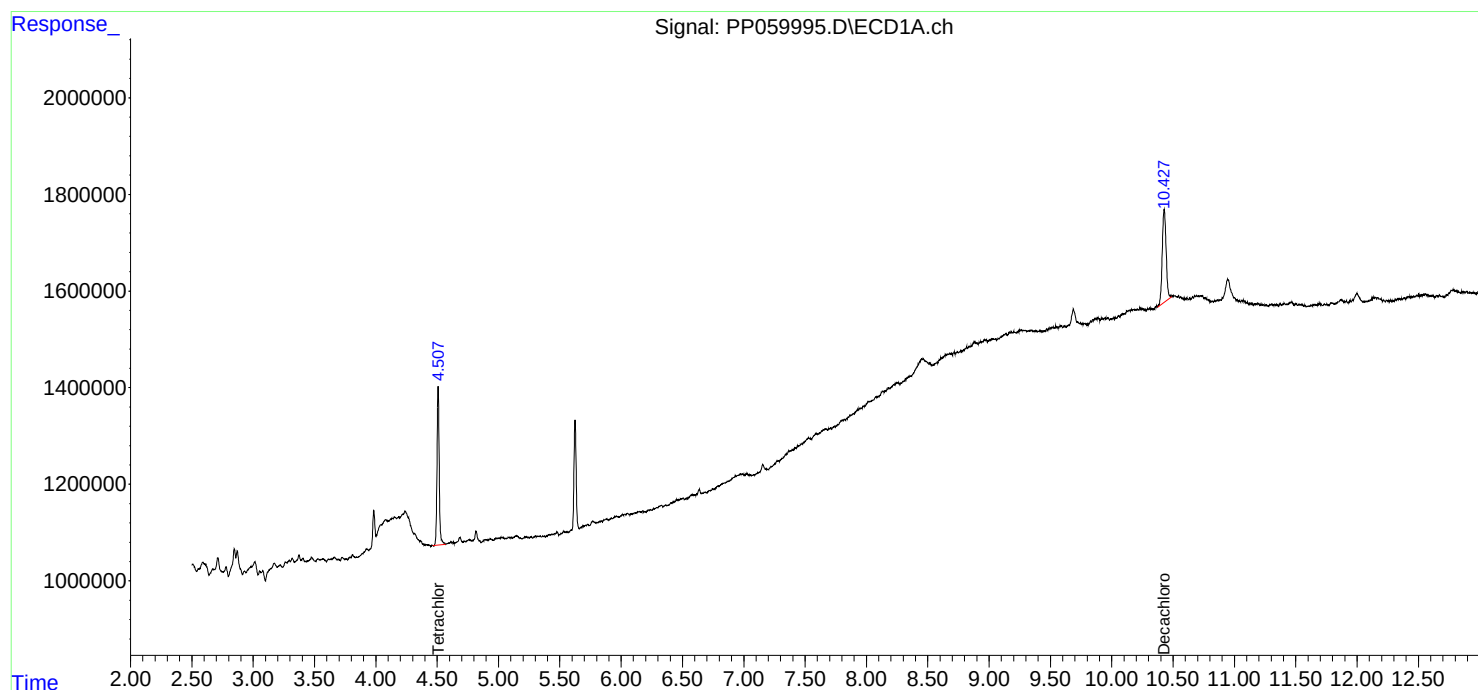


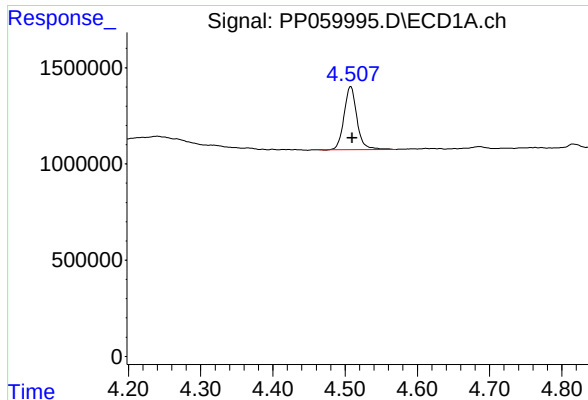

#1 Tetrachloro-m-xylene


R.T.: 4.508 min  
Delta R.T.: -0.002 min  
Response: 4072291  
Conc: 1.96 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
FDA711T-END-1-2

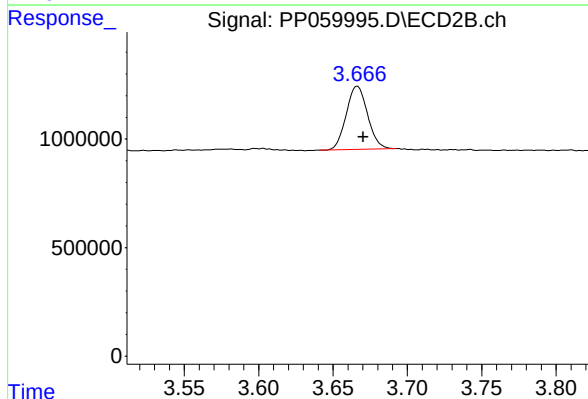


#1 Tetrachloro-m-xylene

R.T.: 3.666 min  
Delta R.T.: -0.004 min  
Response: 2911313  
Conc: 1.79 ng/ml

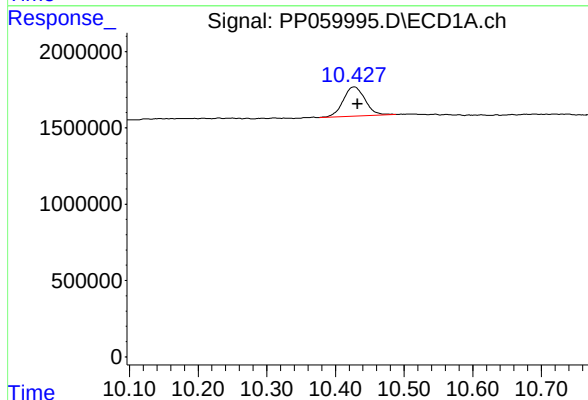

#2 Decachlorobiphenyl

R.T.: 10.427 min  
Delta R.T.: -0.005 min  
Response: 4228980  
Conc: 2.77 ng/ml

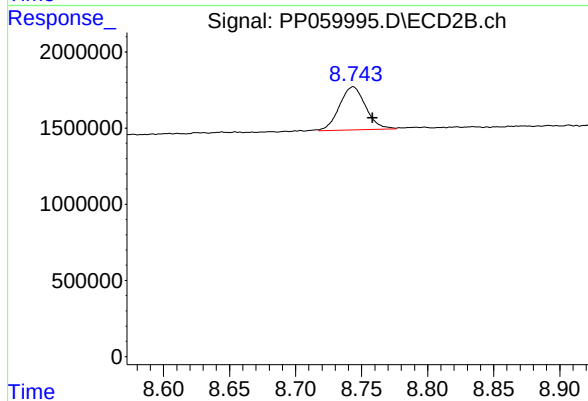

#2 Decachlorobiphenyl

R.T.: 8.744 min  
Delta R.T.: -0.015 min  
Response: 3925448  
Conc: 2.59 ng/ml