

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
 Data File : PP060008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 09:11
 Operator : YP\AJ
 Sample : 04486-06 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC260098LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 11:16:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.508	3.666	3583810	2578725	1.723	1.583
2) SA Decachlor...	10.426	8.742	5021078	3126721	3.292m	2.065 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
Data File : PP060008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 09:11
Operator : YP\AJ
Sample : 04486-06 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC260098LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 11:16:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

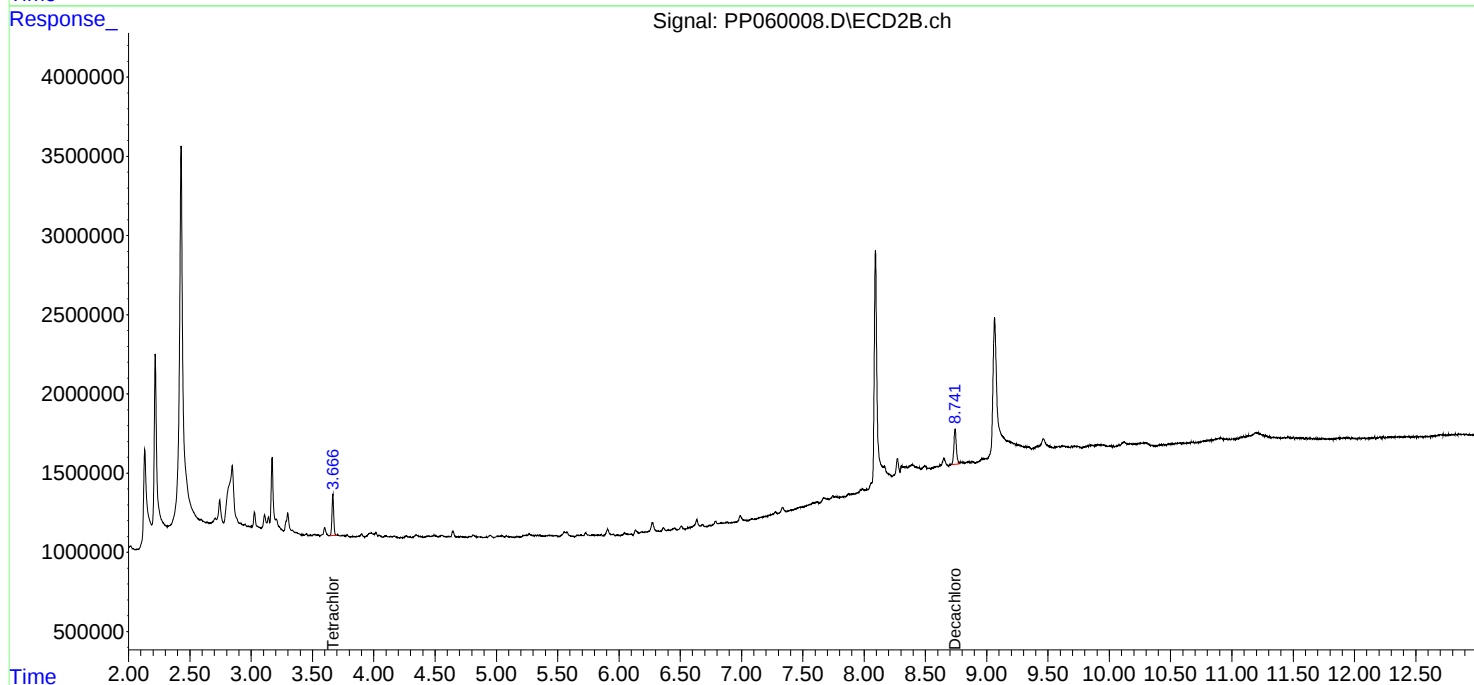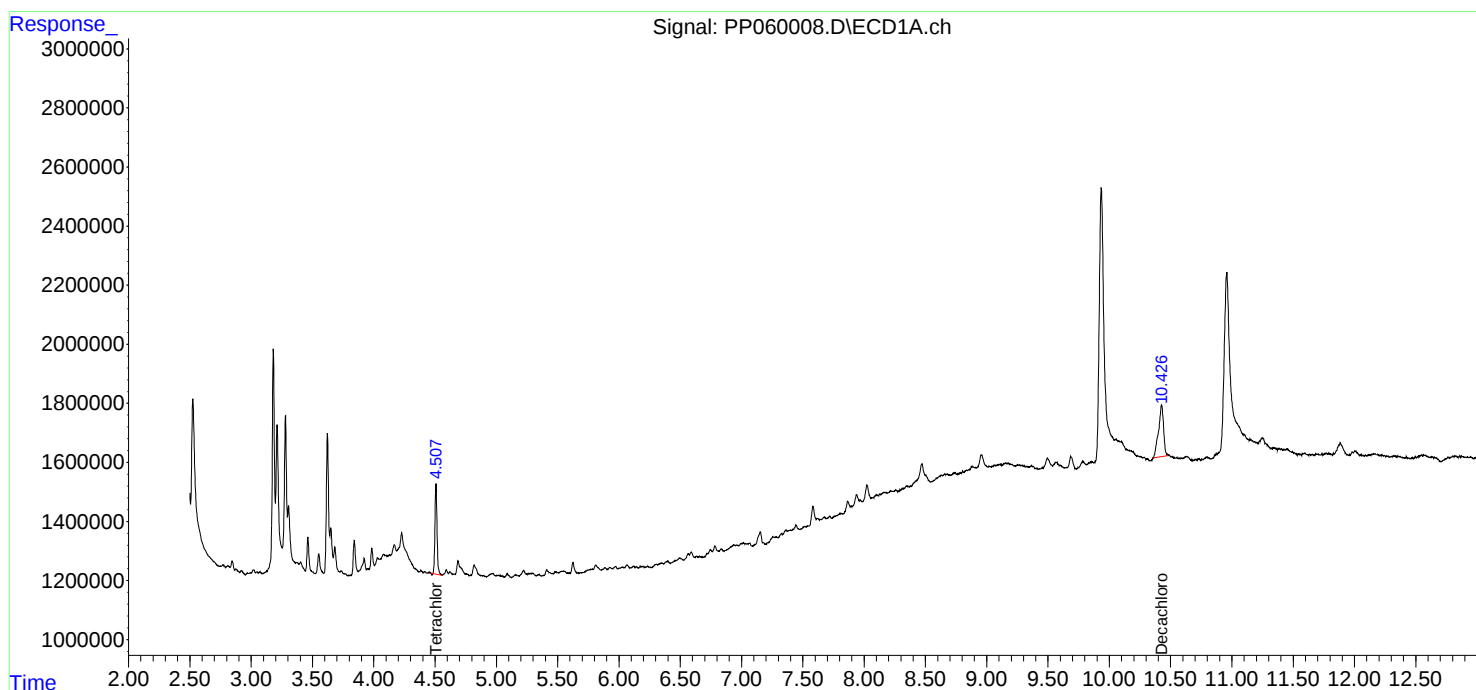

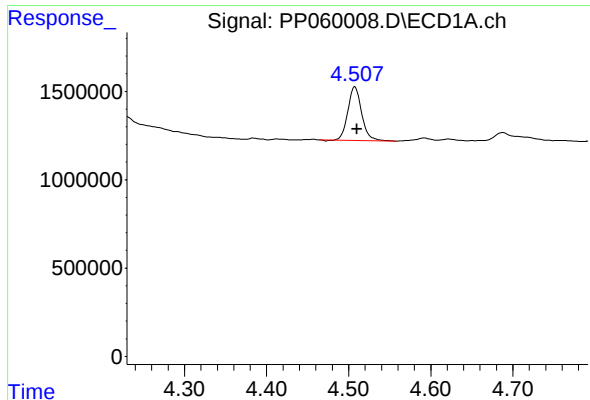


#1 Tetrachloro-m-xylene

R.T.: 4.508 min
Delta R.T.: -0.002 min
Response: 3583810
Conc: 1.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC260098LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

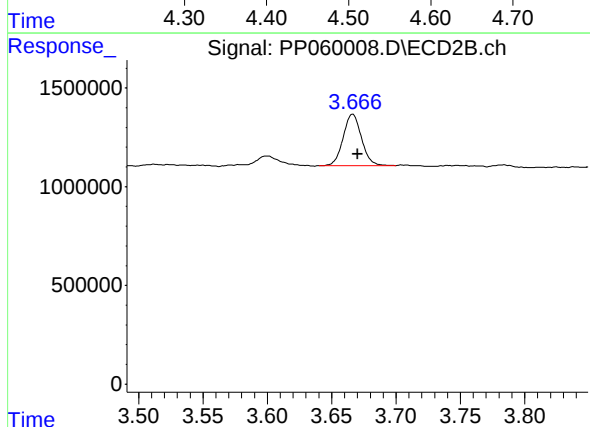


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.004 min
Response: 2578725
Conc: 1.58 ng/ml

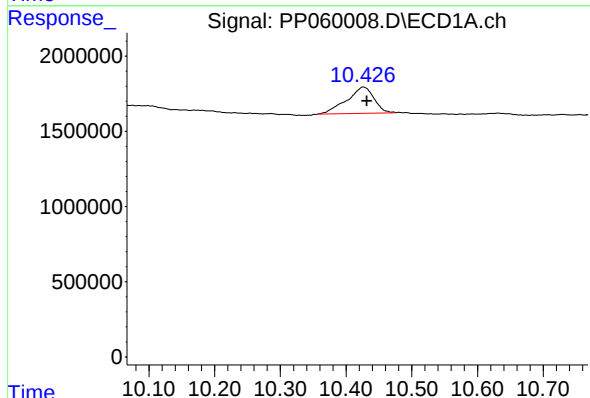

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.006 min
Response: 5021078
Conc: 3.29 ng/ml m

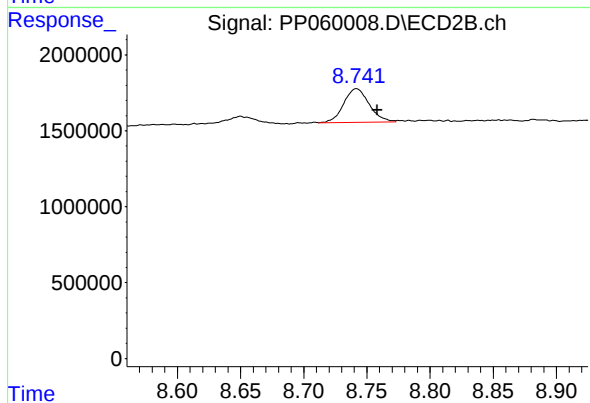

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.017 min
Response: 3126721
Conc: 2.06 ng/ml