

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
 Data File : PP060013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 10:32
 Operator : YP\AJ
 Sample : 04486-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDA711T-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 11:19:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.510	3.668	3873116	2983350	1.862	1.832
2) SA Decachlor...	10.431	8.744	4024018	3656620	2.638	2.415

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091923\
Data File : PP060013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 10:32
Operator : YP\AJ
Sample : 04486-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDA711T-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 11:19:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

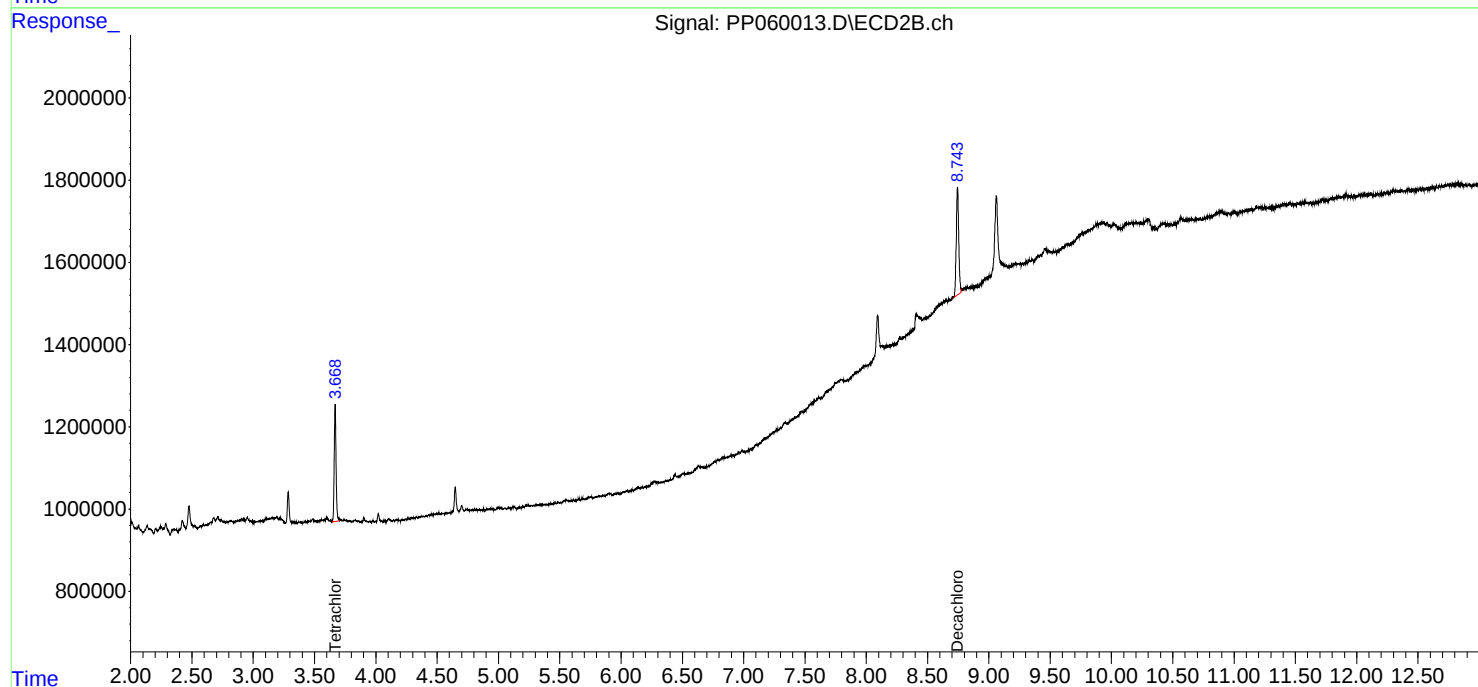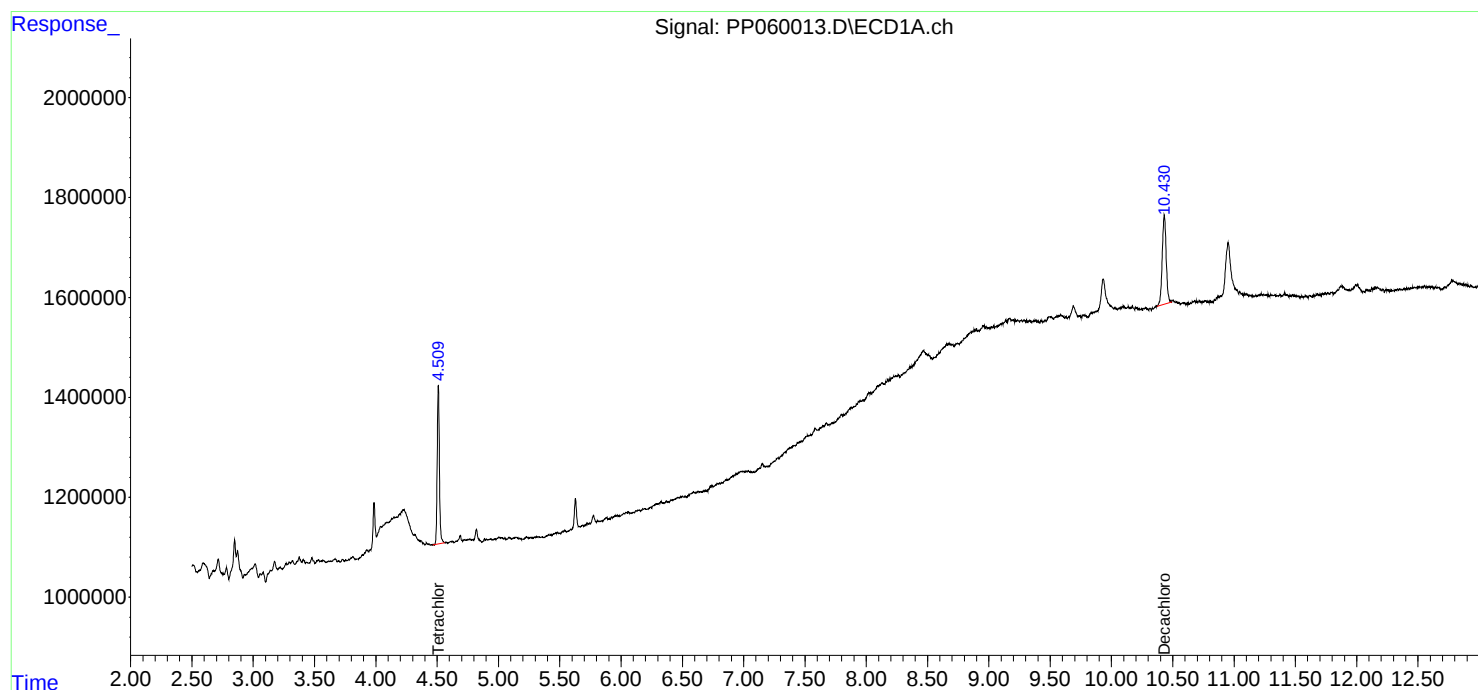


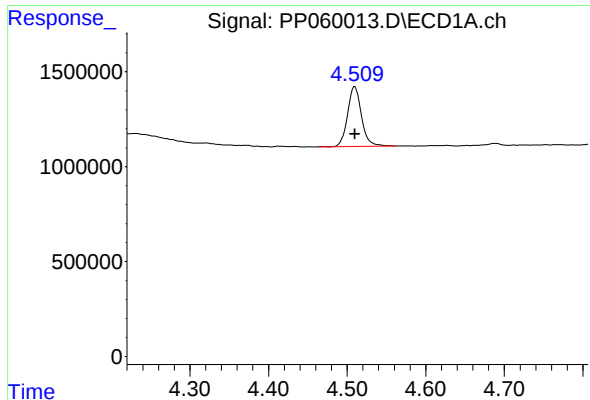

#1 Tetrachloro-m-xylene


R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 3873116
Conc: 1.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA711T-END-1-1

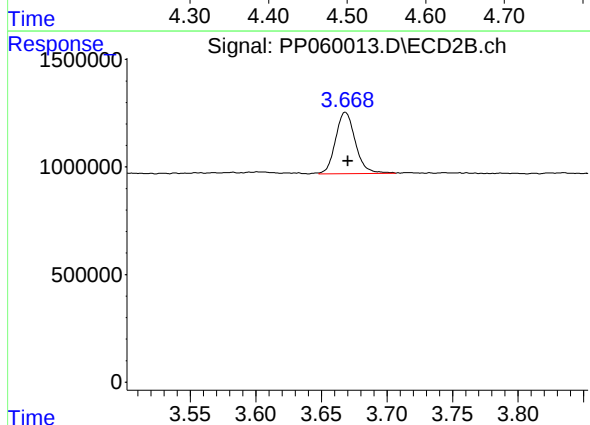


#1 Tetrachloro-m-xylene

R.T.: 3.668 min
Delta R.T.: -0.002 min
Response: 2983350
Conc: 1.83 ng/ml

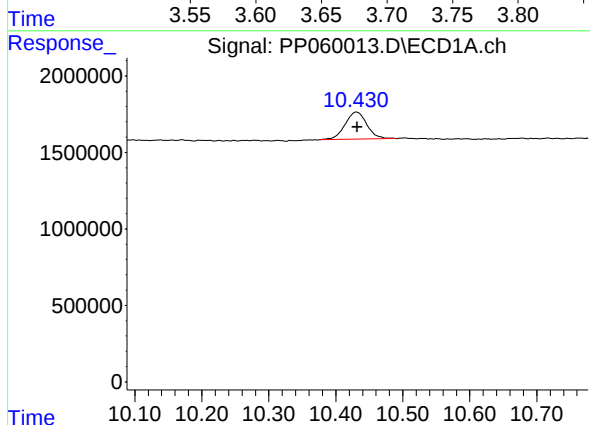

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: -0.001 min
Response: 4024018
Conc: 2.64 ng/ml

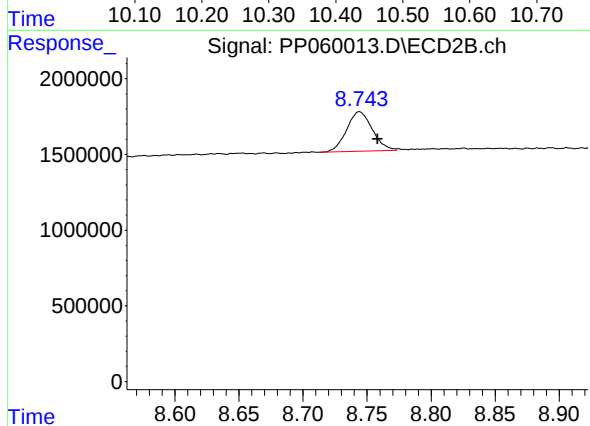

#2 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: -0.014 min
Response: 3656620
Conc: 2.41 ng/ml