

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091925\
 Data File : PP075197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2025 13:03
 Operator : YP\AJ
 Sample : Q3126-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-01-091725

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2025
 Supervised By :mohammad ahmed 09/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 13:51:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 17 02:17:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.651	3.792	26958033	194.1E6	20.941m	34.285 #
2) SA Decachlor...	10.434	8.800	25444703	131.1E6	22.200	16.136 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091925\
Data File : PP075197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2025 13:03
Operator : YP\AJ
Sample : Q3126-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OK-01-091725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2025
Supervised By :mohammad ahmed 09/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 13:51:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 17 02:17:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

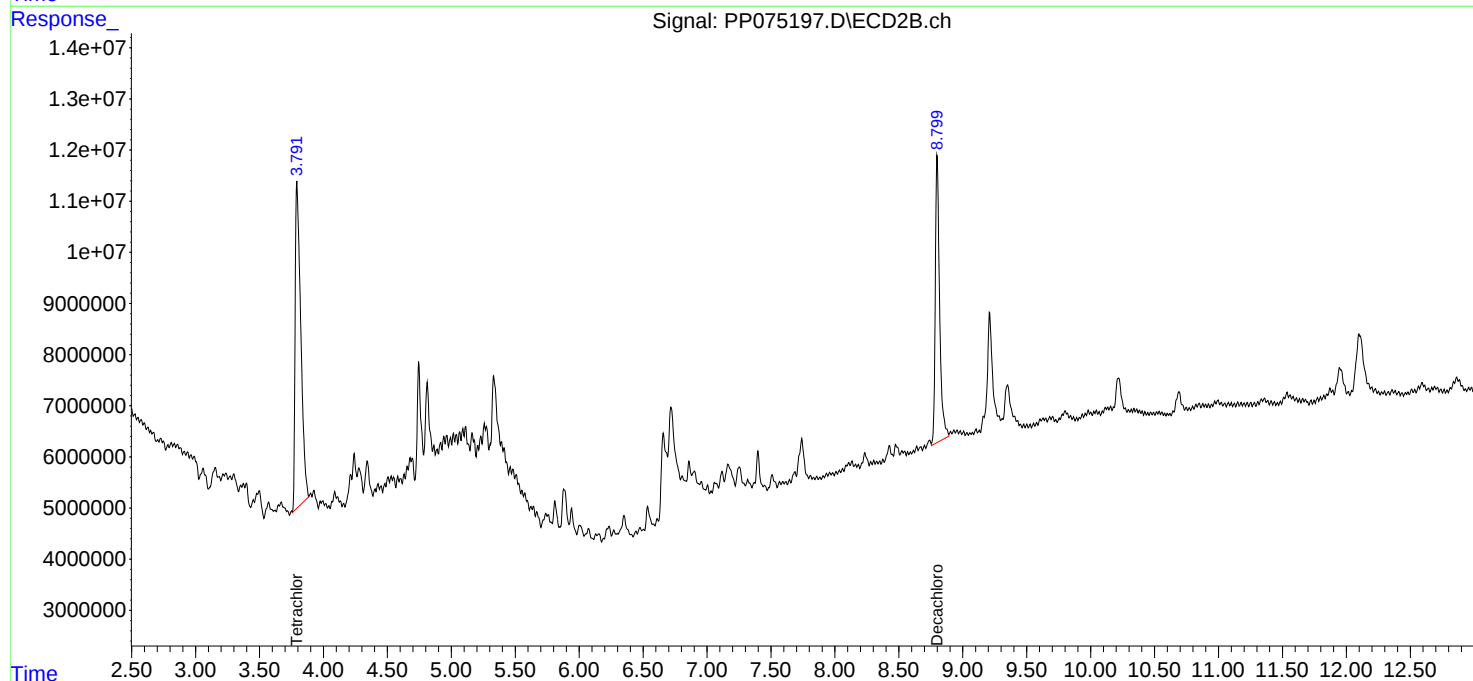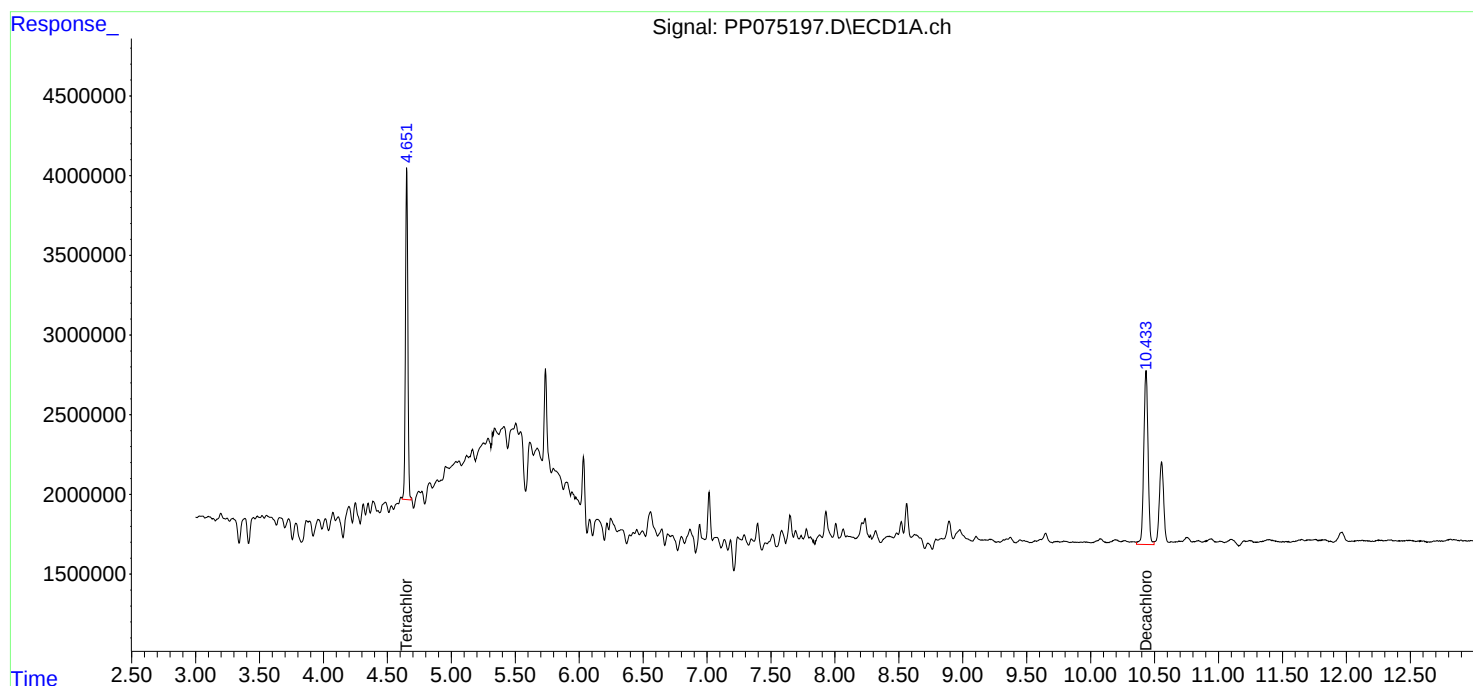

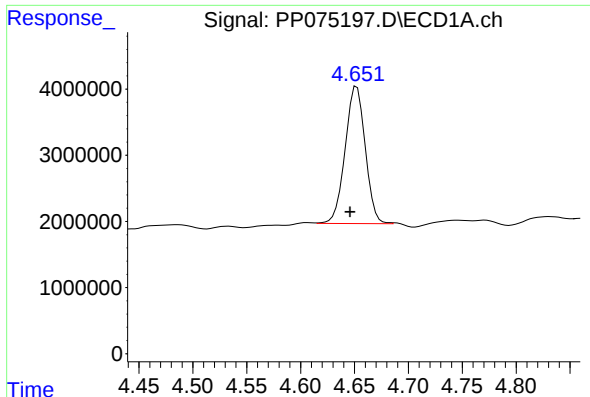


#1 Tetrachloro-m-xylene

R.T.: 4.651 min
Delta R.T.: 0.005 min
Response: 26958033
Conc: 20.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-091725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2025
Supervised By :mohammad ahmed 09/23/2025

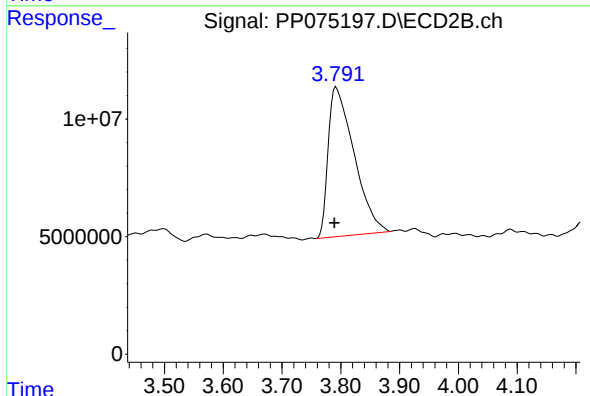


#1 Tetrachloro-m-xylene

R.T.: 3.792 min
Delta R.T.: 0.003 min
Response: 194064041
Conc: 34.28 ng/ml

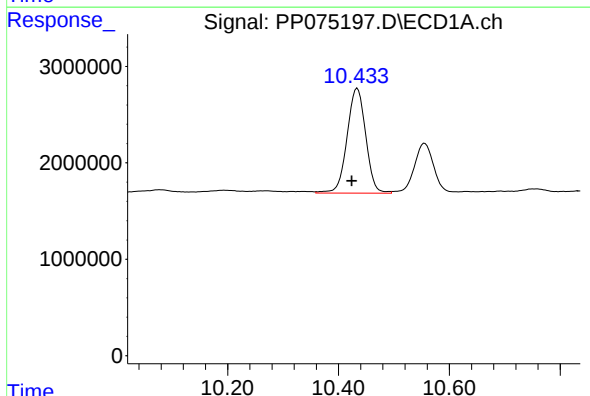

#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.010 min
Response: 25444703
Conc: 22.20 ng/ml

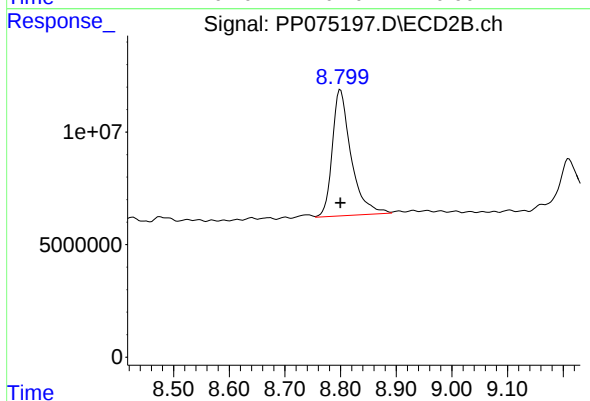

#2 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 131074543
Conc: 16.14 ng/ml