

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
 Data File : PP039369.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Sep 2021 10:35
 Operator : AJ\MA
 Sample : PB139084BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 11:30:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 20 01:59:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.046	4.121	562809	584217	22.440	21.542
2)	SA Decachlor...	11.169	9.498	489171	595200	23.655	22.049
Target Compounds							
8)	L2 AR-1221-1	5.298	0.000	39066	0	125.455	N.D. #
9)	L2 AR-1221-2	0.000	4.477	0	7813	N.D.	32.717 #
24)	L5 AR-1248-4	7.289f	0.000	5700	0	6.594	N.D. #
26)	L6 AR-1254-1	7.289	0.000	5700	0	5.838	N.D. #
28)	L6 AR-1254-3	7.916f	0.000	15559	0	10.210	N.D. #
32)	L7 AR-1260-2	0.000	7.172f	0	5215	N.D.	3.070 #
38)	L8 AR-1262-3	0.000	8.394f	0	3949	N.D.	3.070 #
41)	L9 AR-1268-1	0.000	8.394f	0	3949	N.D.	1.026 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
Data File : PP039369.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Sep 2021 10:35
Operator : AJ\MA
Sample : PB139084BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 11:30:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 20 01:59:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

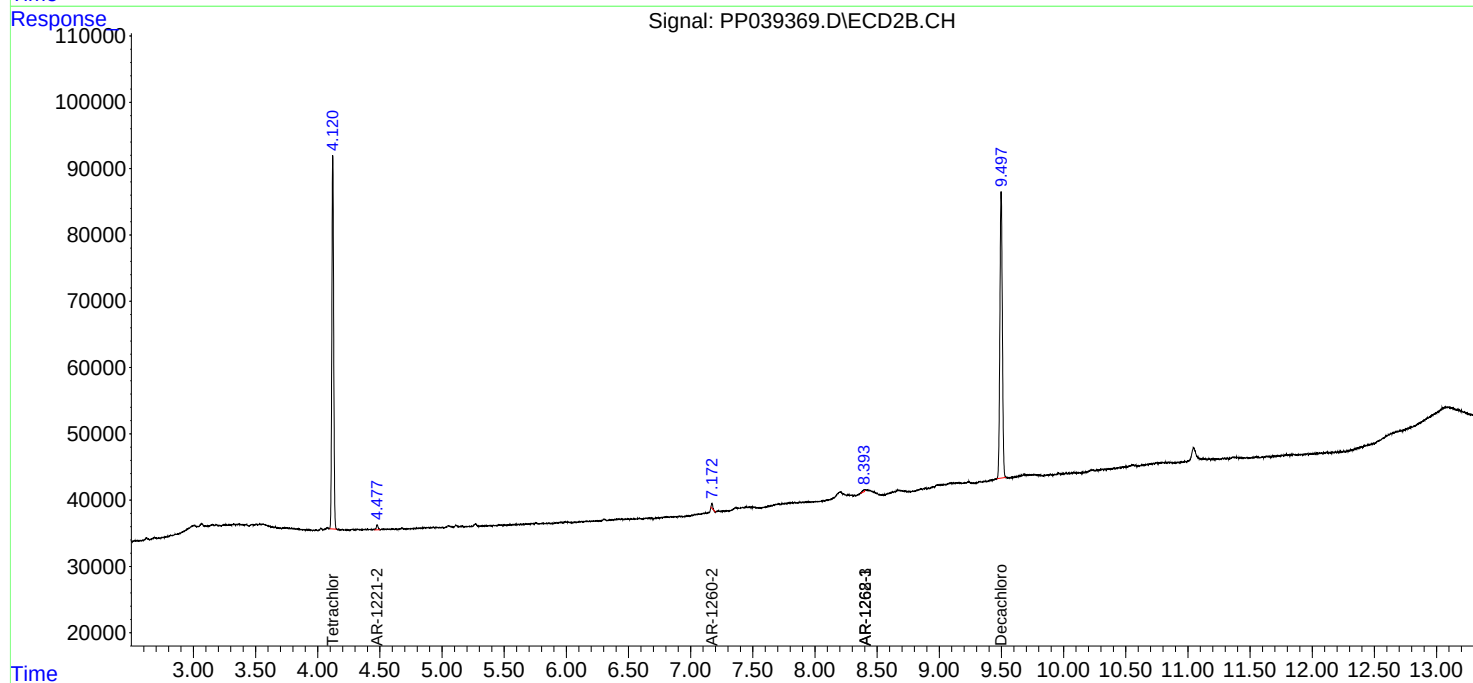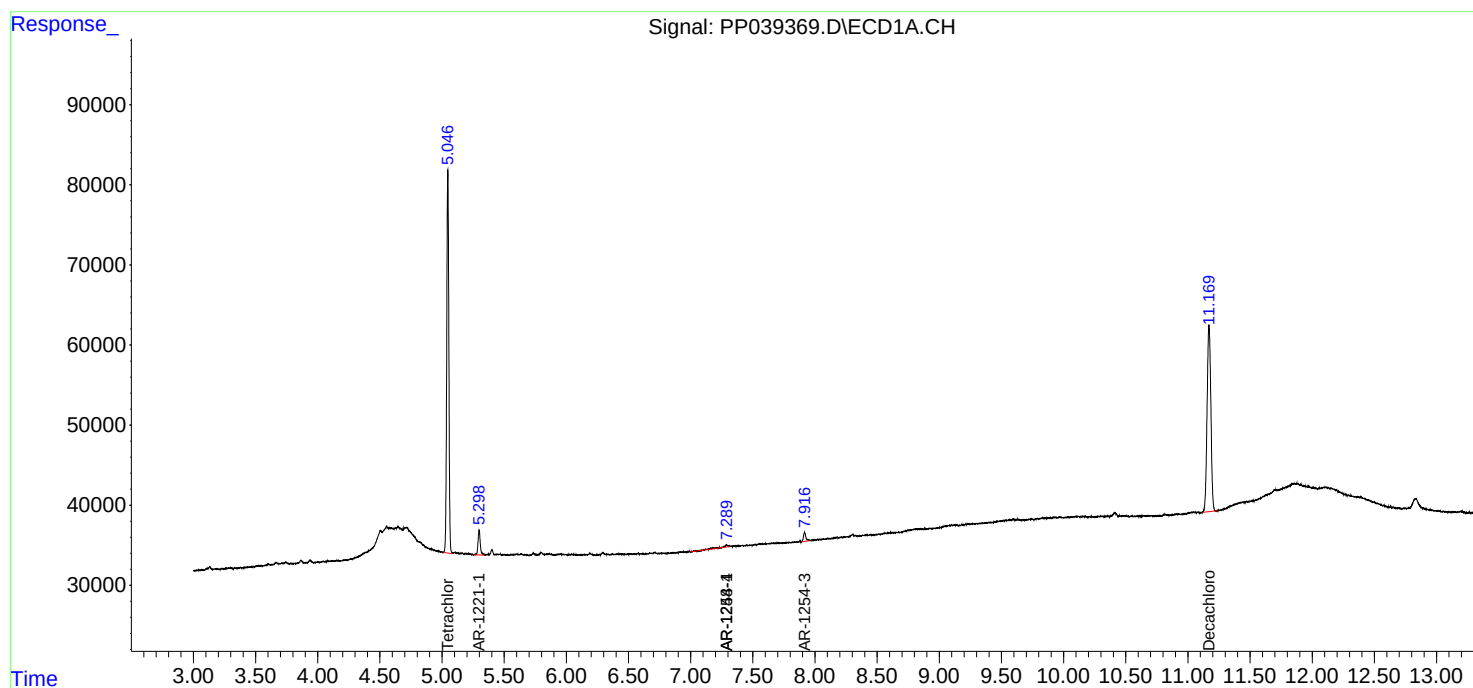


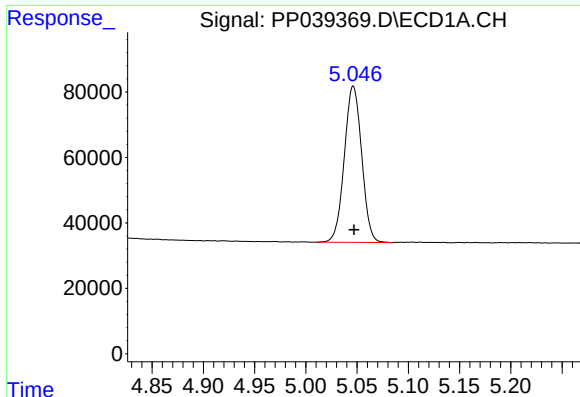

#1 Tetrachloro-m-xylene


R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 562809
Conc: 22.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

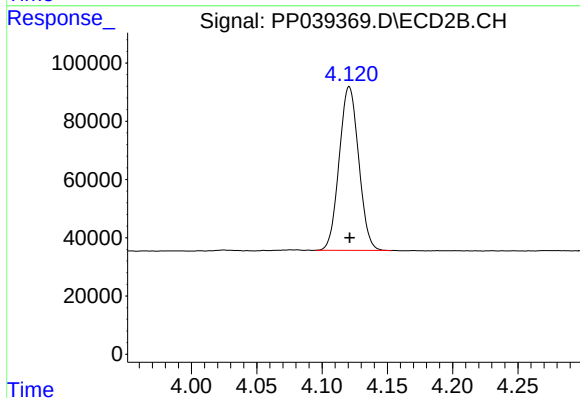


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: 0.000 min
Response: 584217
Conc: 21.54 ng/ml

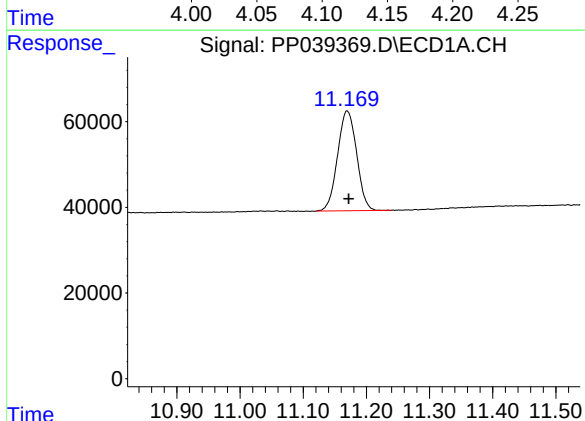


#2 Decachlorobiphenyl

R.T.: 11.169 min
Delta R.T.: -0.003 min
Response: 489171
Conc: 23.66 ng/ml

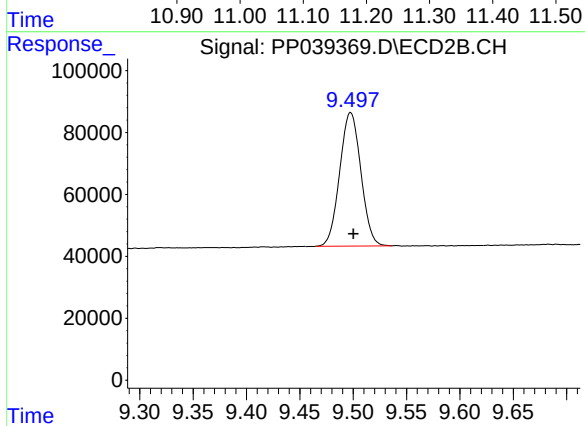

#2 Decachlorobiphenyl


R.T.: 9.498 min
Delta R.T.: -0.003 min
Response: 595200
Conc: 22.05 ng/ml

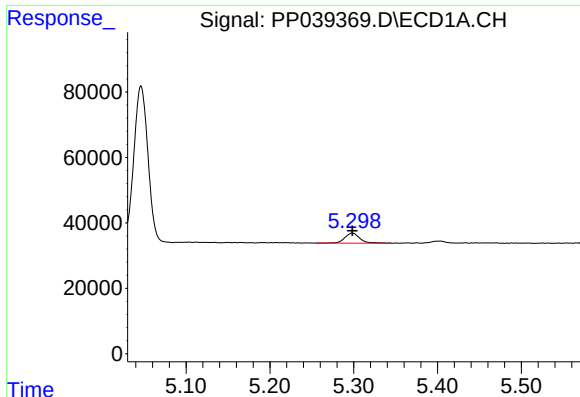

#8 AR-1221-1


R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 39066
Conc: 125.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

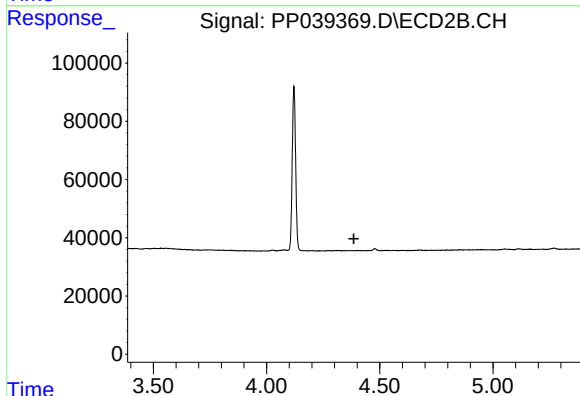


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.385 min
Response: 0
Conc: N.D.

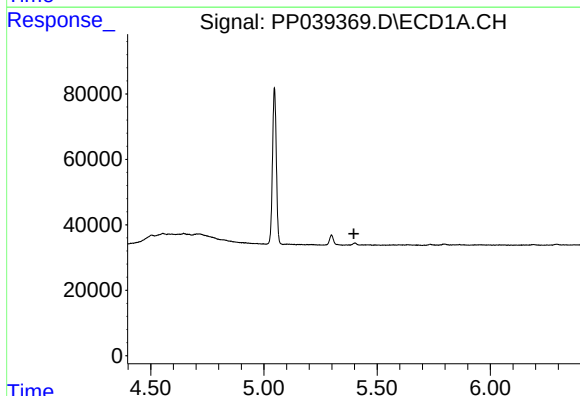


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

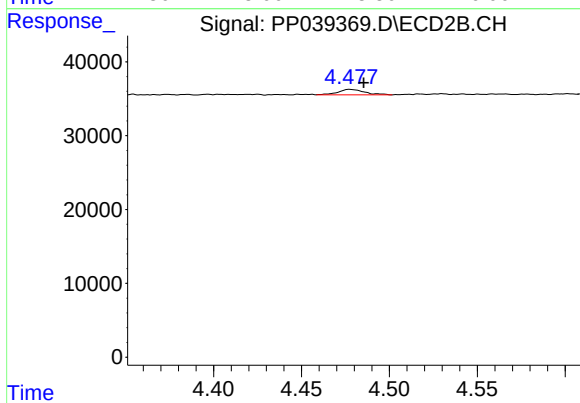

#9 AR-1221-2


R.T.: 4.477 min
Delta R.T.: -0.008 min
Response: 7813
Conc: 32.72 ng/ml

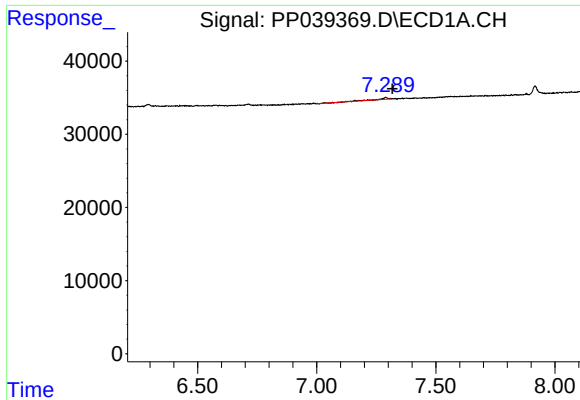

#24 AR-1248-4


R.T.: 7.289 min
Delta R.T.: -0.028 min
Response: 5700
Conc: 6.59 ng/ml

Instrument :
ECD_P
ClientSampleId :

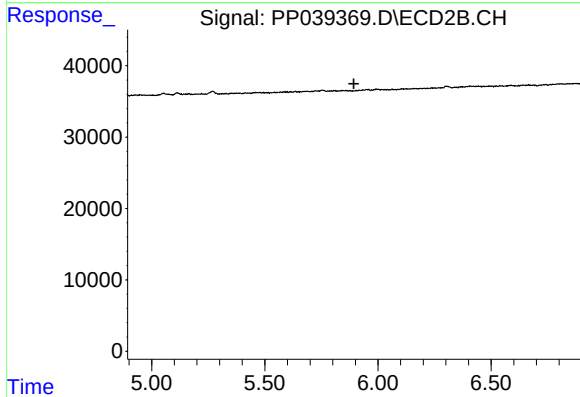


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.894 min
Response: 0
Conc: N.D.

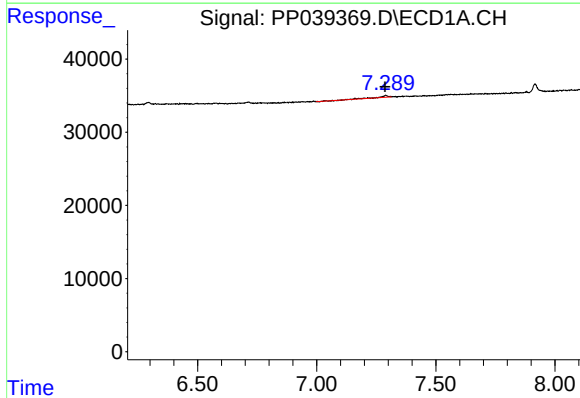


#26 AR-1254-1

R.T.: 7.289 min
Delta R.T.: 0.002 min
Response: 5700
Conc: 5.84 ng/ml

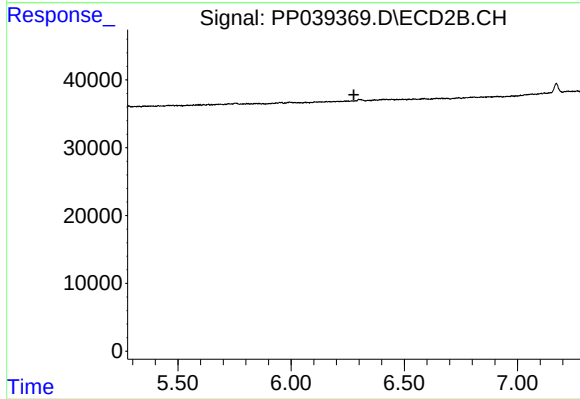

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.277 min
Response: 0
Conc: N.D.

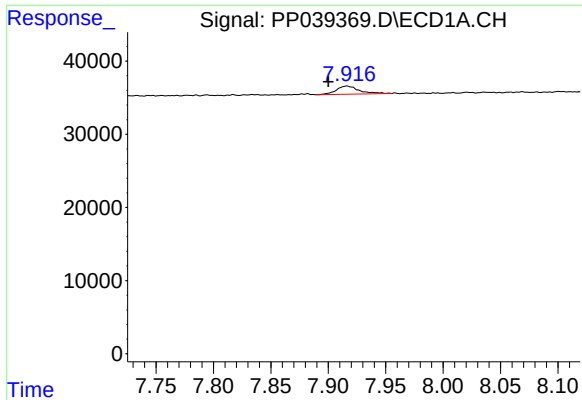

#28 AR-1254-3


R.T.: 7.916 min
Delta R.T.: 0.016 min
Response: 15559
Conc: 10.21 ng/ml

Instrument :
ECD_P
ClientSampleId :

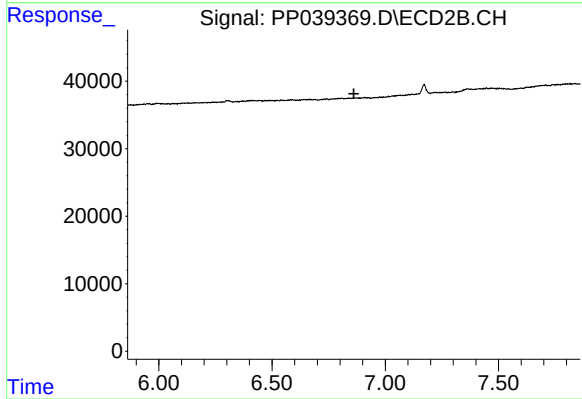


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

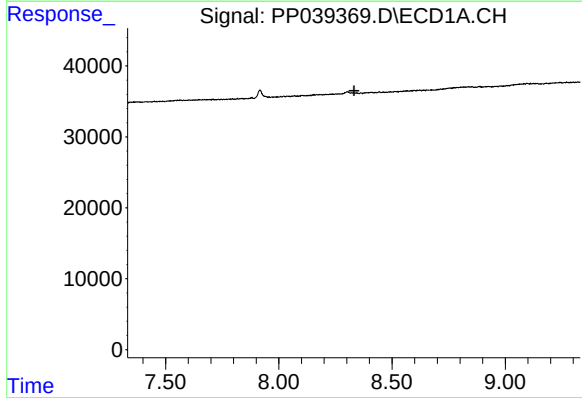


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.332 min
Response: 0
Conc: N.D.

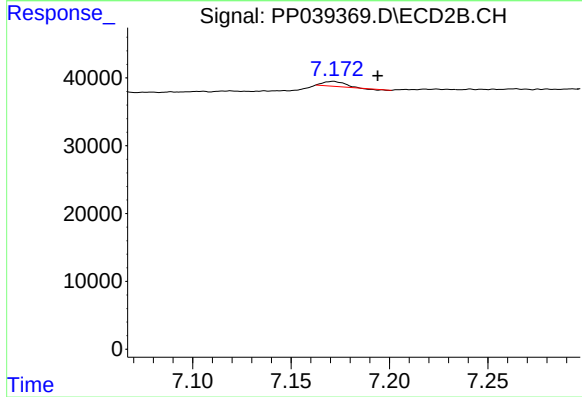

#32 AR-1260-2


R.T.: 7.172 min
Delta R.T.: -0.022 min
Response: 5215
Conc: 3.07 ng/ml

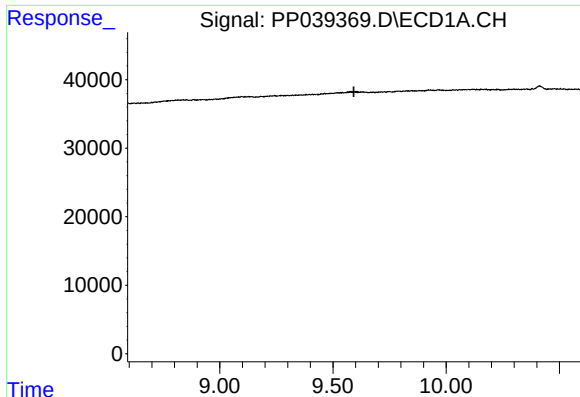

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

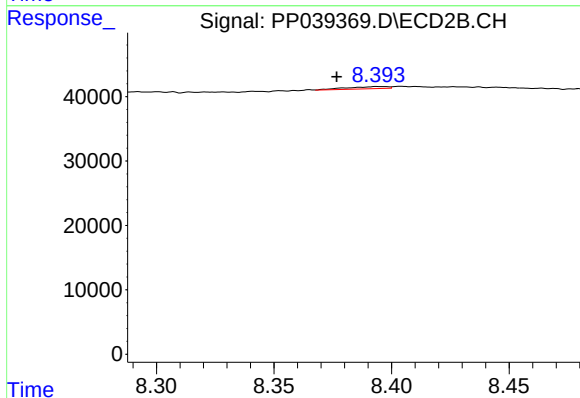


#38 AR-1262-3

R.T.: 8.394 min
Delta R.T.: 0.017 min
Response: 3949
Conc: 3.07 ng/ml

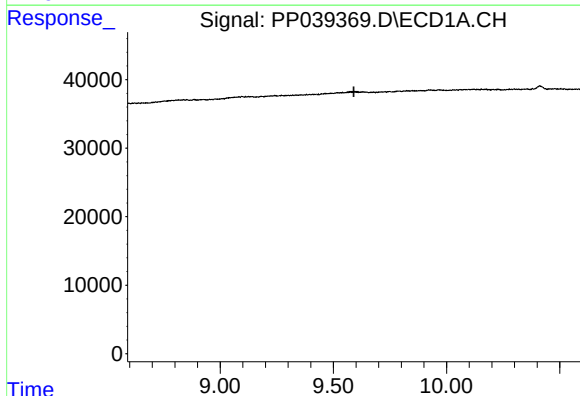

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.591 min
Response: 0
Conc: N.D.

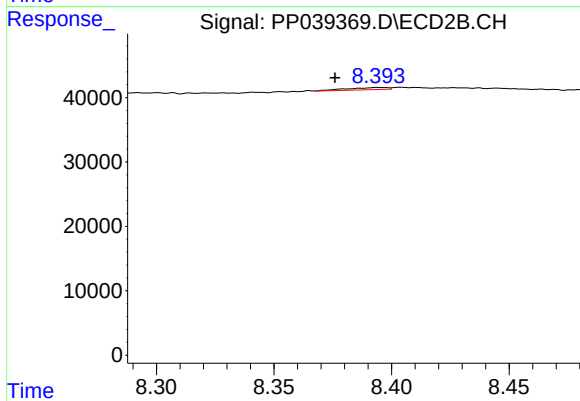

#41 AR-1268-1

R.T.: 8.394 min
Delta R.T.: 0.018 min
Response: 3949
Conc: 1.03 ng/ml