

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
 Data File : PP039376.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Sep 2021 14:11
 Operator : AJ\MA
 Sample : PB139190BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 03:49:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 20 01:59:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.047	4.121	508312	526790	20.267	19.425
2)	SA Decachlor...	11.172	9.497	491641	583992	23.775	21.634
Target Compounds							
8)	L2 AR-1221-1	5.271f	0.000	6553	0	21.043	N.D. #
9)	L2 AR-1221-2	5.420f	4.478	22896	7092	94.789	29.700 #
10)	L2 AR-1221-3	0.000	4.561f	0	19608	N.D.	25.259 #
11)	L3 AR-1232-1	0.000	4.561f	0	19608	N.D.	33.709 #
28)	L6 AR-1254-3	7.916f	0.000	7593	0	4.982	N.D. #
32)	L7 AR-1260-2	0.000	7.171f	0	9490	N.D.	5.587 #
38)	L8 AR-1262-3	0.000	8.381	0	2464	N.D.	1.916 #
41)	L9 AR-1268-1	0.000	8.381	0	2464	N.D.	0.640 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
Data File : PP039376.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Sep 2021 14:11
Operator : AJ\MA
Sample : PB139190BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 03:49:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 20 01:59:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

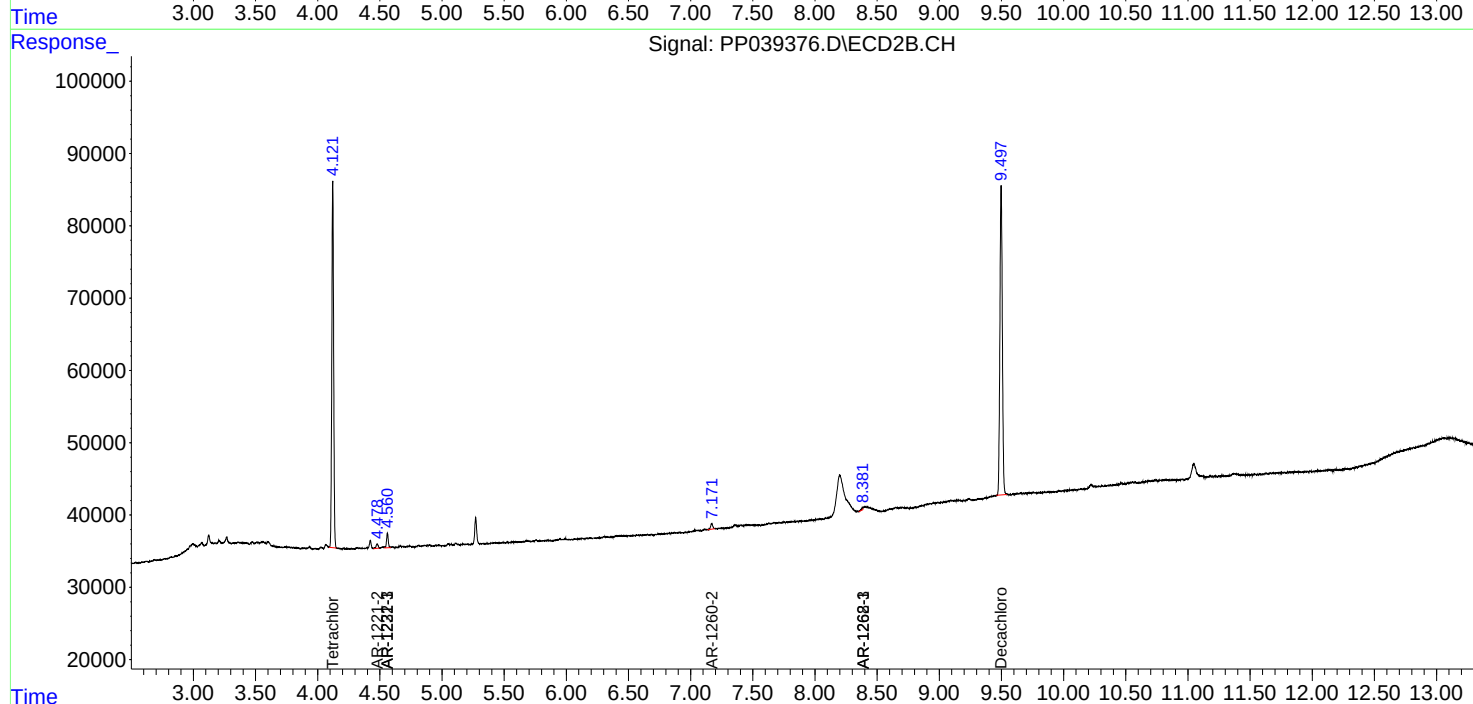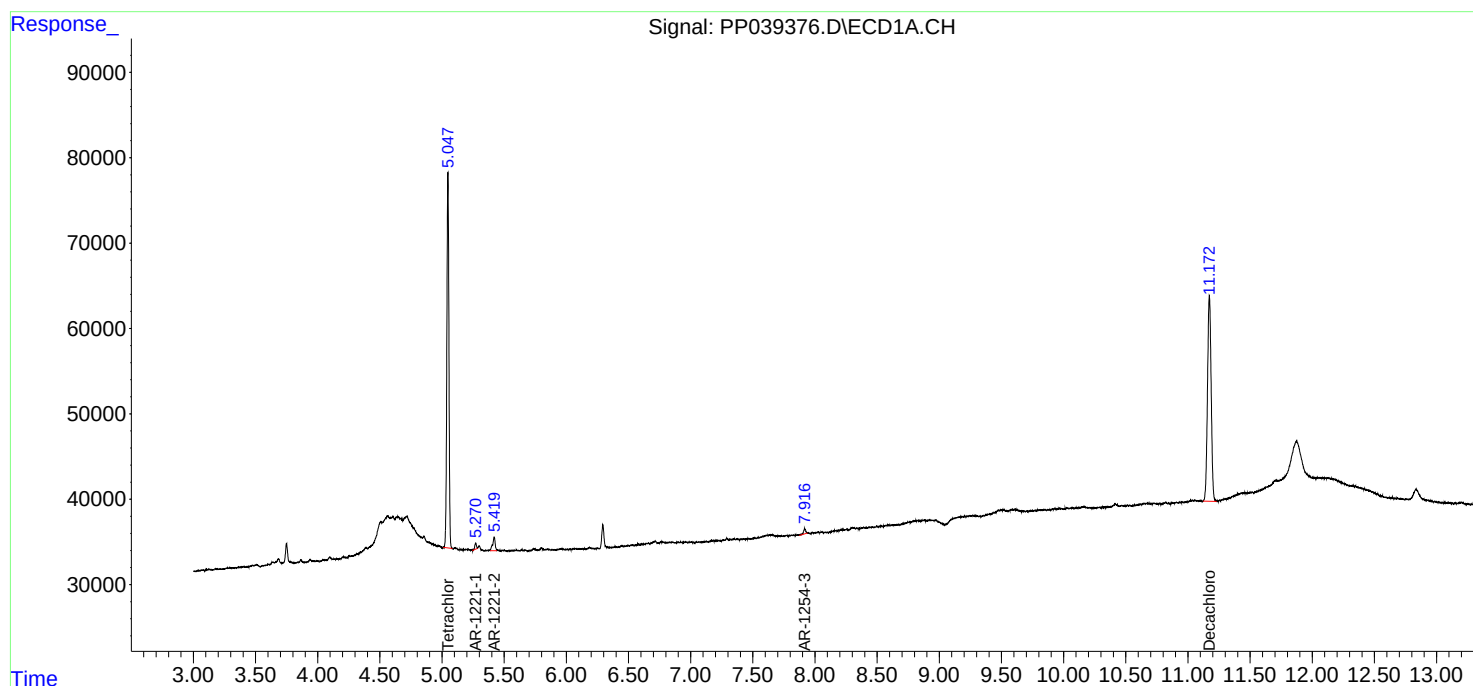


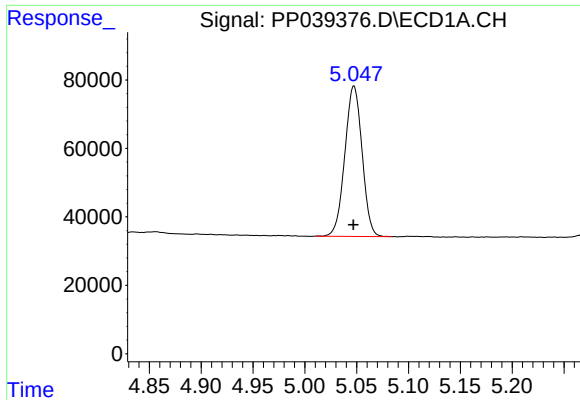

#1 Tetrachloro-m-xylene


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 508312
Conc: 20.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

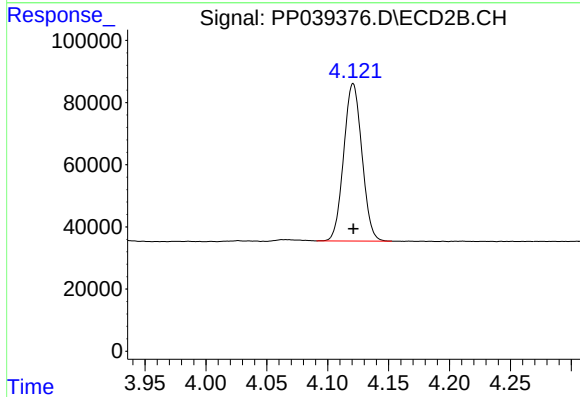


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: 0.000 min
Response: 526790
Conc: 19.42 ng/ml

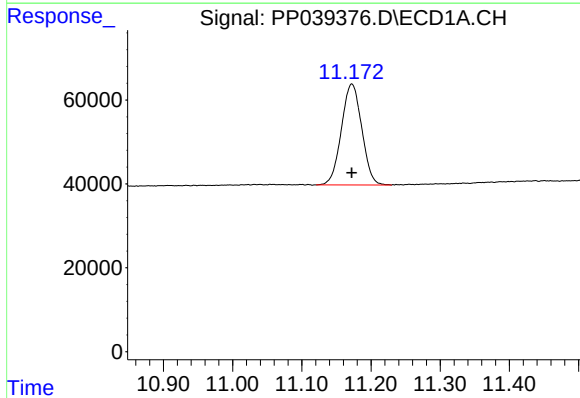


#2 Decachlorobiphenyl

R.T.: 11.172 min
Delta R.T.: 0.000 min
Response: 491641
Conc: 23.77 ng/ml

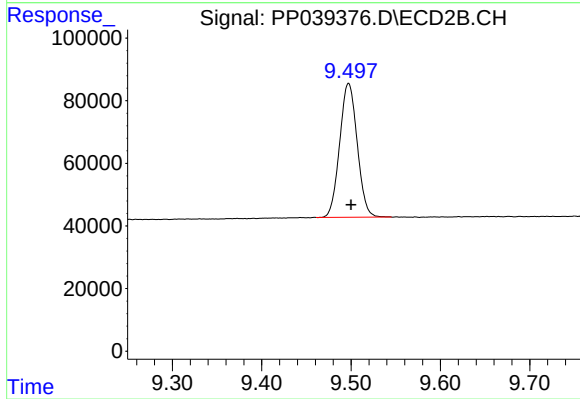

#2 Decachlorobiphenyl


R.T.: 9.497 min
Delta R.T.: -0.003 min
Response: 583992
Conc: 21.63 ng/ml

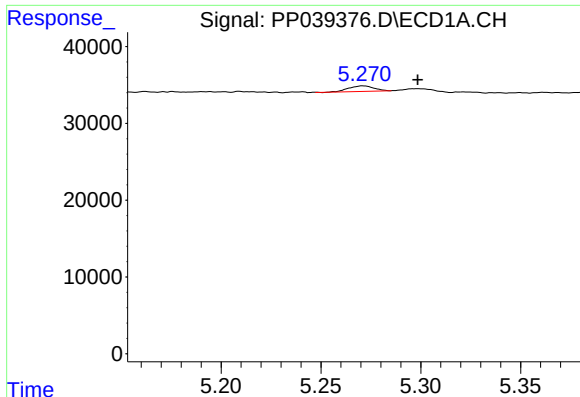

#8 AR-1221-1


R.T.: 5.271 min
Delta R.T.: -0.027 min
Response: 6553
Conc: 21.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

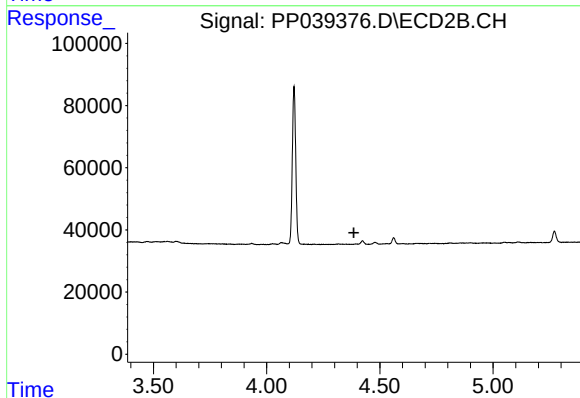


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.385 min
Response: 0
Conc: N.D.

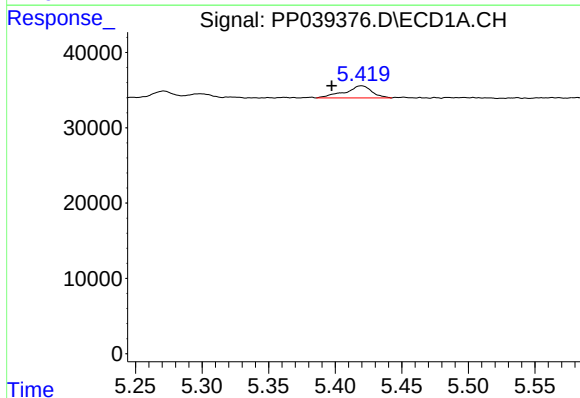


#9 AR-1221-2

R.T.: 5.420 min
Delta R.T.: 0.022 min
Response: 22896
Conc: 94.79 ng/ml

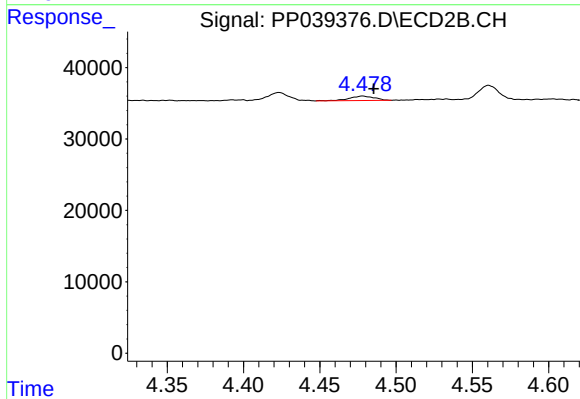

#9 AR-1221-2


R.T.: 4.478 min
Delta R.T.: -0.007 min
Response: 7092
Conc: 29.70 ng/ml

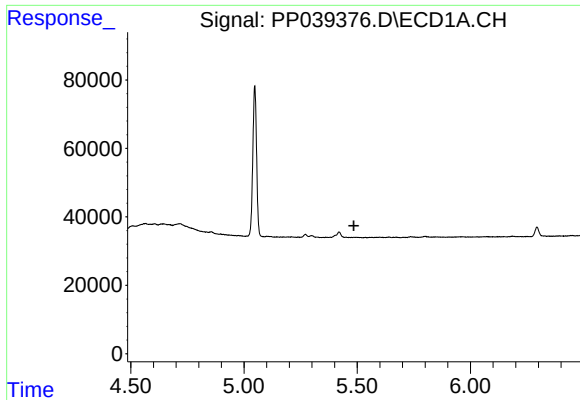

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

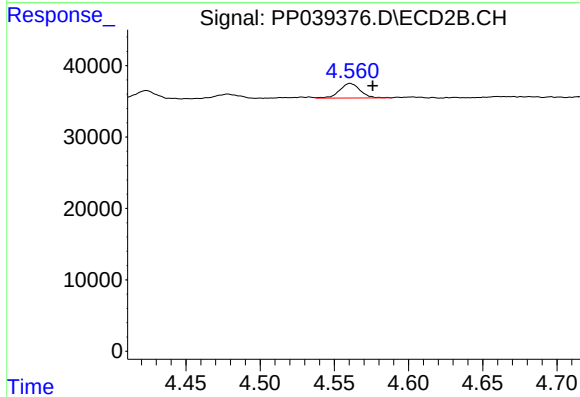


#10 AR-1221-3

R.T.: 4.561 min
Delta R.T.: -0.015 min
Response: 19608
Conc: 25.26 ng/ml

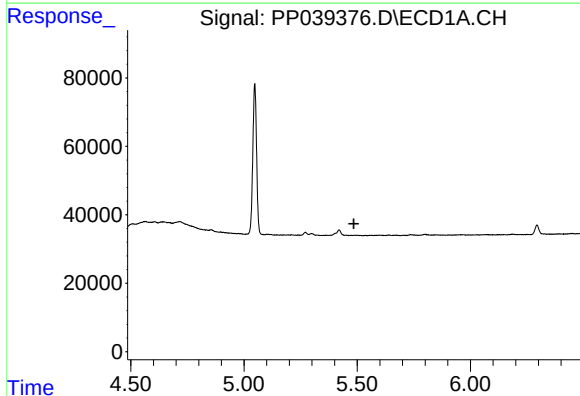


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.485 min
Response: 0
Conc: N.D.

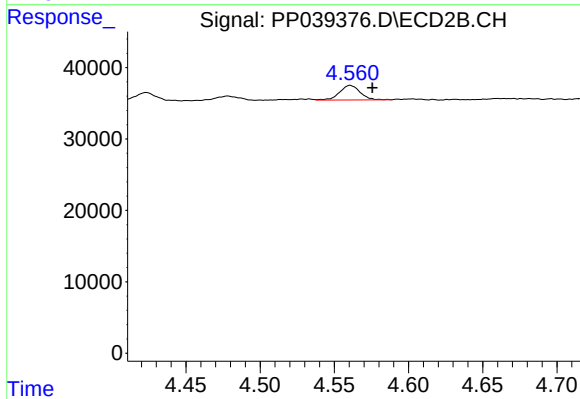

#11 AR-1232-1


R.T.: 4.561 min
Delta R.T.: -0.015 min
Response: 19608
Conc: 33.71 ng/ml

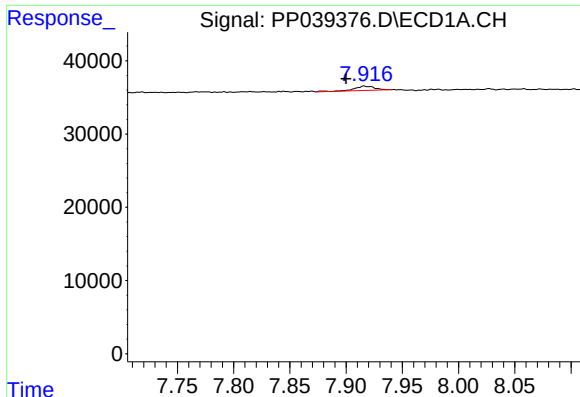

#28 AR-1254-3


R.T.: 7.916 min
Delta R.T.: 0.016 min
Response: 7593
Conc: 4.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

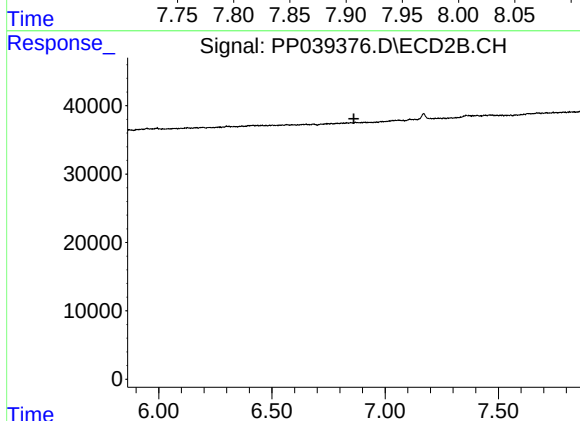


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

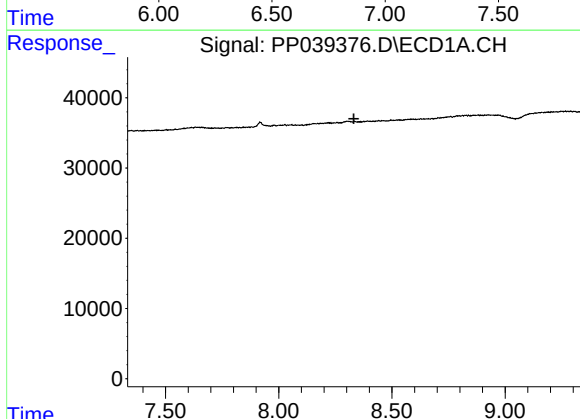


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.332 min
Response: 0
Conc: N.D.

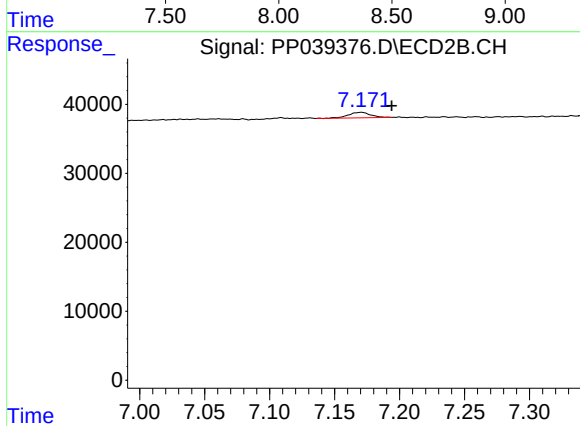

#32 AR-1260-2


R.T.: 7.171 min
Delta R.T.: -0.023 min
Response: 9490
Conc: 5.59 ng/ml

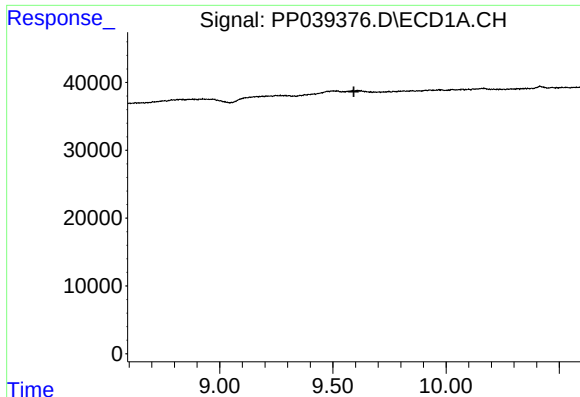

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

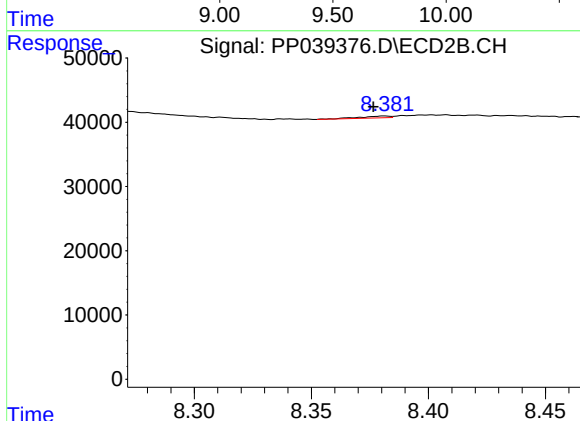


#38 AR-1262-3

R.T.: 8.381 min
Delta R.T.: 0.005 min
Response: 2464
Conc: 1.92 ng/ml

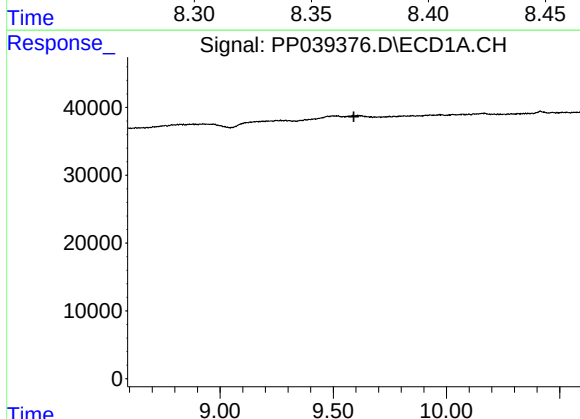

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.591 min
Response: 0
Conc: N.D.

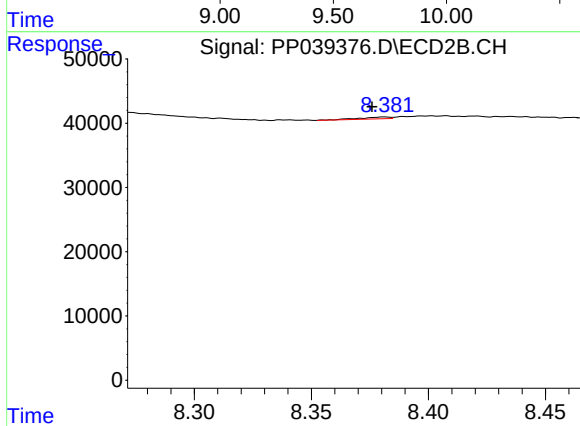

#41 AR-1268-1

R.T.: 8.381 min
Delta R.T.: 0.005 min
Response: 2464
Conc: 0.64 ng/ml