

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
 Data File : PP039375.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Sep 2021 12:54
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 13:14:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Sep 20 01:59:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.047	4.121	629853	661433	25.113	24.390
2) SA Decachlor...	11.171	9.497	602806	720841	29.150	26.703

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092021\
Data File : PP039375.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Sep 2021 12:54
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 13:14:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091721.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Sep 20 01:59:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

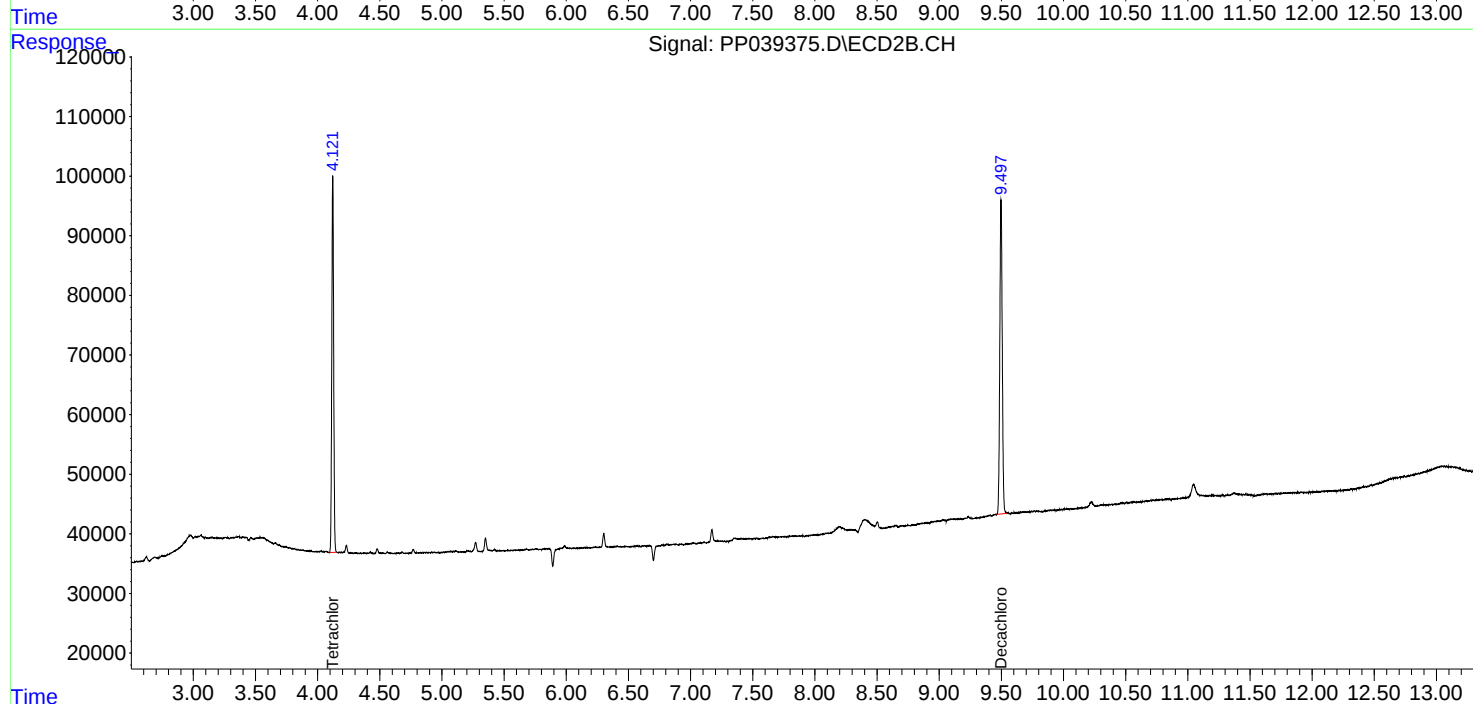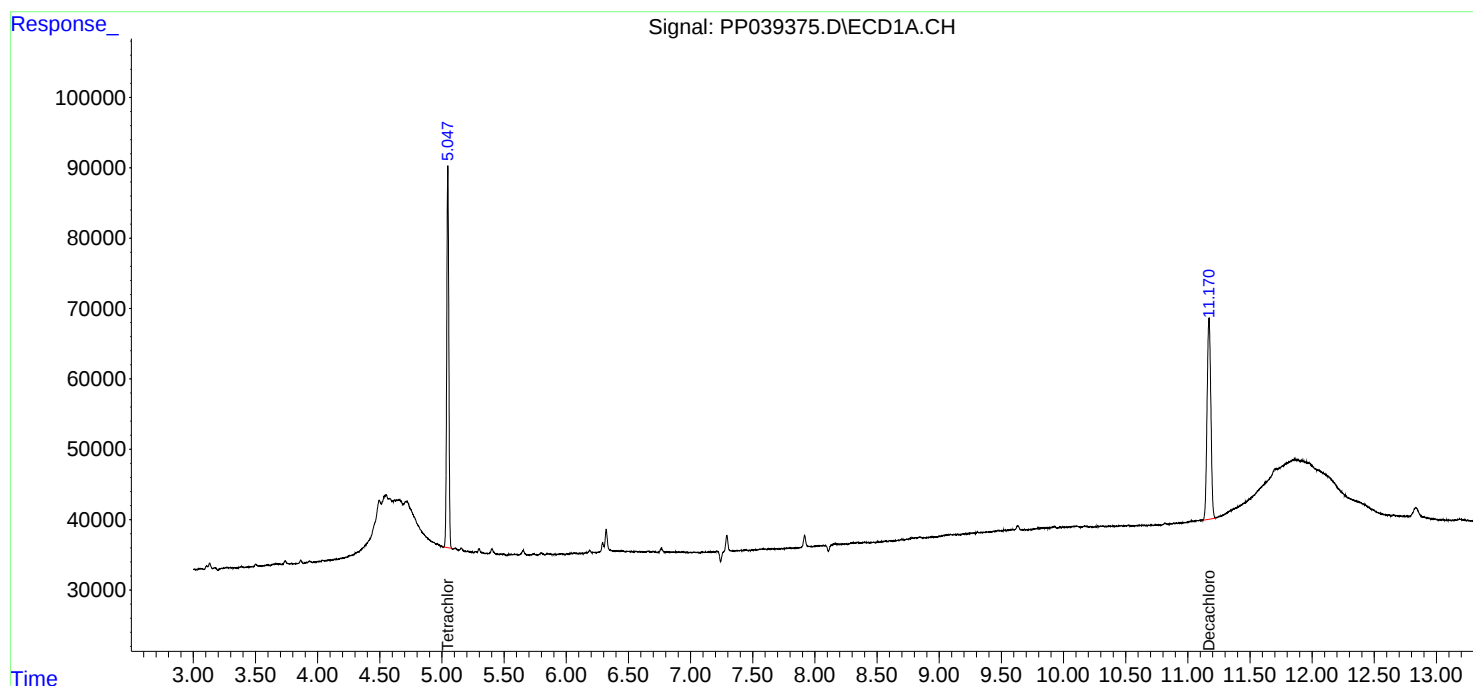


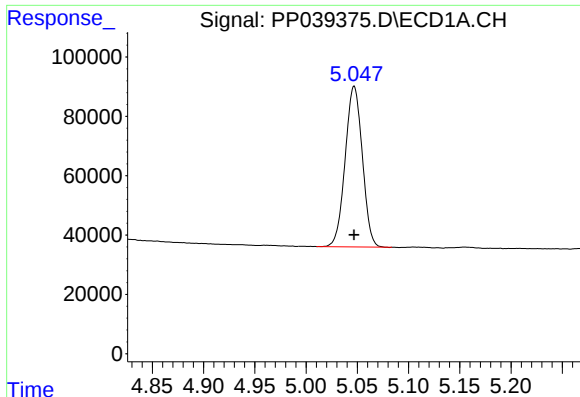

#1 Tetrachloro-m-xylene


R.T.: 5.047 min
Delta R.T.: 0.000 min
Response: 629853
Conc: 25.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

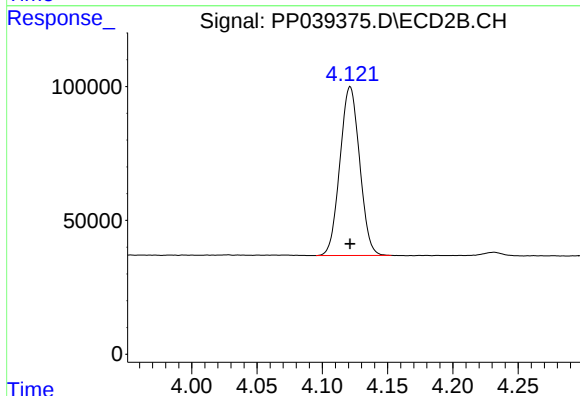


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: 0.000 min
Response: 661433
Conc: 24.39 ng/ml

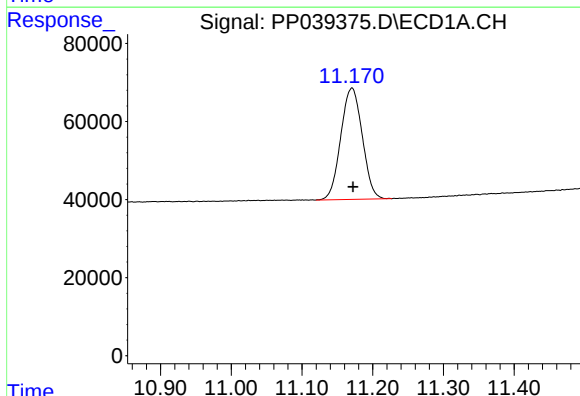

#2 Decachlorobiphenyl

R.T.: 11.171 min
Delta R.T.: -0.001 min
Response: 602806
Conc: 29.15 ng/ml

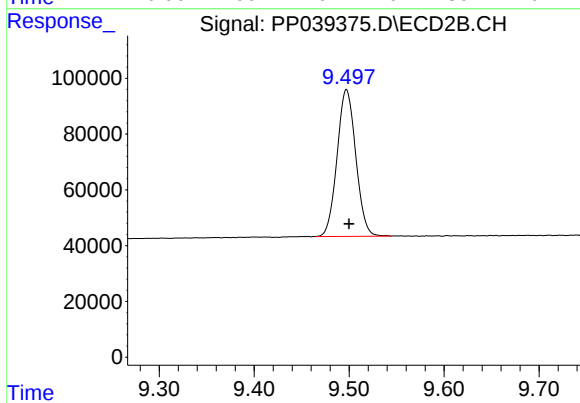

#2 Decachlorobiphenyl

R.T.: 9.497 min
Delta R.T.: -0.003 min
Response: 720841
Conc: 26.70 ng/ml