

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
 Data File : PP051468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 15:56
 Operator : YP\AJ
 Sample : N4714-01
 Misc : PP20775
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-01-091922

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:28:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.686	40320546	33728928	22.689	22.329
2) SA Decachlor...	10.256	8.787	30790792	23067912	19.923	19.252

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
Data File : PP051468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 15:56
Operator : YP\AJ
Sample : N4714-01
Misc : PP20775
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OK-01-091922

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:28:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

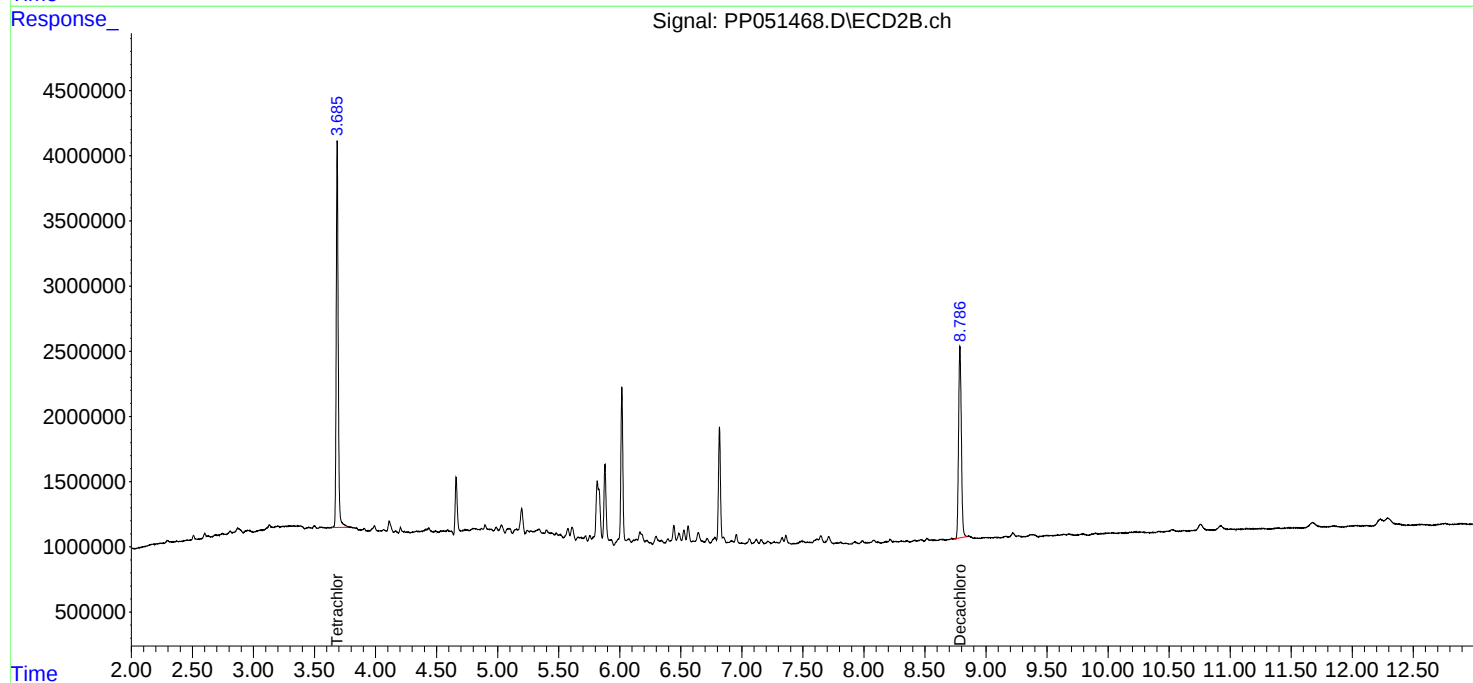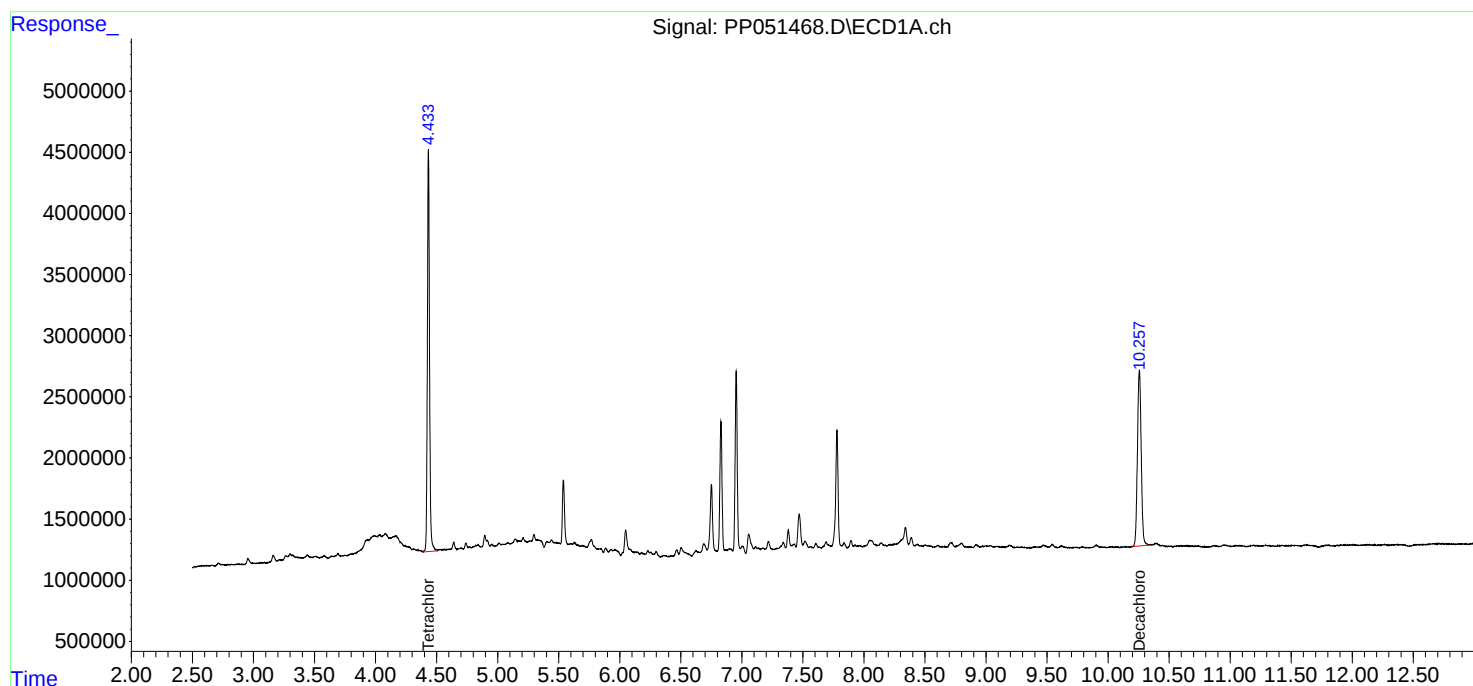


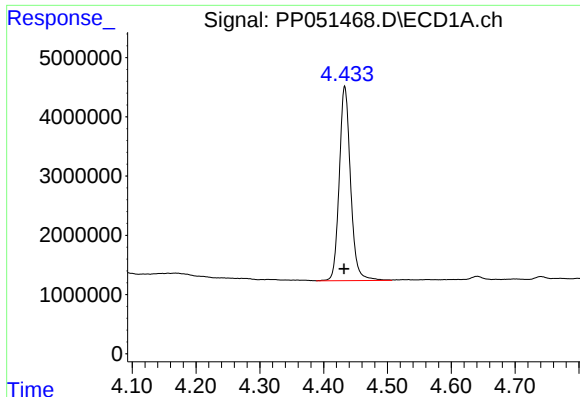

#1 Tetrachloro-m-xylene


R.T.: 4.433 min
Delta R.T.: 0.001 min
Response: 40320546
Conc: 22.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-01-091922

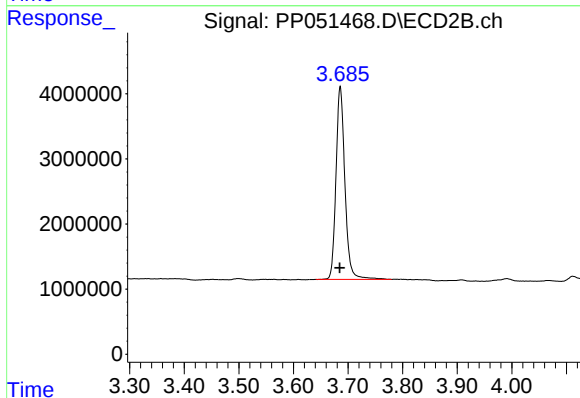


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: 0.001 min
Response: 33728928
Conc: 22.33 ng/ml

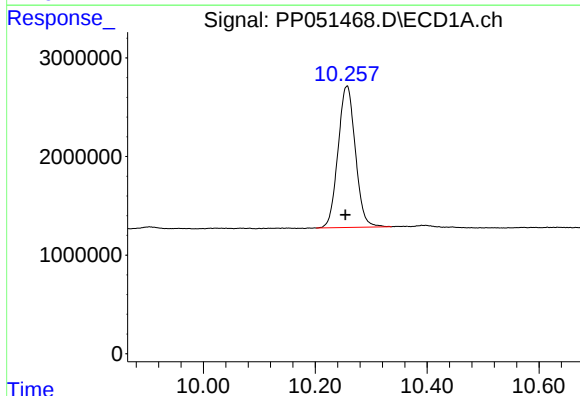

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.003 min
Response: 30790792
Conc: 19.92 ng/ml

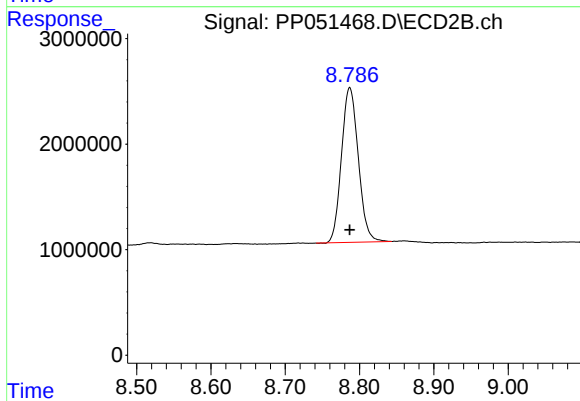

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 23067912
Conc: 19.25 ng/ml