

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
 Data File : PP051470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 16:30
 Operator : YP\AJ
 Sample : AR1221 250 PPB TEST
 Misc : PP20776
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221 250 PPB TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:29:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) L2	AR-1221-1	4.643	3.905	5533188	4627131	246.274 254.687
9) L2	AR-1221-2	4.729	3.992	3650794	2968896	214.503 215.574
10) L2	AR-1221-3	4.806	4.069	13537638	10804828	266.561 254.985



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
Data File : PP051470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 16:30
Operator : YP\AJ
Sample : AR1221 250 PPB TEST
Misc : PP20776
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221 250 PPB TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:29:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

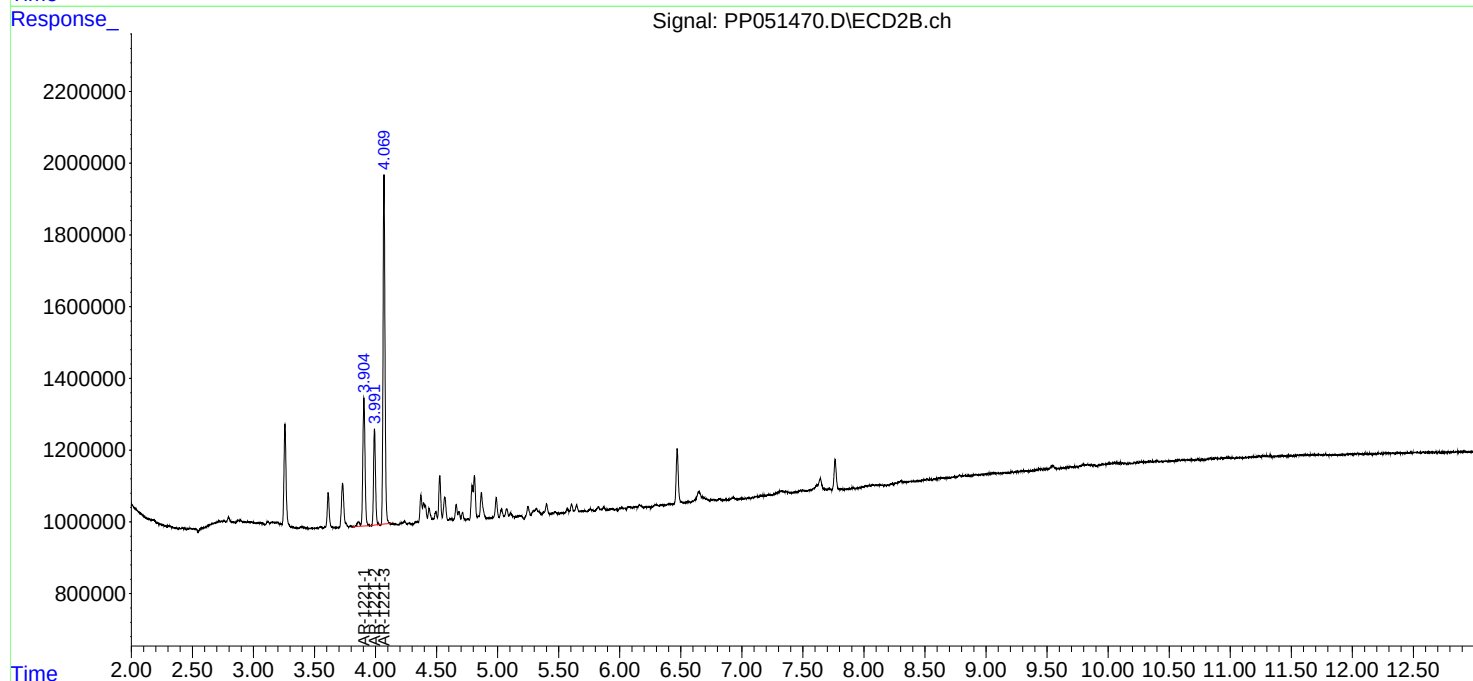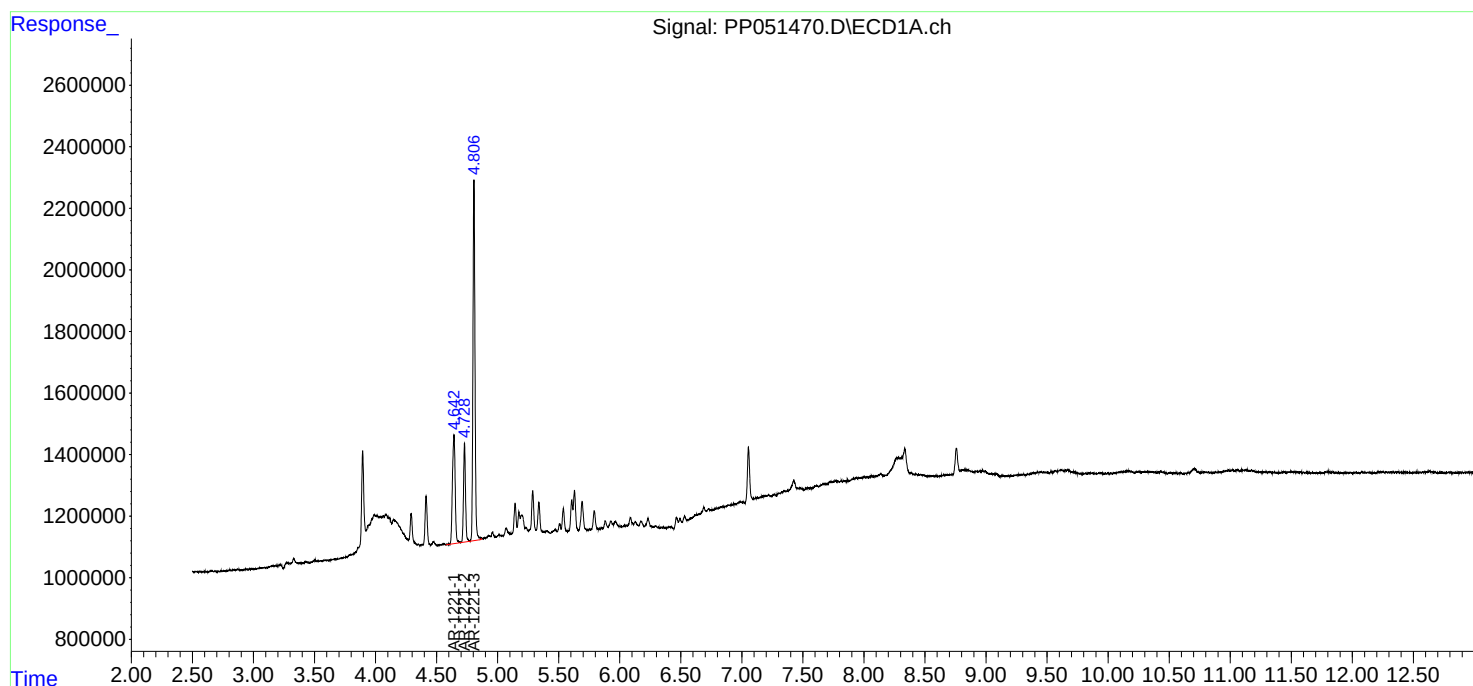


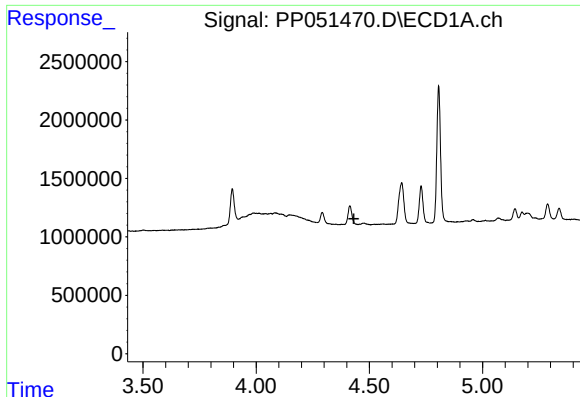

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1221 250 PPB TEST

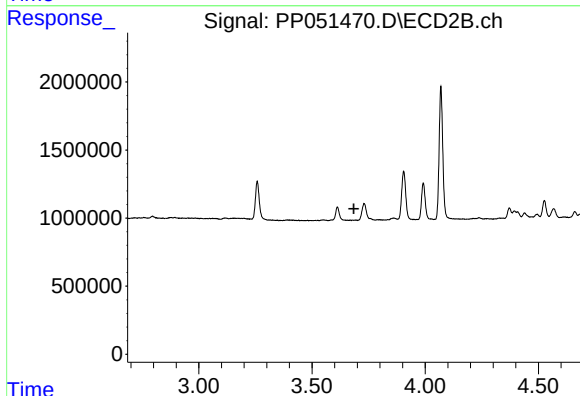


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.685 min
Response: 0
Conc: N.D.

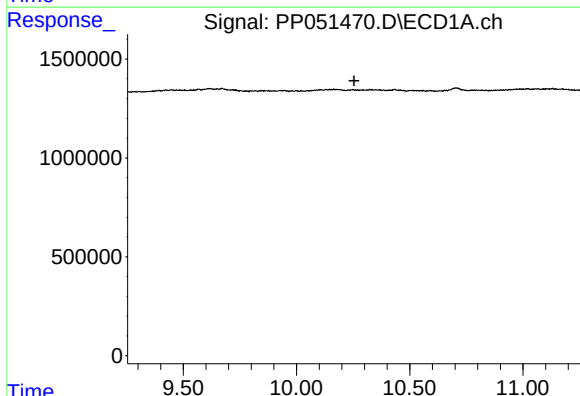


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.254 min
Response: 0
Conc: N.D.

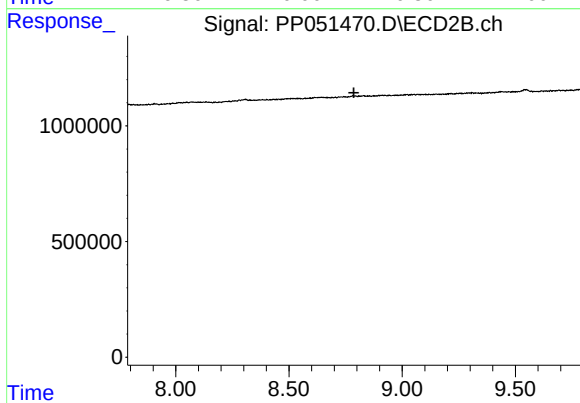

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.787 min
Response: 0
Conc: N.D.

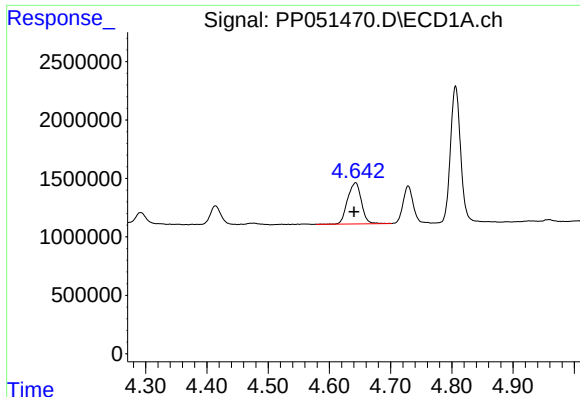

#8 AR-1221-1


R.T.: 4.643 min
Delta R.T.: 0.002 min
Response: 5533188
Conc: 246.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221 250 PPB TEST

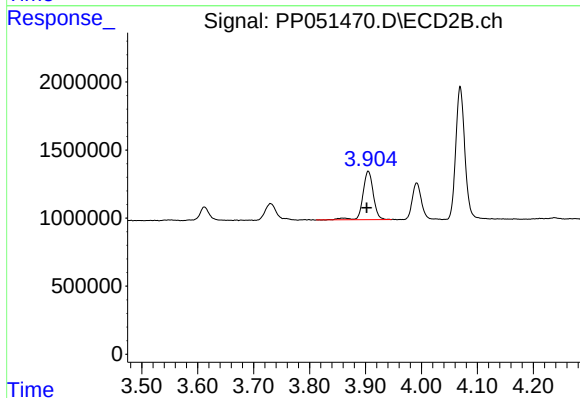


#8 AR-1221-1

R.T.: 3.905 min
Delta R.T.: 0.003 min
Response: 4627131
Conc: 254.69 ng/ml

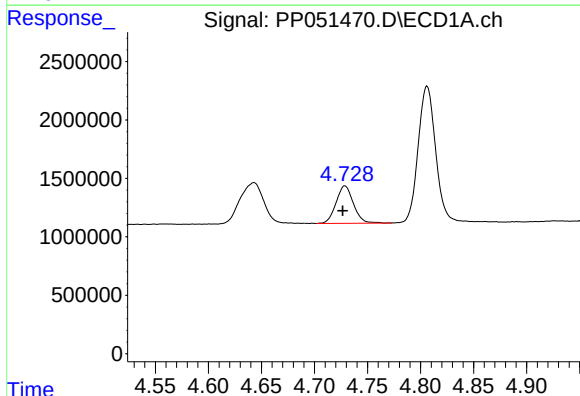


#9 AR-1221-2

R.T.: 4.729 min
Delta R.T.: 0.002 min
Response: 3650794
Conc: 214.50 ng/ml

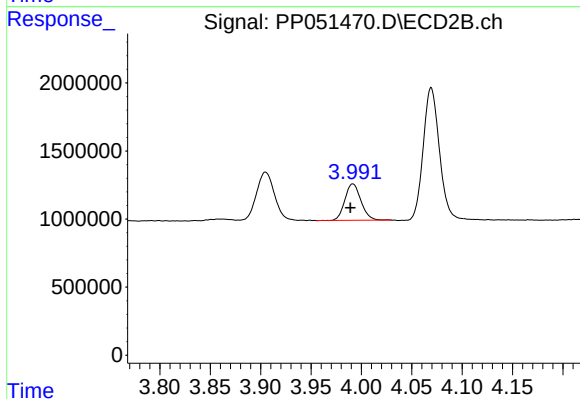

#9 AR-1221-2


R.T.: 3.992 min
Delta R.T.: 0.002 min
Response: 2968896
Conc: 215.57 ng/ml

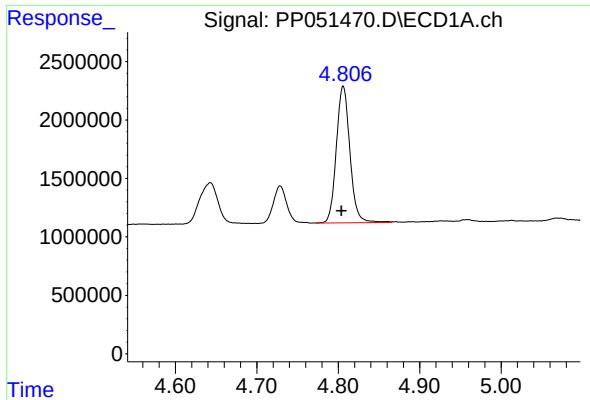

#10 AR-1221-3

R.T.: 4.806 min
Delta R.T.: 0.002 min
Response: 13537638
Conc: 266.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221 250 PPB TEST

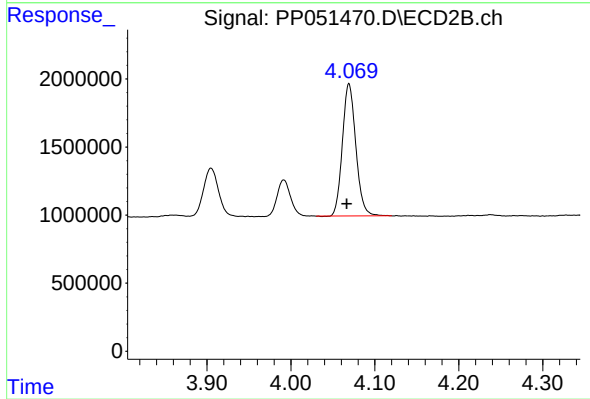

#10 AR-1221-3

R.T.: 4.069 min
Delta R.T.: 0.003 min
Response: 10804828
Conc: 254.99 ng/ml