

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
 Data File : PP051471.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 16:46
 Operator : YP\AJ
 Sample : AR1232 250 PPB TEST
 Misc : PP20777
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232 250 PPB TEST

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2022
 Supervised By :Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:30:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
11)	L3	AR-1232-1	4.805	4.068	11565267	9033484	277.281	261.866
12)	L3	AR-1232-2	5.337	4.809	5652052	7727344	261.045	251.582
13)	L3	AR-1232-3	5.629	4.988	9909123	4007443	262.549	252.470m
14)	L3	AR-1232-4	5.791	5.072	4594795	3853907	253.384	259.661m
15)	L3	AR-1232-5	5.881	5.248	3877634	4213443	258.497	249.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
Data File : PP051471.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 16:46
Operator : YP\AJ
Sample : AR1232 250 PPB TEST
Misc : PP20777
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1232 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:30:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

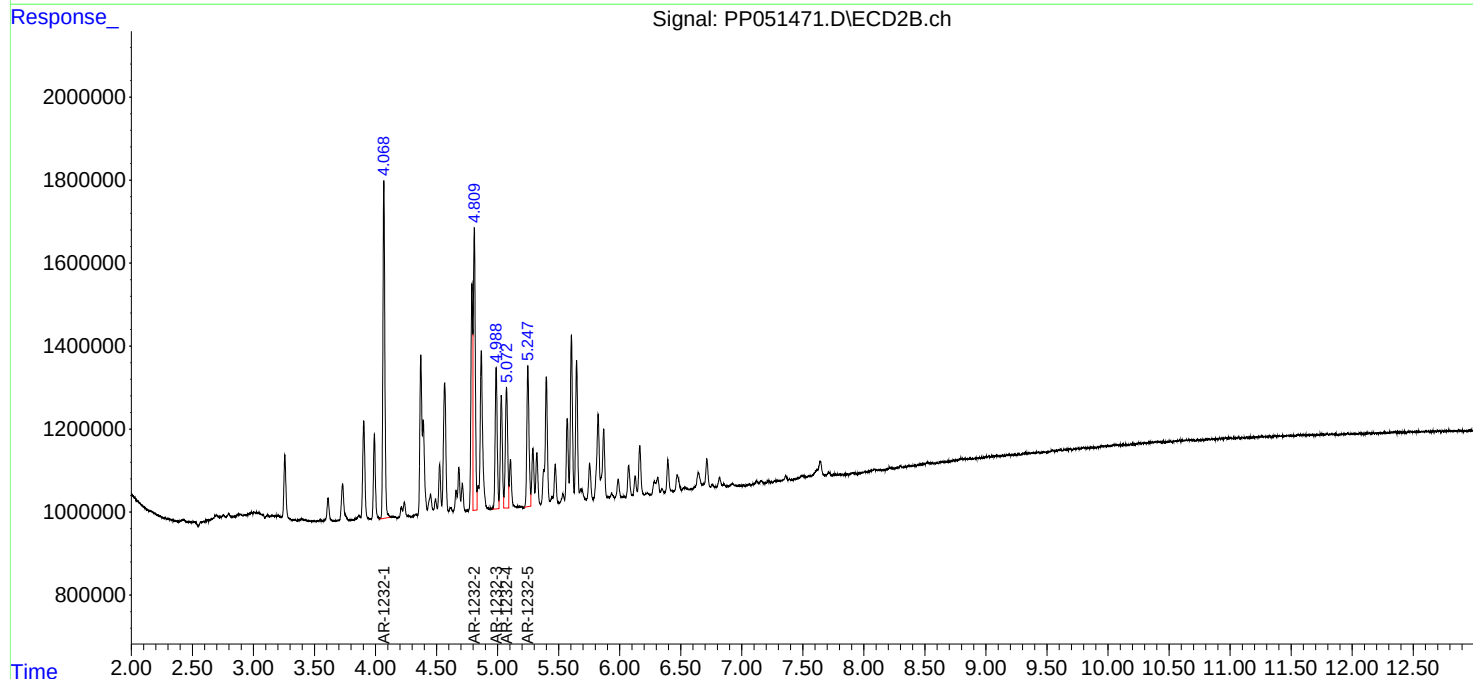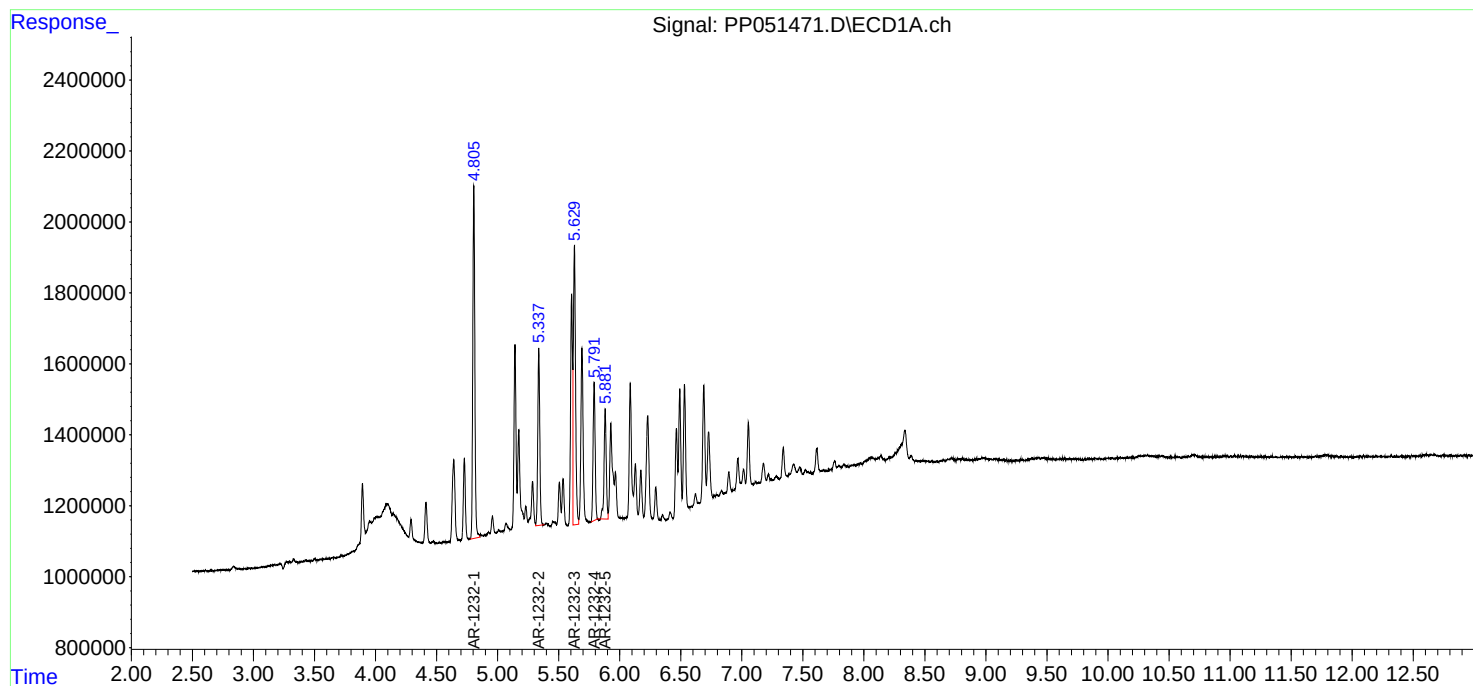

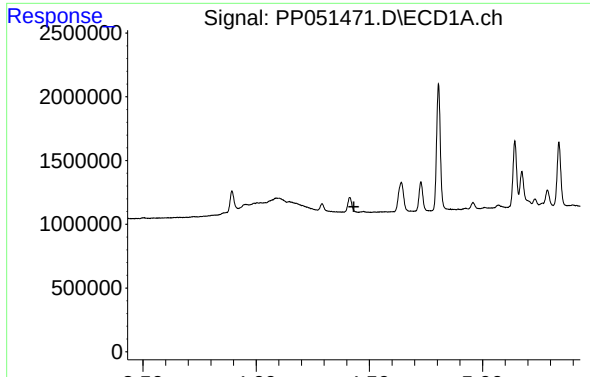


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1232 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

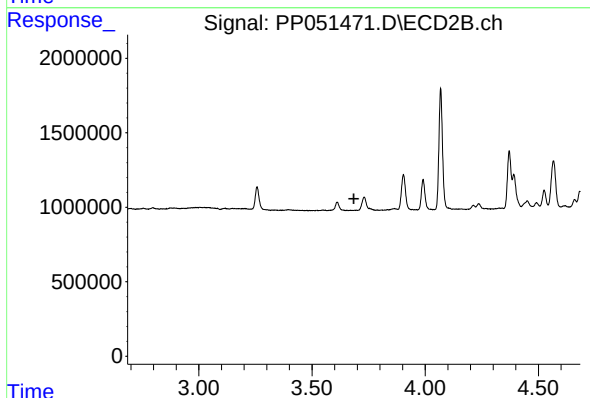


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.685 min
Response: 0
Conc: N.D.

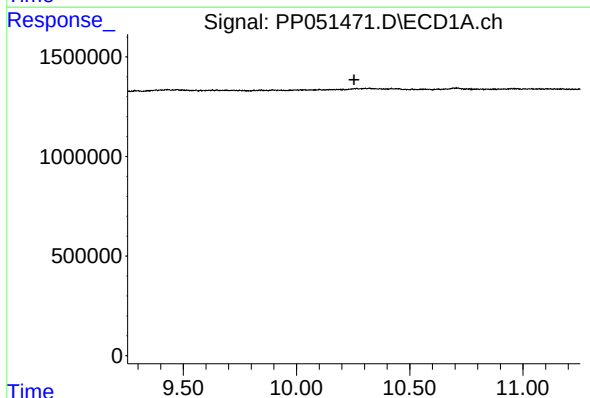


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.254 min
Response: 0
Conc: N.D.

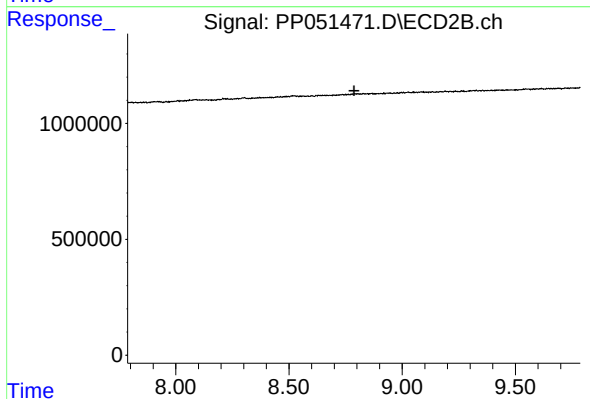

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.787 min
Response: 0
Conc: N.D.

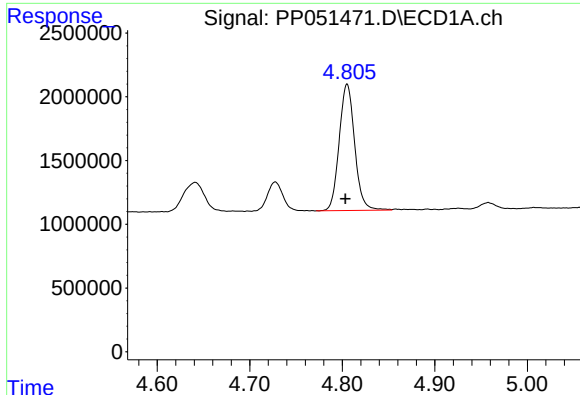


#11 AR-1232-1

R.T.: 4.805 min
Delta R.T.: 0.002 min
Response: 11565267
Conc: 277.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1232 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

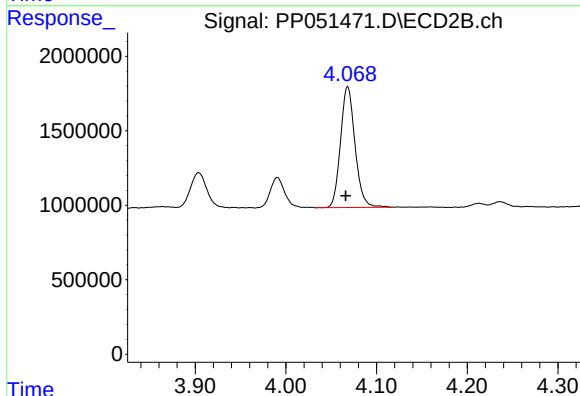


#11 AR-1232-1

R.T.: 4.068 min
Delta R.T.: 0.002 min
Response: 9033484
Conc: 261.87 ng/ml

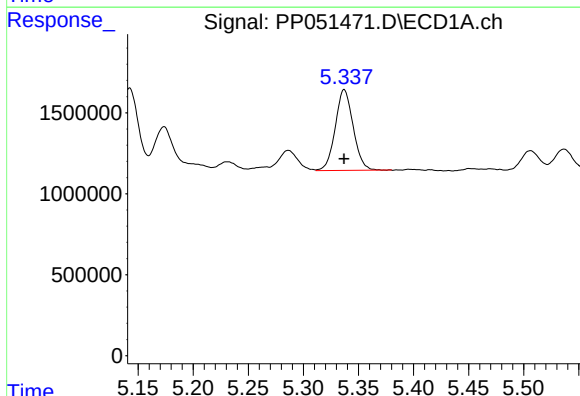


#12 AR-1232-2

R.T.: 5.337 min
Delta R.T.: 0.000 min
Response: 5652052
Conc: 261.04 ng/ml

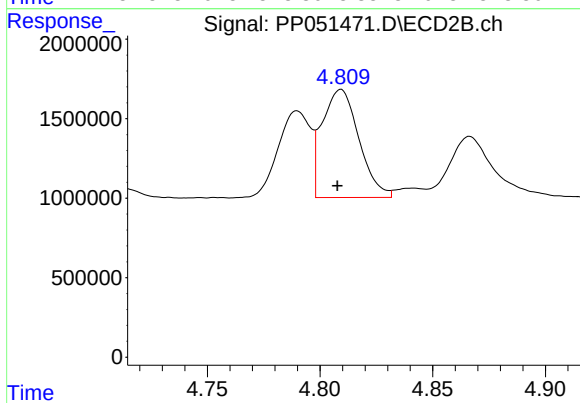

#12 AR-1232-2

R.T.: 4.809 min
Delta R.T.: 0.002 min
Response: 7727344
Conc: 251.58 ng/ml

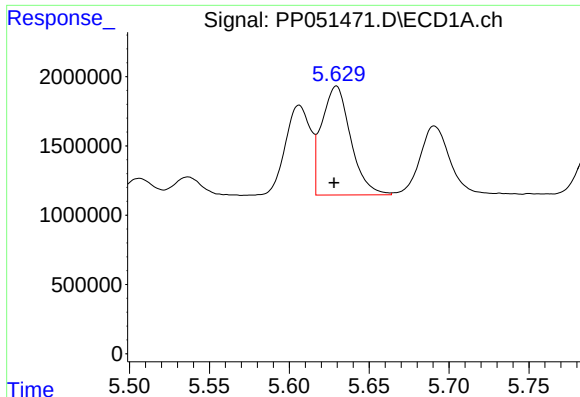


#13 AR-1232-3

R.T.: 5.629 min
Delta R.T.: 0.001 min
Response: 9909123
Conc: 262.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1232 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

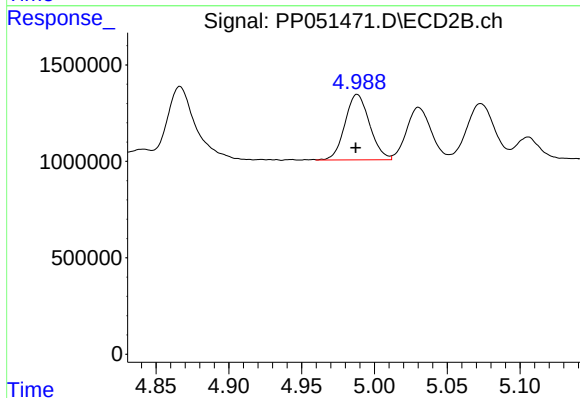


#13 AR-1232-3

R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 4007443
Conc: 252.47 ng/ml m

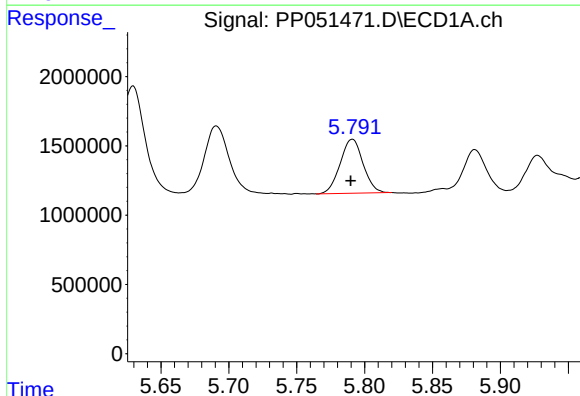


#14 AR-1232-4

R.T.: 5.791 min
Delta R.T.: 0.001 min
Response: 4594795
Conc: 253.38 ng/ml

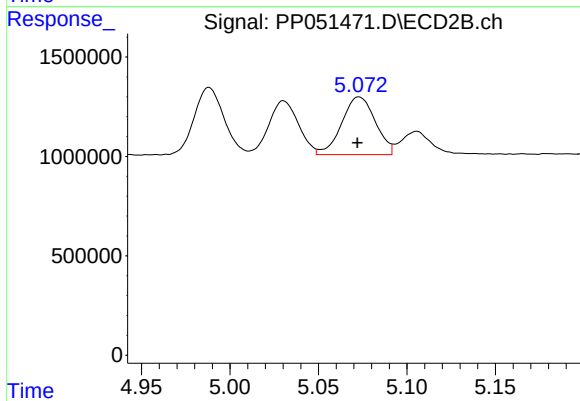

#14 AR-1232-4

R.T.: 5.072 min
Delta R.T.: 0.000 min
Response: 3853907
Conc: 259.66 ng/ml m

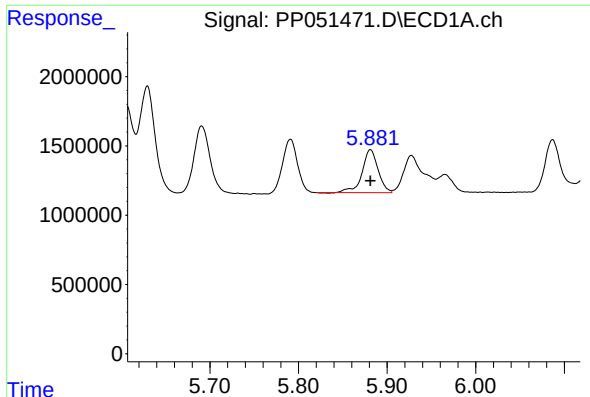


#15 AR-1232-5

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 3877634
Conc: 258.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1232 250 PPB TEST

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

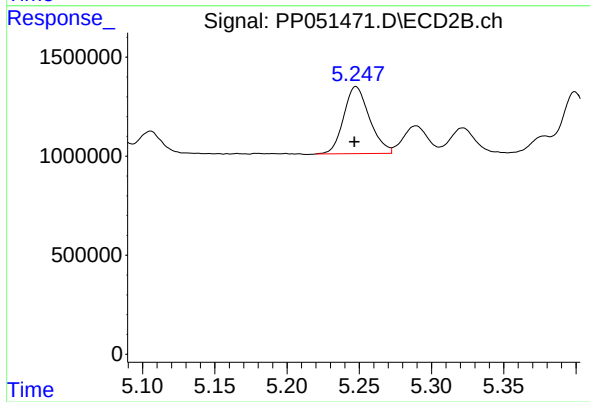

#15 AR-1232-5

R.T.: 5.248 min
Delta R.T.: 0.001 min
Response: 4213443
Conc: 249.90 ng/ml