

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
 Data File : PP051474.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 17:36
 Operator : YP\AJ
 Sample : AR1254 250 PPB TEST
 Misc : PP20780
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254 250 PPB TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:31:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
26)	L6	AR-1254-1	6.466	5.606	13989350	17577210	225.163	216.389
27)	L6	AR-1254-2	6.686	5.755	23844196	15228641	206.566	216.695
28)	L6	AR-1254-3	7.053	6.165	25302292	23990488	207.850	213.766
29)	L6	AR-1254-4	7.339	6.395	17239048	13770523	208.157	212.153
30)	L6	AR-1254-5	7.760	6.818	19349159	19997356	217.178	213.881



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
Data File : PP051474.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 17:36
Operator : YP\AJ
Sample : AR1254 250 PPB TEST
Misc : PP20780
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254 250 PPB TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:31:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

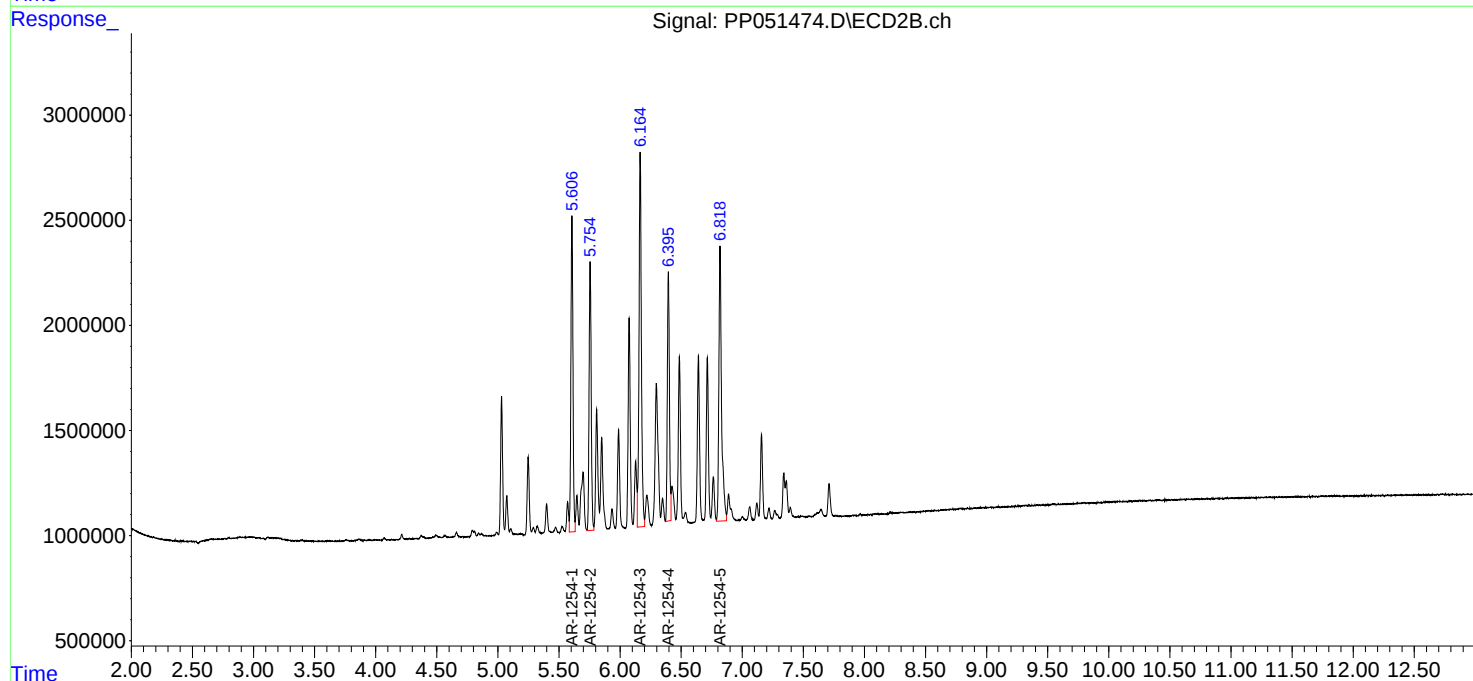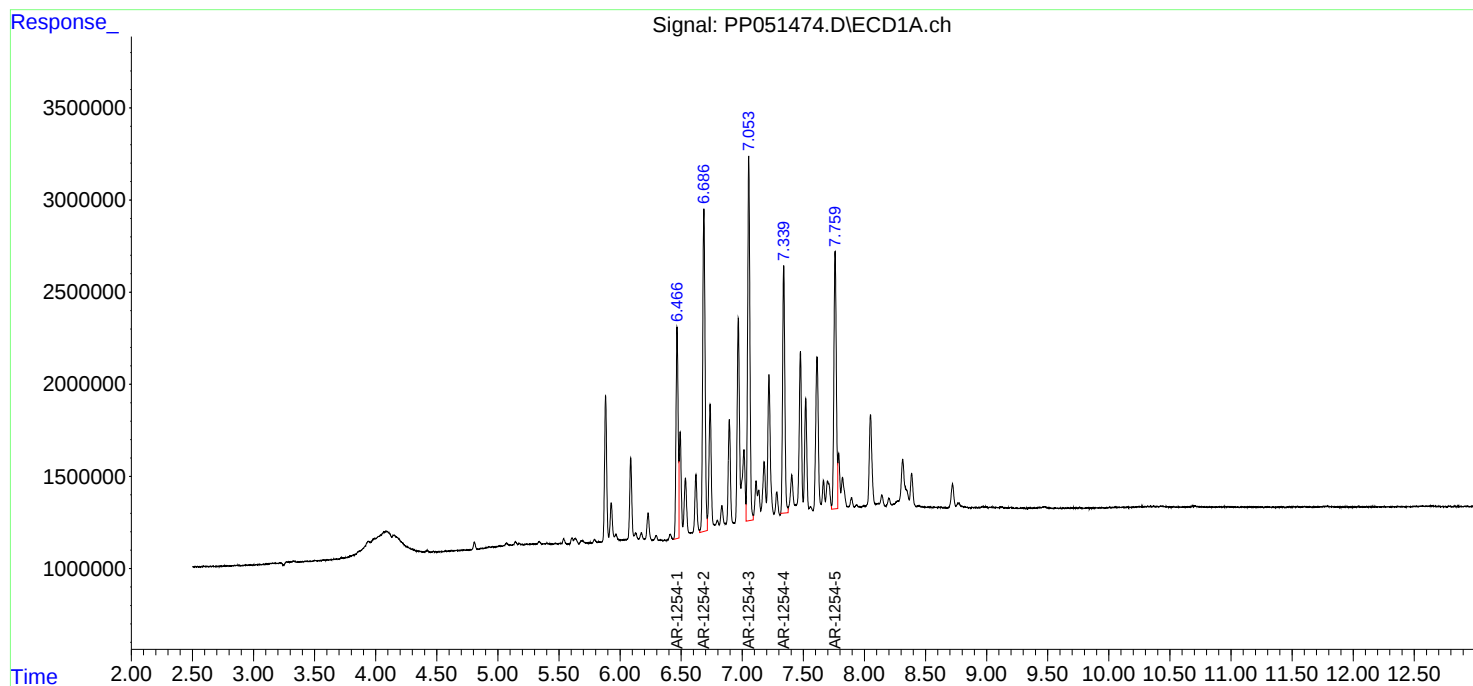


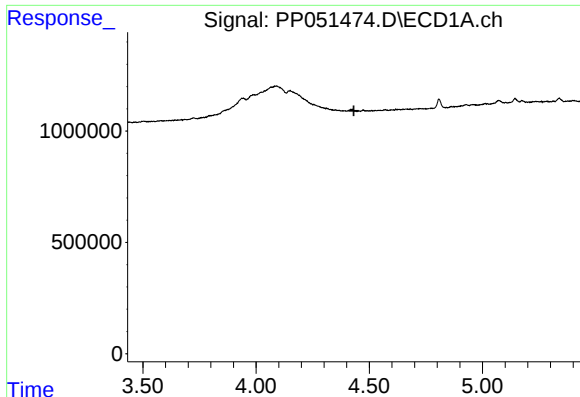

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1254 250 PPB TEST

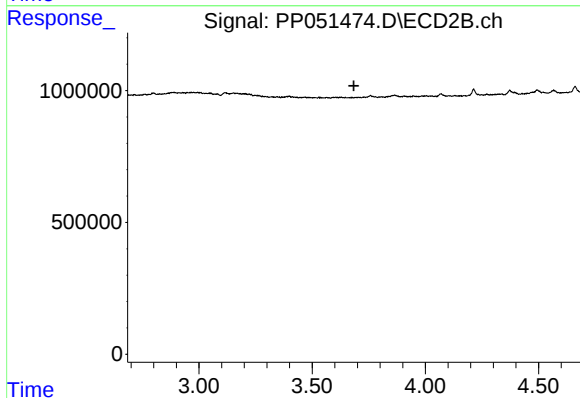


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.685 min
Response: 0
Conc: N.D.

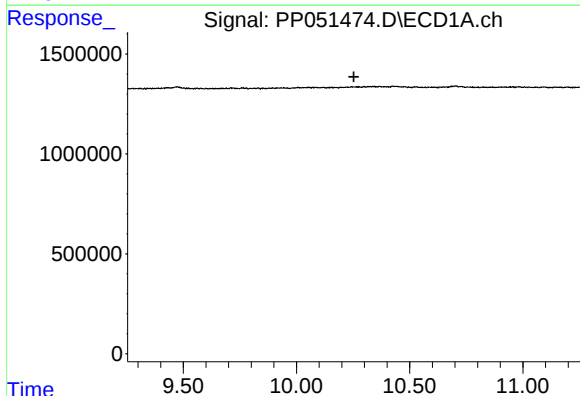


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.254 min
Response: 0
Conc: N.D.

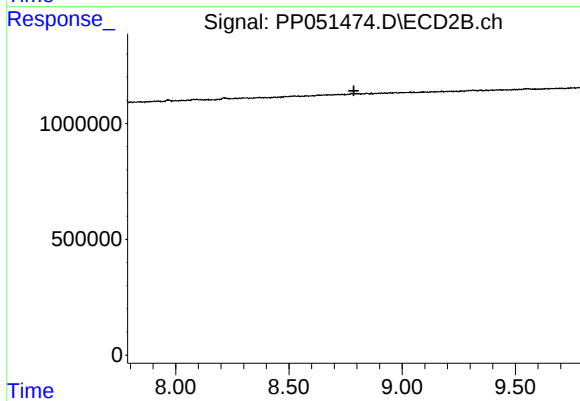

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.787 min
Response: 0
Conc: N.D.

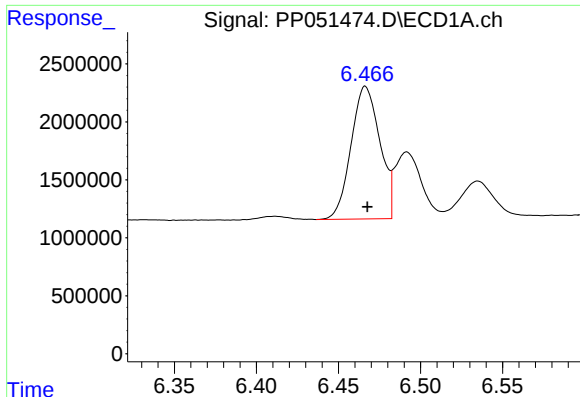

#26 AR-1254-1


R.T.: 6.466 min
Delta R.T.: -0.001 min
Response: 13989350
Conc: 225.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254 250 PPB TEST

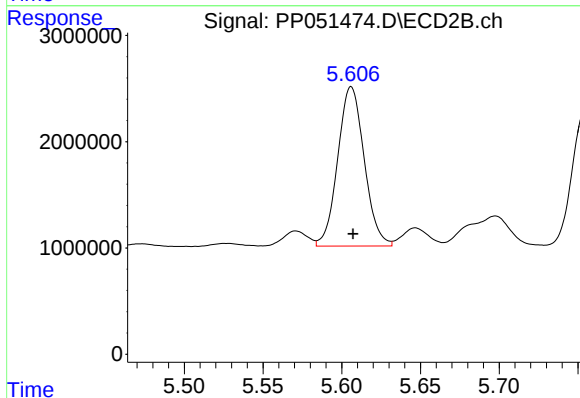


#26 AR-1254-1

R.T.: 5.606 min
Delta R.T.: -0.001 min
Response: 17577210
Conc: 216.39 ng/ml

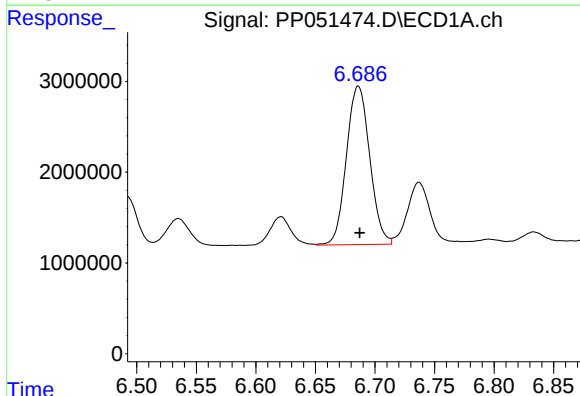


#27 AR-1254-2

R.T.: 6.686 min
Delta R.T.: -0.001 min
Response: 23844196
Conc: 206.57 ng/ml

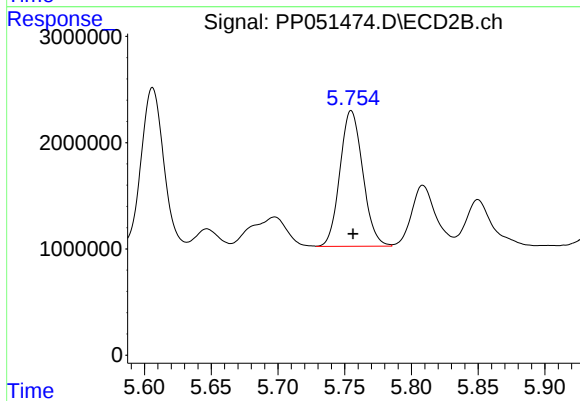

#27 AR-1254-2


R.T.: 5.755 min
Delta R.T.: -0.001 min
Response: 15228641
Conc: 216.69 ng/ml

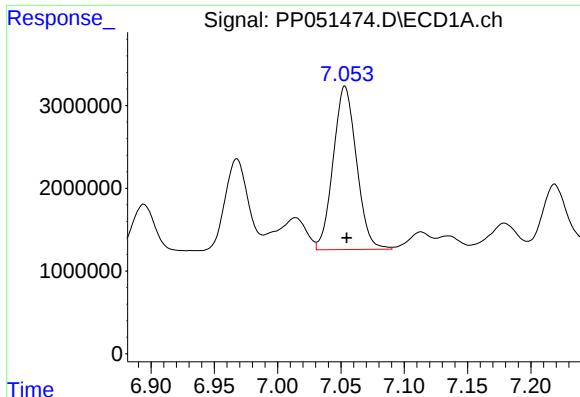

#28 AR-1254-3


R.T.: 7.053 min
Delta R.T.: -0.001 min
Response: 25302292
Conc: 207.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254 250 PPB TEST

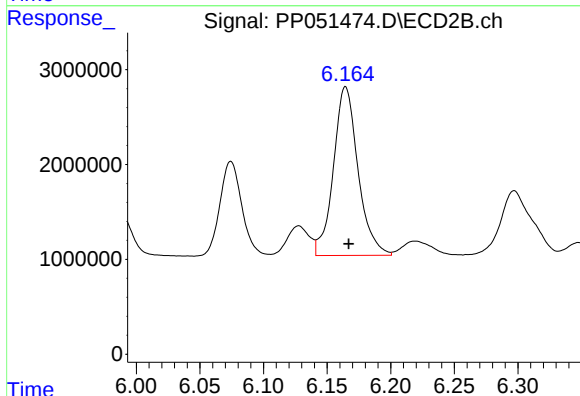


#28 AR-1254-3

R.T.: 6.165 min
Delta R.T.: -0.003 min
Response: 23990488
Conc: 213.77 ng/ml

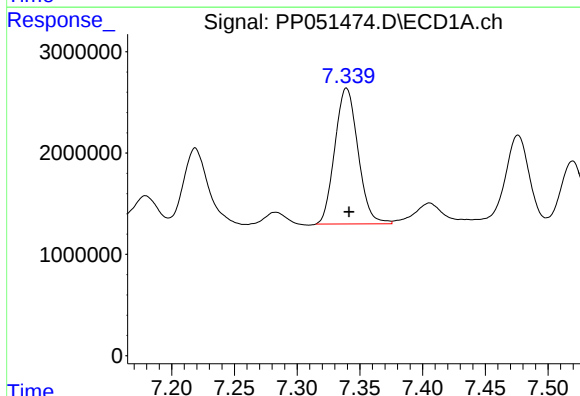


#29 AR-1254-4

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 17239048
Conc: 208.16 ng/ml

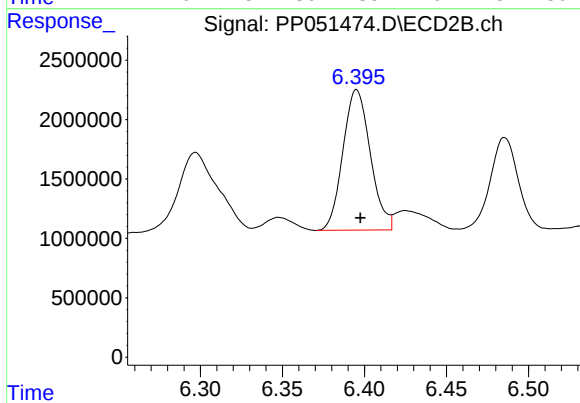

#29 AR-1254-4


R.T.: 6.395 min
Delta R.T.: -0.002 min
Response: 13770523
Conc: 212.15 ng/ml

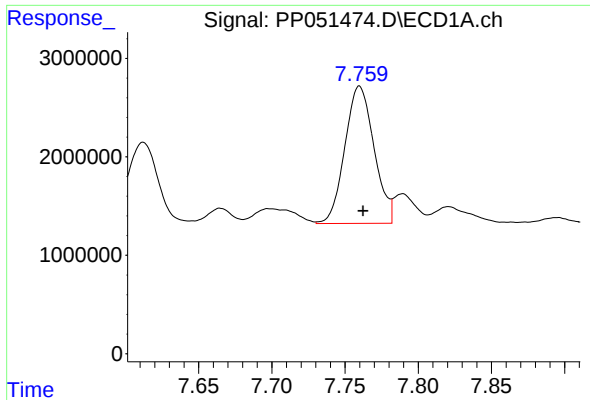

#30 AR-1254-5

R.T.: 7.760 min
Delta R.T.: -0.002 min
Response: 19349159
Conc: 217.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254 250 PPB TEST

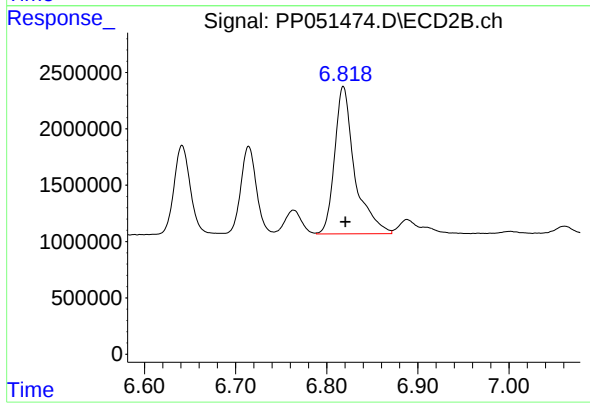

#30 AR-1254-5

R.T.: 6.818 min
Delta R.T.: -0.002 min
Response: 19997356
Conc: 213.88 ng/ml