

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
 Data File : PP051475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2022 17:52
 Operator : YP\AJ
 Sample : AR1262 250 PPB TEST
 Misc : PP20781
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1262 250 PPB TEST

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2022
 Supervised By :Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 01:32:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
36)	L8	AR-1262-1	7.835	6.856	25708435 23021377	250.766 245.553
37)	L8	AR-1262-2	8.386	7.119	39378969 20550639	248.078 243.883
38)	L8	AR-1262-3	8.707	7.647	28880138 16156140	249.592 249.173
39)	L8	AR-1262-4	8.798	7.712	13059618 28301579	263.352m 238.675
40)	L8	AR-1262-5	9.471	8.213	15606474 13056476	249.091 248.139m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092022\
Data File : PP051475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2022 17:52
Operator : YP\AJ
Sample : AR1262 250 PPB TEST
Misc : PP20781
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1262 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 01:32:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

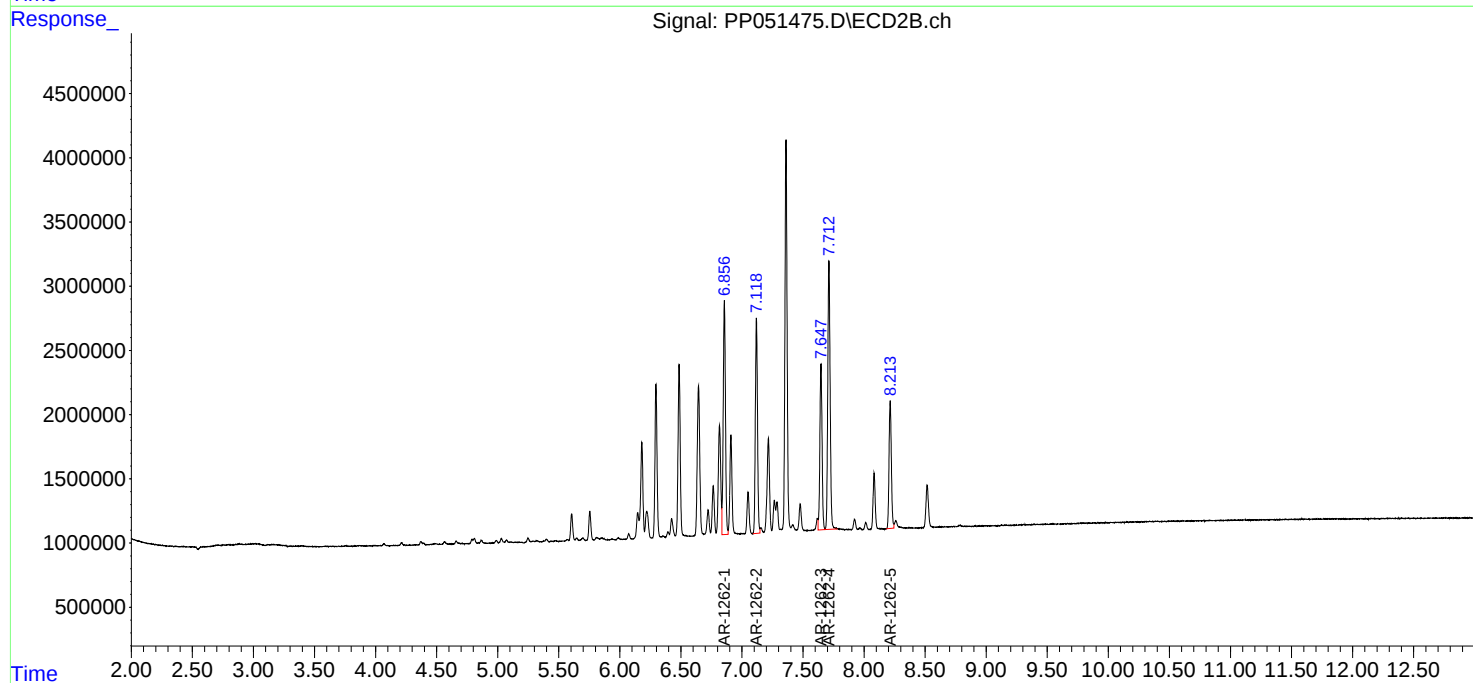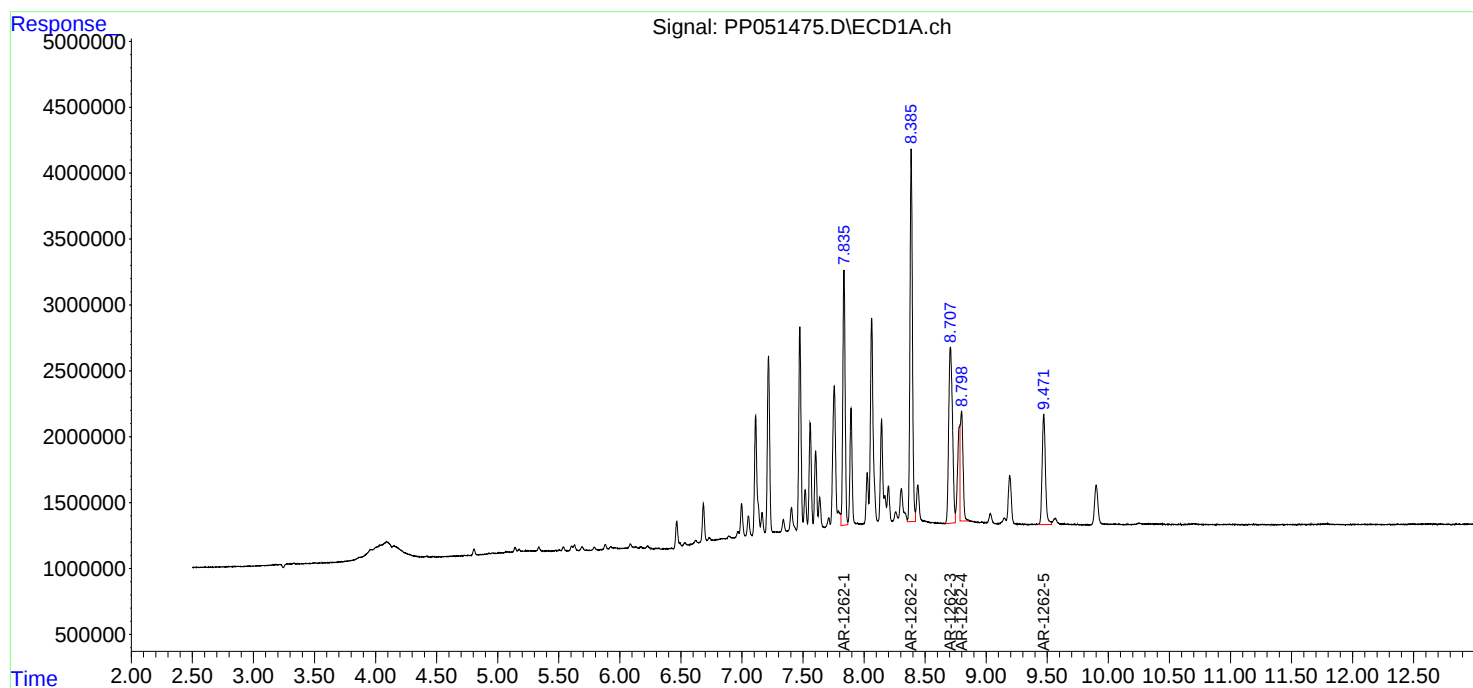

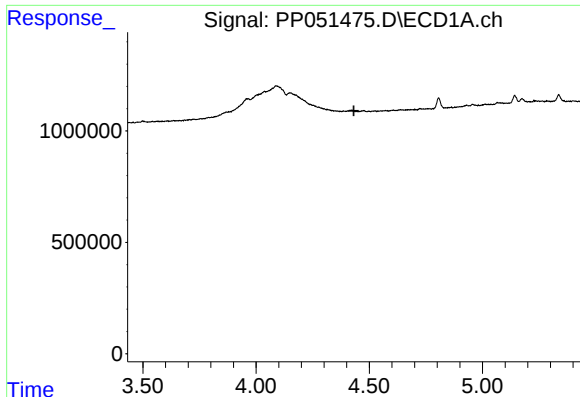


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
AR1262 250 PPB TEST

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

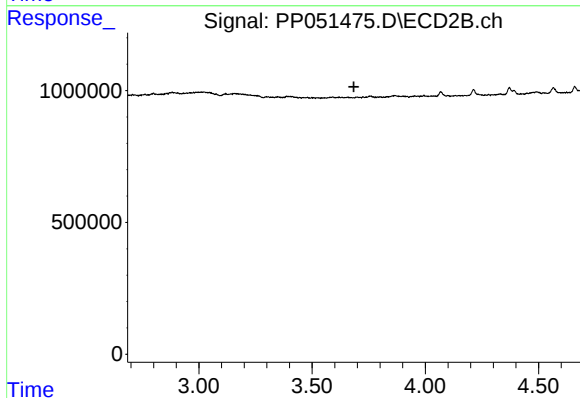


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.685 min
Response: 0
Conc: N.D.


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.254 min
Response: 0
Conc: N.D.

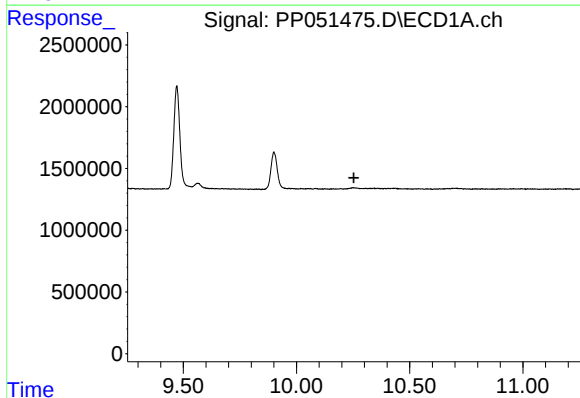

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.787 min
Response: 0
Conc: N.D.

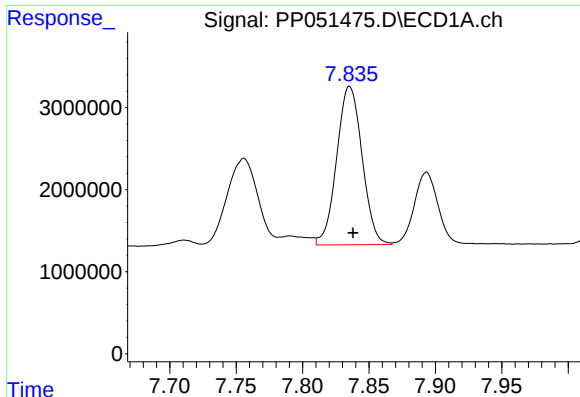


#36 AR-1262-1

R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 25708435
Conc: 250.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

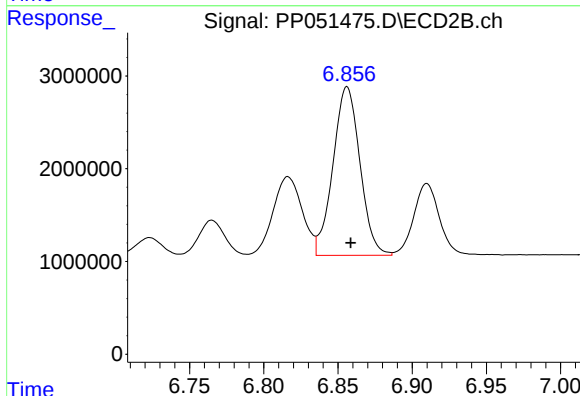


#36 AR-1262-1

R.T.: 6.856 min
Delta R.T.: -0.003 min
Response: 23021377
Conc: 245.55 ng/ml

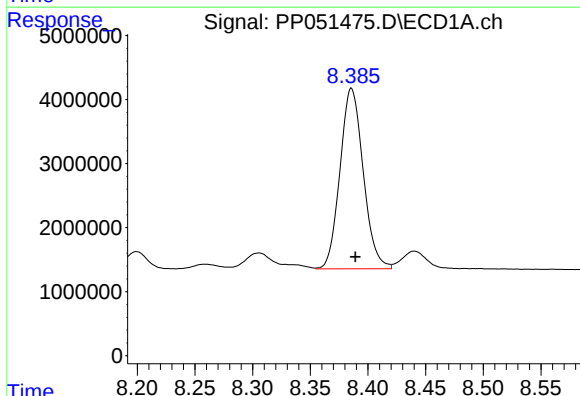


#37 AR-1262-2

R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 39378969
Conc: 248.08 ng/ml

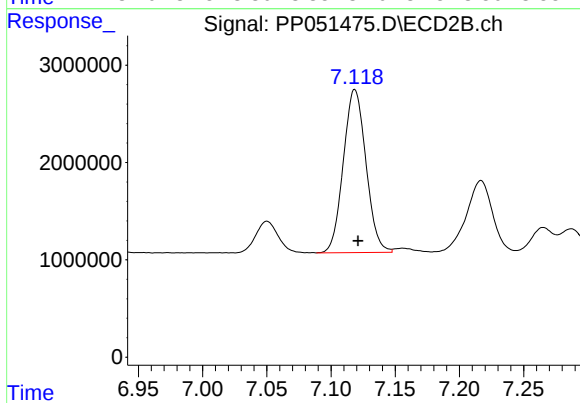

#37 AR-1262-2

R.T.: 7.119 min
Delta R.T.: -0.003 min
Response: 20550639
Conc: 243.88 ng/ml

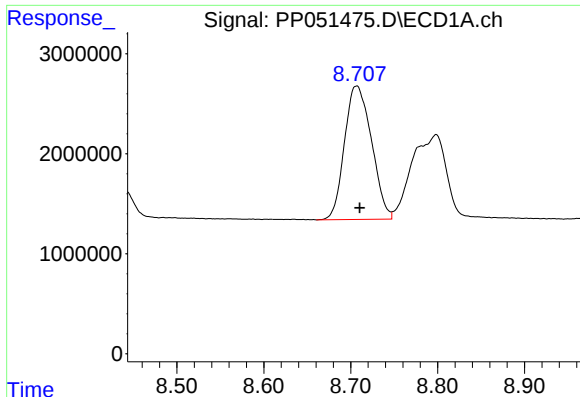


#38 AR-1262-3

R.T.: 8.707 min
Delta R.T.: -0.004 min
Response: 28880138
Conc: 249.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262 250 PPB TEST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

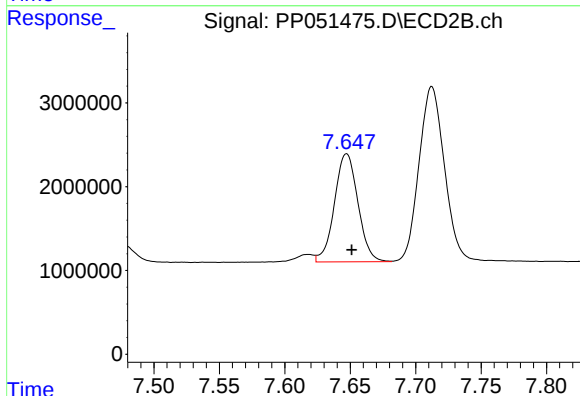


#38 AR-1262-3

R.T.: 7.647 min
Delta R.T.: -0.004 min
Response: 16156140
Conc: 249.17 ng/ml

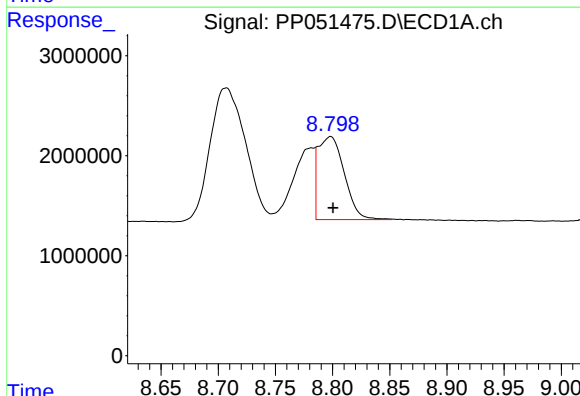


#39 AR-1262-4

R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 13059618
Conc: 263.35 ng/ml m

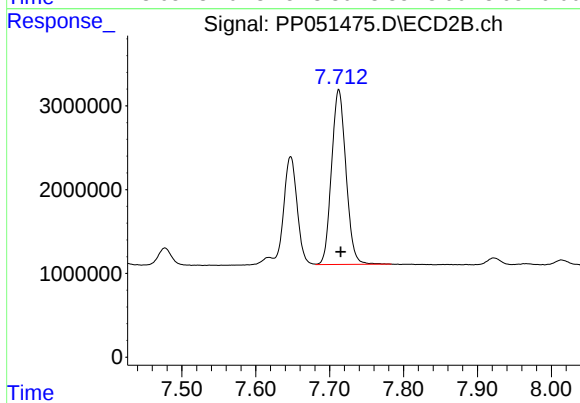

#39 AR-1262-4

R.T.: 7.712 min
Delta R.T.: -0.003 min
Response: 28301579
Conc: 238.68 ng/ml

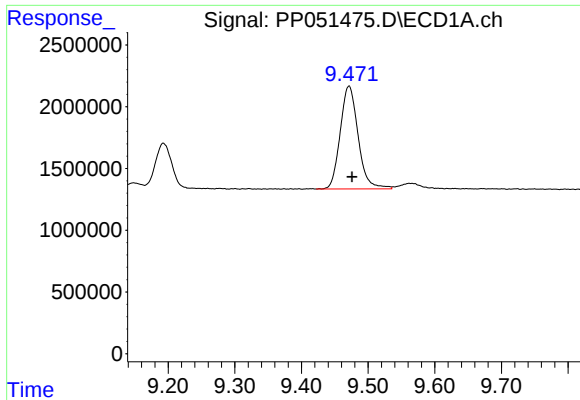


#40 AR-1262-5

R.T.: 9.471 min
Delta R.T.: -0.005 min
Response: 15606474
Conc: 249.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1262 250 PPB TEST

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

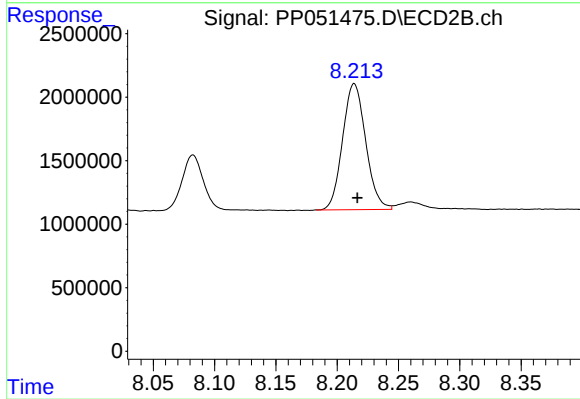

#40 AR-1262-5

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 13056476
Conc: 248.14 ng/ml m