

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092023\
 Data File : PP060033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 17:35
 Operator : YP\AJ
 Sample : 04501-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 02:13:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.510	3.668	37034359	29478915	17.803	18.098
2) SA Decachlor...	10.429	8.742	23742785	22175718	15.566m	14.645m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092023\
Data File : PP060033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 17:35
Operator : YP\AJ
Sample : 04501-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 02:13:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

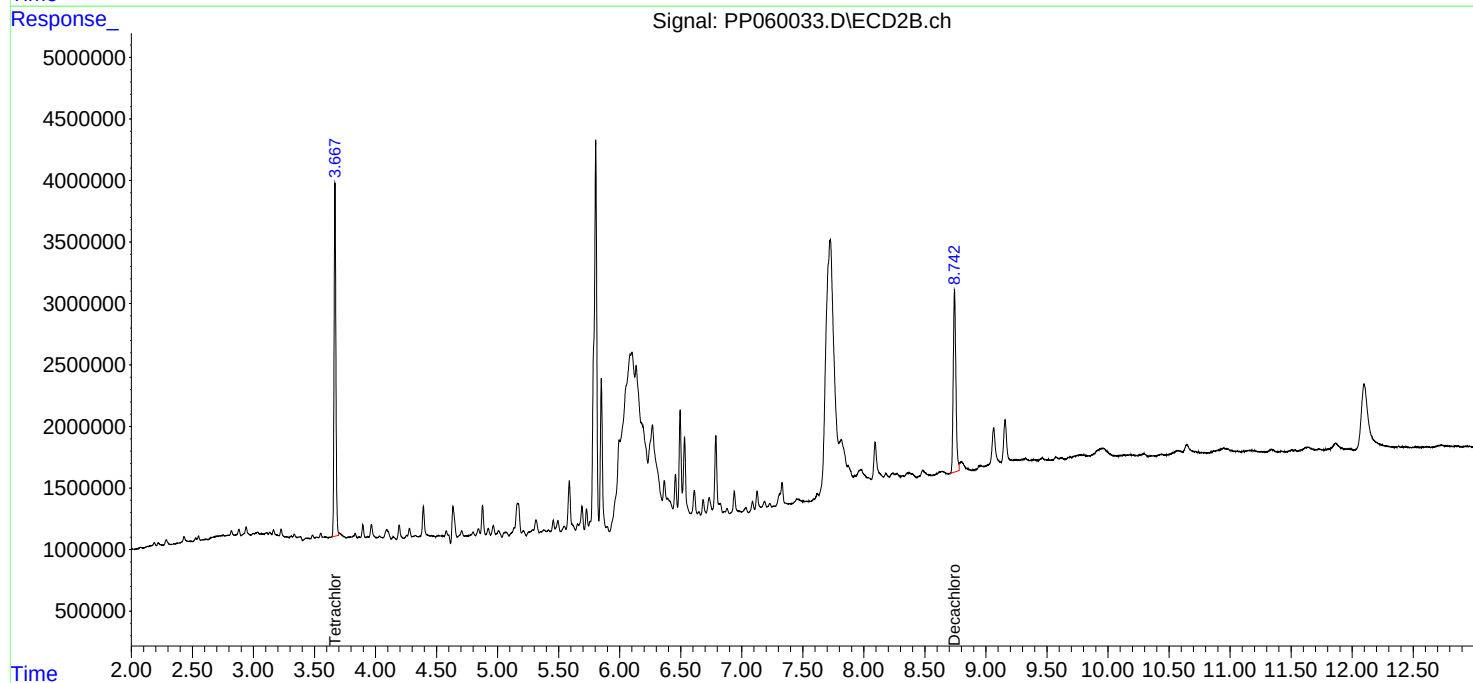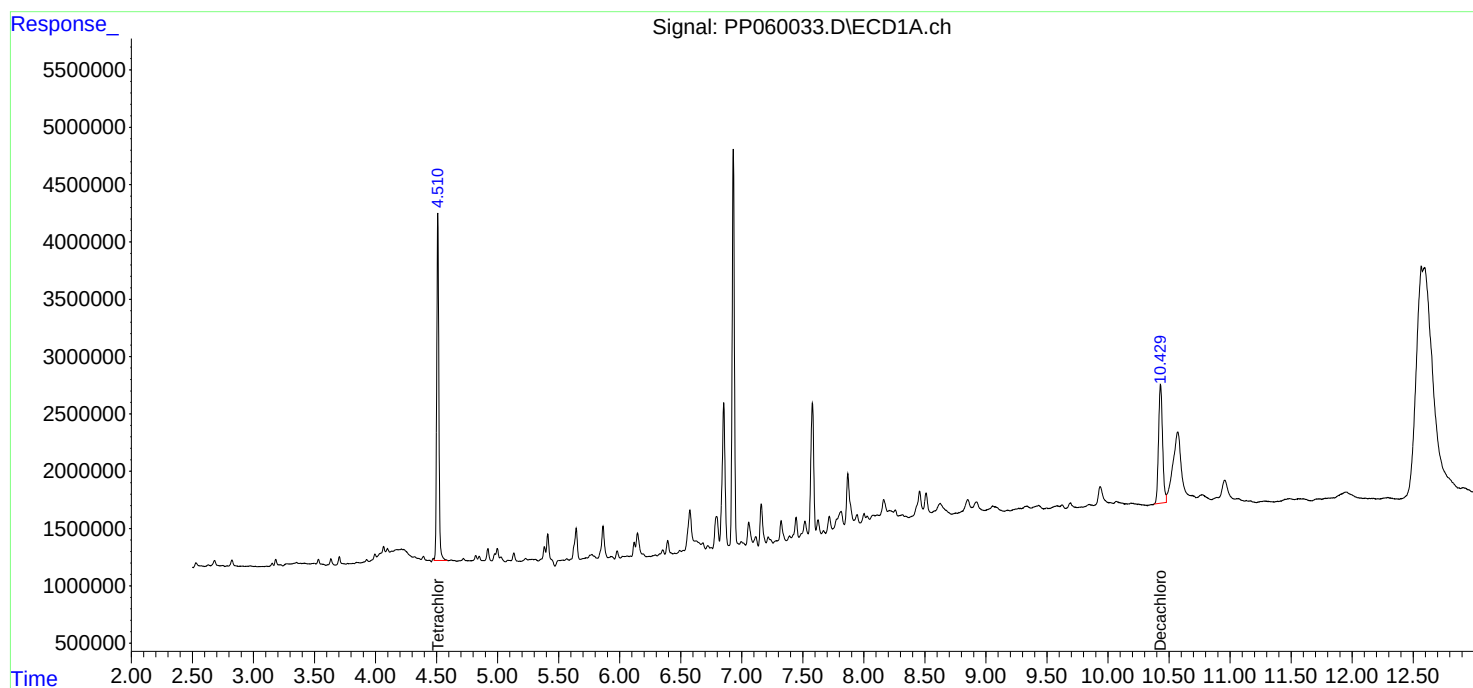

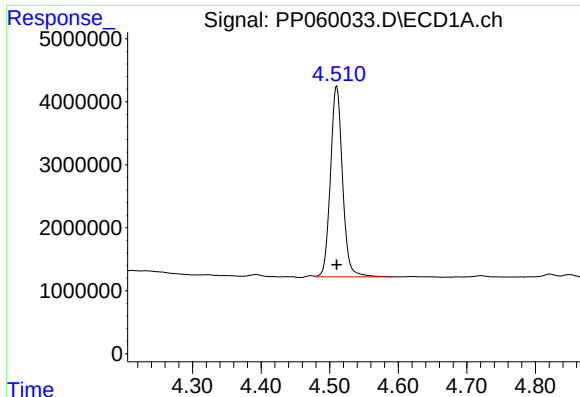


#1 Tetrachloro-m-xylene

R.T.: 4.510 min
Delta R.T.: 0.000 min
Response: 37034359
Conc: 17.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

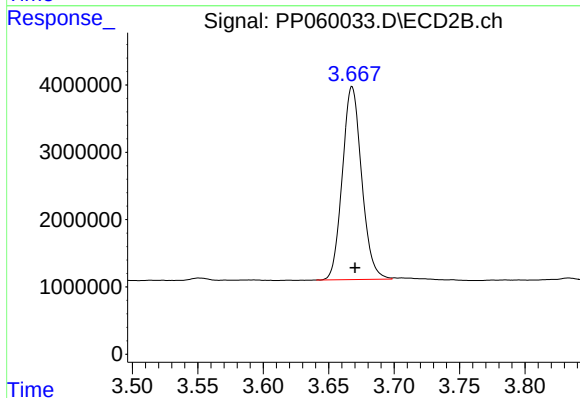


#1 Tetrachloro-m-xylene

R.T.: 3.668 min
Delta R.T.: -0.002 min
Response: 29478915
Conc: 18.10 ng/ml

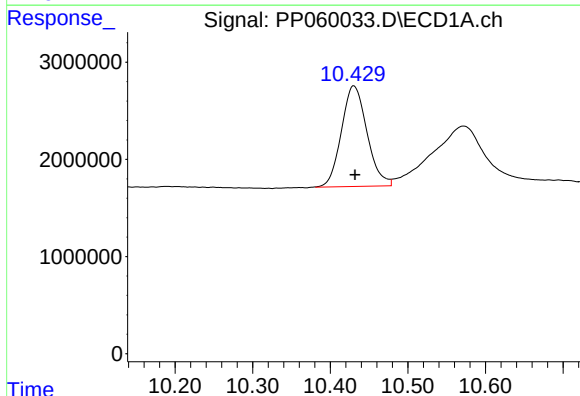

#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: -0.003 min
Response: 23742785
Conc: 15.57 ng/ml m

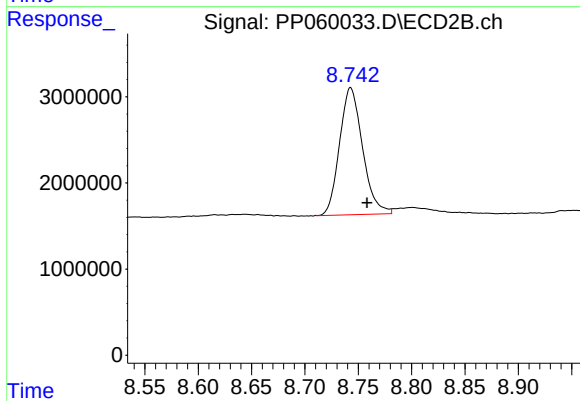

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.016 min
Response: 22175718
Conc: 14.65 ng/ml m