

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092023\
 Data File : PP060044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2023 21:05
 Operator : YP\AJ
 Sample : 04512-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 214

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2023
 Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 02:29:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.667	4178692	3276948	2.009	2.012
2) SA Decachlor...	10.432	8.742	4134765	3646536	2.711	2.408
Target Compounds						
31) L7 AR-1260-1	7.324	6.269	1500142	1812196	16.643	19.462
32) L7 AR-1260-2	7.583	6.459	3490165	2561004	34.021	23.359 #
33) L7 AR-1260-3	7.946	6.613	2777901	1852052	35.271	18.007 #
34) L7 AR-1260-4	8.172	7.090	4562519	1972291	50.909m	23.682 #
35) L7 AR-1260-5	8.510	7.332	6348513	5376158	37.200m	27.942

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092023\
Data File : PP060044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2023 21:05
Operator : YP\AJ
Sample : 04512-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
214


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 02:29:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

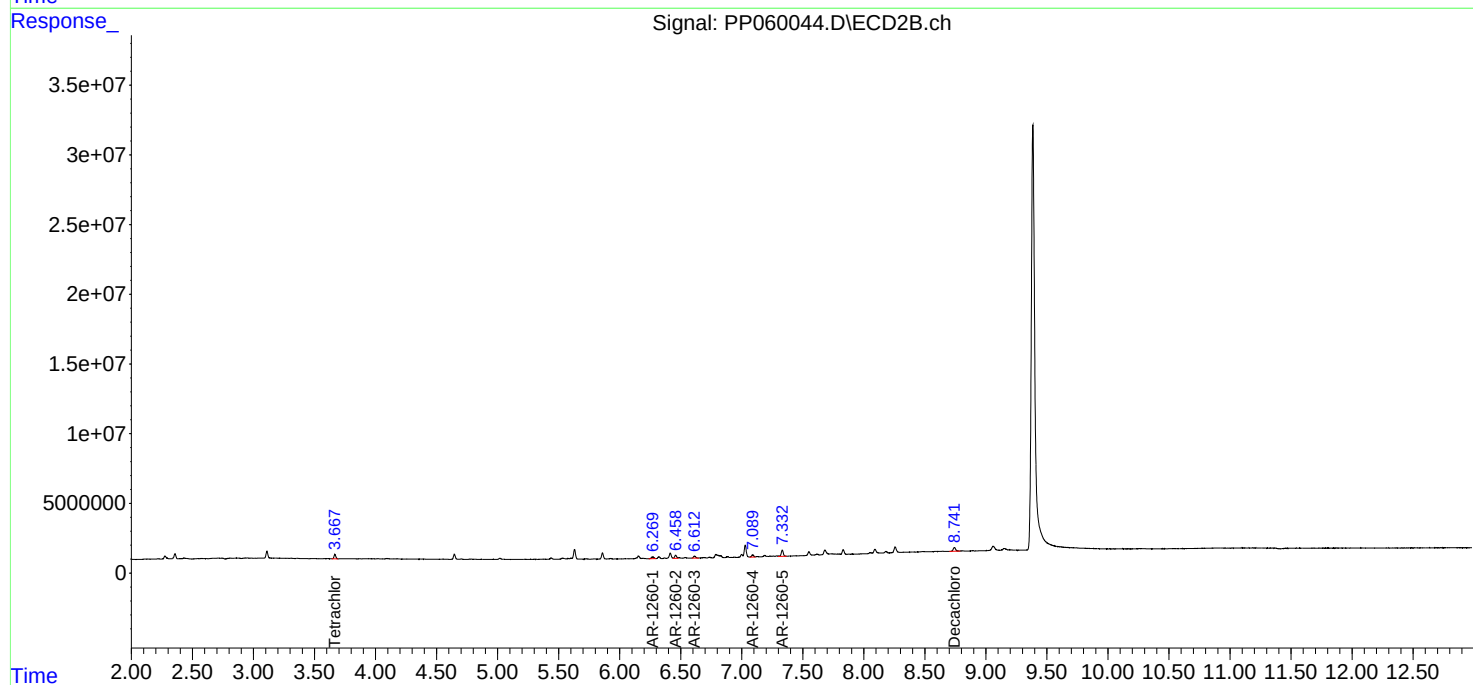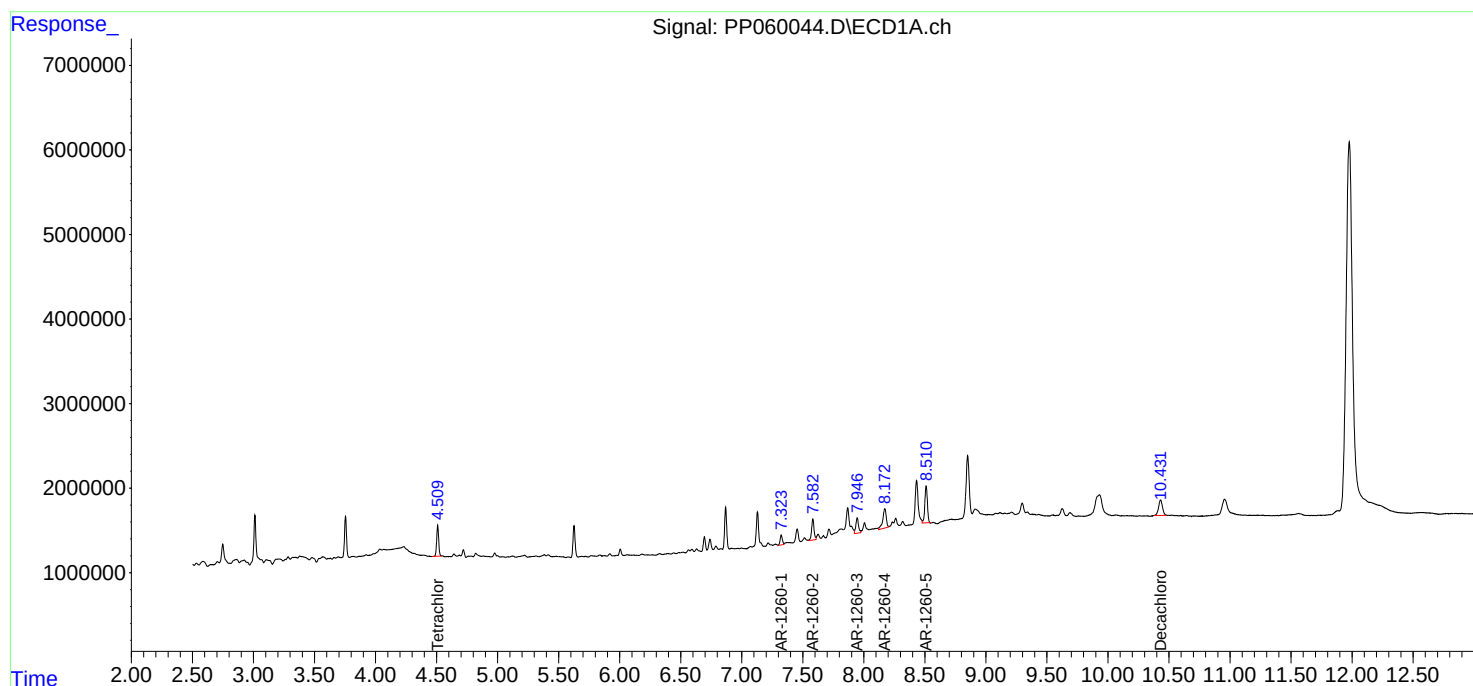

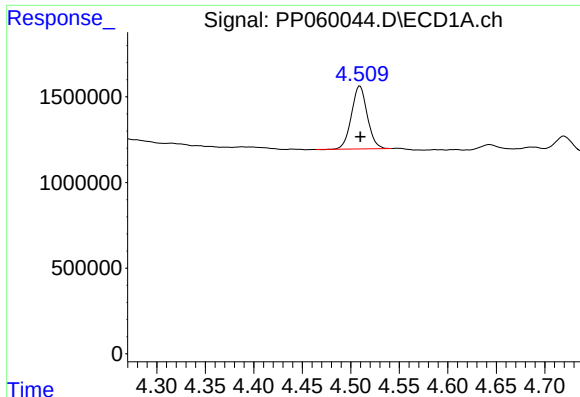


#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: 0.000 min
Response: 4178692
Conc: 2.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
214


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

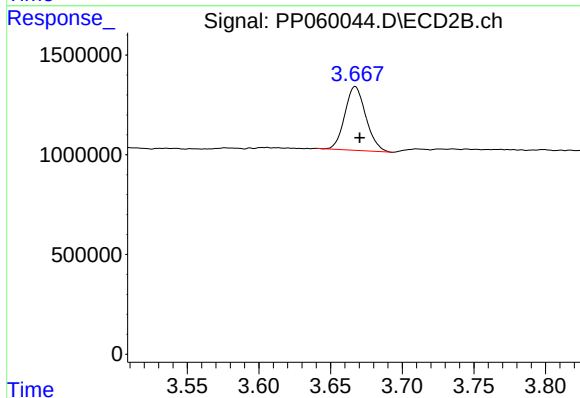


#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: -0.003 min
Response: 3276948
Conc: 2.01 ng/ml

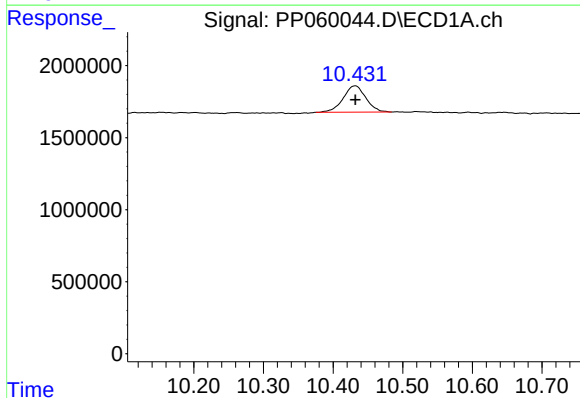


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 4134765
Conc: 2.71 ng/ml

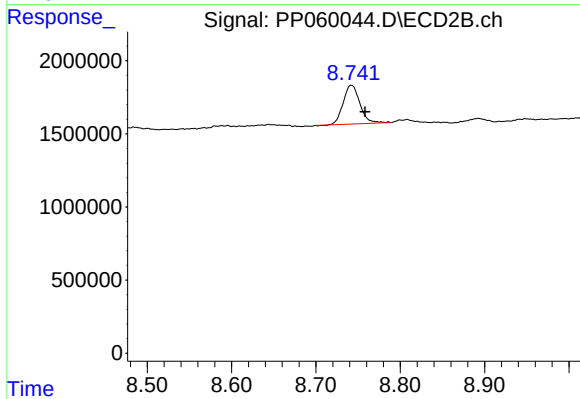

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.016 min
Response: 3646536
Conc: 2.41 ng/ml

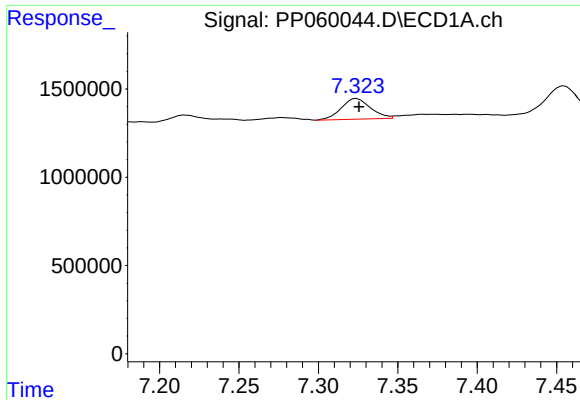


#31 AR-1260-1

R.T.: 7.324 min
Delta R.T.: -0.002 min
Response: 1500142
Conc: 16.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
214


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

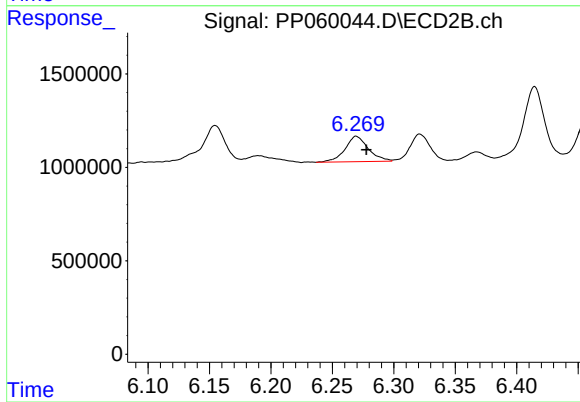


#31 AR-1260-1

R.T.: 6.269 min
Delta R.T.: -0.008 min
Response: 1812196
Conc: 19.46 ng/ml

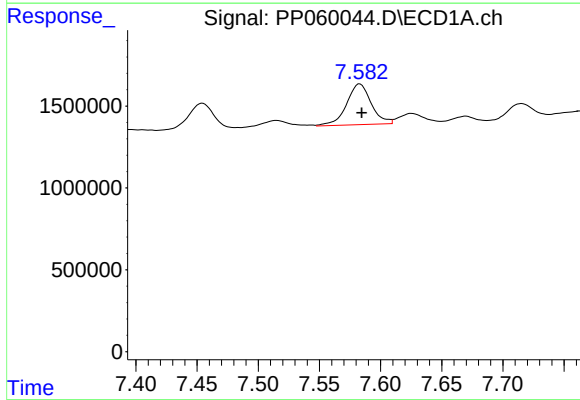


#32 AR-1260-2

R.T.: 7.583 min
Delta R.T.: -0.002 min
Response: 3490165
Conc: 34.02 ng/ml

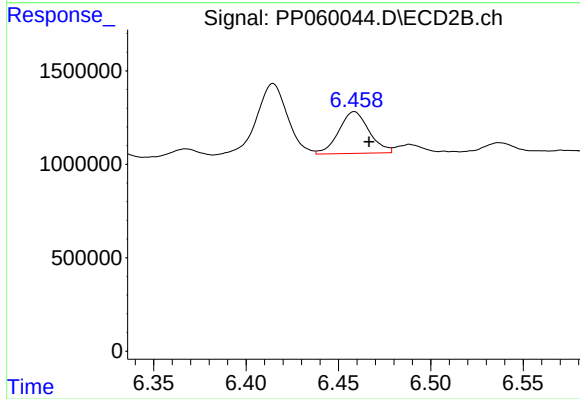

#32 AR-1260-2

R.T.: 6.459 min
Delta R.T.: -0.008 min
Response: 2561004
Conc: 23.36 ng/ml

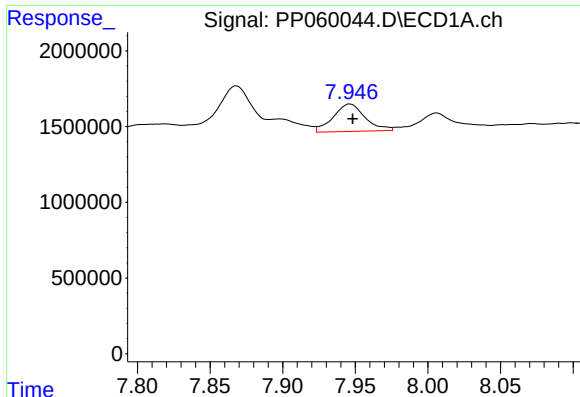


#33 AR-1260-3

R.T.: 7.946 min
Delta R.T.: -0.002 min
Response: 2777901
Conc: 35.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
214


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

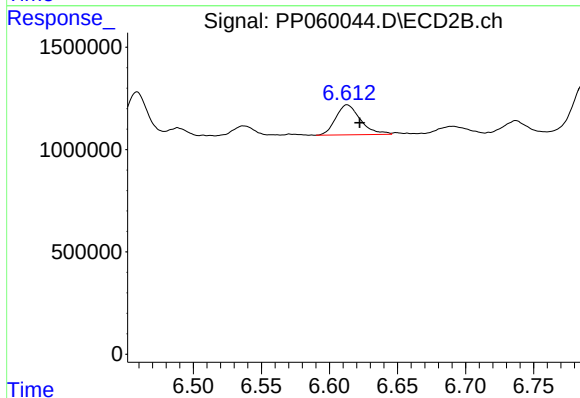


#33 AR-1260-3

R.T.: 6.613 min
Delta R.T.: -0.009 min
Response: 1852052
Conc: 18.01 ng/ml

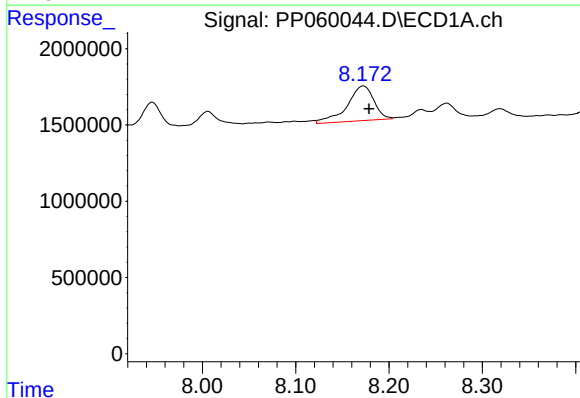


#34 AR-1260-4

R.T.: 8.172 min
Delta R.T.: -0.007 min
Response: 4562519
Conc: 50.91 ng/ml m

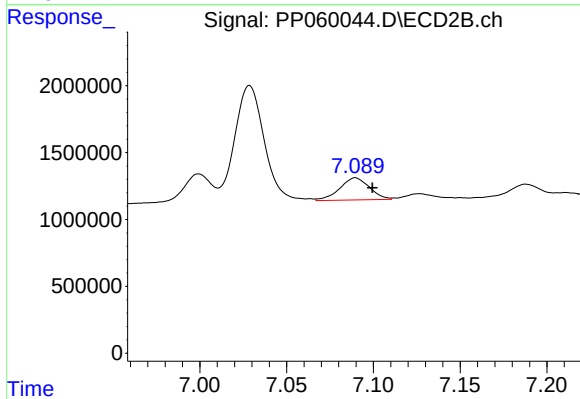

#34 AR-1260-4

R.T.: 7.090 min
Delta R.T.: -0.010 min
Response: 1972291
Conc: 23.68 ng/ml

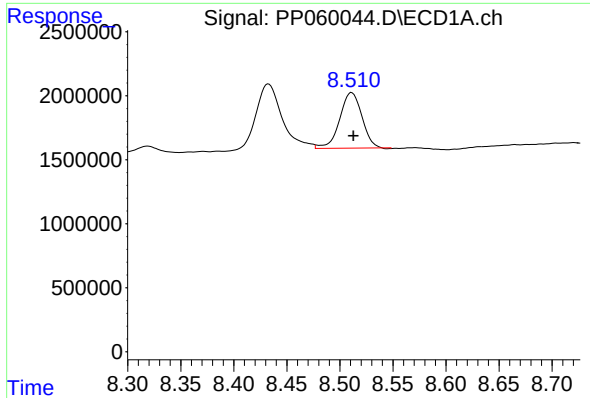


#35 AR-1260-5

R.T.: 8.510 min
Delta R.T.: -0.002 min
Response: 6348513
Conc: 37.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
214

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2023
Supervised By :Ankita Jodhani 09/21/2023

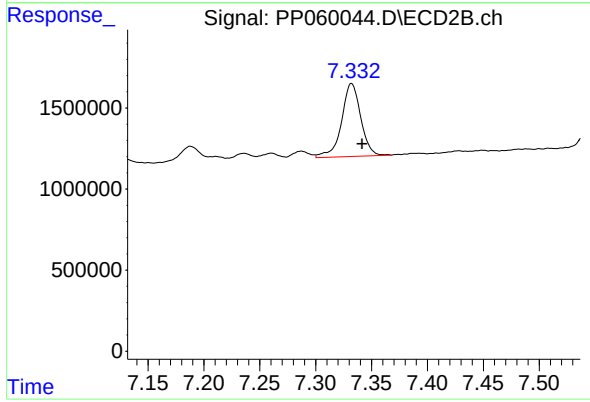

#35 AR-1260-5

R.T.: 7.332 min
Delta R.T.: -0.009 min
Response: 5376158
Conc: 27.94 ng/ml