

Data Path : P:\HPCHEM1\ECD_P\Data\PP092115\
Data File : PP011780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 17:45
Operator : IZ/UA
Sample : G3708-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MGP201-40-41

Manual Integrations
APPROVED

ugo
9/22/2015 11:59:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:44:39 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 19 00:23:08 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.166	4.186	985596	956556	22.540m	16.658 #
2) SA Decachlor...	11.476	9.277	572110	1506423	14.957m	26.522m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_P\Data\PP092115\
Data File : PP011780.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 17:45
Operator : IZ/UA
Sample : G3708-10
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
MGP201-40-41


Manual Integrations
APPROVED

ugo
9/22/2015 11:59:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:44:39 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 19 00:23:08 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

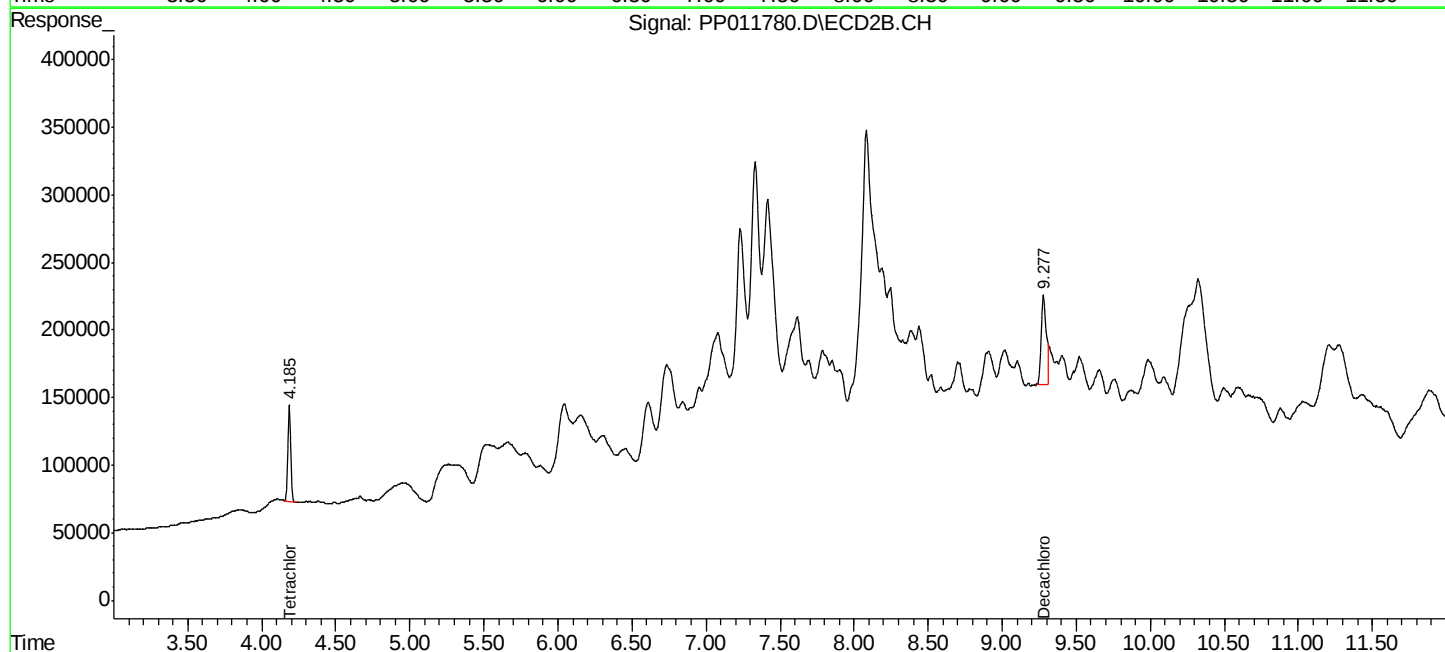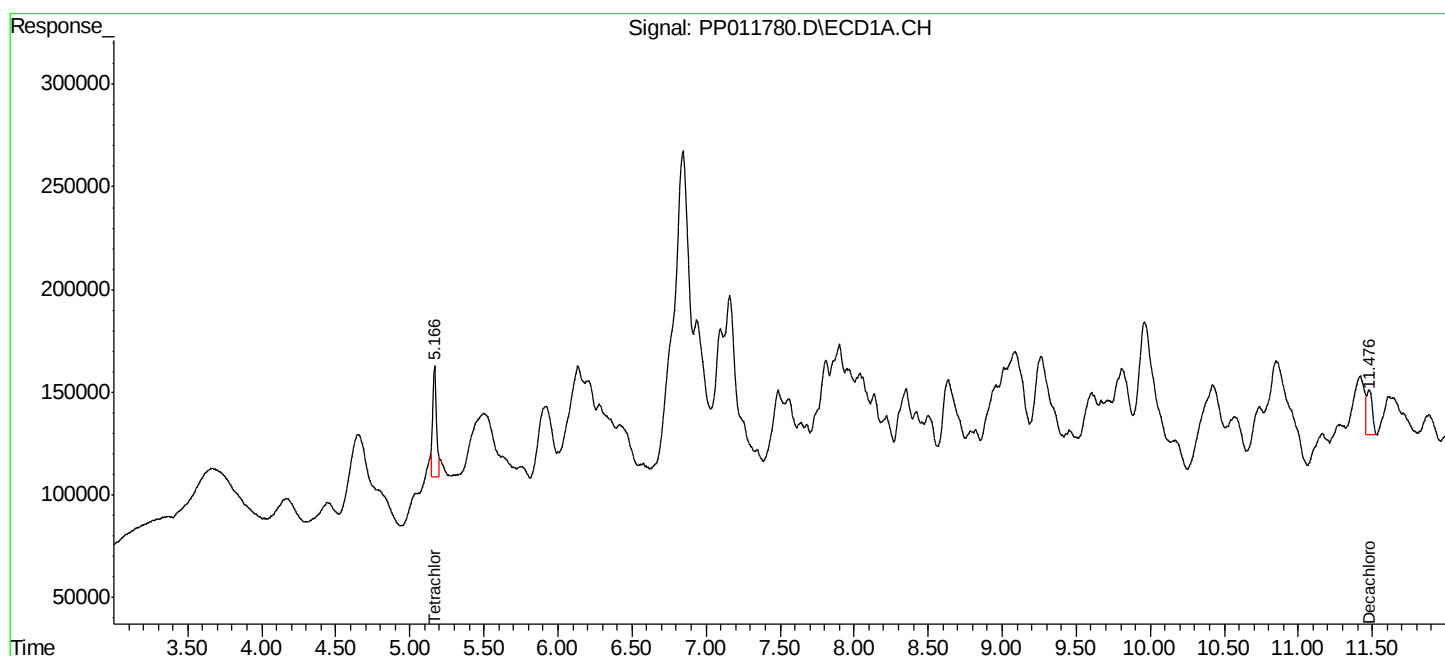

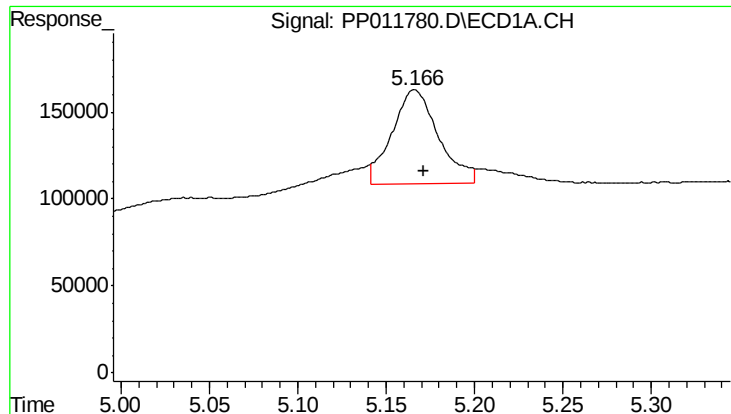


#1 Tetrachloro-m-xylene

R.T.: 5.166 min
Delta R.T.: -0.005 min
Response: 985596
Conc: 22.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MGP201-40-41


Manual Integrations
APPROVED

ugo
9/22/2015 11:59:02 AM

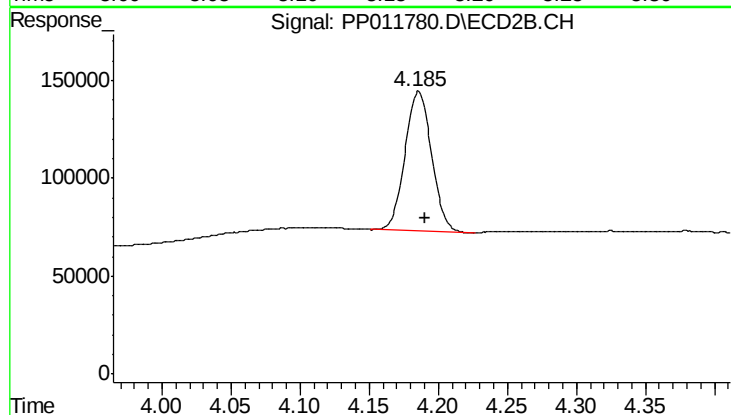


#1 Tetrachloro-m-xylene

R.T.: 4.186 min
Delta R.T.: -0.005 min
Response: 956556
Conc: 16.66 ng/ml

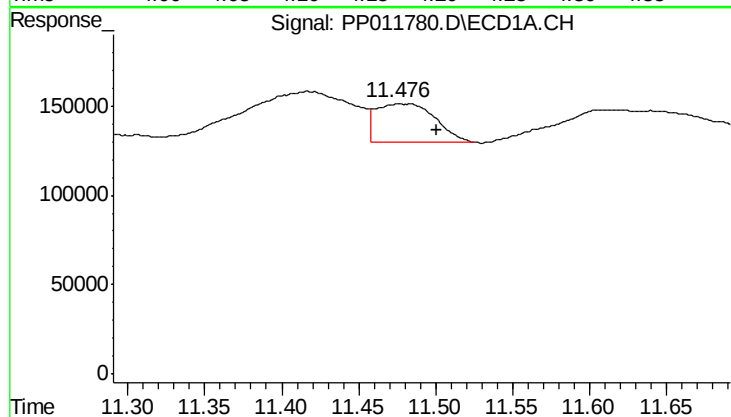

#2 Decachlorobiphenyl

R.T.: 11.476 min
Delta R.T.: -0.025 min
Response: 572110
Conc: 14.96 ng/ml m

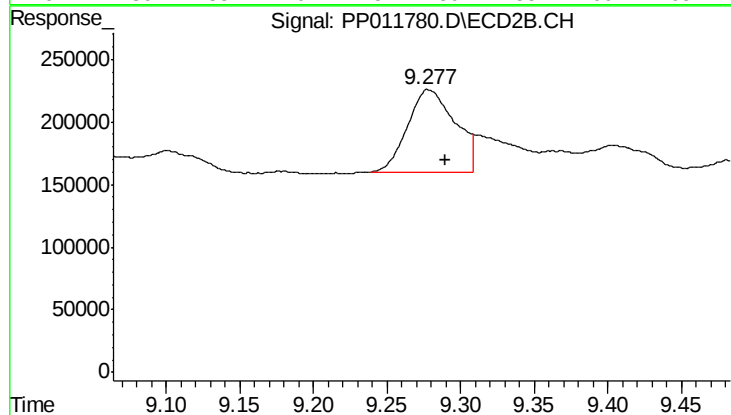

#2 Decachlorobiphenyl

R.T.: 9.277 min
Delta R.T.: -0.012 min
Response: 1506423
Conc: 26.52 ng/ml m