

Data Path : P:\HPCHEM1\ECD_P\Data\PP092115\
Data File : PP011783.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 18:31
Operator : IZ/UA
Sample : G3748-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MGP202-42-44

Manual Integrations
APPROVED

ugo
9/22/2015 11:59:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:48:56 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 19 00:23:08 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.167	4.186	839429	1151127	19.197m	20.047
2) SA Decachlor...	11.492	9.277	630672	728764	16.488m	12.831m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_P\Data\PP092115\
Data File : PP011783.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Sep 2015 18:31
Operator : IZ/UA
Sample : G3748-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MGP202-42-44


Manual Integrations
APPROVED

ugo
9/22/2015 11:59:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 10:48:56 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 19 00:23:08 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

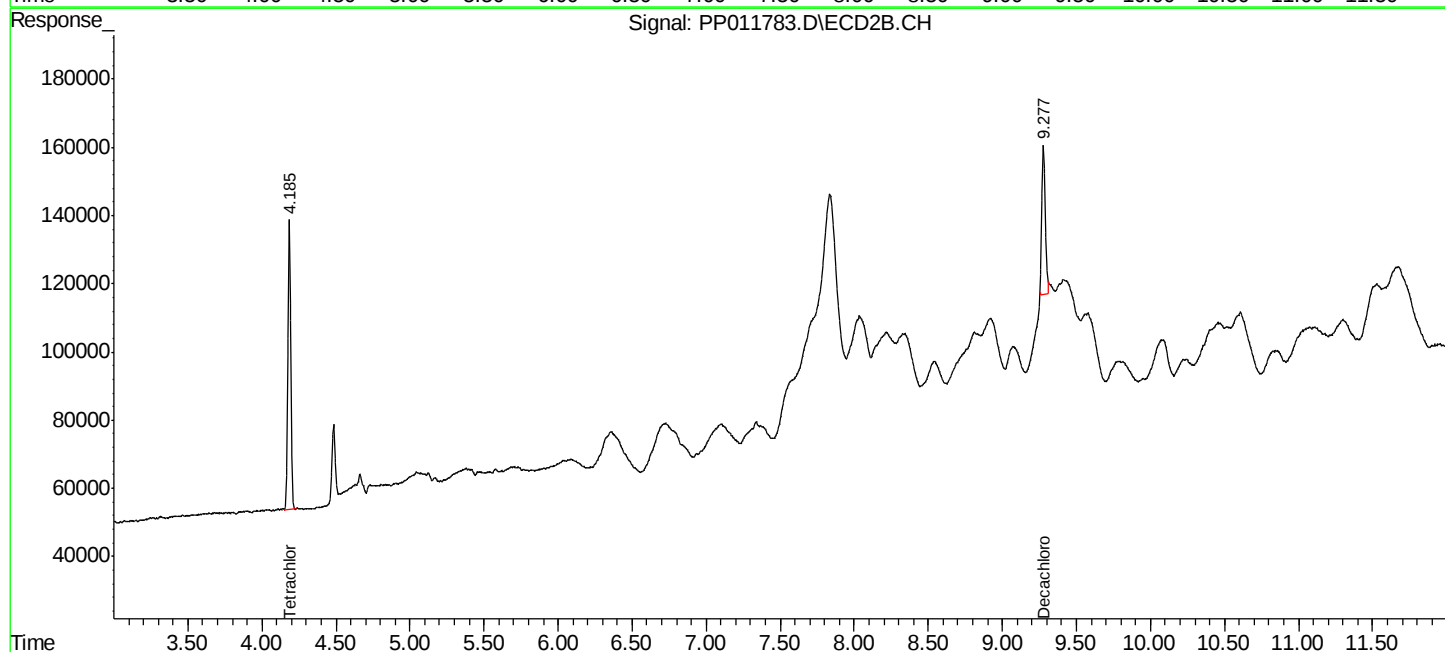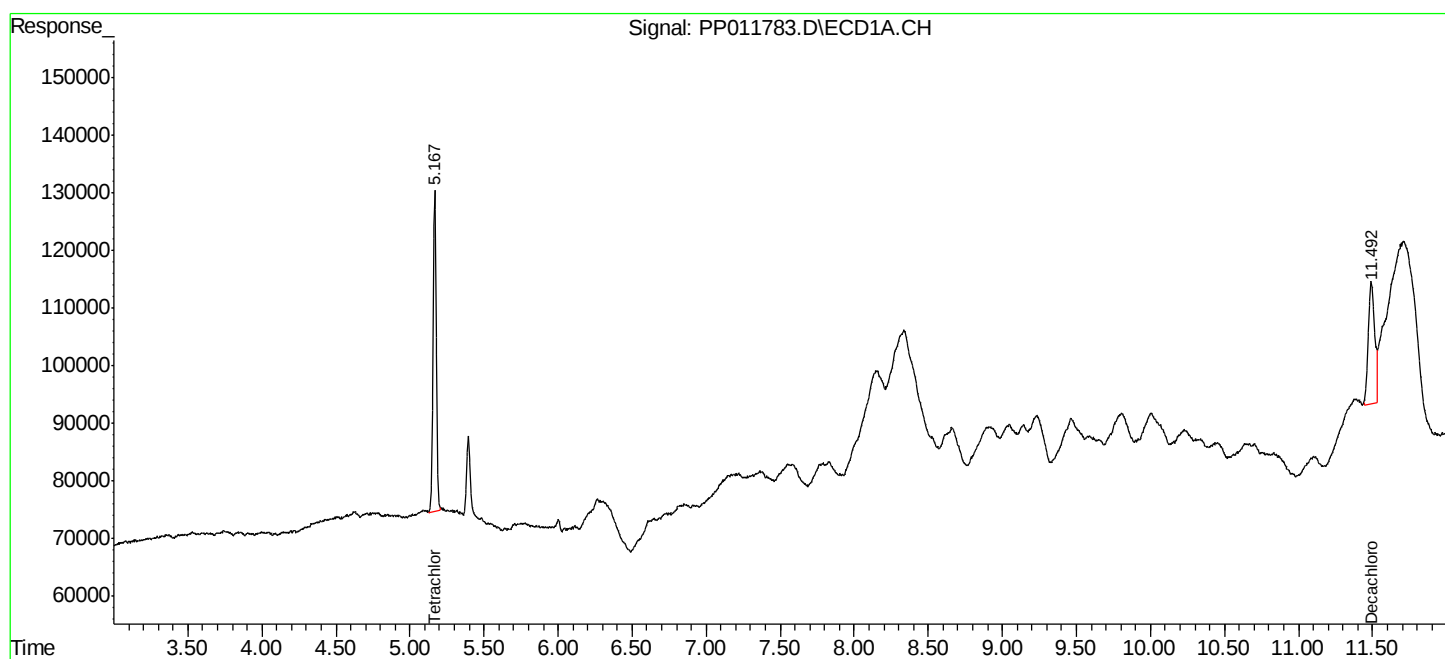

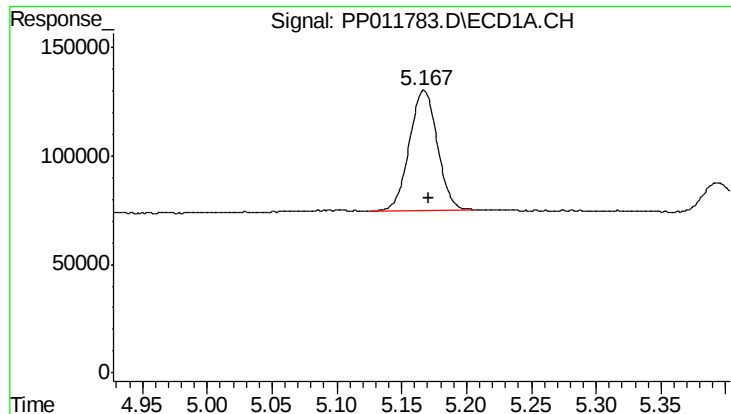


#1 Tetrachloro-m-xylene

R.T.: 5.167 min
Delta R.T.: -0.005 min
Response: 839429
Conc: 19.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MGP202-42-44


Manual Integrations
APPROVED

ugo
9/22/2015 11:59:10 AM

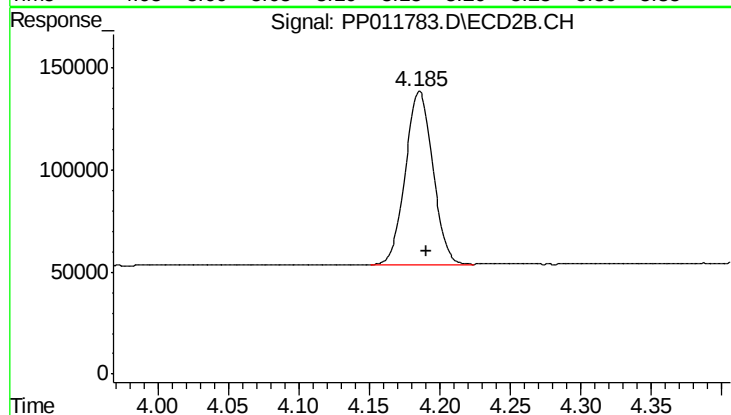


#1 Tetrachloro-m-xylene

R.T.: 4.186 min
Delta R.T.: -0.005 min
Response: 1151127
Conc: 20.05 ng/ml

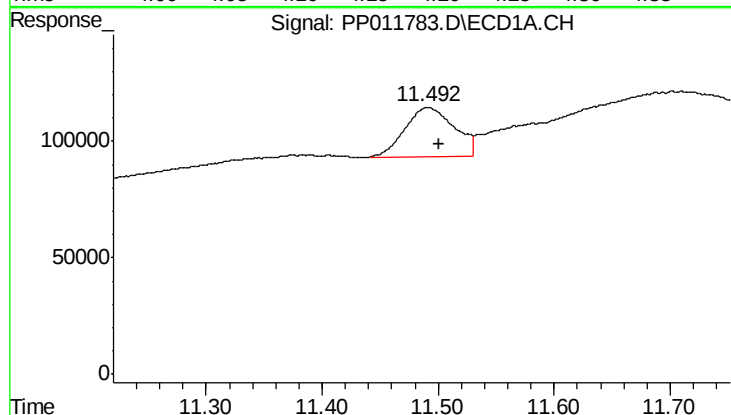

#2 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: -0.009 min
Response: 630672
Conc: 16.49 ng/ml m

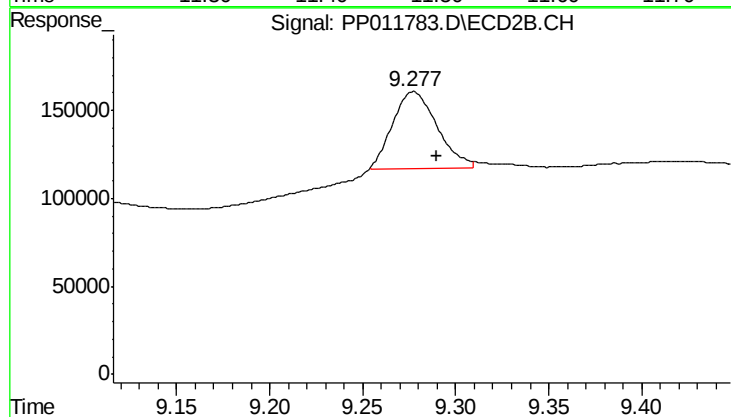

#2 Decachlorobiphenyl

R.T.: 9.277 min
Delta R.T.: -0.012 min
Response: 728764
Conc: 12.83 ng/ml m