

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092122\
 Data File : PP051488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2022 13:20
 Operator : YP\AJ
 Sample : N4715-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZZ106O-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2022
 Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 21 13:58:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.683	3797233	3082785	2.137m	2.041
2) SA Decachlor...	10.250	8.786	3469808	2393968	2.245m	1.998

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092122\
Data File : PP051488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2022 13:20
Operator : YP\AJ
Sample : N4715-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZZ106O-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 21 13:58:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

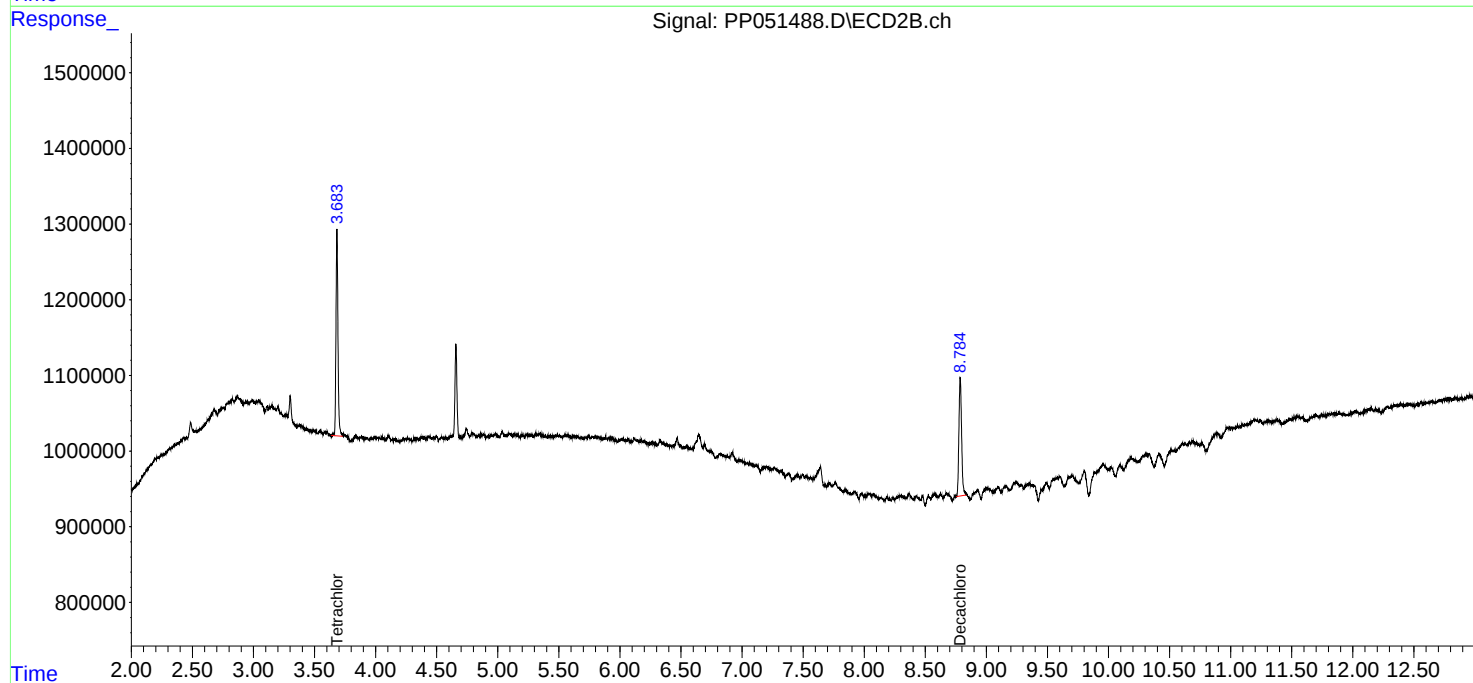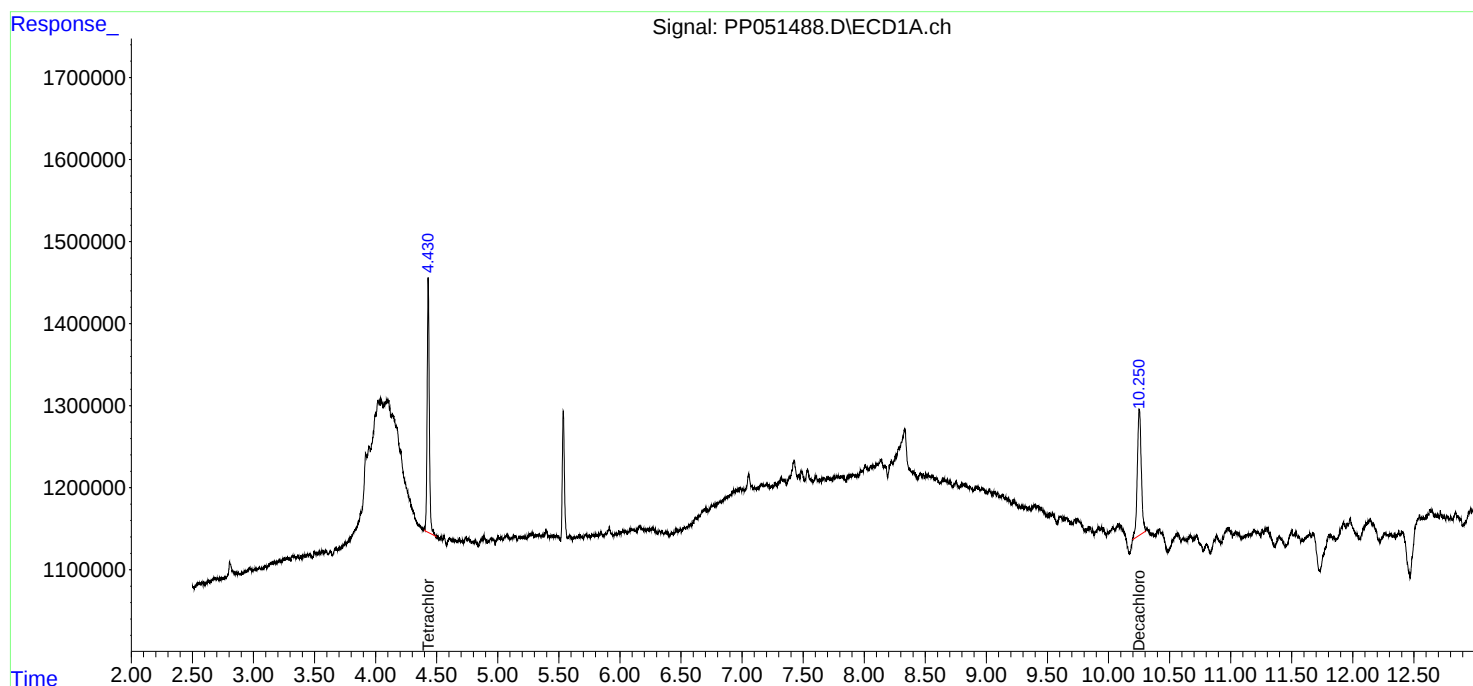

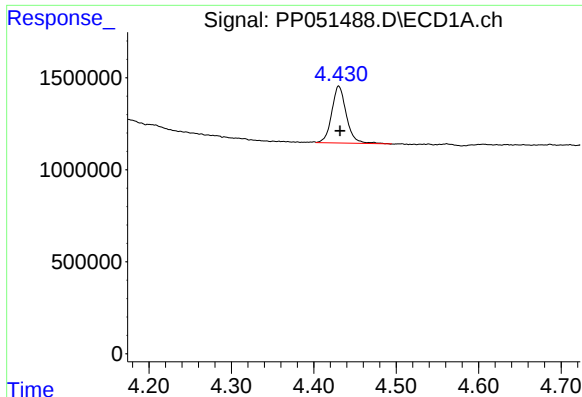

#1 Tetrachloro-m-xylene

R.T.: 4.430 min
Delta R.T.: -0.002 min
Response: 3797233
Conc: 2.14 ng/ml

Instrument :

ECD_P


ClientSampleId :

KZZ106O-1-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

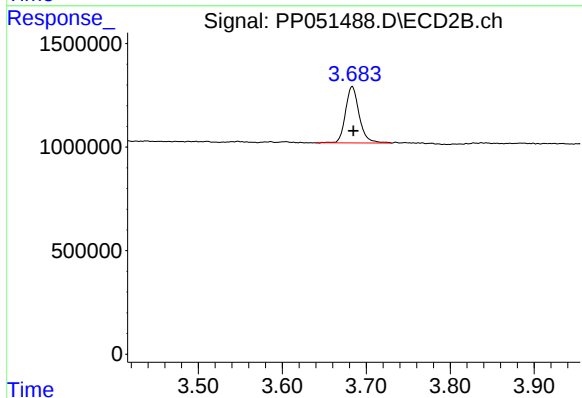


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: -0.001 min
Response: 3082785
Conc: 2.04 ng/ml

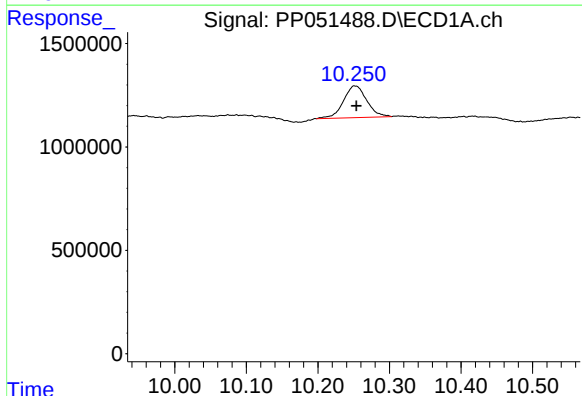

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: -0.004 min
Response: 3469808
Conc: 2.25 ng/ml m

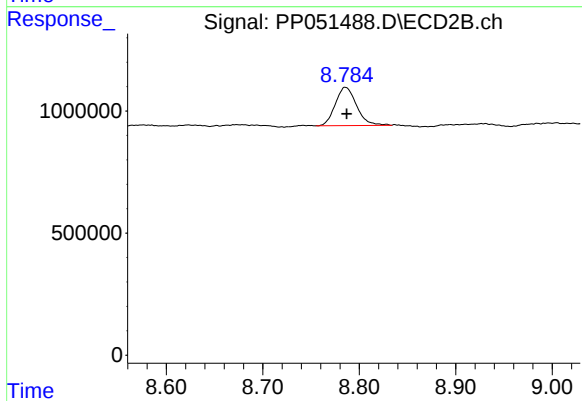

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.001 min
Response: 2393968
Conc: 2.00 ng/ml