

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092122\
 Data File : PP051508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Sep 2022 21:19
 Operator : YP\AJ
 Sample : N4726-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-0120

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/22/2022
 Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 01:13:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.691	10835470	8008401	6.097	5.302
2) SA Decachlor...	10.265	8.795	8576657	4482171	5.550	3.741m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092122\
Data File : PP051508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Sep 2022 21:19
Operator : YP\AJ
Sample : N4726-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-0120


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 01:13:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

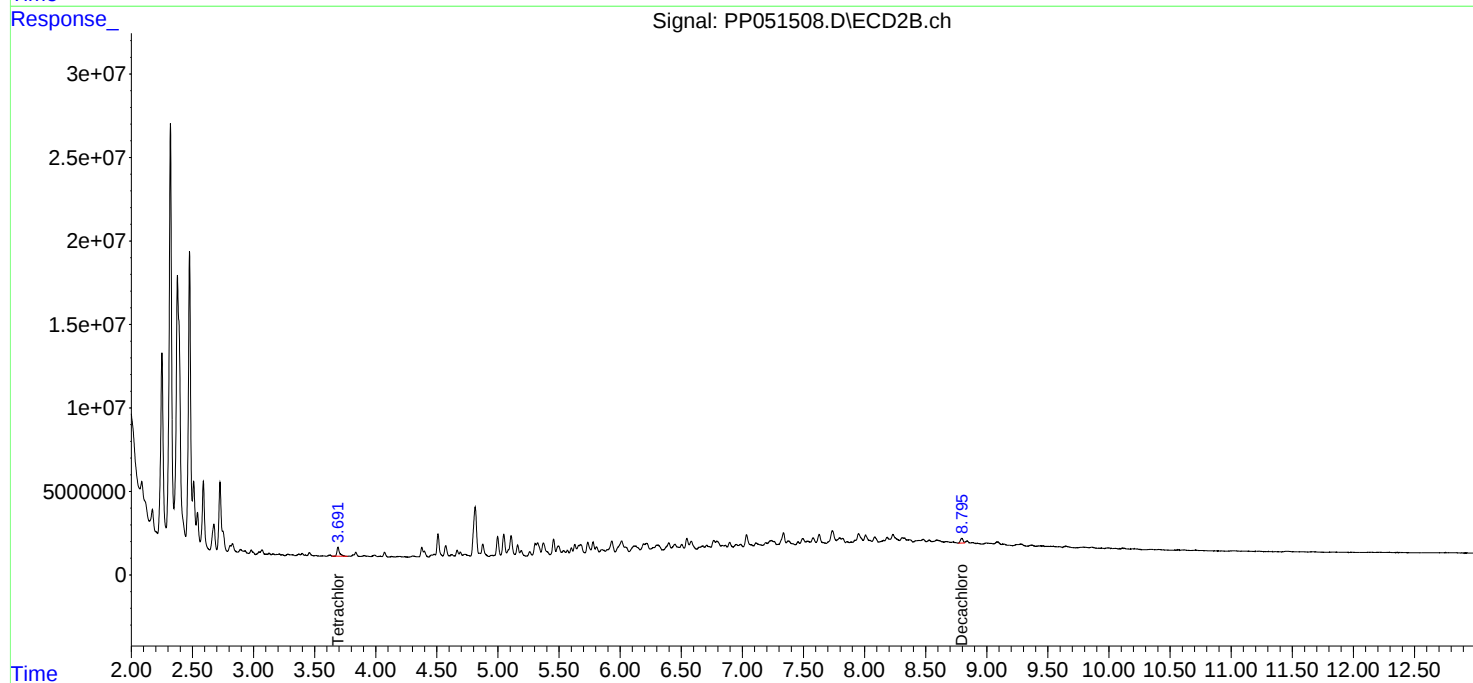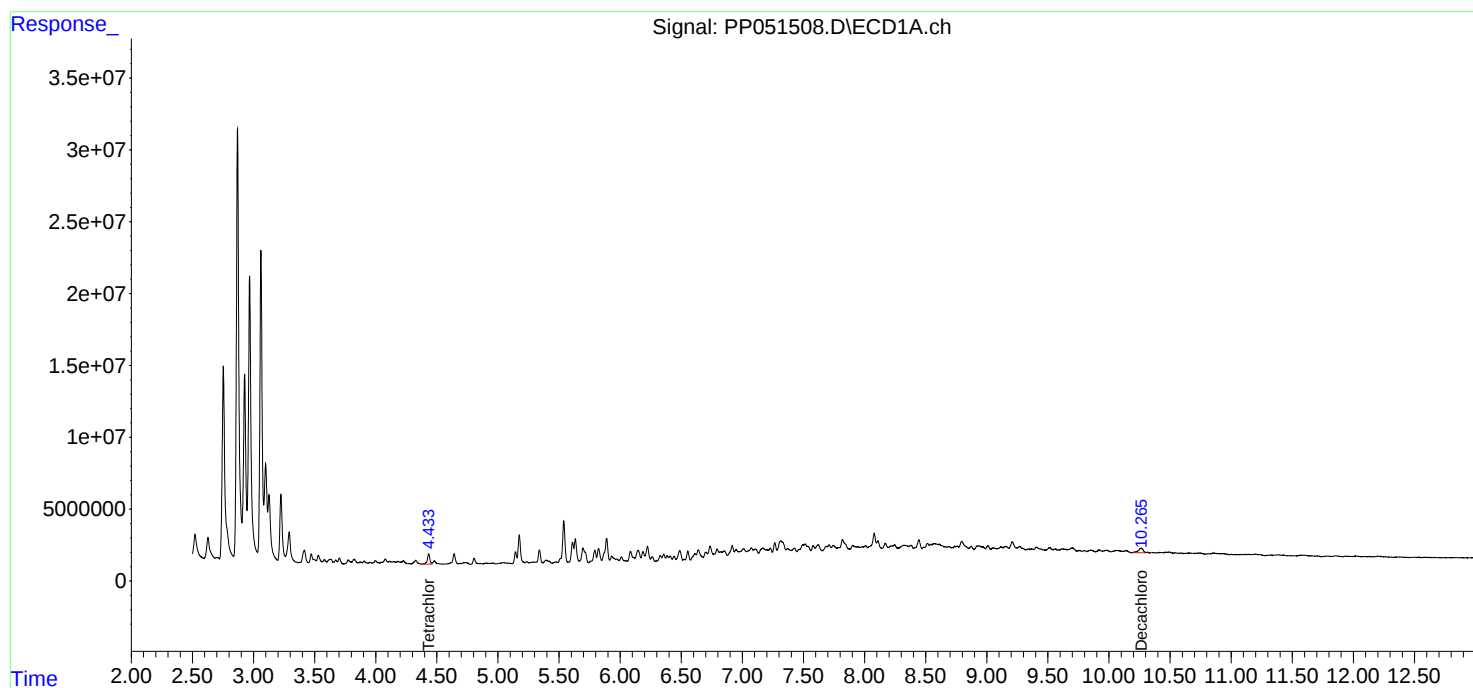

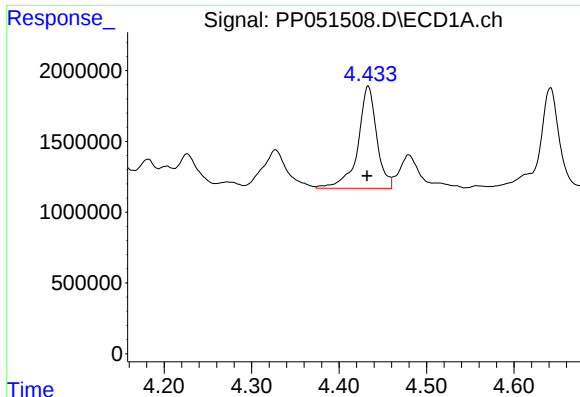


#1 Tetrachloro-m-xylene

R.T.: 4.433 min
Delta R.T.: 0.001 min
Response: 10835470
Conc: 6.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-0120


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/22/2022
Supervised By :Ankita Jodhani 09/22/2022

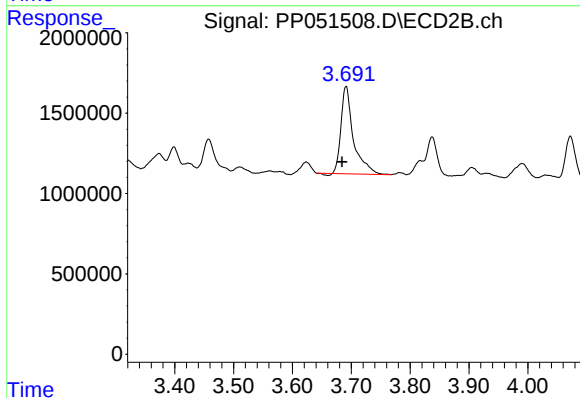


#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: 0.006 min
Response: 8008401
Conc: 5.30 ng/ml

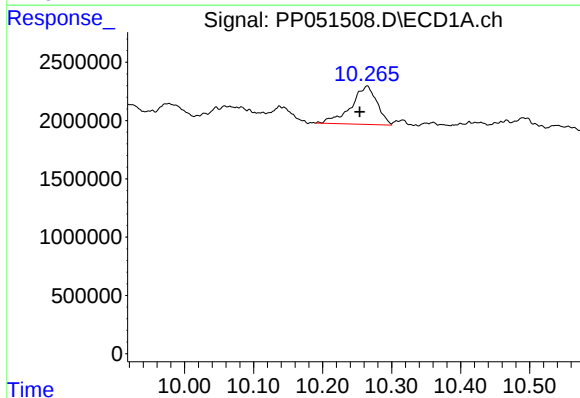

#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.011 min
Response: 8576657
Conc: 5.55 ng/ml

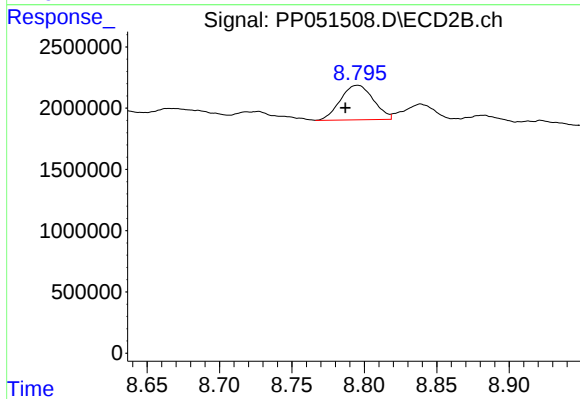

#2 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: 0.008 min
Response: 4482171
Conc: 3.74 ng/ml m