

Data Path : P:\HPCHEM1\ECD_P\Data\PP092215\
Data File : PP011793.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2015 11:37
Operator : IZ/UA
Sample : G3748-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MGP205-10-12RE

Manual Integrations
APPROVED

ugo
9/23/2015 1:11:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 13:18:02 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 03 15:00:38 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.169	4.191	1012744	518832	23.160m	9.034m#
2) SA Decachlor...	11.496	9.277	302729	418533	7.915	7.369m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_P\Data\PP092215\
Data File : PP011793.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Sep 2015 11:37
Operator : IZ/UA
Sample : G3748-04RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MGP205-10-12RE


Manual Integrations
APPROVED

ugo
9/23/2015 1:11:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 13:18:02 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 03 15:00:38 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

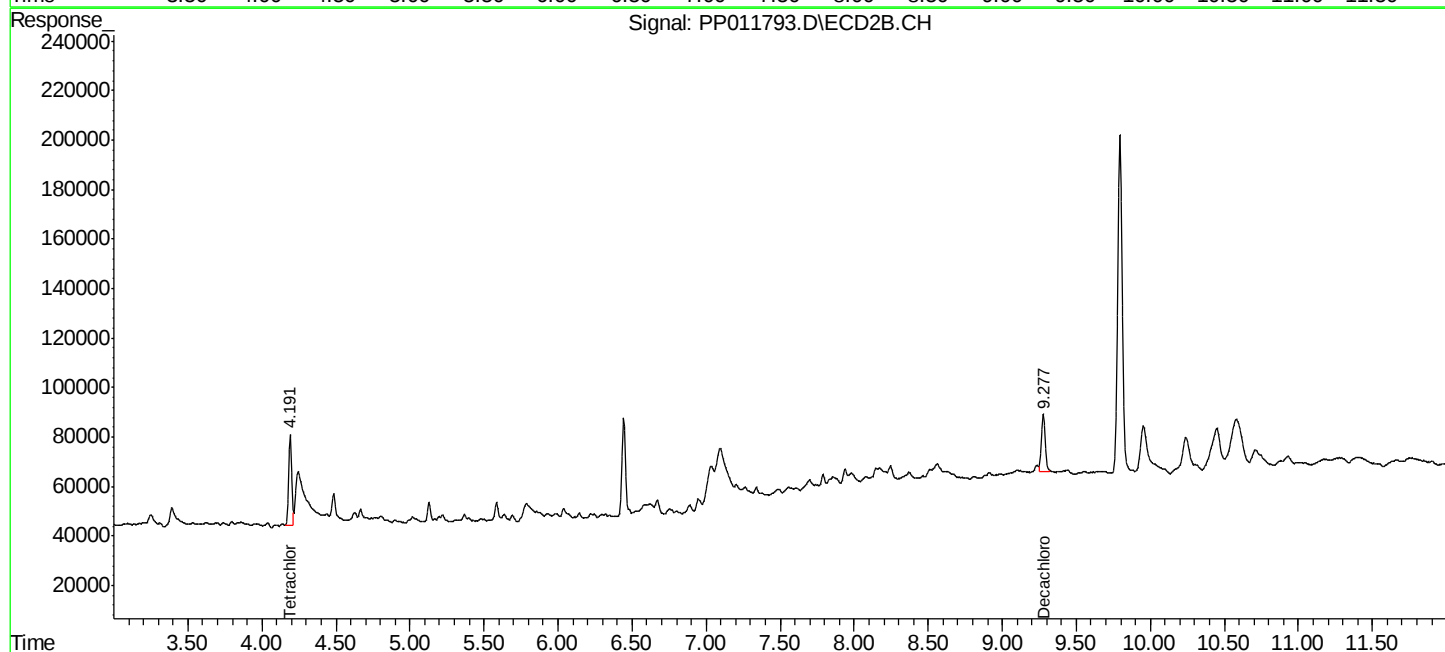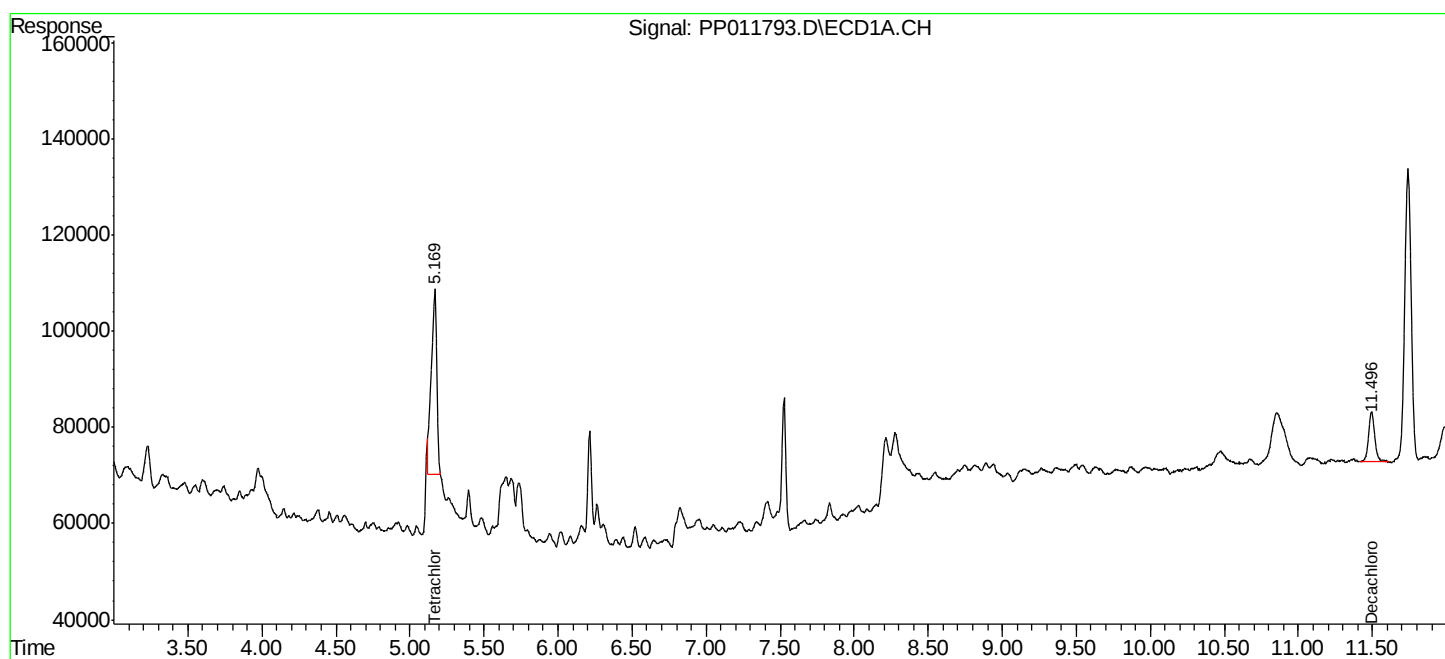

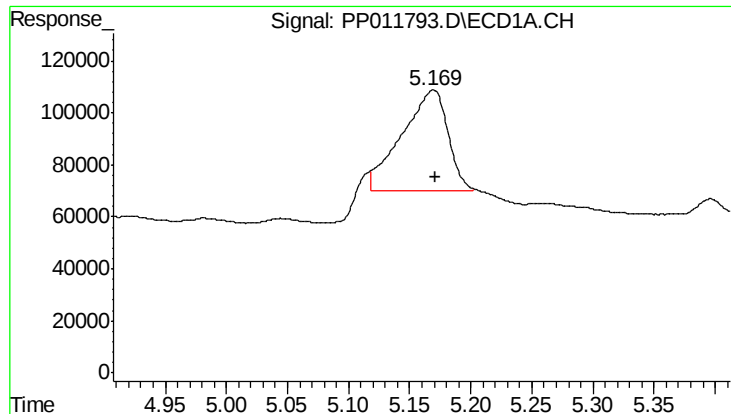


#1 Tetrachloro-m-xylene

R.T.: 5.169 min
Delta R.T.: -0.002 min
Response: 1012744
Conc: 23.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MGP205-10-12RE


Manual Integrations
APPROVED

ugo
9/23/2015 1:11:33 PM

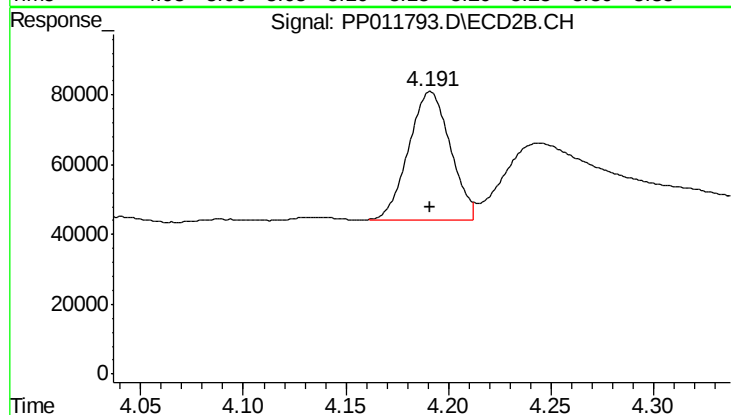


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 518832
Conc: 9.03 ng/ml m

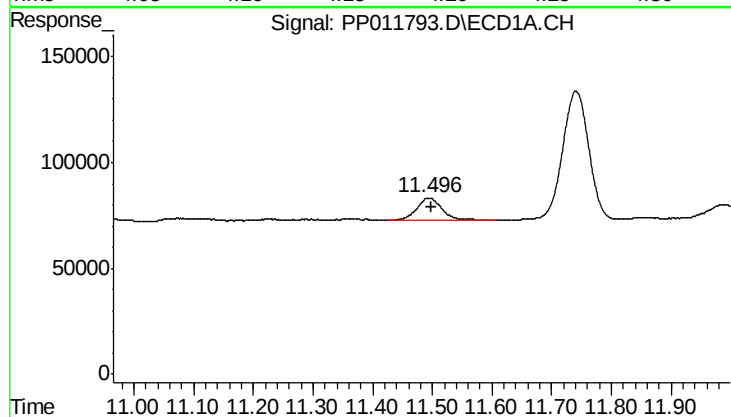

#2 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: -0.003 min
Response: 302729
Conc: 7.91 ng/ml

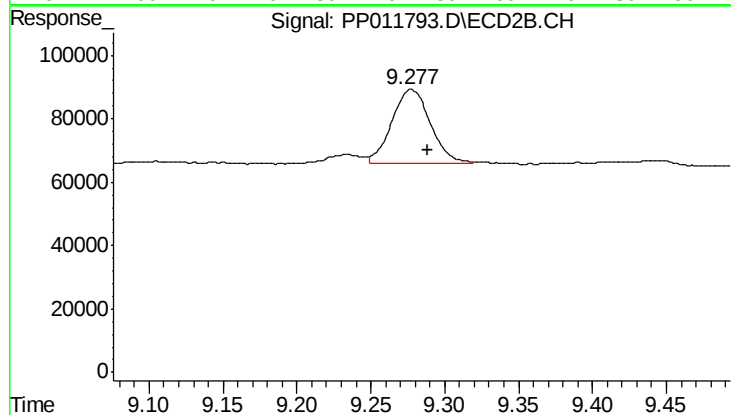

#2 Decachlorobiphenyl

R.T.: 9.277 min
Delta R.T.: -0.012 min
Response: 418533
Conc: 7.37 ng/ml m