

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092222\
 Data File : PP051523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2022 10:57
 Operator : YP\AJ
 Sample : N4726-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-0120

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/23/2022
 Supervised By :Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 16:10:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.435	3.692	12733094	9468196	7.165	6.268
2) SA Decachlor...	10.271	8.799	12423738	6629757	8.039m	5.533m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092222\
Data File : PP051523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2022 10:57
Operator : YP\AJ
Sample : N4726-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-0120


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2022
Supervised By :Ankita Jodhani 09/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 16:10:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

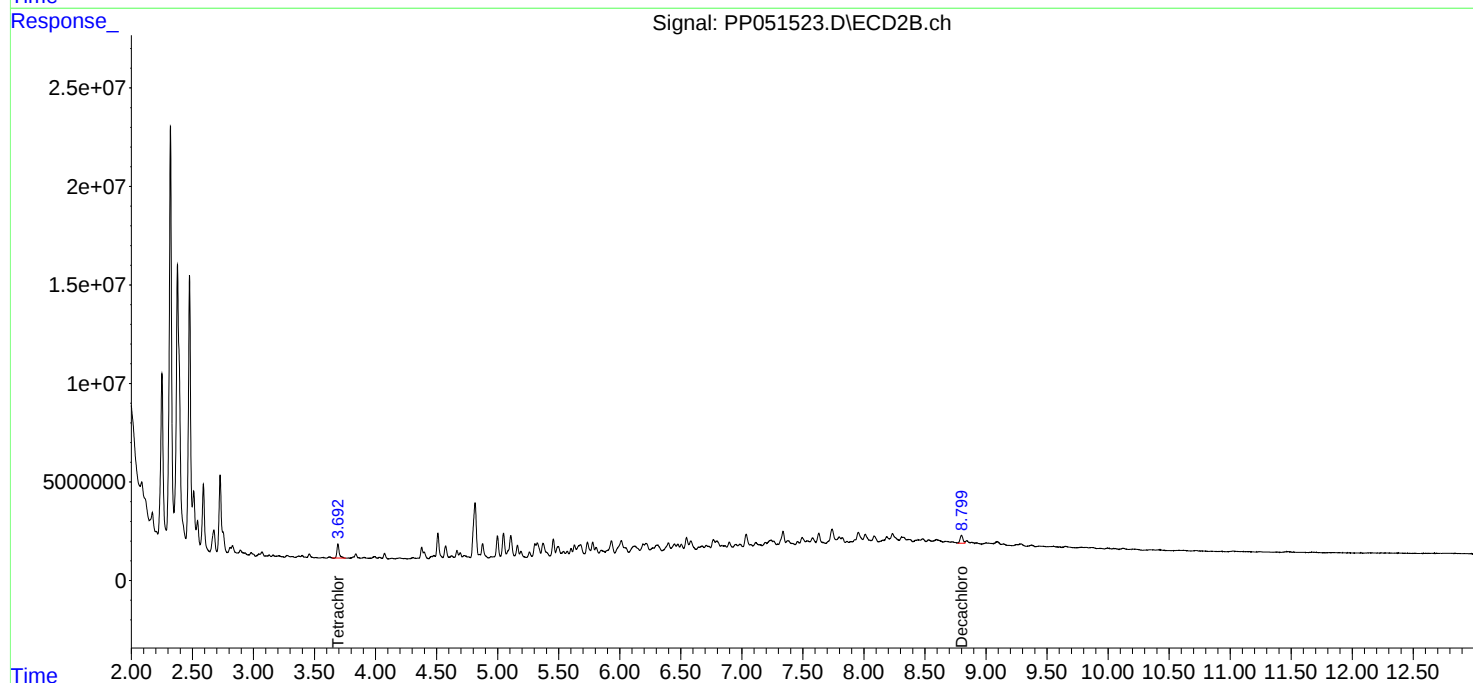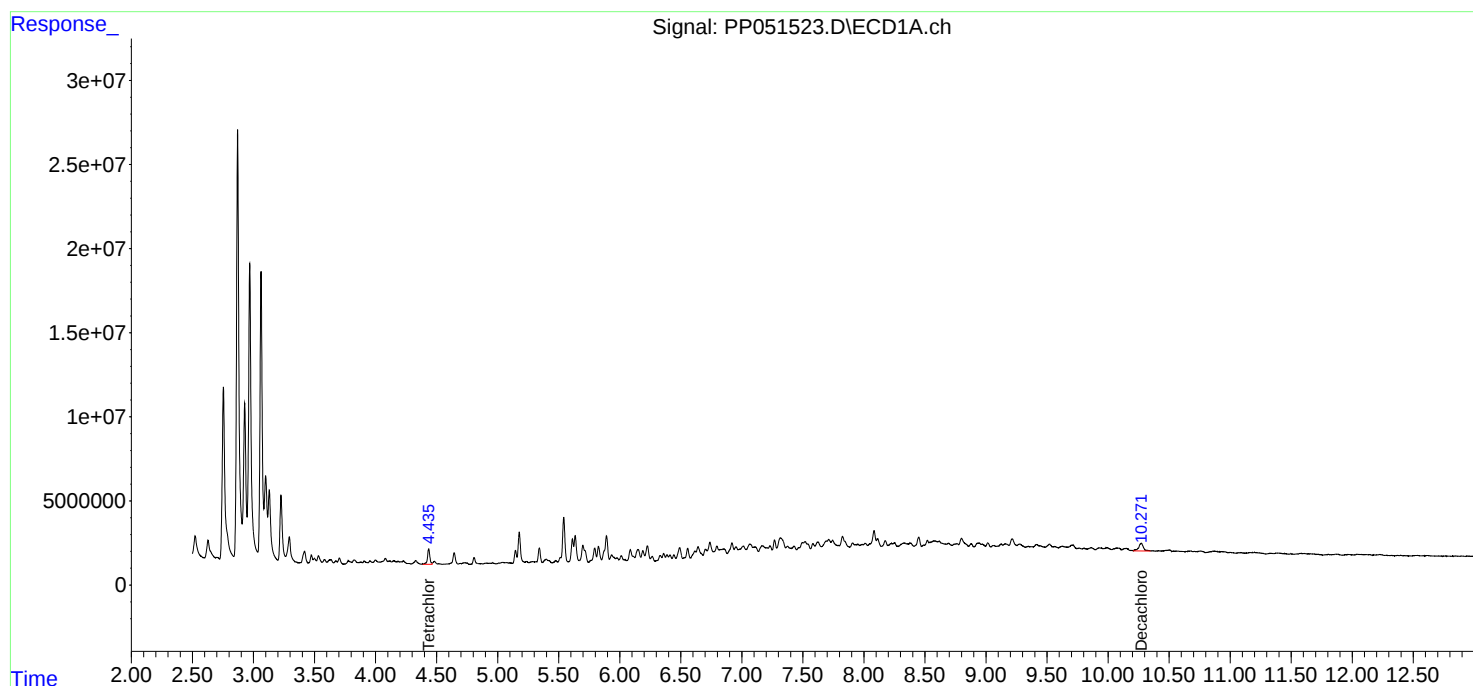

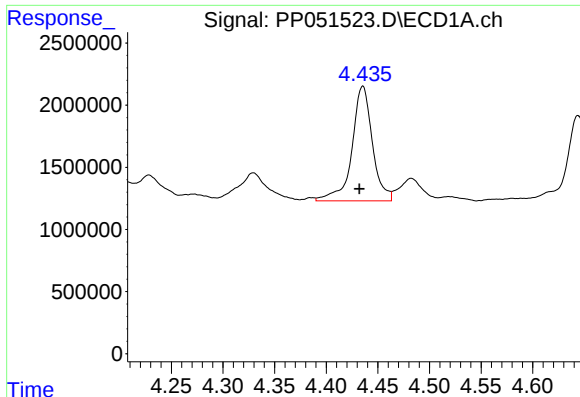


#1 Tetrachloro-m-xylene

R.T.: 4.435 min
Delta R.T.: 0.003 min
Response: 12733094
Conc: 7.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-0120


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/23/2022
Supervised By :Ankita Jodhani 09/23/2022

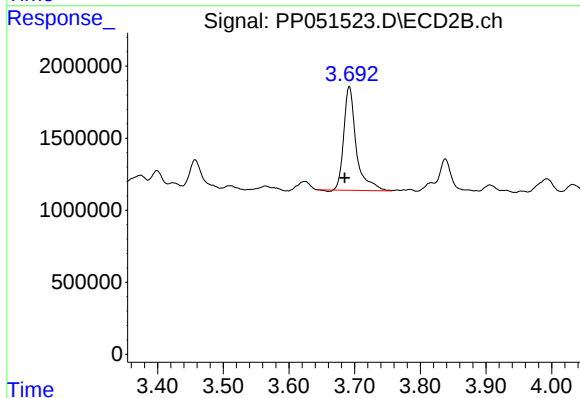


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: 0.007 min
Response: 9468196
Conc: 6.27 ng/ml

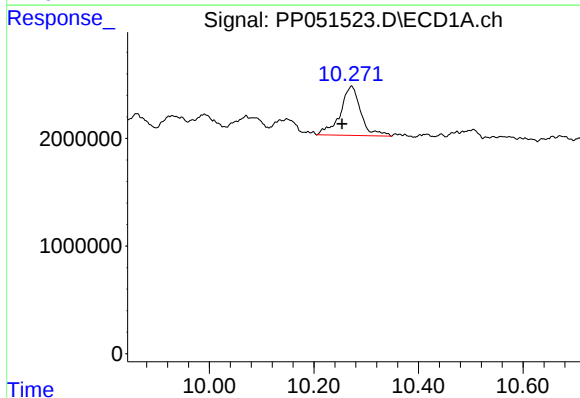

#2 Decachlorobiphenyl

R.T.: 10.271 min
Delta R.T.: 0.018 min
Response: 12423738
Conc: 8.04 ng/ml m

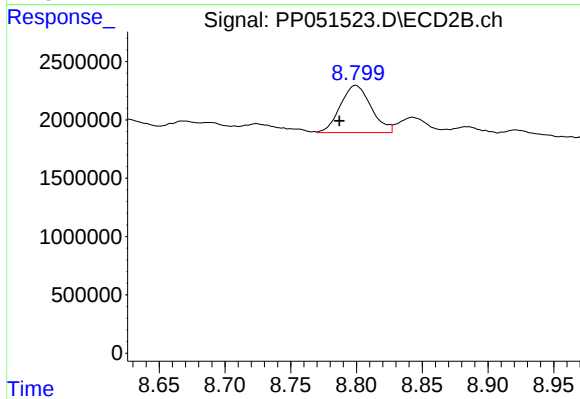

#2 Decachlorobiphenyl

R.T.: 8.799 min
Delta R.T.: 0.012 min
Response: 6629757
Conc: 5.53 ng/ml m