

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092322\
 Data File : PP051570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2022 10:44
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 11:20:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.680	26055683	21791088	14.662	14.426
2) SA Decachlor...	10.248	8.779	22050421	18738916	14.268	15.639
Target Compounds						
5) L1 AR-1016-3	5.672f	0.000	404976	0	7.402	N.D. #
9) L2 AR-1221-2	4.734	0.000	399528	0	23.474	N.D. #
12) L3 AR-1232-2	5.309f	0.000	134342	0	6.205	N.D. #
15) L3 AR-1232-5	5.910f	0.000	172350	0	11.490	N.D. #
18) L4 AR-1242-3	5.672f	0.000	404976	0	8.556	N.D. #
22) L5 AR-1248-2	5.910f	0.000	172350	0	3.038	N.D. #
32) L7 AR-1260-2	7.479	0.000	177655	0	1.683	N.D. #
35) L7 AR-1260-5	8.386	0.000	56102	0	0.365	N.D. #
37) L8 AR-1262-2	8.386	0.000	56102	0	0.353	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092322\
Data File : PP051570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2022 10:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 11:20:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

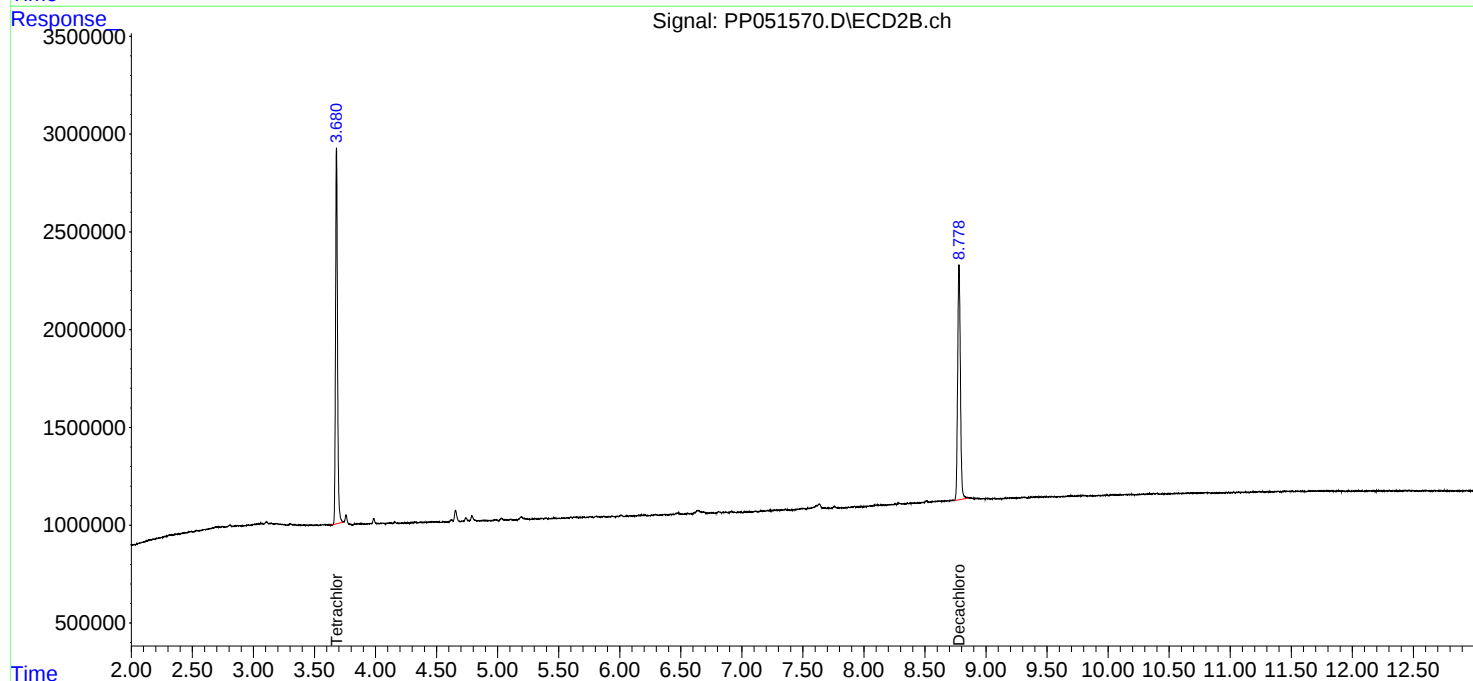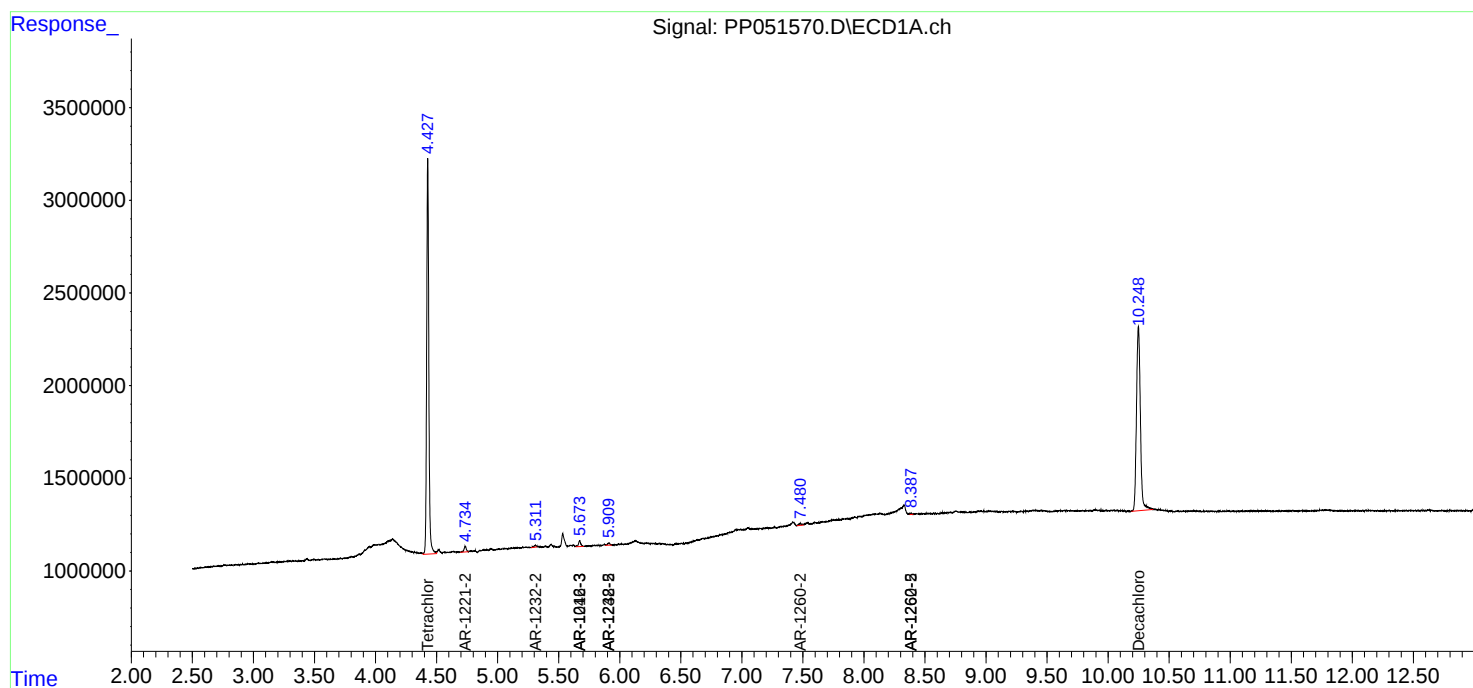


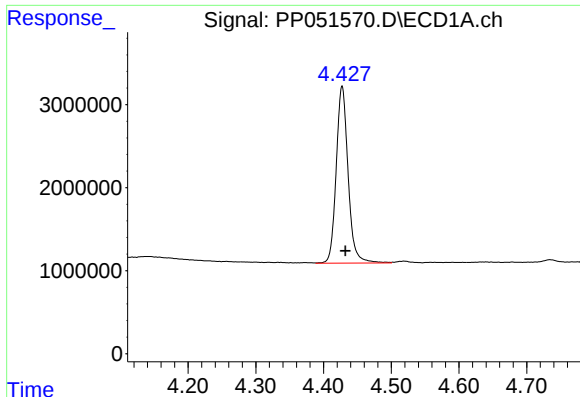

#1 Tetrachloro-m-xylene


R.T.: 4.427 min
Delta R.T.: -0.005 min
Response: 26055683
Conc: 14.66 ng/ml

Instrument :
ECD_P
ClientSampleId :

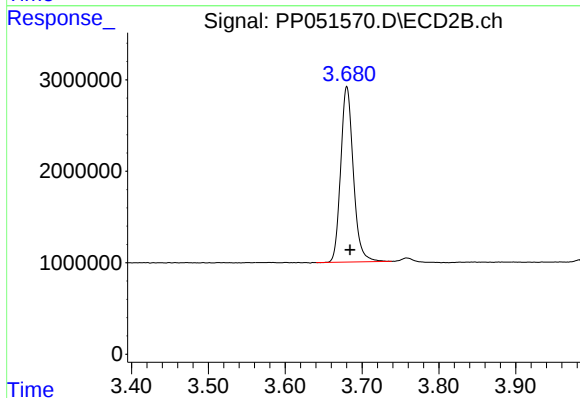


#1 Tetrachloro-m-xylene

R.T.: 3.680 min
Delta R.T.: -0.004 min
Response: 21791088
Conc: 14.43 ng/ml

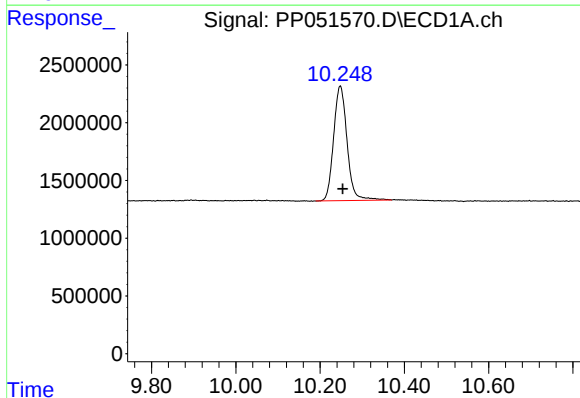


#2 Decachlorobiphenyl

R.T.: 10.248 min
Delta R.T.: -0.006 min
Response: 22050421
Conc: 14.27 ng/ml

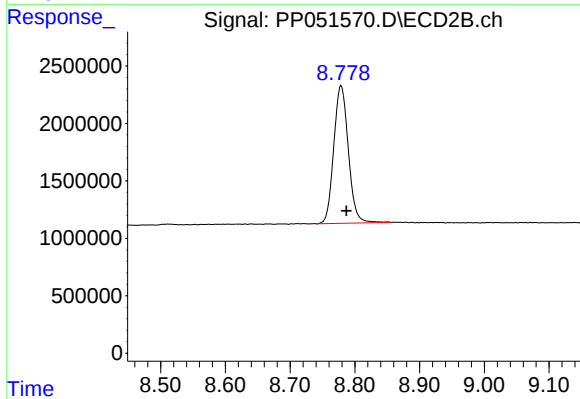

#2 Decachlorobiphenyl


R.T.: 8.779 min
Delta R.T.: -0.008 min
Response: 18738916
Conc: 15.64 ng/ml

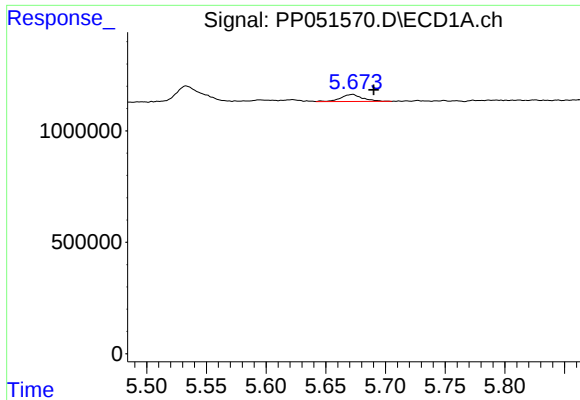

#5 AR-1016-3


R.T.: 5.672 min
Delta R.T.: -0.018 min
Response: 404976
Conc: 7.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

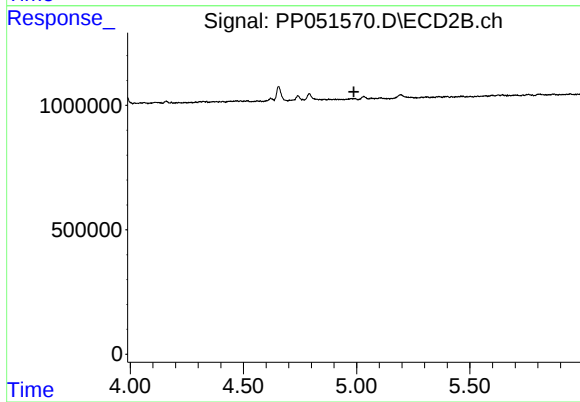


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

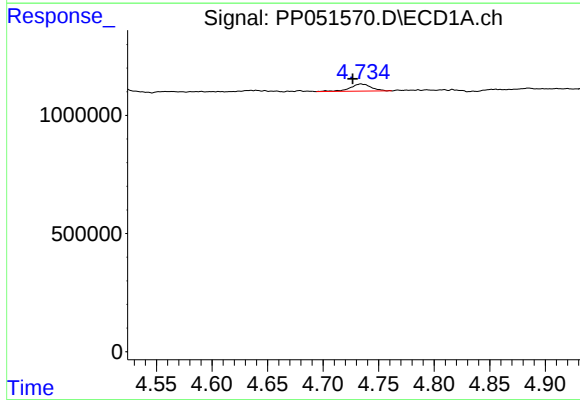


#9 AR-1221-2

R.T.: 4.734 min
Delta R.T.: 0.007 min
Response: 399528
Conc: 23.47 ng/ml

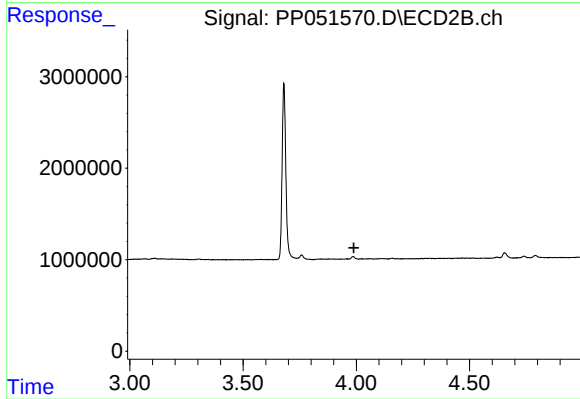

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.989 min
Response: 0
Conc: N.D.

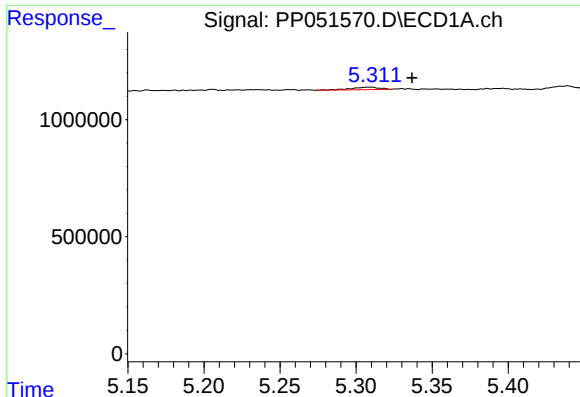

#12 AR-1232-2


R.T.: 5.309 min
Delta R.T.: -0.028 min
Response: 134342
Conc: 6.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

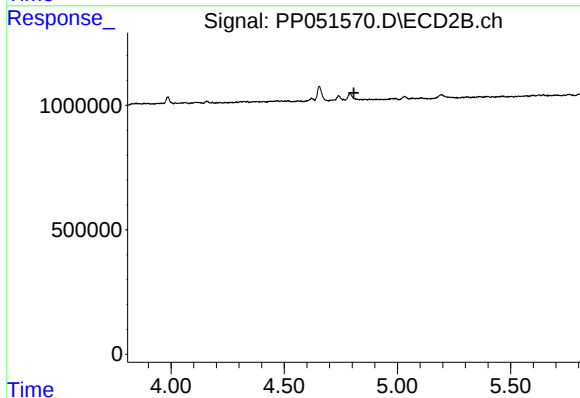


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.808 min
Response: 0
Conc: N.D.

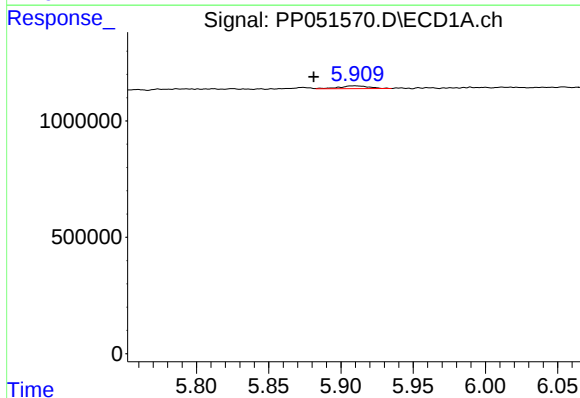


#15 AR-1232-5

R.T.: 5.910 min
Delta R.T.: 0.029 min
Response: 172350
Conc: 11.49 ng/ml

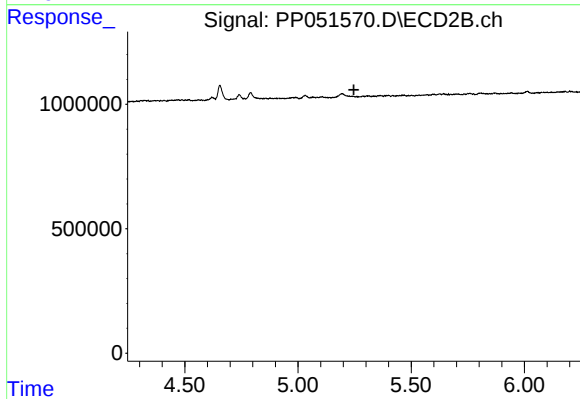

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.247 min
Response: 0
Conc: N.D.

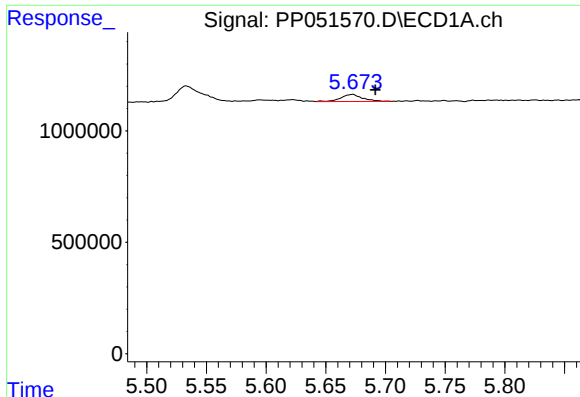

#18 AR-1242-3


R.T.: 5.672 min
Delta R.T.: -0.019 min
Response: 404976
Conc: 8.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

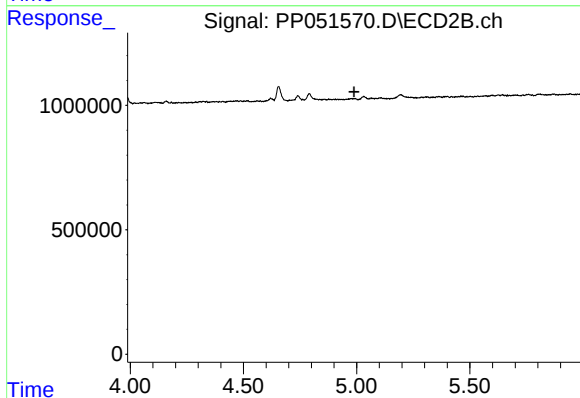


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

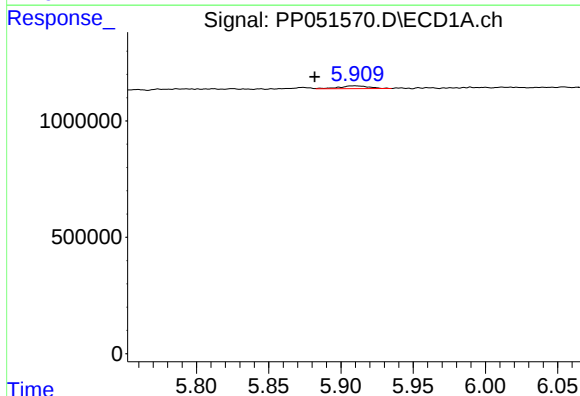


#22 AR-1248-2

R.T.: 5.910 min
Delta R.T.: 0.028 min
Response: 172350
Conc: 3.04 ng/ml

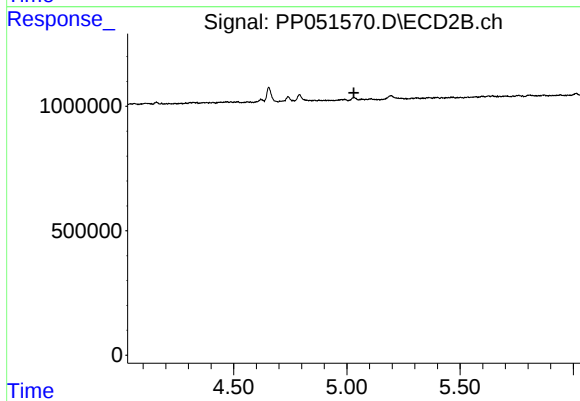

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.031 min
Response: 0
Conc: N.D.

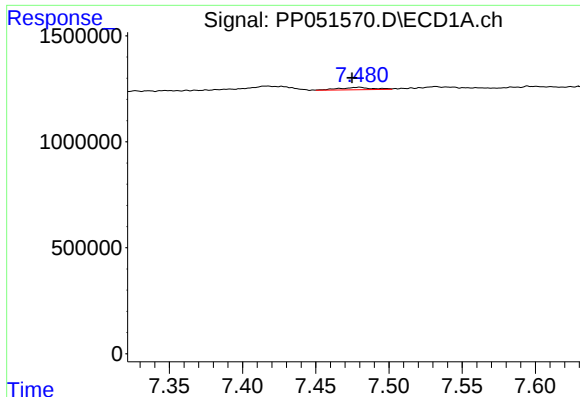

#32 AR-1260-2


R.T.: 7.479 min
Delta R.T.: 0.004 min
Response: 177655
Conc: 1.68 ng/ml

Instrument :
ECD_P
ClientSampleId :

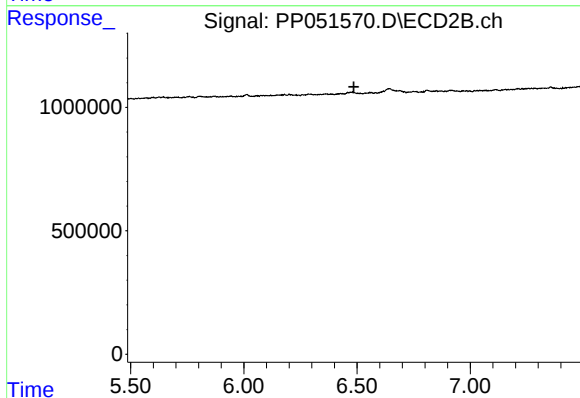


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

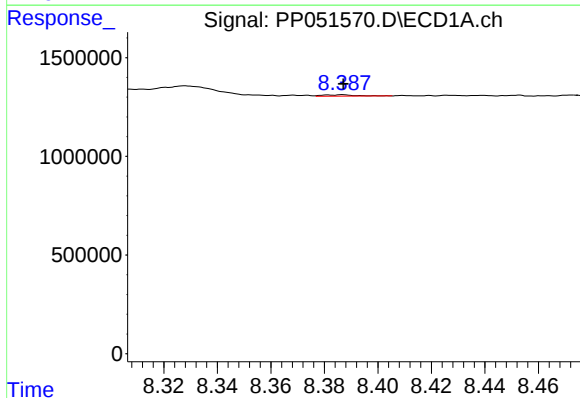


#35 AR-1260-5

R.T.: 8.386 min
Delta R.T.: -0.002 min
Response: 56102
Conc: 0.36 ng/ml

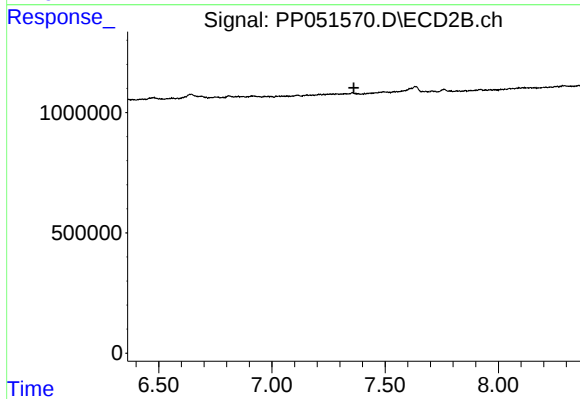

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

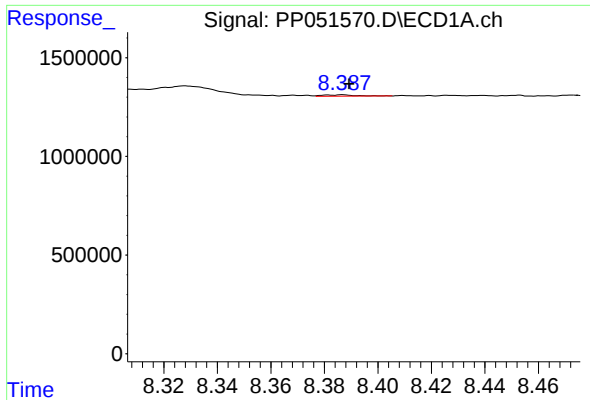

#37 AR-1262-2

R.T.: 8.386 min
Delta R.T.: -0.004 min
Response: 56102
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

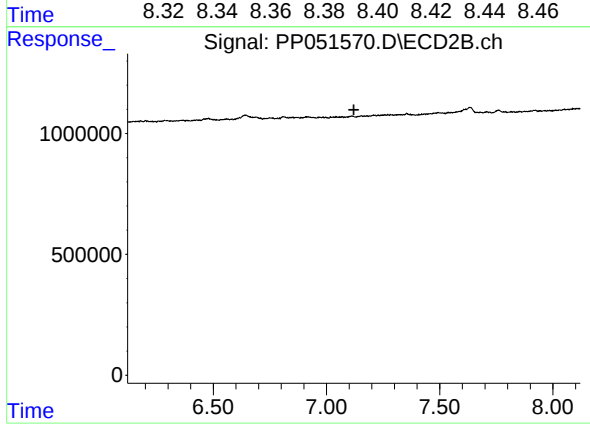

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.121 min
Response: 0
Conc: N.D.