

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092421\
 Data File : PP039491.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Sep 2021 9:37
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 18:33:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 24 18:31:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
24)	L5	AR-1248-4	7.148f	0.000	18028	0	16.606 N.D. #
26)	L6	AR-1254-1	7.148	0.000	18028	0	16.516 N.D. #
28)	L6	AR-1254-3	7.769f	0.000	10714	0	6.439 N.D. #
29)	L6	AR-1254-4	8.071f	0.000	25829	0	21.145 N.D. #
32)	L7	AR-1260-2	8.206f	0.000	37444	0	27.046 N.D. #
33)	L7	AR-1260-3	8.551	7.213	2197	51301	2.656 42.642 #
36)	L8	AR-1262-1	8.551	0.000	2197	0	1.645 N.D. #
39)	L8	AR-1262-4	9.496	0.000	1056	0	1.765 N.D. #
42)	L9	AR-1268-2	9.496f	0.000	1056	0	0.410 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092421\
Data File : PP039491.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Sep 2021 9:37
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 18:33:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 24 18:31:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

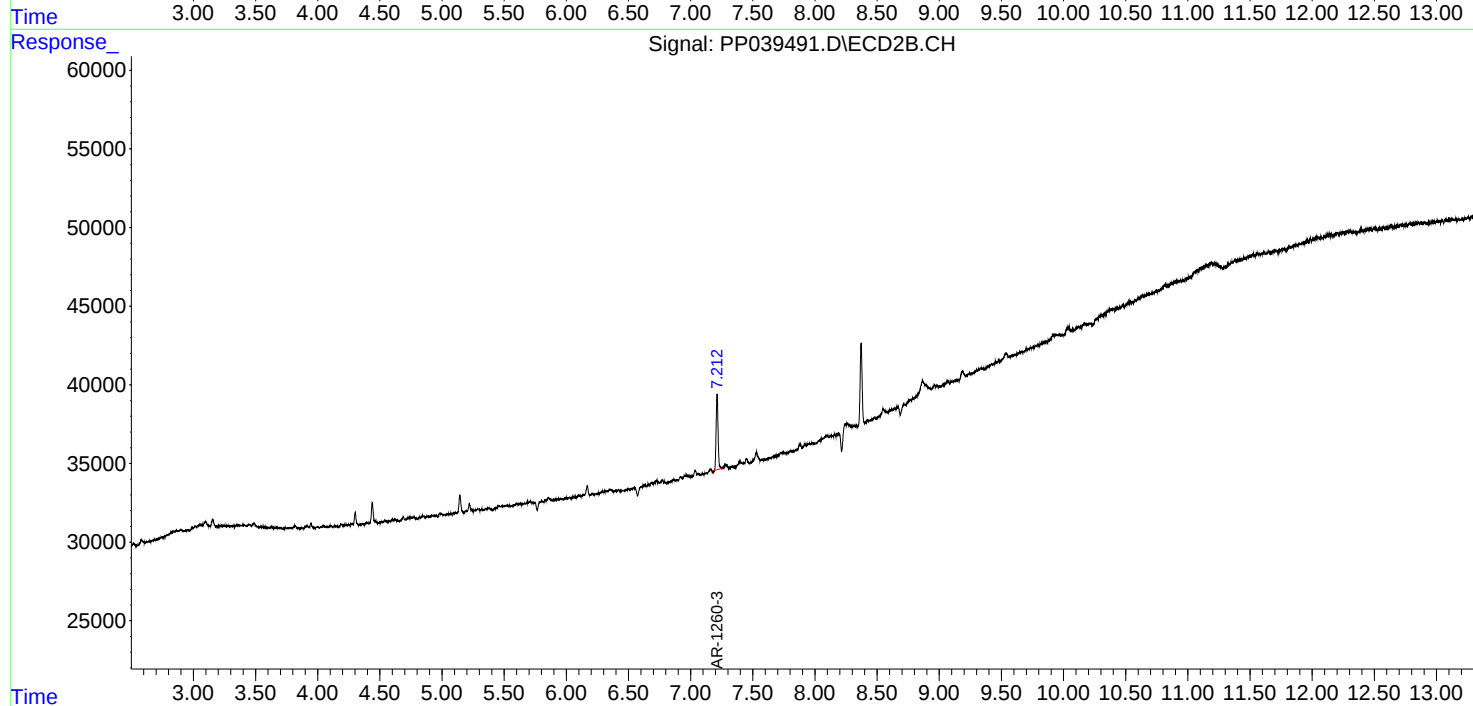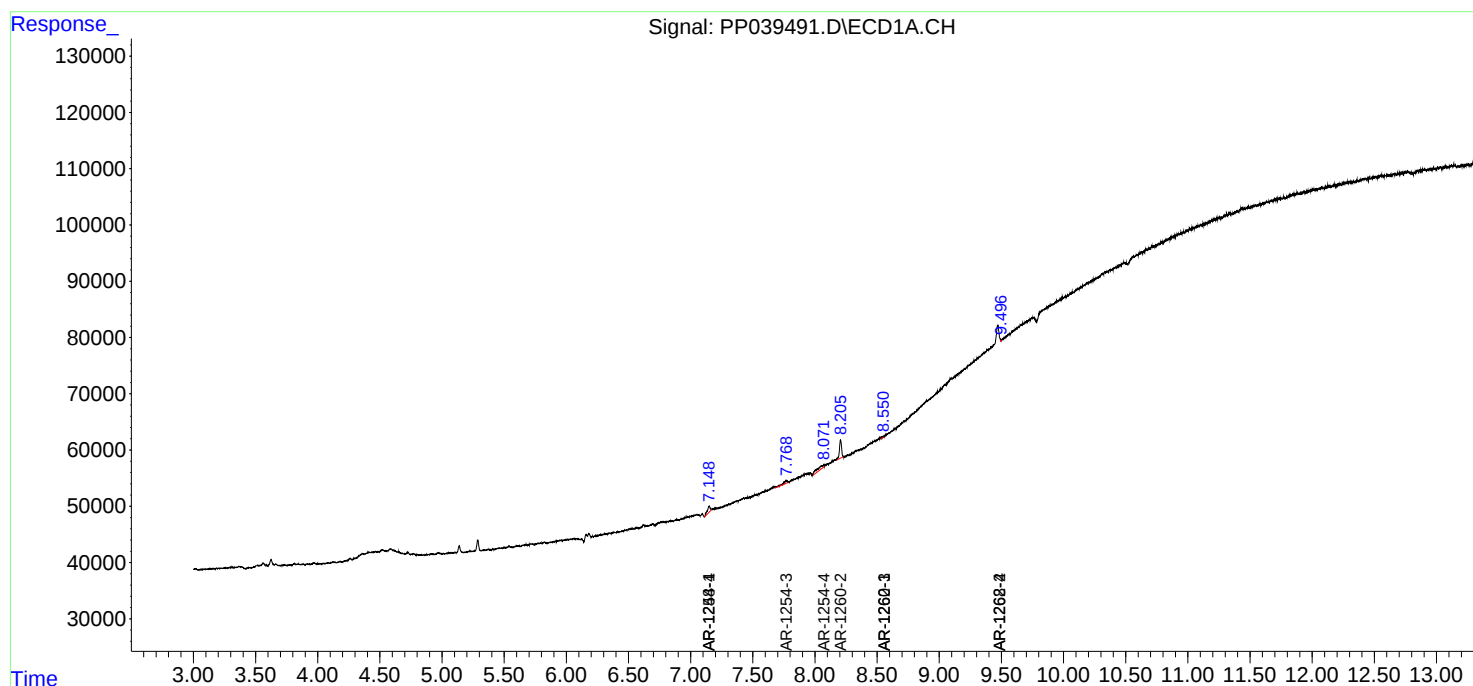


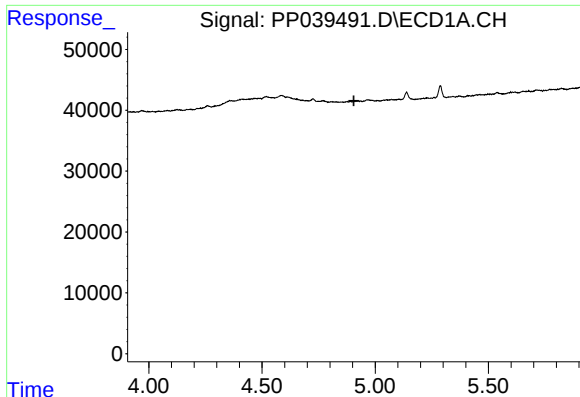

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.906 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

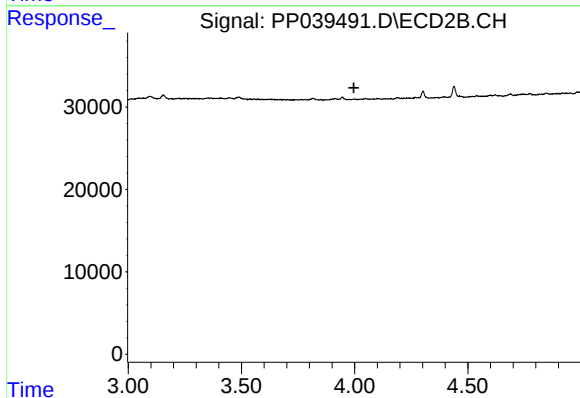


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

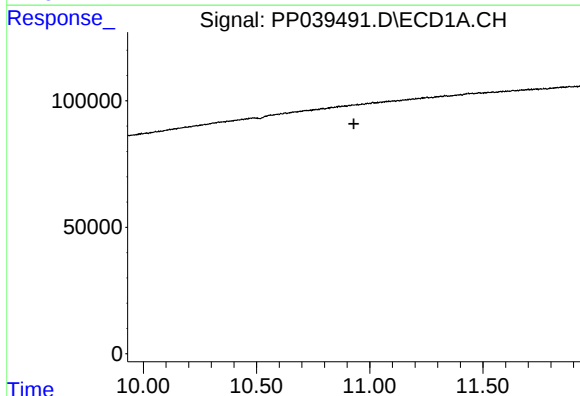


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.930 min
Response: 0
Conc: N.D.

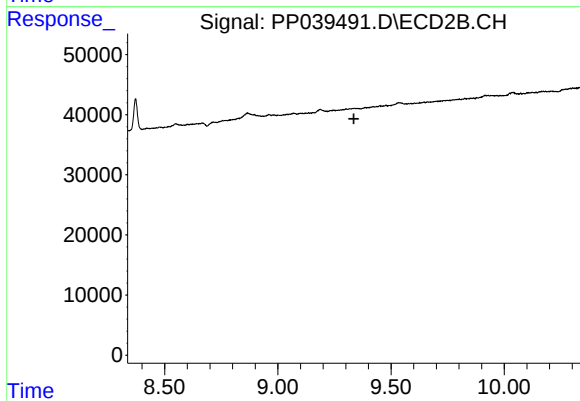

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

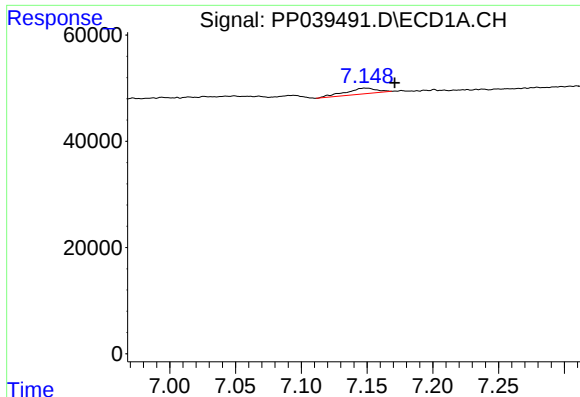

#24 AR-1248-4


R.T.: 7.148 min
Delta R.T.: -0.023 min
Response: 18028
Conc: 16.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

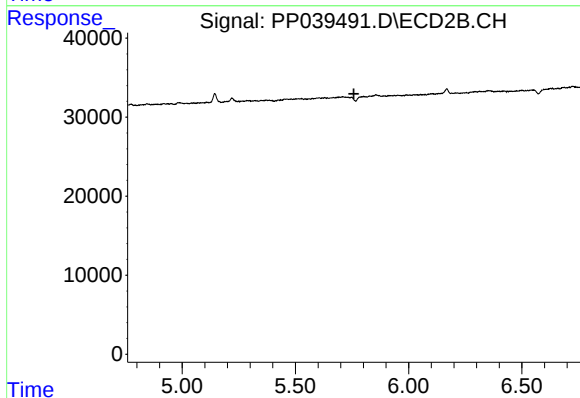


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.758 min
Response: 0
Conc: N.D.

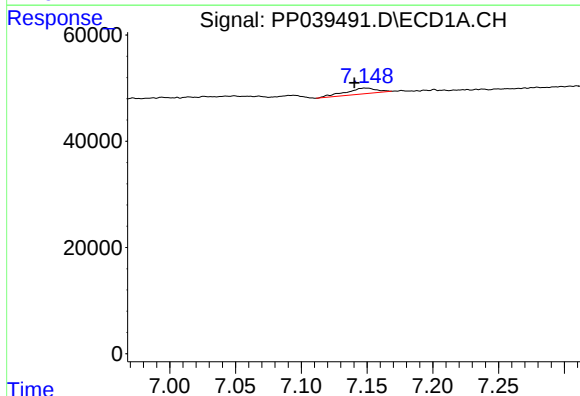


#26 AR-1254-1

R.T.: 7.148 min
Delta R.T.: 0.008 min
Response: 18028
Conc: 16.52 ng/ml

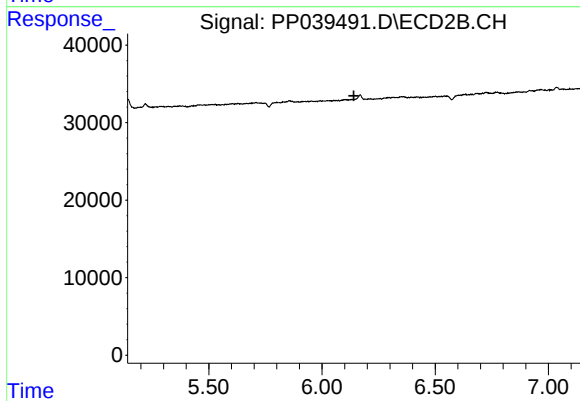

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

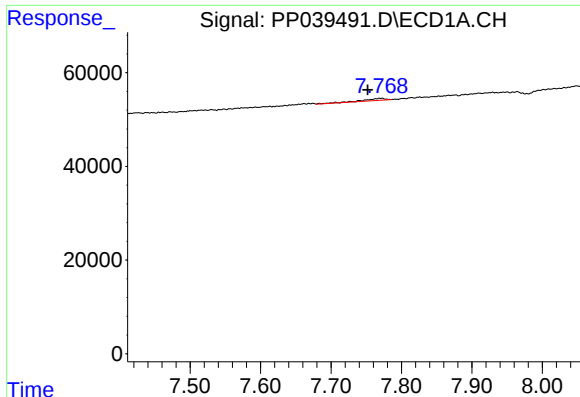

#28 AR-1254-3


R.T.: 7.769 min
Delta R.T.: 0.016 min
Response: 10714
Conc: 6.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

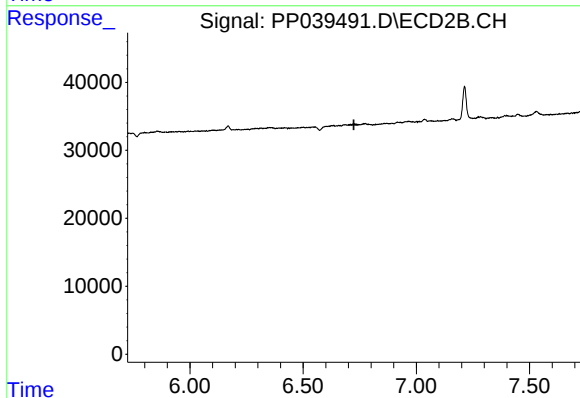


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

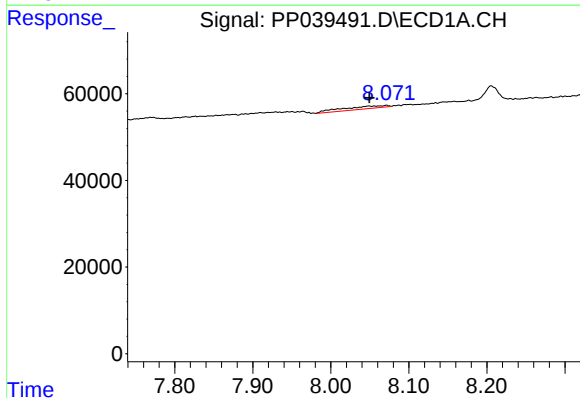


#29 AR-1254-4

R.T.: 8.071 min
Delta R.T.: 0.022 min
Response: 25829
Conc: 21.15 ng/ml

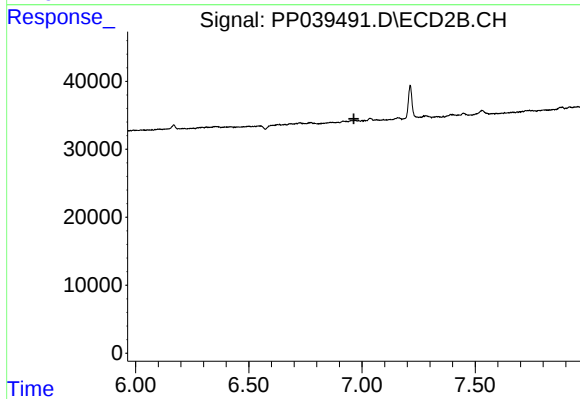

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

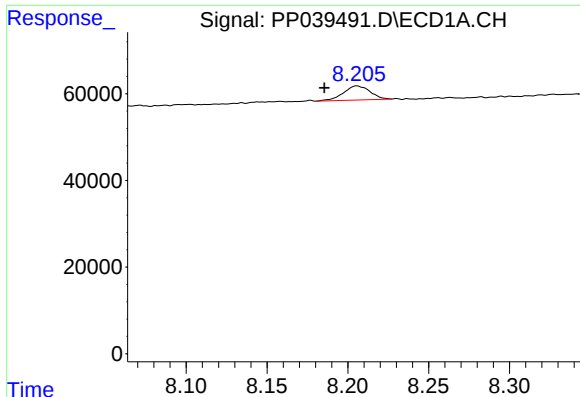

#32 AR-1260-2


R.T.: 8.206 min
Delta R.T.: 0.020 min
Response: 37444
Conc: 27.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

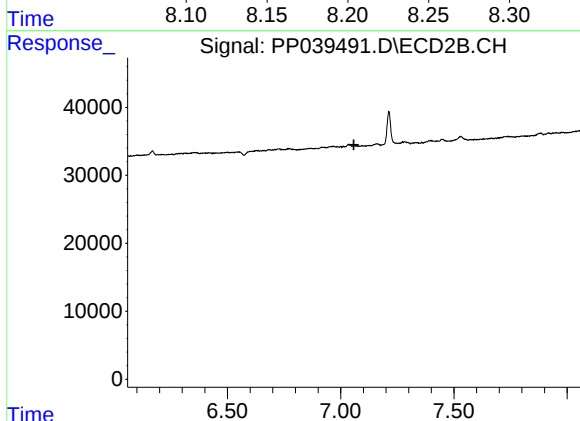


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.058 min
Response: 0
Conc: N.D.

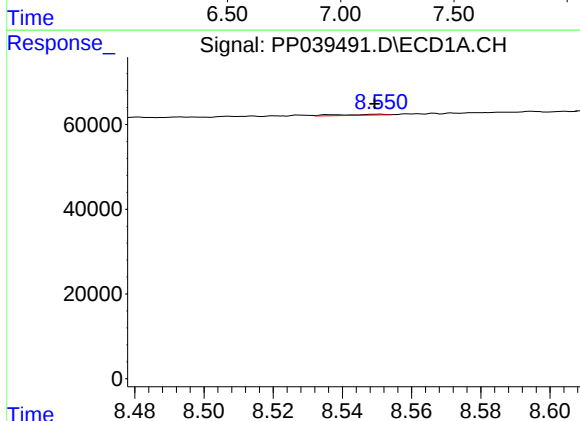


#33 AR-1260-3

R.T.: 8.551 min
Delta R.T.: 0.001 min
Response: 2197
Conc: 2.66 ng/ml

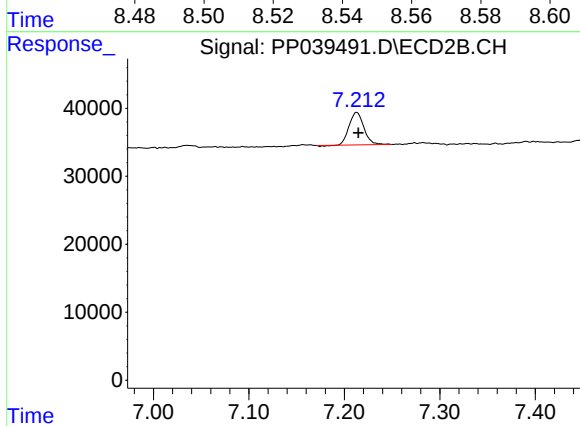

#33 AR-1260-3


R.T.: 7.213 min
Delta R.T.: -0.002 min
Response: 51301
Conc: 42.64 ng/ml

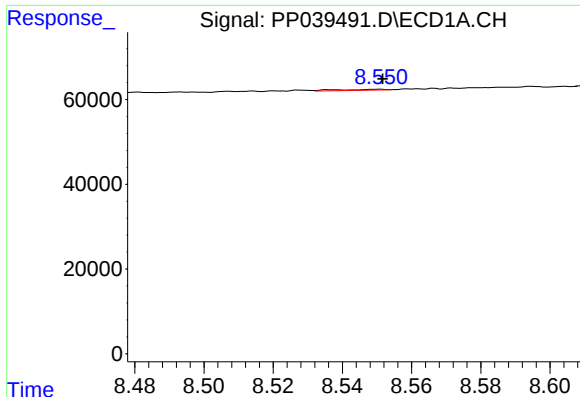

#36 AR-1262-1


R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 2197
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

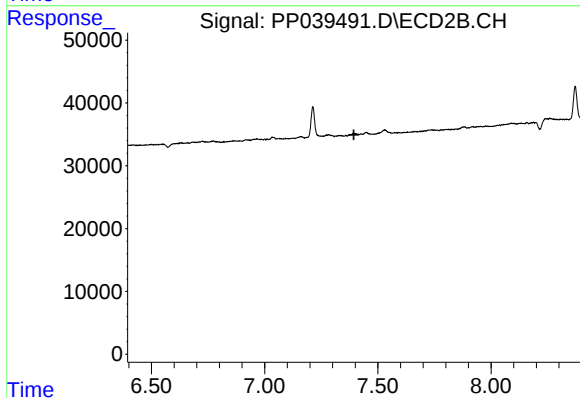


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.394 min
Response: 0
Conc: N.D.

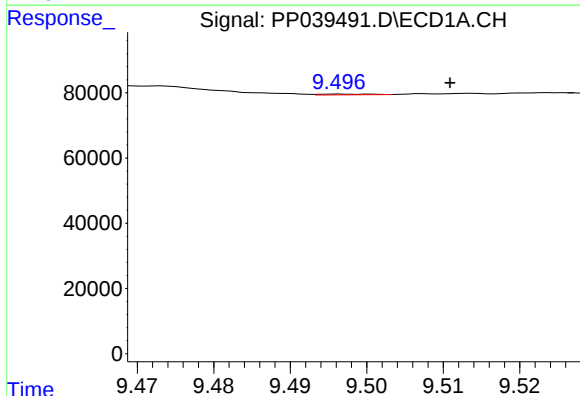


#39 AR-1262-4

R.T.: 9.496 min
Delta R.T.: -0.015 min
Response: 1056
Conc: 1.76 ng/ml

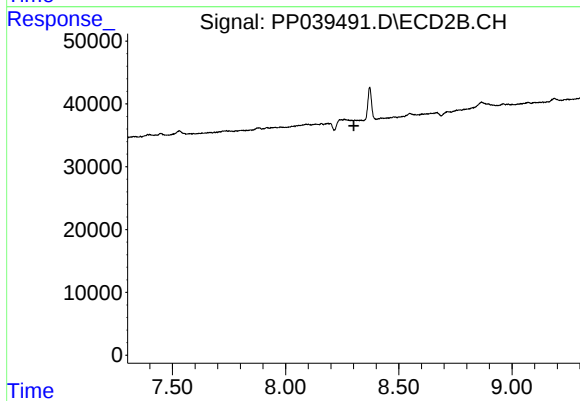

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.302 min
Response: 0
Conc: N.D.

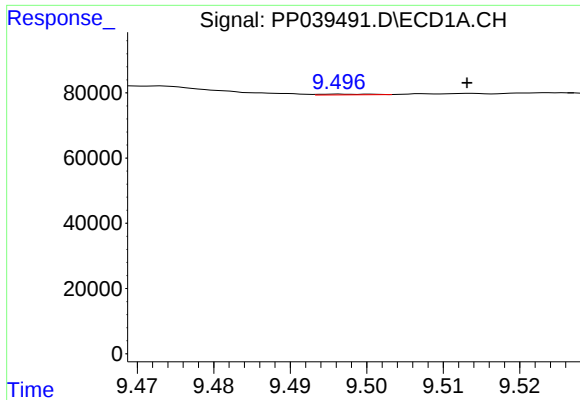

#42 AR-1268-2

R.T.: 9.496 min
Delta R.T.: -0.017 min
Response: 1056
Conc: 0.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

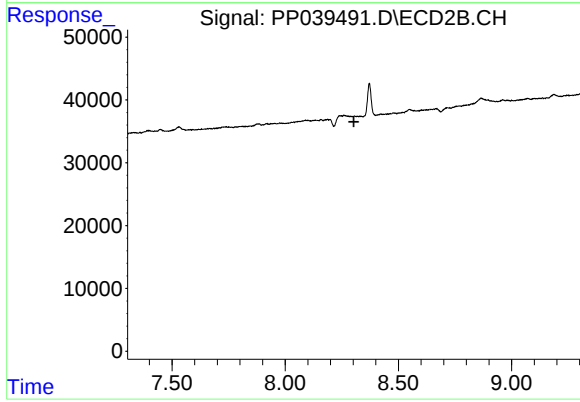

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.303 min
Response: 0
Conc: N.D.