

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092424\
Data File : PP067227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 00:35
Operator : YP\AJ
Sample : P4163-12
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RV-15(4.0-4.5)

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 09:05:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091224.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 13 08:31:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.751	4.054	22642968	23664374	18.370m	16.950
2) SA Decachlor...	10.660	9.228	29528545	27740248	22.675	20.919

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092424\
Data File : PP067227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 00:35
Operator : YP\AJ
Sample : P4163-12
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RV-15(4.0-4.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 09:05:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091224.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 13 08:31:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

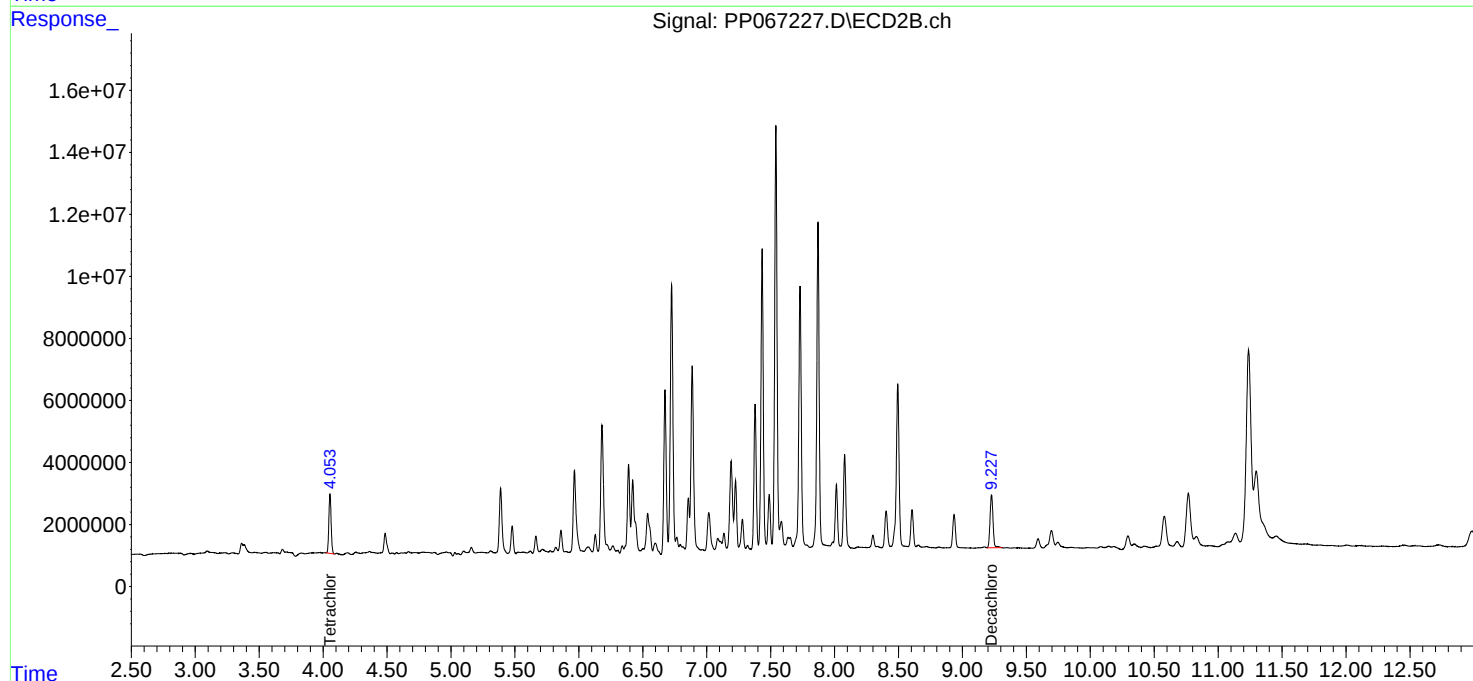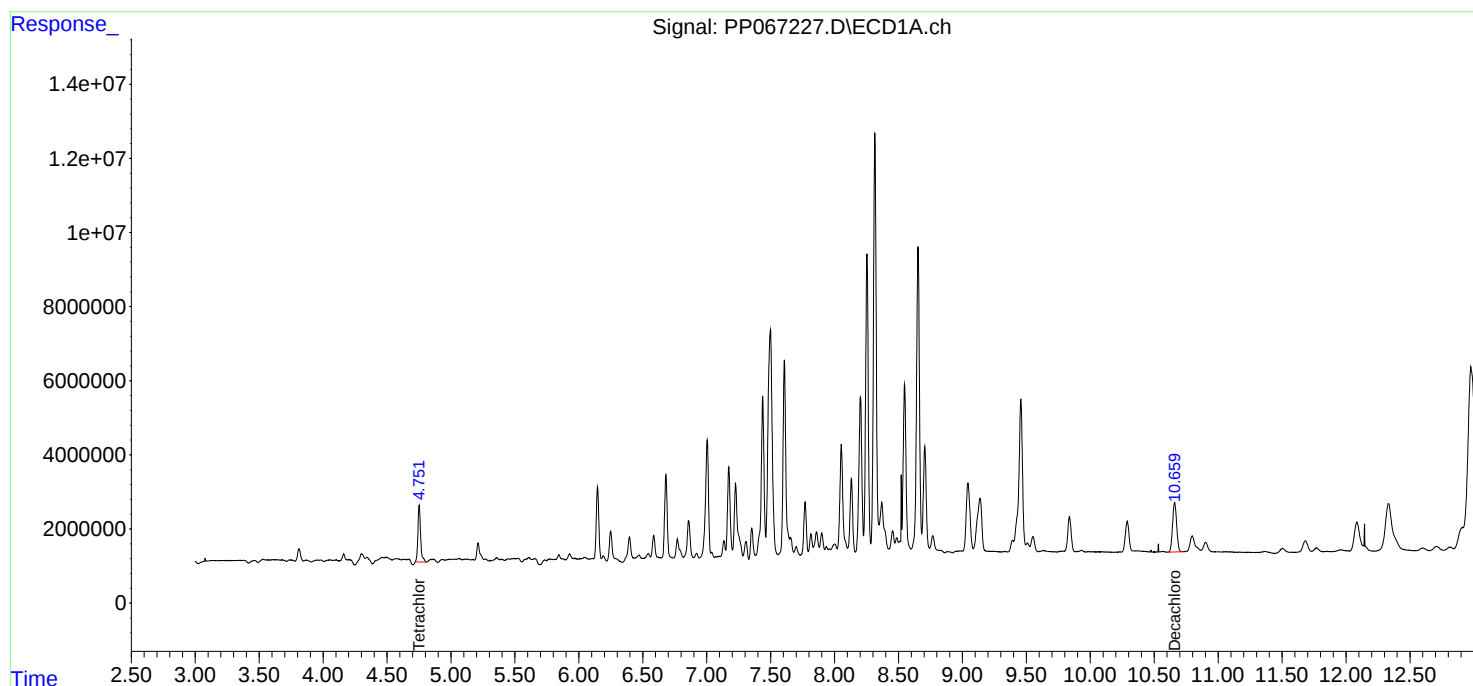

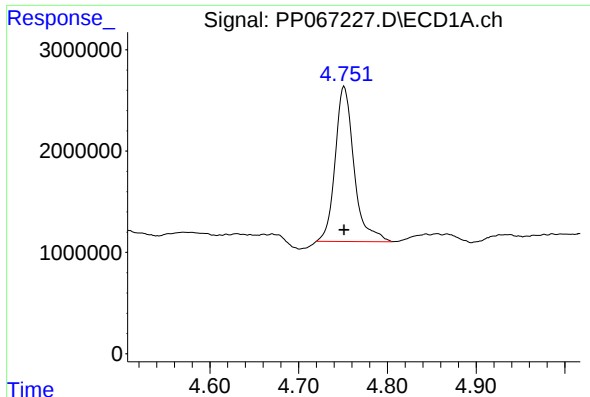


#1 Tetrachloro-m-xylene

R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 22642968
Conc: 18.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
RV-15(4.0-4.5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :Ankita Jodhani 09/25/2024

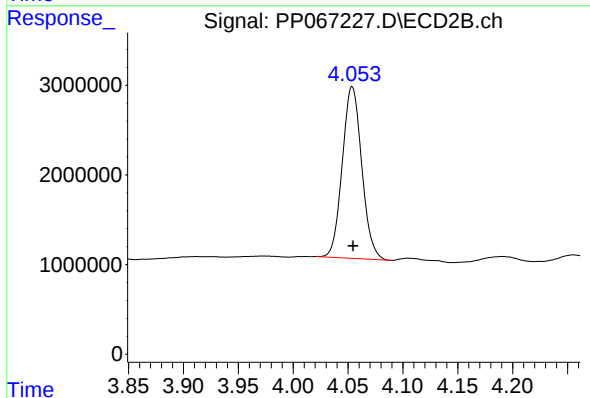


#1 Tetrachloro-m-xylene

R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 23664374
Conc: 16.95 ng/ml

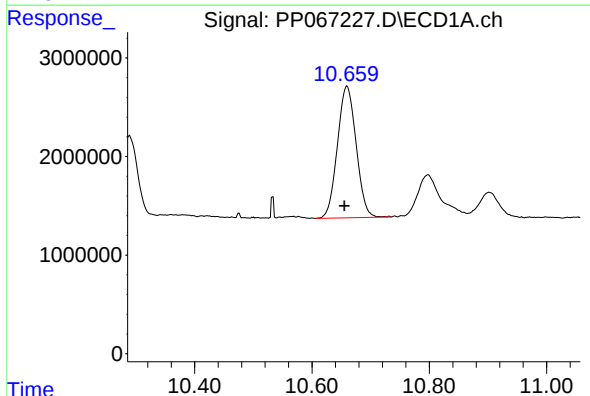

#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: 0.005 min
Response: 29528545
Conc: 22.67 ng/ml

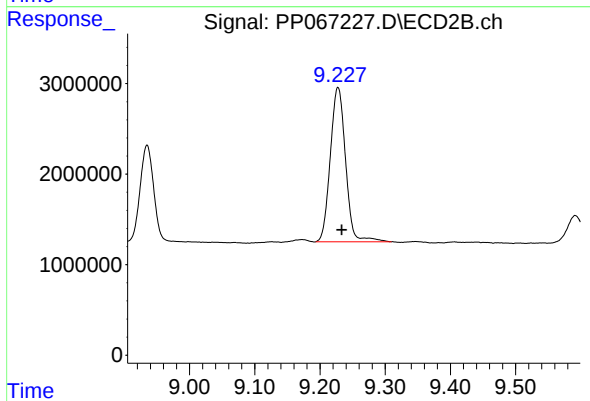

#2 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.006 min
Response: 27740248
Conc: 20.92 ng/ml