

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092425\
 Data File : PP075296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2025 15:28
 Operator : YP\AJ
 Sample : Q3167-03 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT3997

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/26/2025
 Supervised By :Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 03:03:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.810	2474980	12143022	1.891	1.990m
2) SA Decachlor...	10.442	8.808	1860060	11230676	1.865	1.862

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092425\
Data File : PP075296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2025 15:28
Operator : YP\AJ
Sample : Q3167-03 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RT3997


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 03:03:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

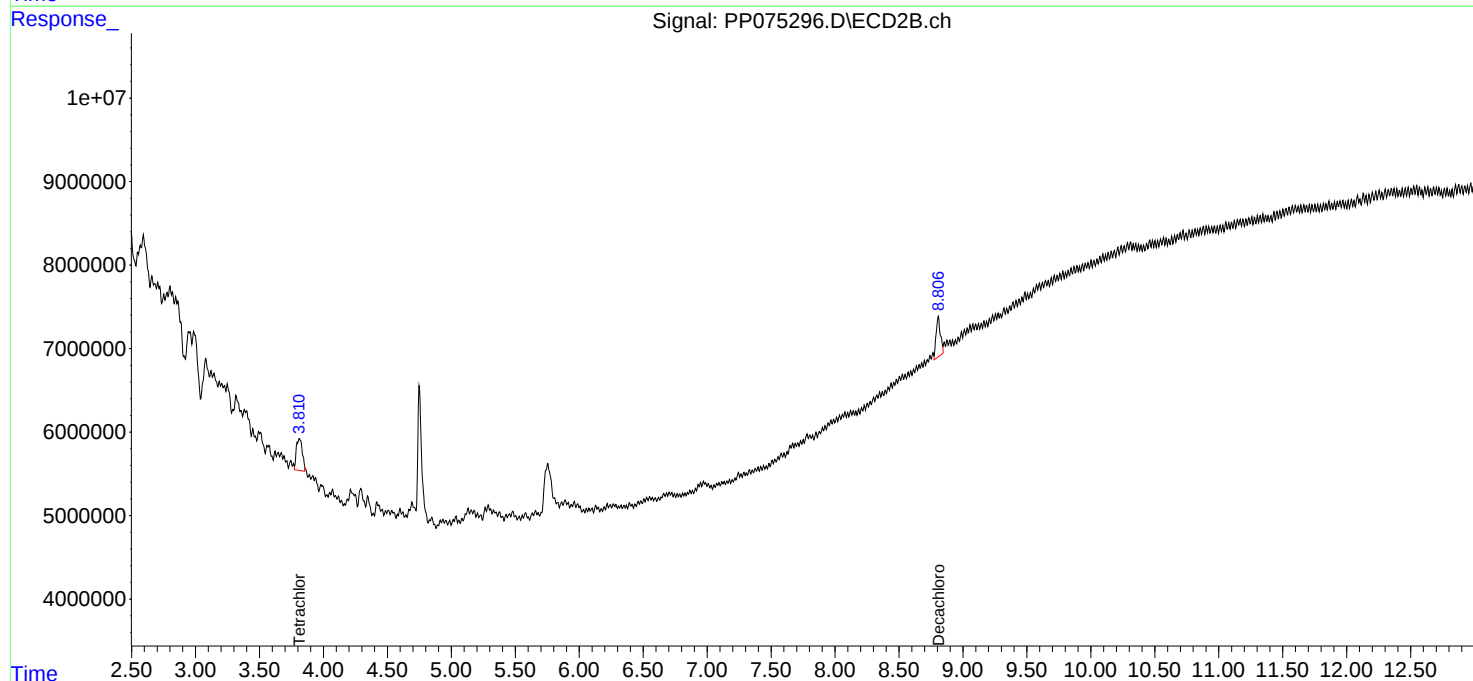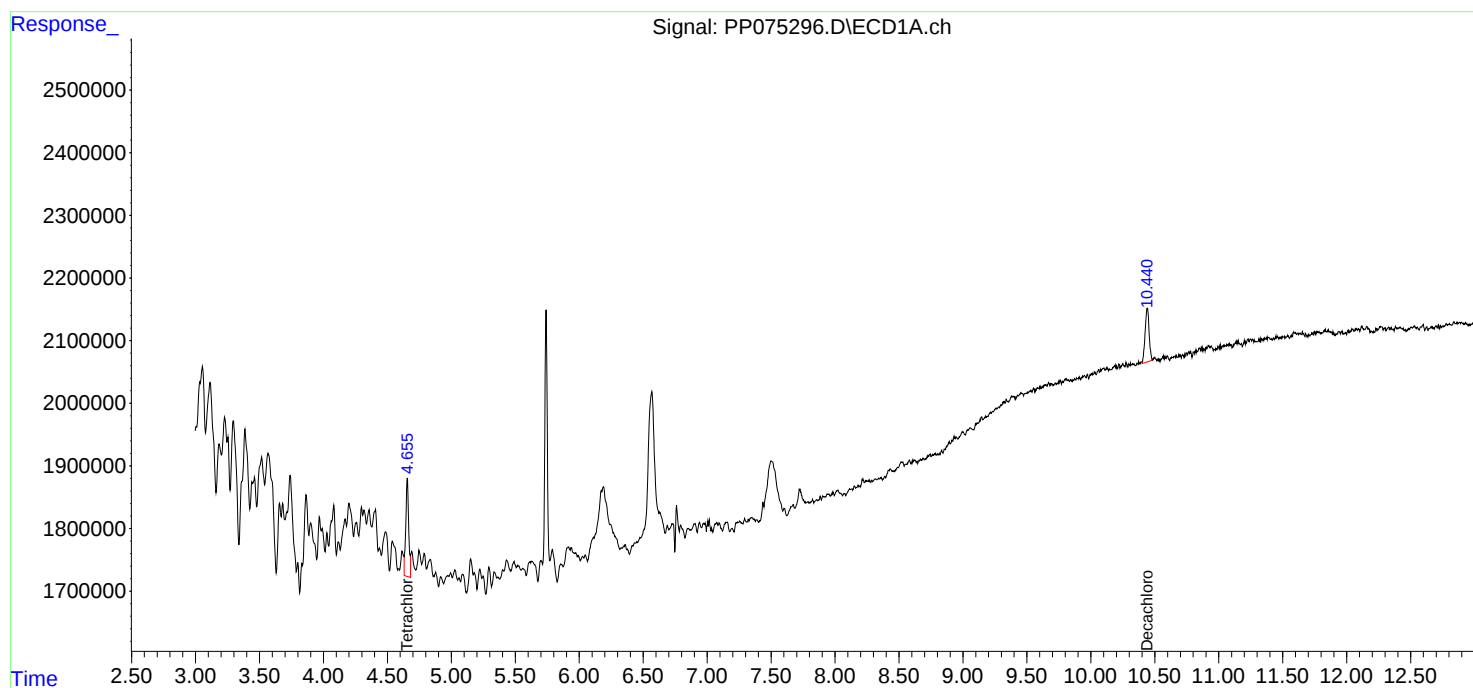

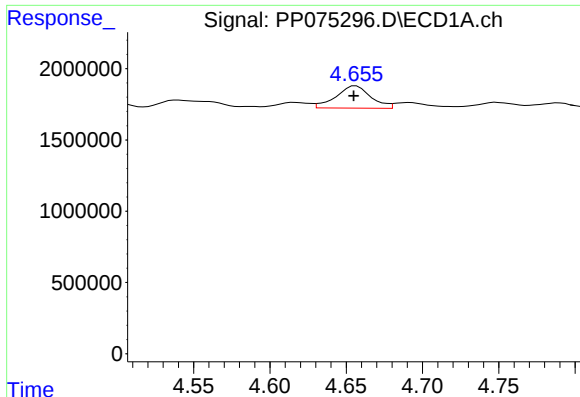


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: 0.001 min
Response: 2474980
Conc: 1.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
RT3997


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

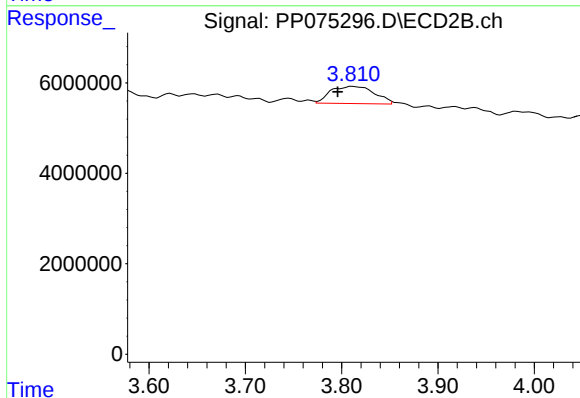


#1 Tetrachloro-m-xylene

R.T.: 3.810 min
Delta R.T.: 0.014 min
Response: 12143022
Conc: 1.99 ng/ml m

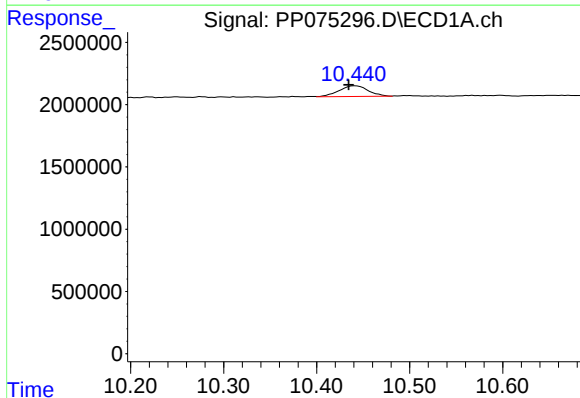

#2 Decachlorobiphenyl

R.T.: 10.442 min
Delta R.T.: 0.007 min
Response: 1860060
Conc: 1.86 ng/ml

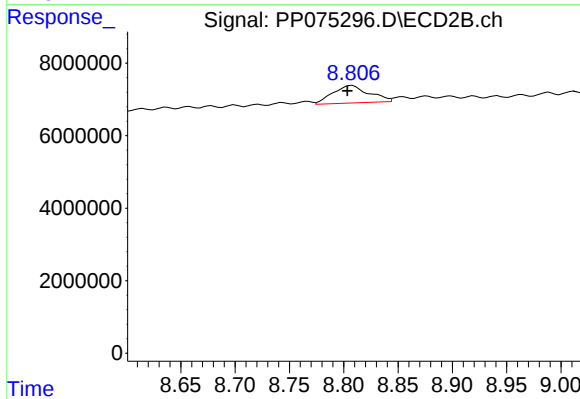

#2 Decachlorobiphenyl

R.T.: 8.808 min
Delta R.T.: 0.004 min
Response: 11230676
Conc: 1.86 ng/ml