

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092518\
 Data File : PP027517.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Sep 2018 3:59
 Operator : EI\MA
 Sample : J4770-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 05:54:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092418.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 25 01:51:01 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.045	12.158	101.3E6	142.5E6	399.510	329.201
Target Compounds							
1) T	Dalapon	3.273	2.947	77048939	135.5E6	128.995	249.209 #
6) T	MCPD	12.727	0.000	27041220	0	61.415	N.D. #
7) T	MCPA	12.984	12.980	3133345	43612849	11.787	32.486 #
8) T	DICHLORPROP	13.539	13.592	3692517	18944276	10.192	45.663 #
12) T	2,4,5-T	0.000	15.885	0	17820138	N.D.	9.005 #
13) T	2,4-DB	16.355	0.000	10450070	0	55.137	N.D. #
14) T	DINOSEB	17.833	0.000	10630269	0	5.522	N.D. #
15) T	Picloram	17.593	18.266	4482887	32358889	1.459	12.926 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092518\
Data File : PP027517.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Sep 2018 3:59
Operator : EI\MA
Sample : J4770-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 05:54:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092418.M
Quant Title : 8080.M
QLast Update : Tue Sep 25 01:51:01 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

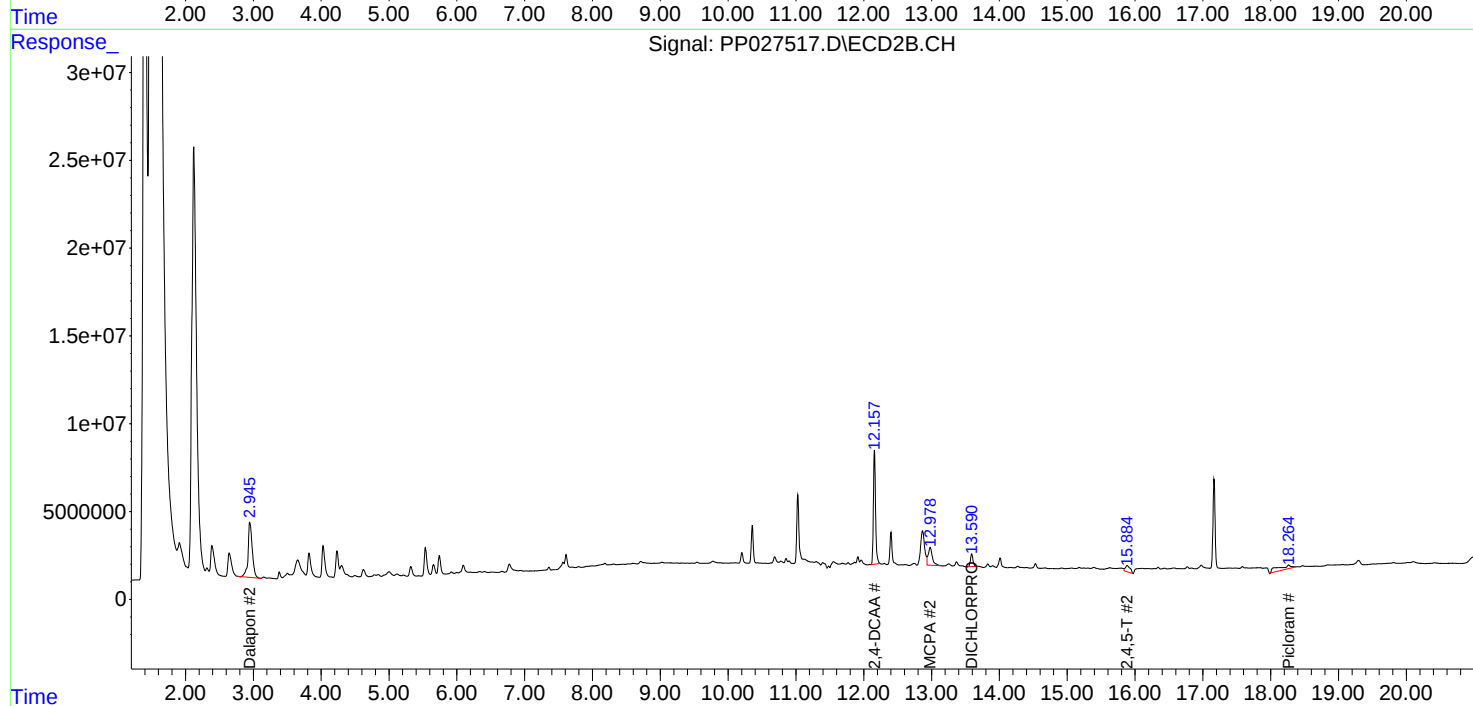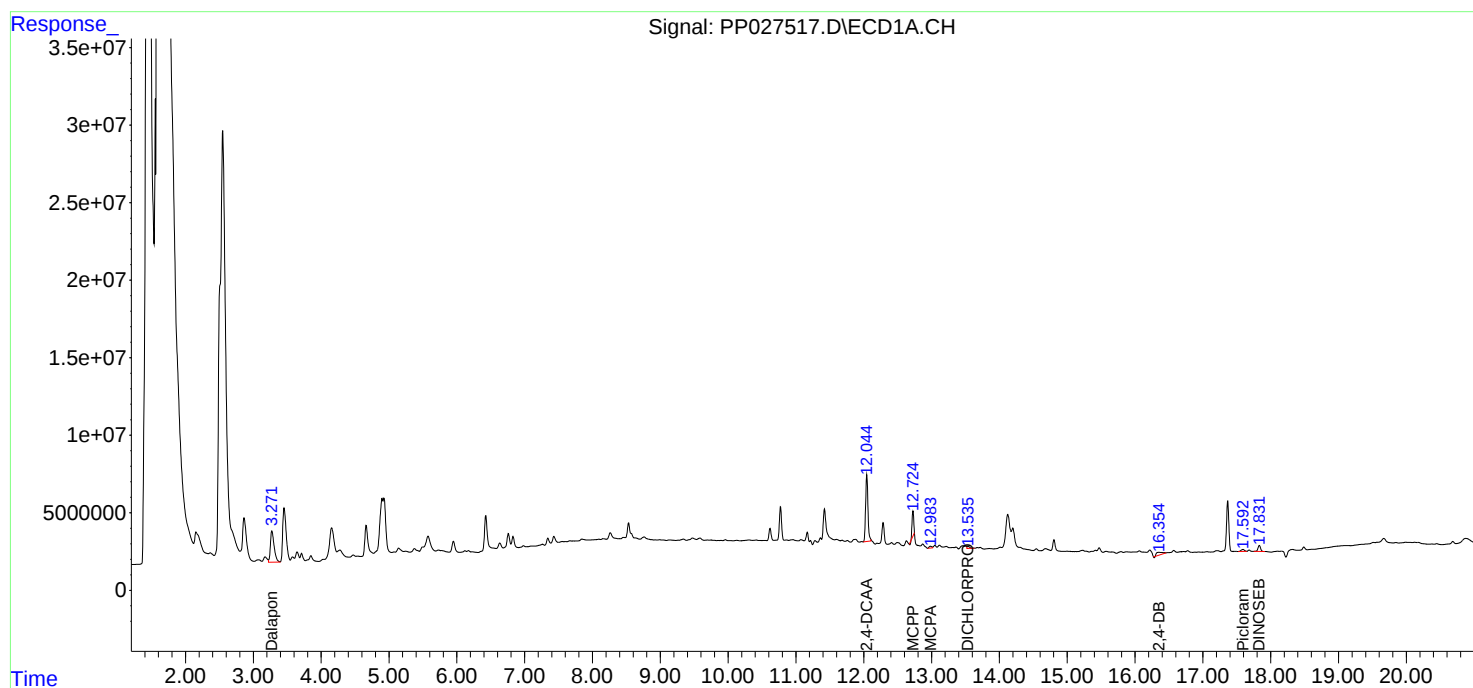


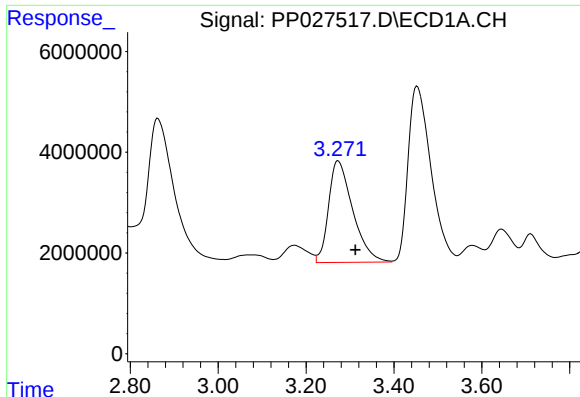

#1 Dalapon


R.T.: 3.273 min
Delta R.T.: -0.039 min
Response: 77048939
Conc: 129.00 ng/ml

Instrument :
ECD_P
ClientSampleId :

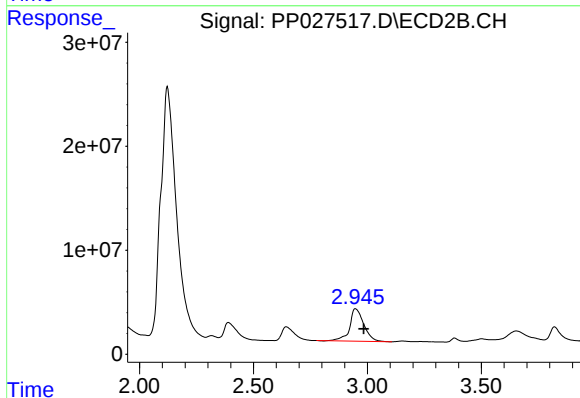


#1 Dalapon

R.T.: 2.947 min
Delta R.T.: -0.036 min
Response: 135543356
Conc: 249.21 ng/ml

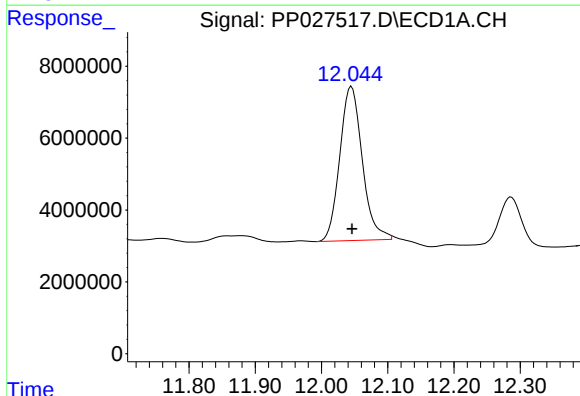


#4 2,4-DCAA

R.T.: 12.045 min
Delta R.T.: -0.001 min
Response: 101321402
Conc: 399.51 ng/ml

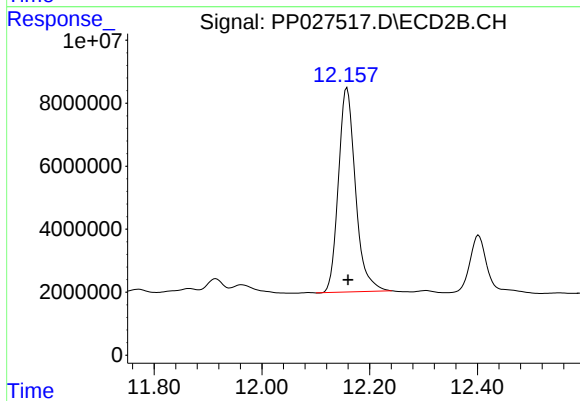

#4 2,4-DCAA


R.T.: 12.158 min
Delta R.T.: -0.002 min
Response: 142487361
Conc: 329.20 ng/ml

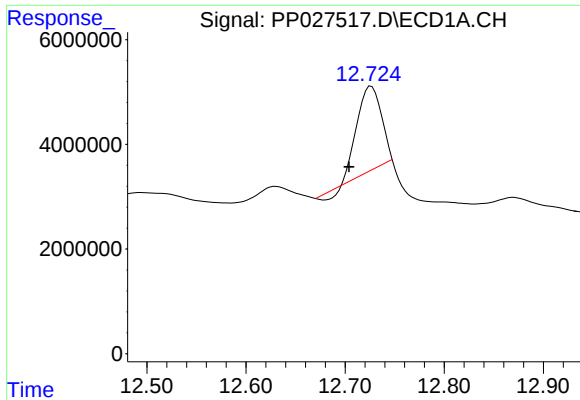

#6 MCPP


R.T.: 12.727 min
Delta R.T.: 0.022 min
Response: 27041220
Conc: 61.42 ug/ml

Instrument :
ECD_P
ClientSampleId :

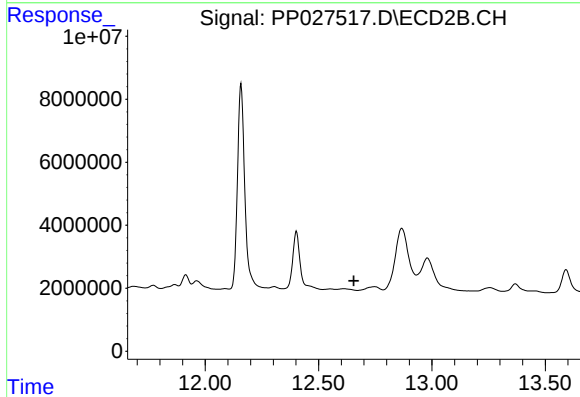


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.656 min
Response: 0
Conc: N.D.

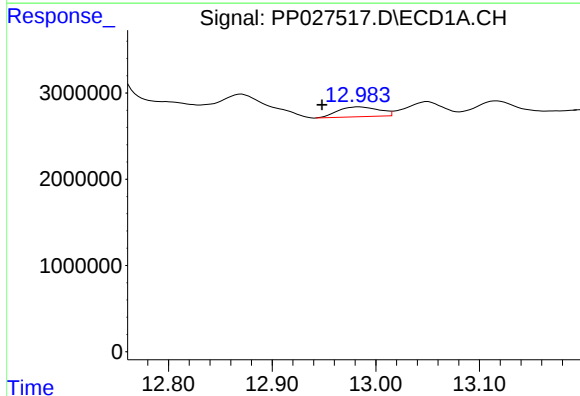


#7 MCPA

R.T.: 12.984 min
Delta R.T.: 0.036 min
Response: 3133345
Conc: 11.79 ug/ml

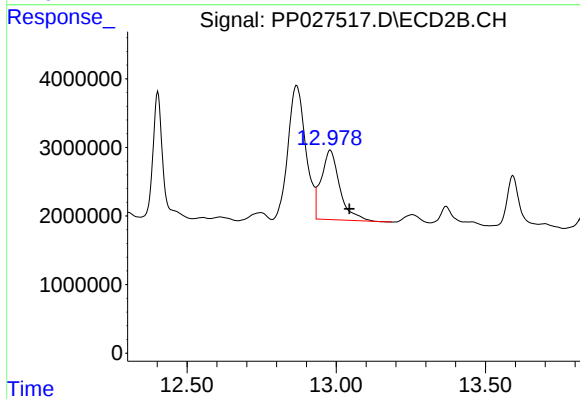

#7 MCPA


R.T.: 12.980 min
Delta R.T.: -0.064 min
Response: 43612849
Conc: 32.49 ug/ml

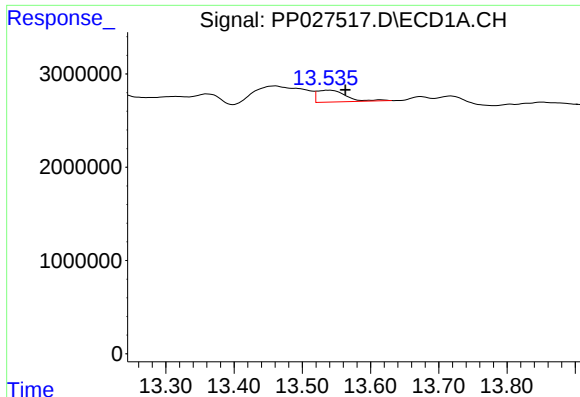

#8 DICHLORPROP


R.T.: 13.539 min
Delta R.T.: -0.024 min
Response: 3692517
Conc: 10.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

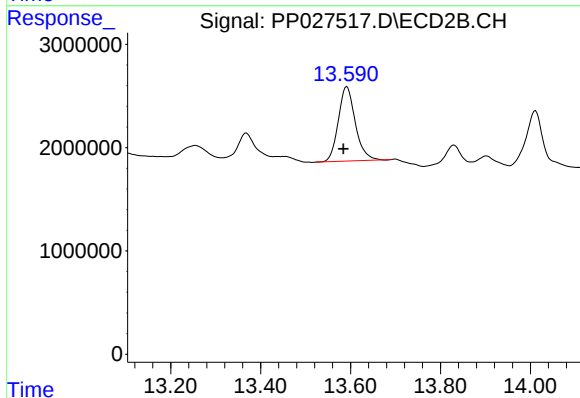


#8 DICHLORPROP

R.T.: 13.592 min
Delta R.T.: 0.008 min
Response: 18944276
Conc: 45.66 ng/ml

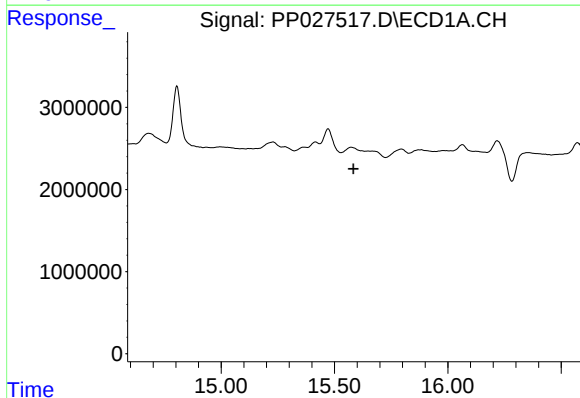


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.584 min
Response: 0
Conc: N.D.

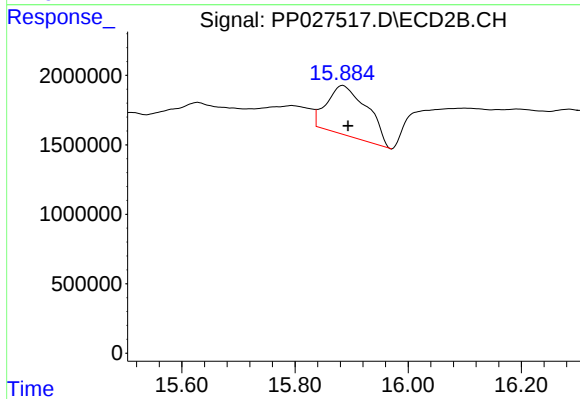

#12 2,4,5-T


R.T.: 15.885 min
Delta R.T.: -0.009 min
Response: 17820138
Conc: 9.00 ng/ml

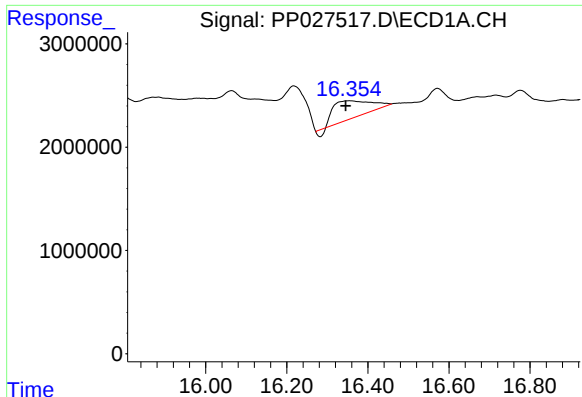

#13 2,4-DB


R.T.: 16.355 min
Delta R.T.: 0.009 min
Response: 10450070
Conc: 55.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

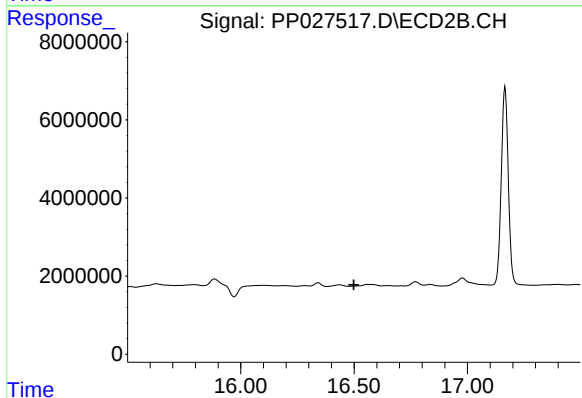


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.498 min
Response: 0
Conc: N.D.

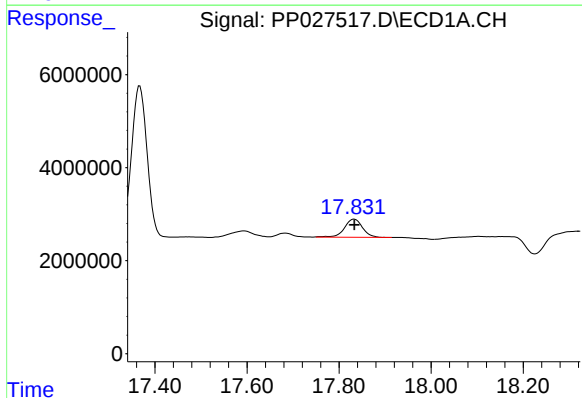


#14 DINOSEB

R.T.: 17.833 min
Delta R.T.: 0.000 min
Response: 10630269
Conc: 5.52 ng/ml

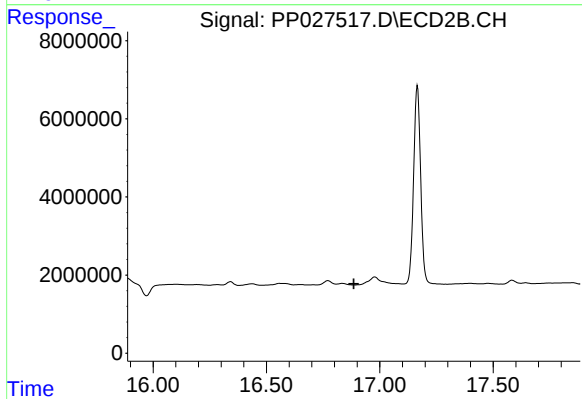

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.885 min
Response: 0
Conc: N.D.

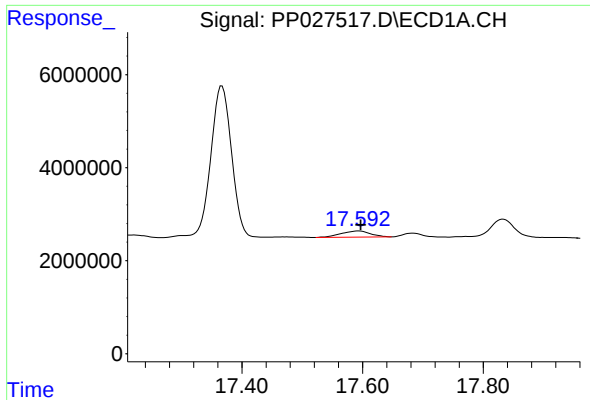

#15 Picloram

R.T.: 17.593 min
Delta R.T.: -0.003 min
Response: 4482887
Conc: 1.46 ng/ml

Instrument :
ECD_P
ClientSampleId :

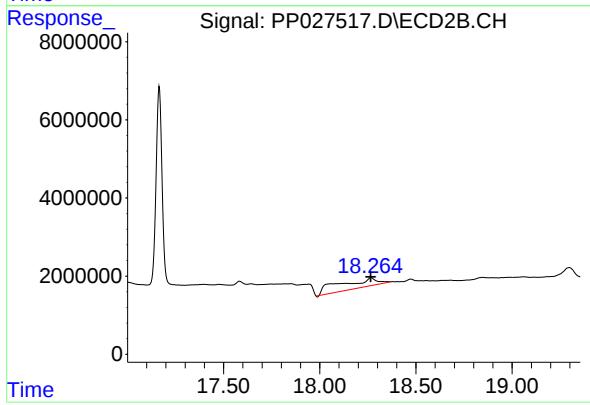

#15 Picloram

R.T.: 18.266 min
Delta R.T.: 0.000 min
Response: 32358889
Conc: 12.93 ng/ml