

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092523\
 Data File : PP060222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 19:01
 Operator : YP\AJ
 Sample : 04577-24
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DUP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/26/2023
 Supervised By :Ankita Jodhani 09/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 04:32:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 09:22:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.663	34779052	25282128	16.718	15.521
2) SA Decachlor...	10.423	8.728	23688987	23118041	15.530	15.268

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092523\
Data File : PP060222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 19:01
Operator : YP\AJ
Sample : 04577-24
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
DUP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2023
Supervised By :Ankita Jodhani 09/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 04:32:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 09:22:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

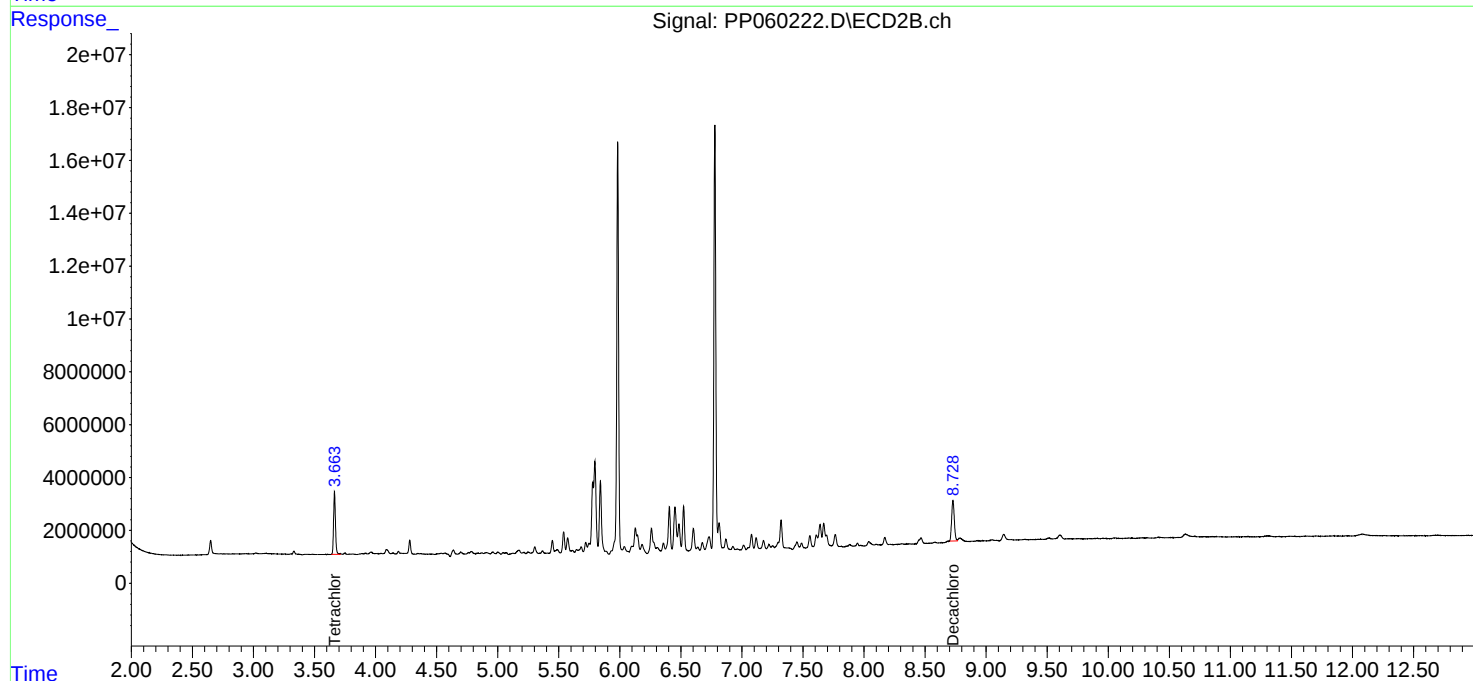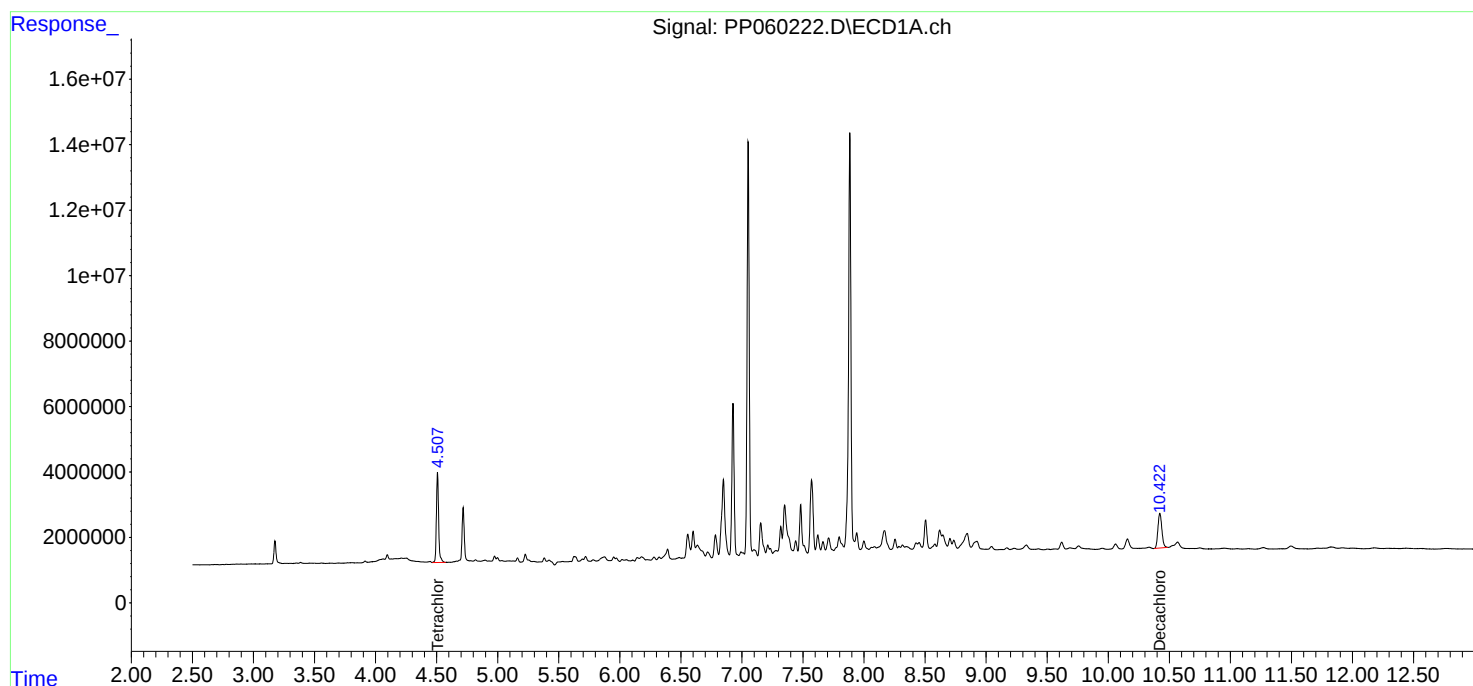

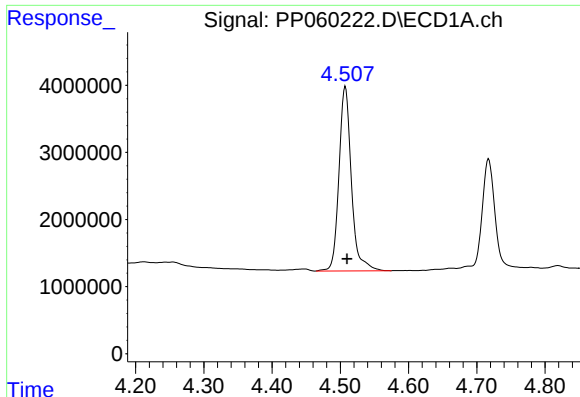


#1 Tetrachloro-m-xylene

R.T.: 4.507 min
Delta R.T.: -0.003 min
Response: 34779052
Conc: 16.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
DUP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2023
Supervised By :Ankita Jodhani 09/26/2023

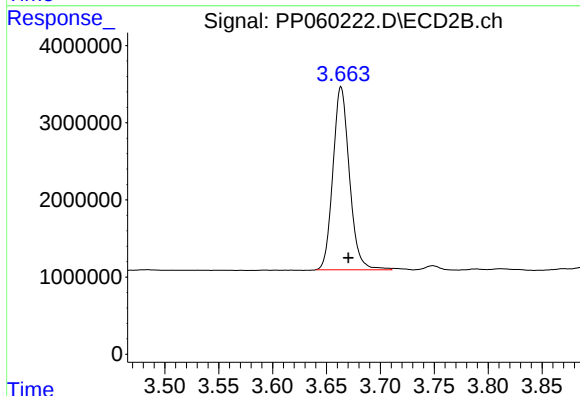


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.007 min
Response: 25282128
Conc: 15.52 ng/ml

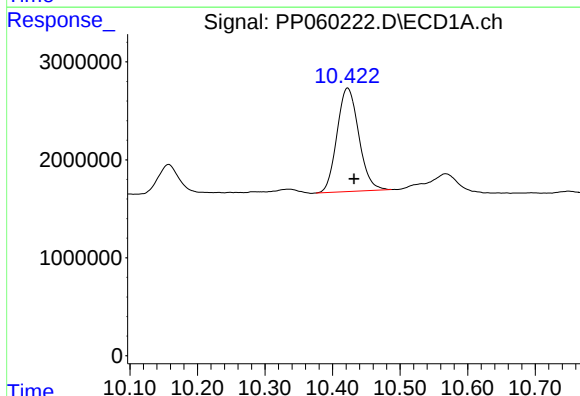

#2 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: -0.009 min
Response: 23688987
Conc: 15.53 ng/ml

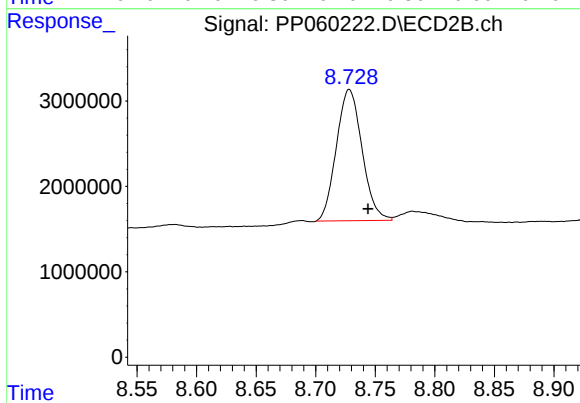

#2 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: -0.016 min
Response: 23118041
Conc: 15.27 ng/ml