Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092525\
Data File : PP075315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2025 10:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 08:15:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.654	3.798	25277161	97183761	19.318m	15.929
2)	SA Decachlor...	10.435	8.804	20472831	132.3E6	20.523	21.938
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092525\
Data File : PP075315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2025 10:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 08:15:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

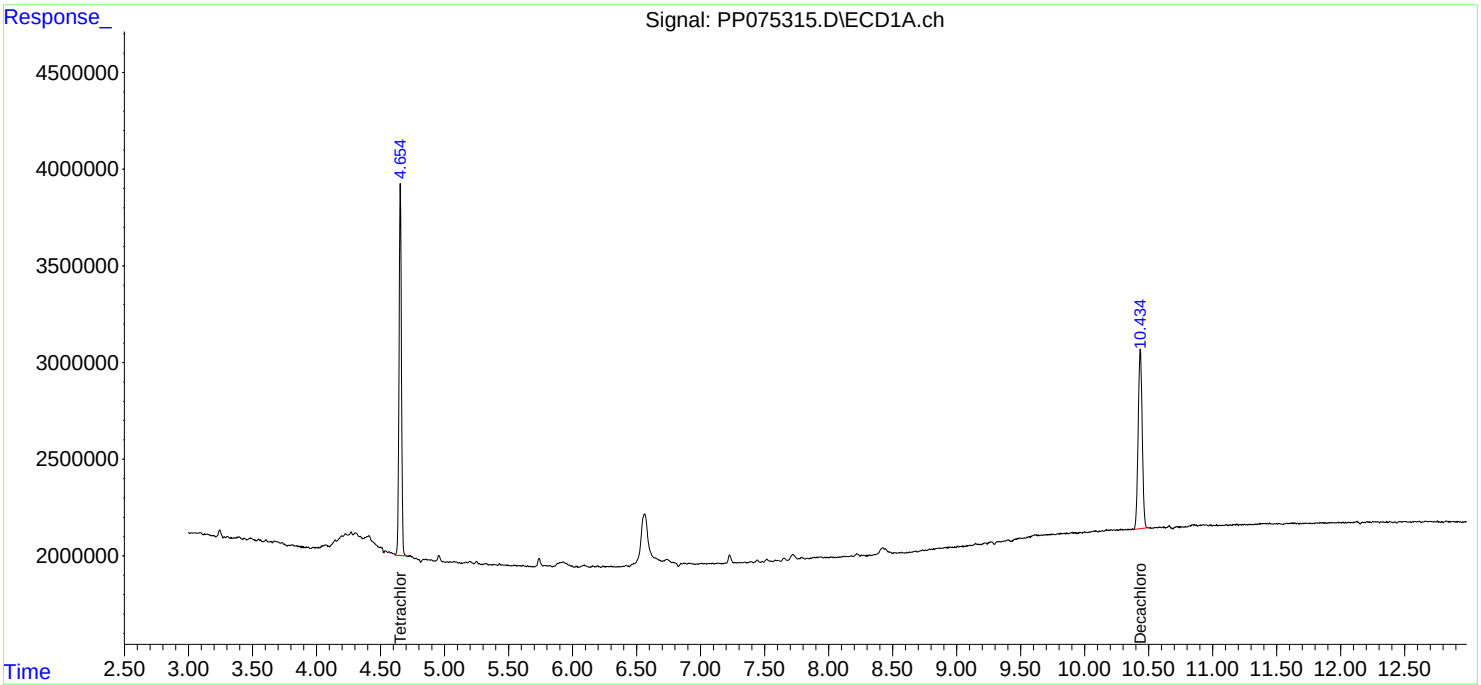

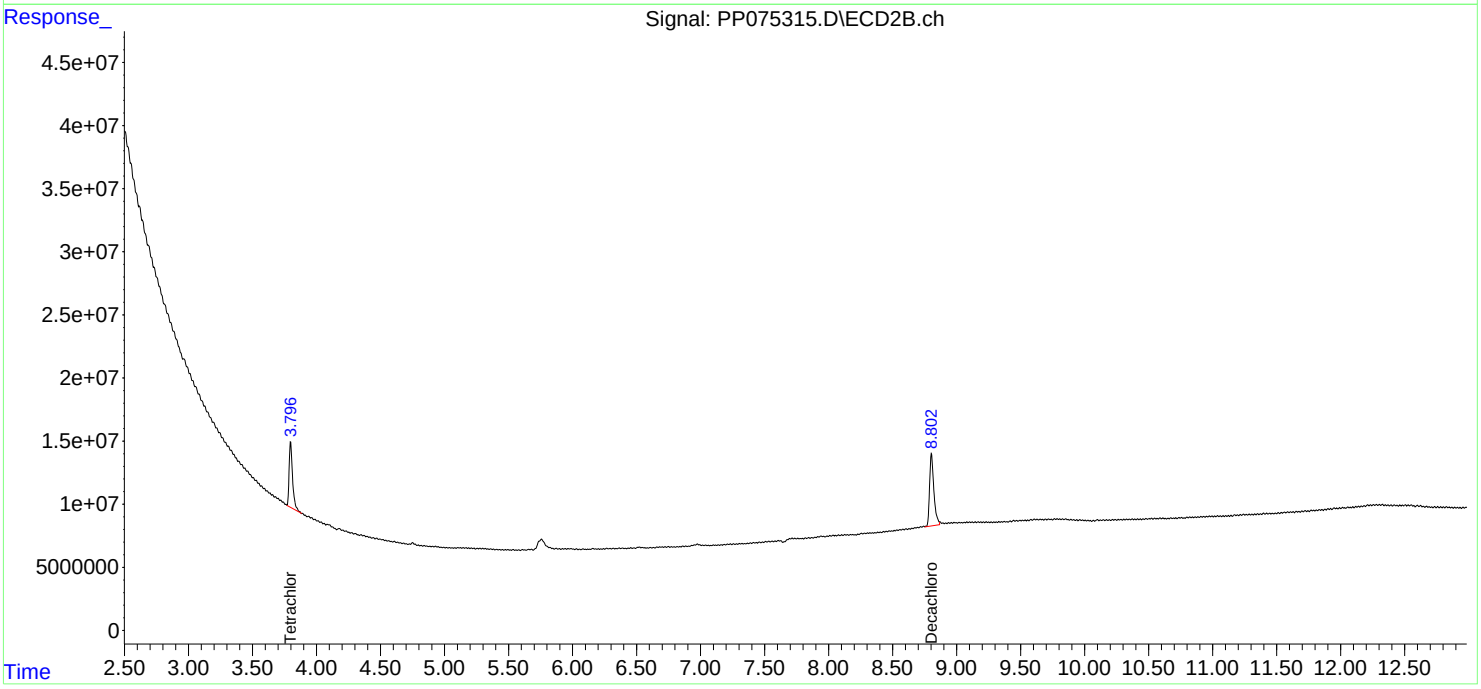

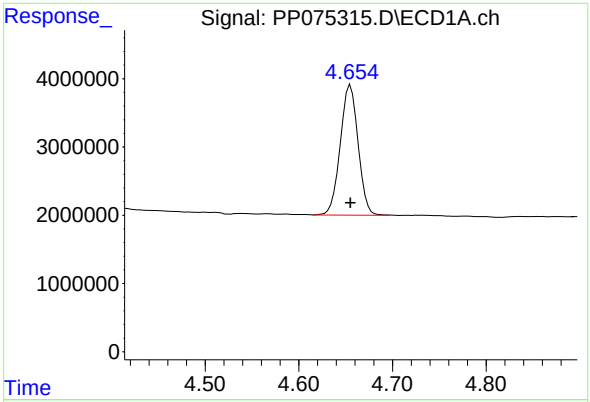

#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: -0.001 min
Response: 25277161
Conc: 19.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/26/2025
Supervised By :Sohil Jodhani 09/26/2025

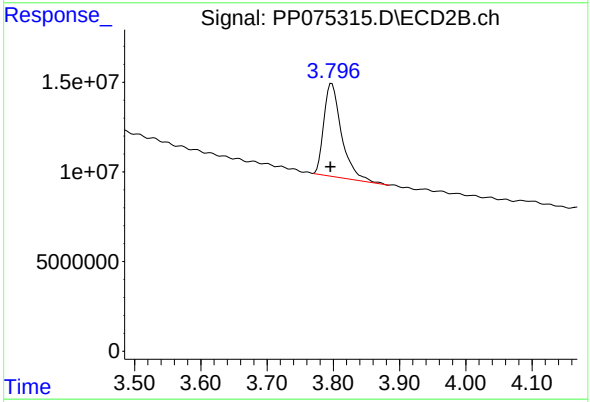

#1 Tetrachloro-m-xylene

R.T.: 3.798 min
Delta R.T.: 0.002 min
Response: 97183761
Conc: 15.93 ng/ml

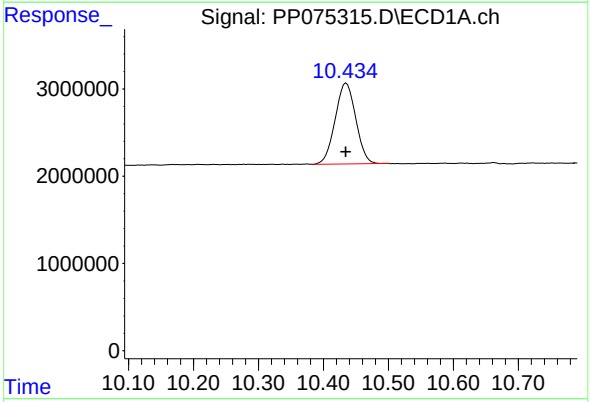

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.000 min
Response: 20472831
Conc: 20.52 ng/ml

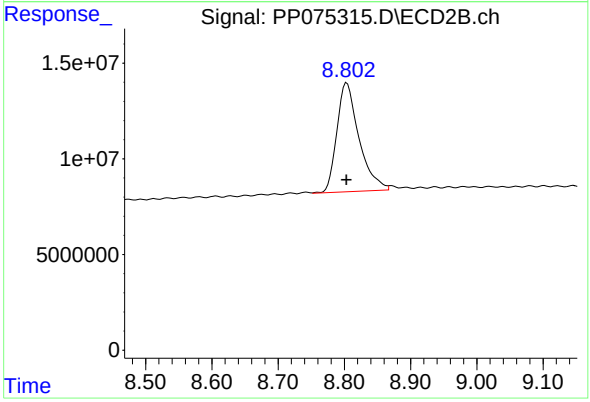

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: 0.000 min
Response: 132338596
Conc: 21.94 ng/ml