

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092622\
 Data File : PP051664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 20:42
 Operator : YP\AJ
 Sample : N4818-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-092022-AP-02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/27/2022
 Supervised By :Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 06:23:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.681	41305370	34502659	23.244	22.841
2) SA Decachlor...	10.255	8.781	38253166	20963811	24.752m	17.496m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092622\
Data File : PP051664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 20:42
Operator : YP\AJ
Sample : N4818-02
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-092022-AP-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2022
Supervised By :Ankita Jodhani 09/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 06:23:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

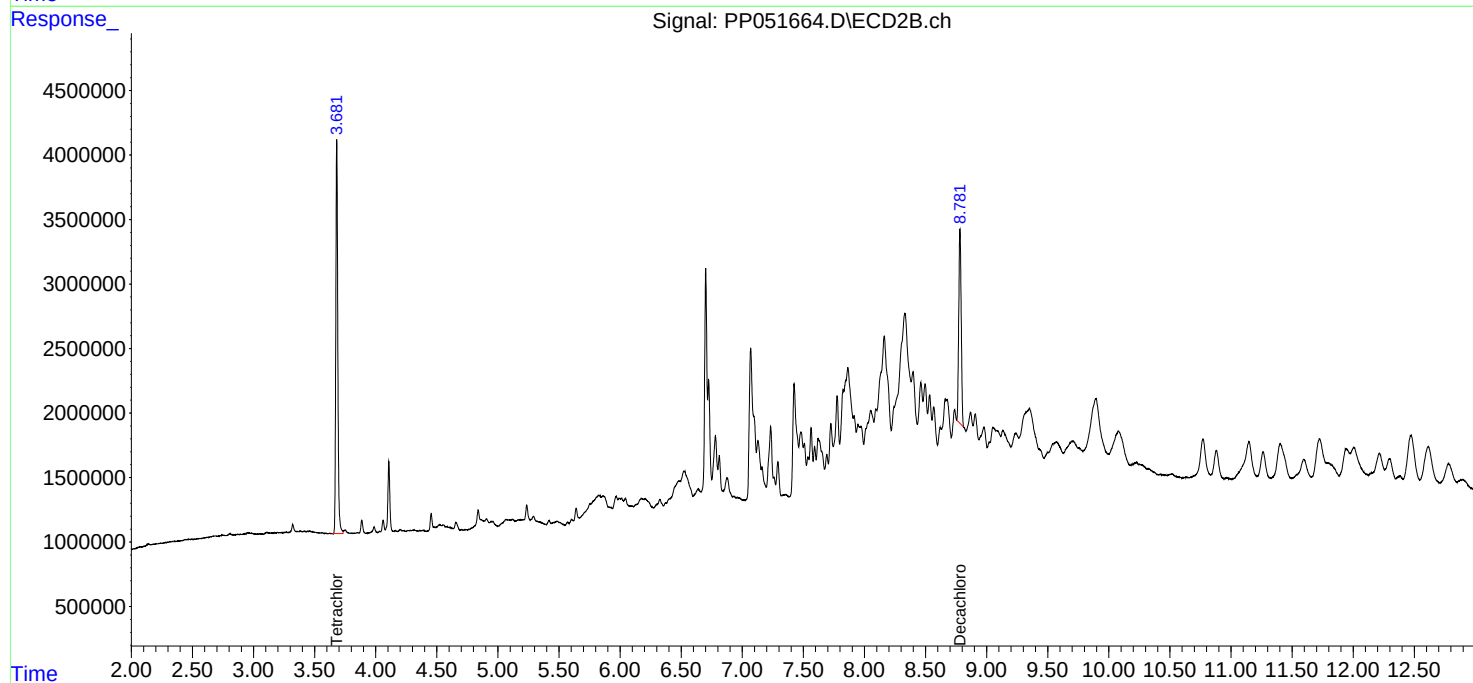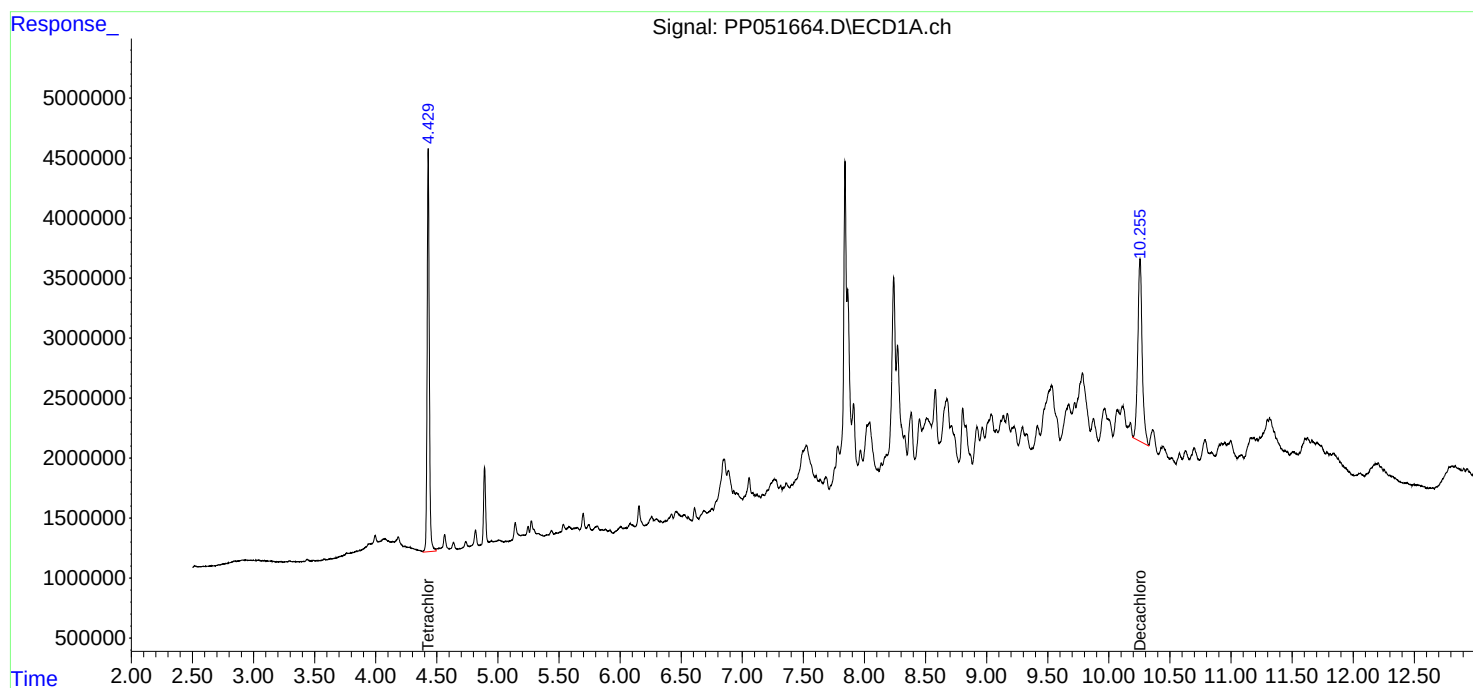

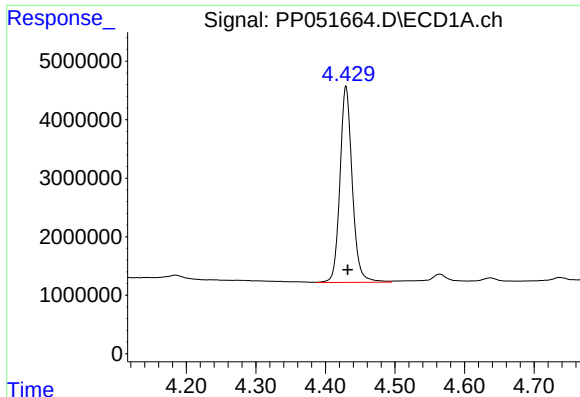


#1 Tetrachloro-m-xylene

R.T.: 4.430 min
Delta R.T.: -0.002 min
Response: 41305370
Conc: 23.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-092022-AP-02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/27/2022
Supervised By :Ankita Jodhani 09/27/2022

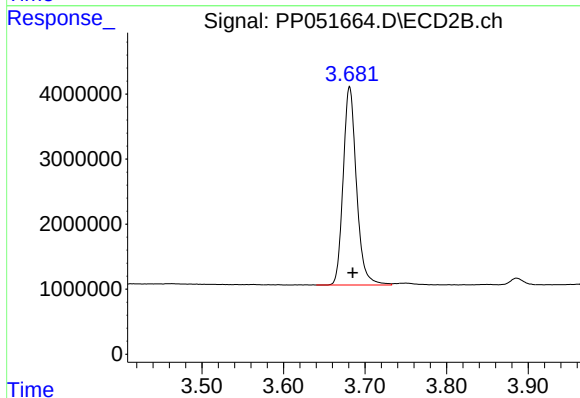


#1 Tetrachloro-m-xylene

R.T.: 3.681 min
Delta R.T.: -0.004 min
Response: 34502659
Conc: 22.84 ng/ml

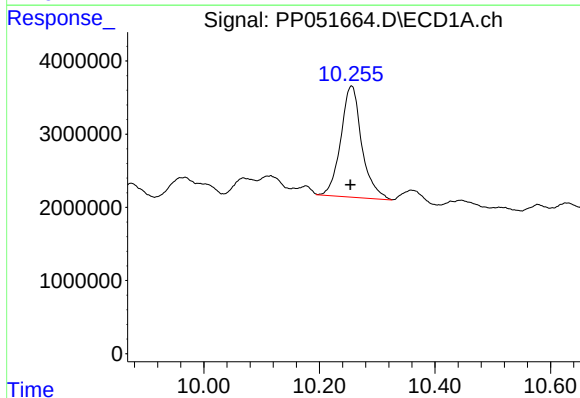

#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: 0.001 min
Response: 38253166
Conc: 24.75 ng/ml m

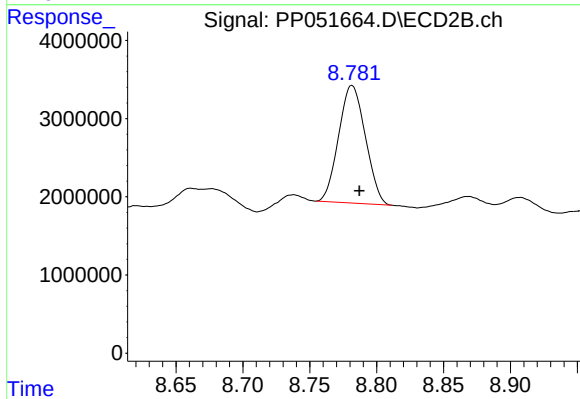

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: -0.006 min
Response: 20963811
Conc: 17.50 ng/ml m