

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092622\
 Data File : PP051666.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2022 21:15
 Operator : YP\AJ
 Sample : N4818-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-092022-AP-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 06:26:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 14:37:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.430	3.682	37647993	32784707	21.186	21.704
2) SA Decachlor...	10.256	8.782	28873724	23066360	18.683	19.251

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092622\
Data File : PP051666.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2022 21:15
Operator : YP\AJ
Sample : N4818-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-092022-AP-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 06:26:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 14:37:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

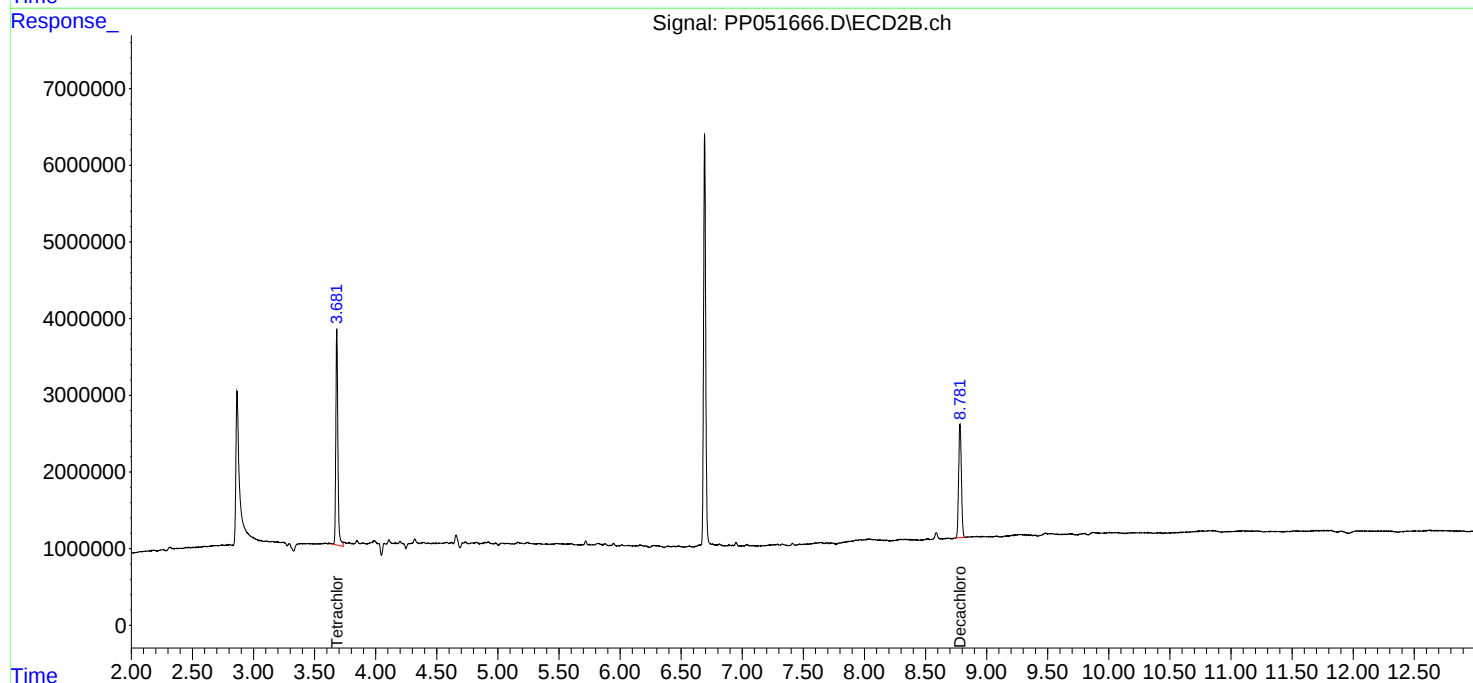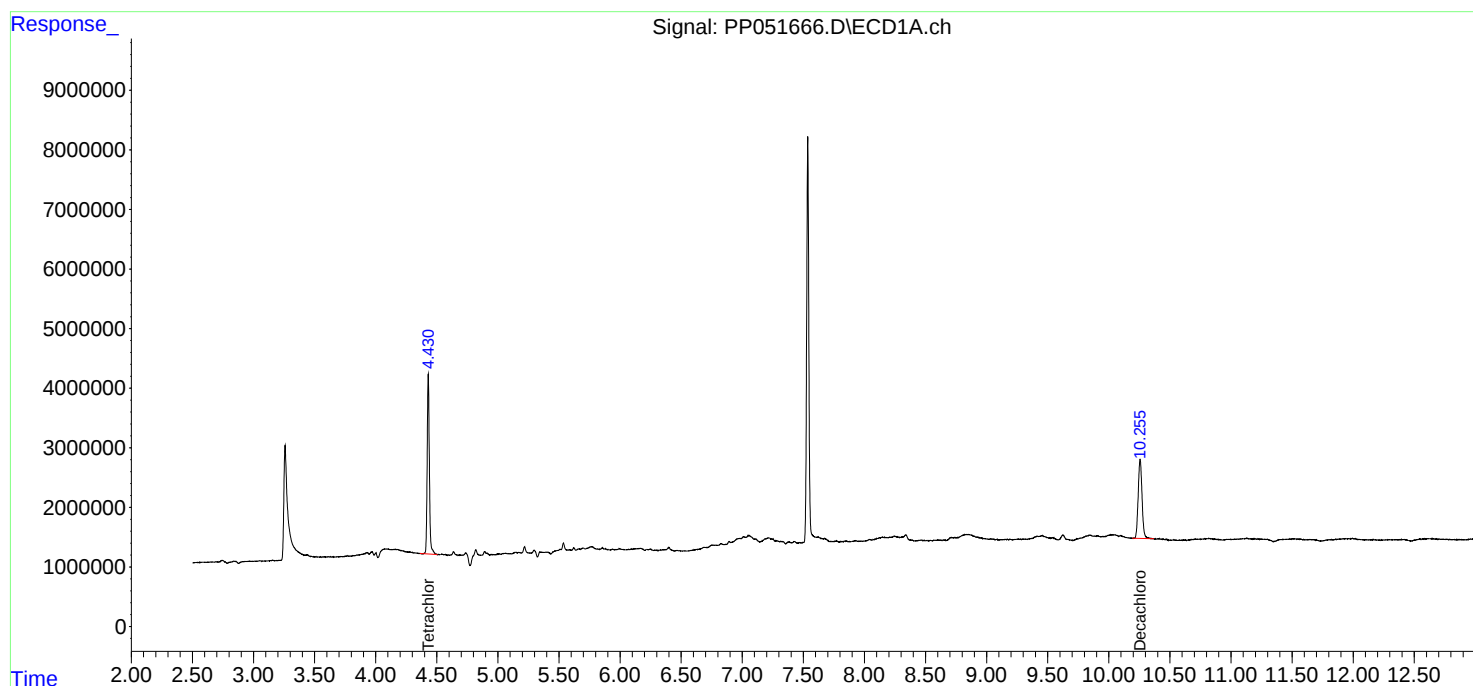


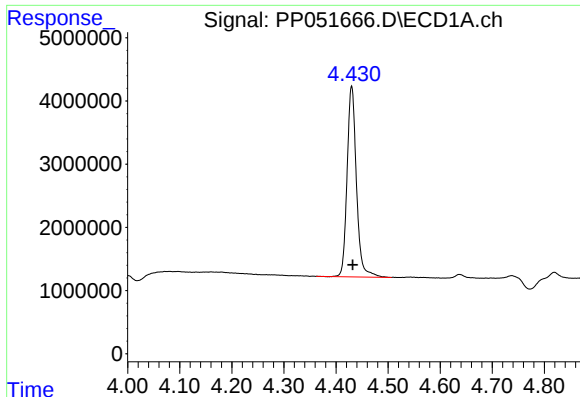

#1 Tetrachloro-m-xylene


R.T.: 4.430 min
Delta R.T.: -0.002 min
Response: 37647993
Conc: 21.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-092022-AP-04

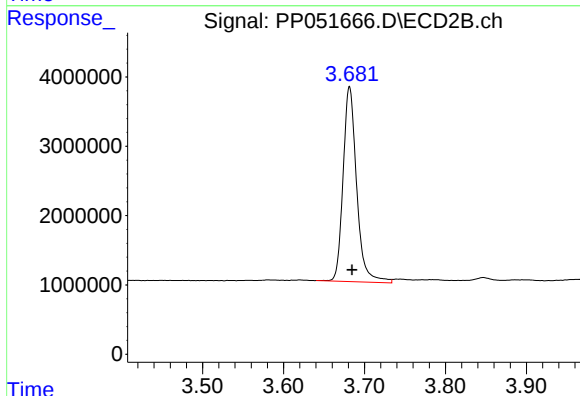


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.003 min
Response: 32784707
Conc: 21.70 ng/ml

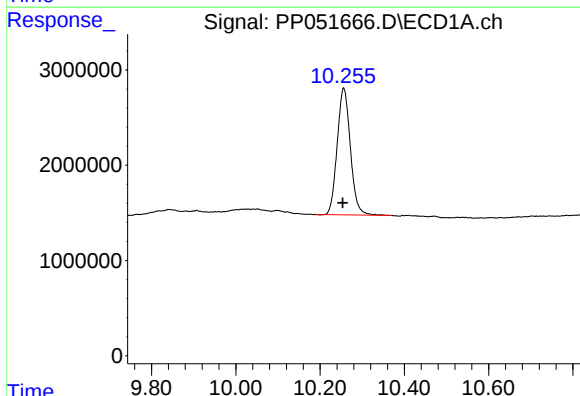

#2 Decachlorobiphenyl

R.T.: 10.256 min
Delta R.T.: 0.002 min
Response: 28873724
Conc: 18.68 ng/ml

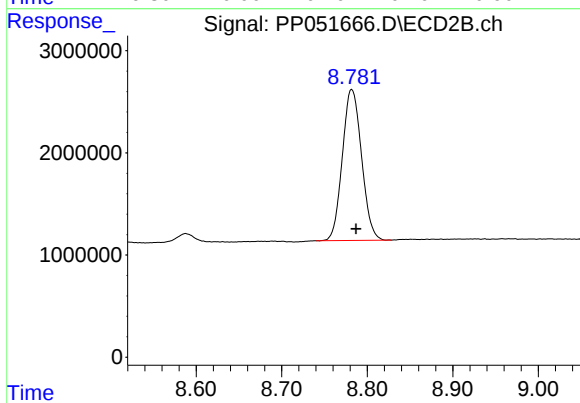

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 23066360
Conc: 19.25 ng/ml