

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
 Data File : PP075372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2025 00:17
 Operator : YP\AJ
 Sample : PB169860BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB169860BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2025
 Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 02:06:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.665	3.797	24298889	118.3E6	18.570m	19.388
2) SA Decachlor...	10.460	8.809	18934534	132.1E6	18.981m	21.904

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
Data File : PP075372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2025 00:17
Operator : YP\AJ
Sample : PB169860BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB169860BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2025
Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 02:06:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

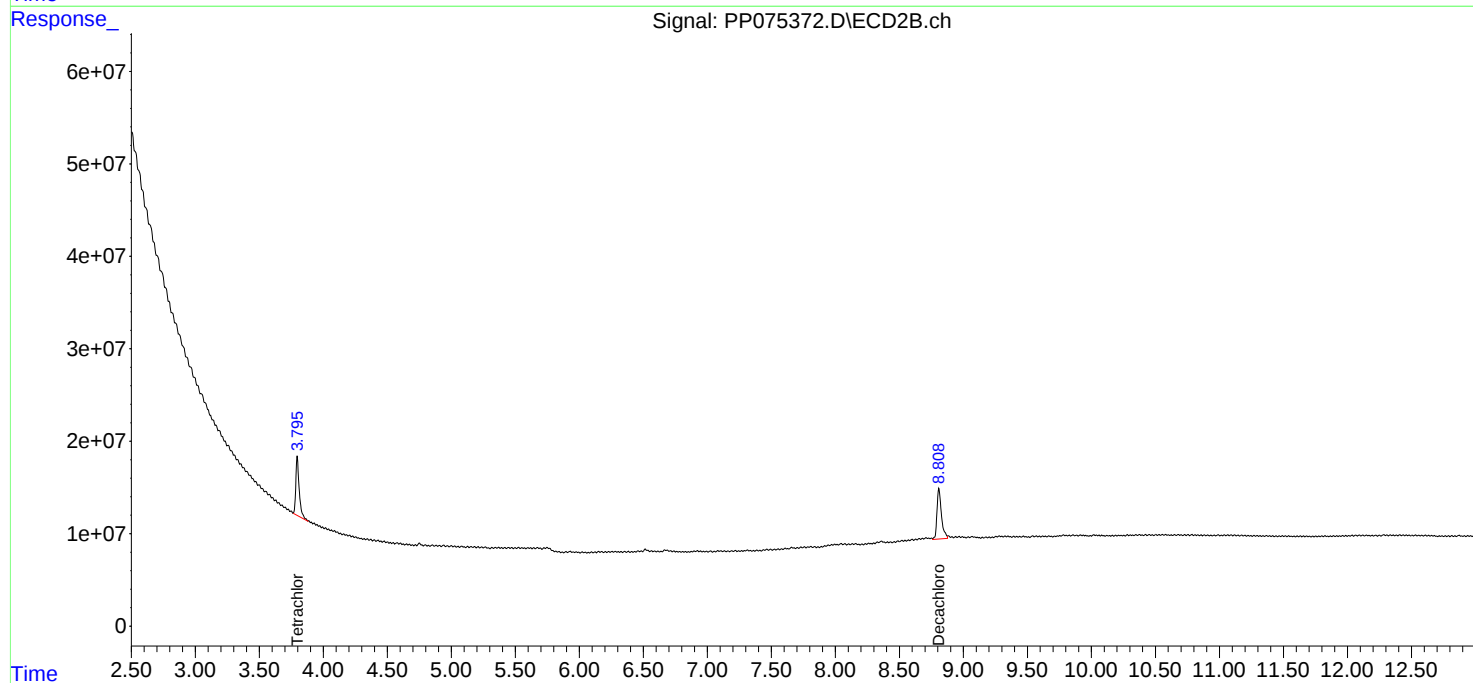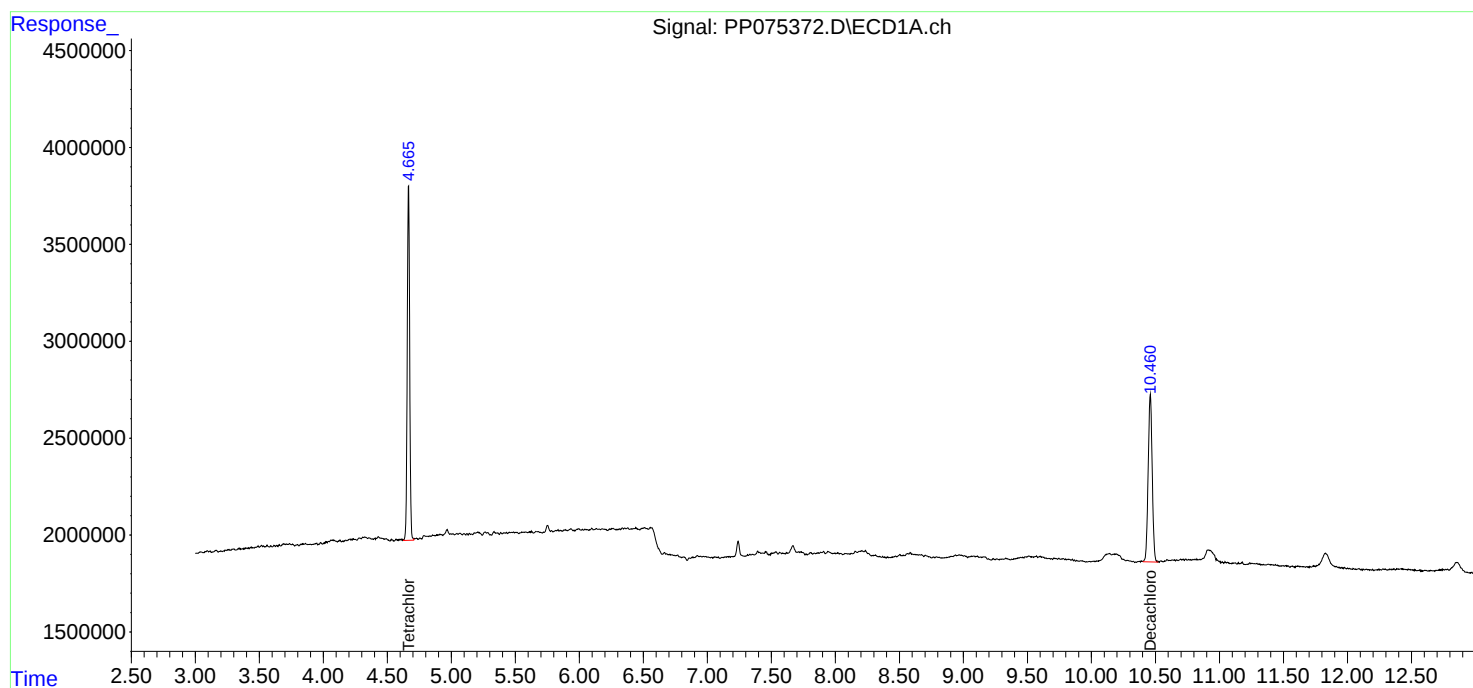

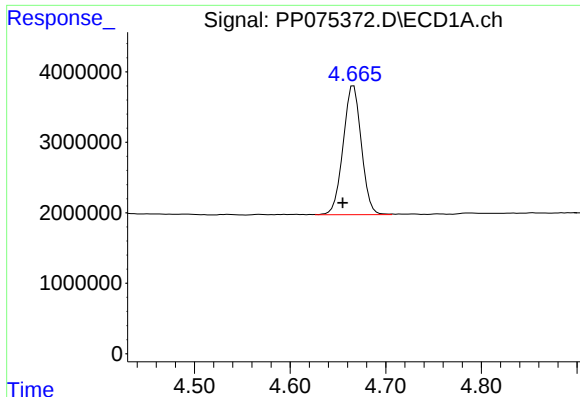

#1 Tetrachloro-m-xylene

R.T.: 4.665 min
Delta R.T.: 0.010 min
Response: 24298889
Conc: 18.57 ng/ml

Instrument :

ECD_P

ClientSampleId :


PB169860BL

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 09/29/2025

Supervised By :mohammad ahmed 09/30/2025

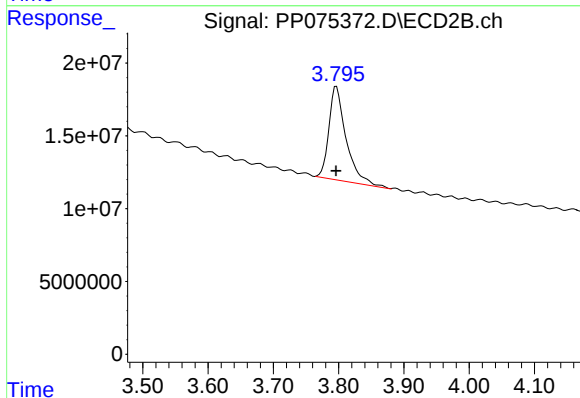


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: 0.000 min
Response: 118285738
Conc: 19.39 ng/ml

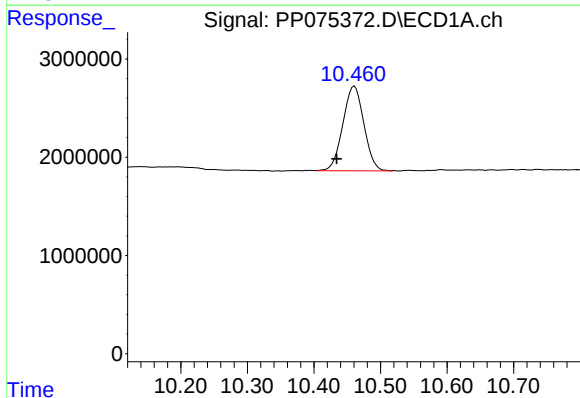

#2 Decachlorobiphenyl

R.T.: 10.460 min
Delta R.T.: 0.025 min
Response: 18934534
Conc: 18.98 ng/ml m

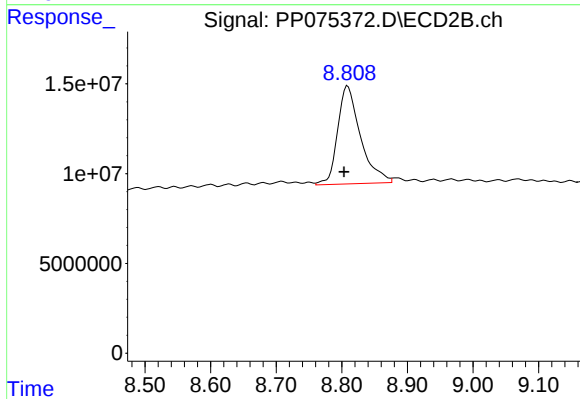

#2 Decachlorobiphenyl

R.T.: 8.809 min
Delta R.T.: 0.005 min
Response: 132138441
Conc: 21.90 ng/ml