

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
 Data File : PP075376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2025 01:22
 Operator : YP\AJ
 Sample : Q3196-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-FMC-9-24-25-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 03:21:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.657	3.791	32463586	1036.2E6	24.810	169.852 #
2) SA Decachlor...	10.438	8.801	12399599	76146535	12.430	12.623

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
Data File : PP075376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2025 01:22
Operator : YP\AJ
Sample : Q3196-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TOTE-FMC-9-24-25-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 03:21:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

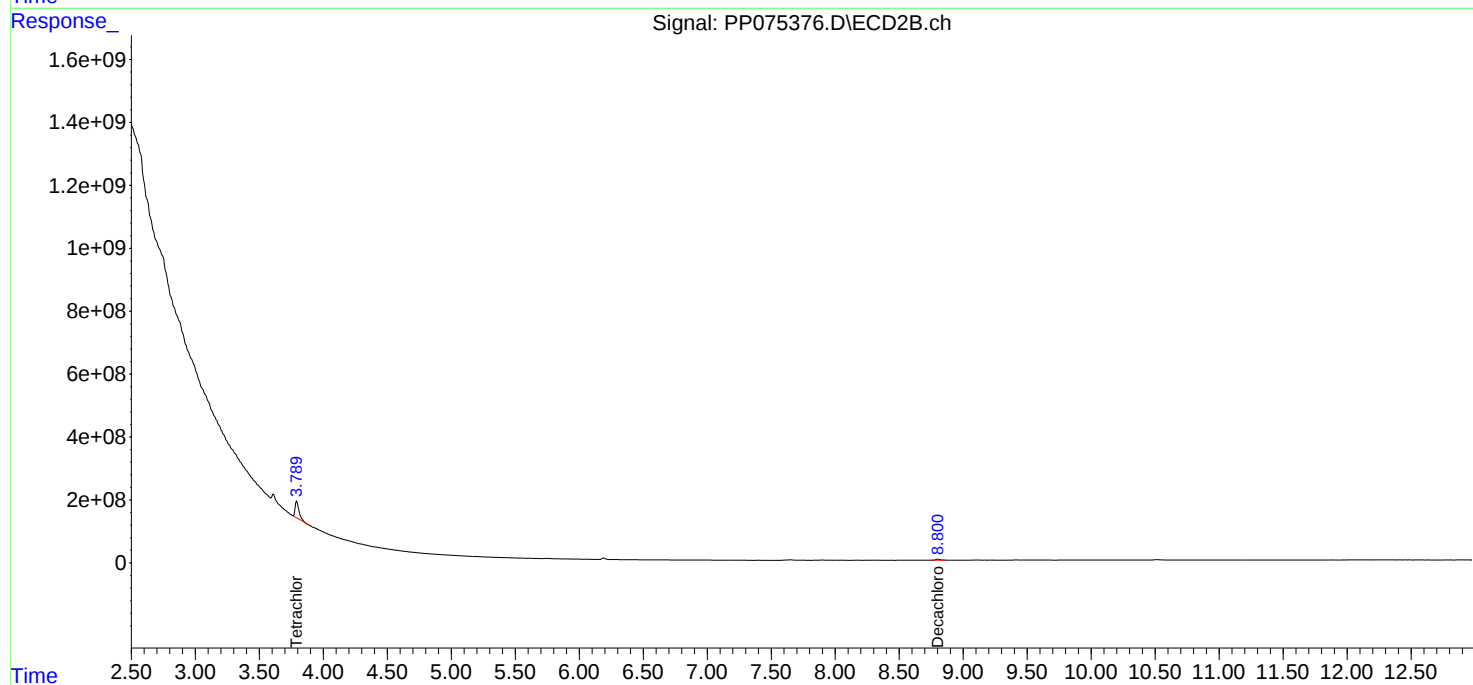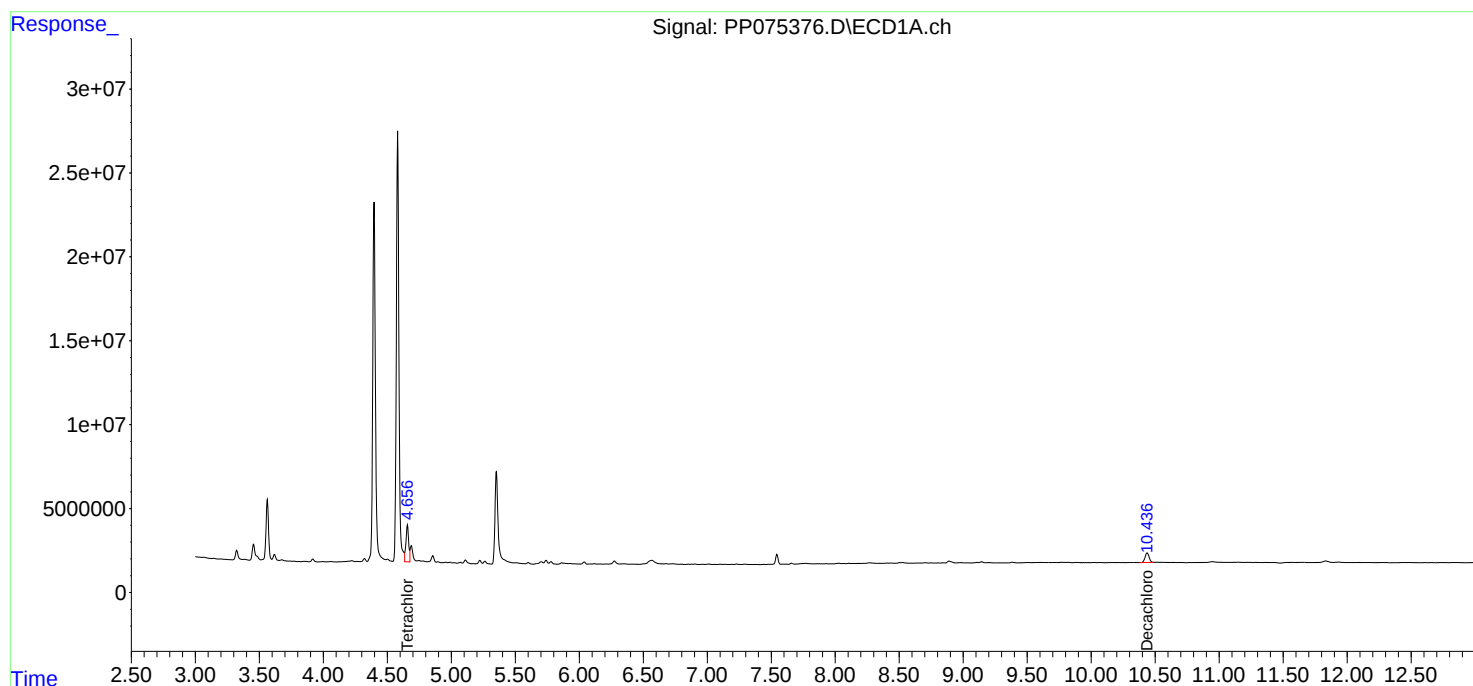


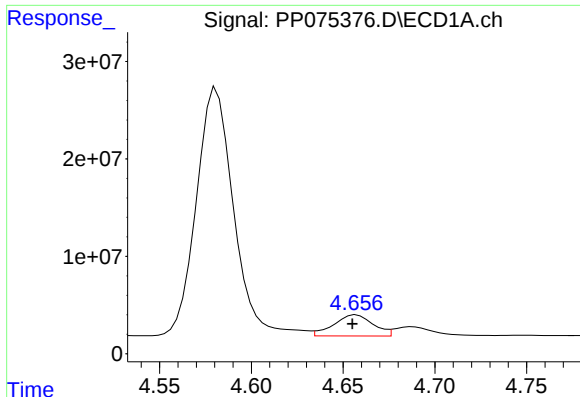

#1 Tetrachloro-m-xylene


R.T.: 4.657 min
Delta R.T.: 0.002 min
Response: 32463586
Conc: 24.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE-FMC-9-24-25-2

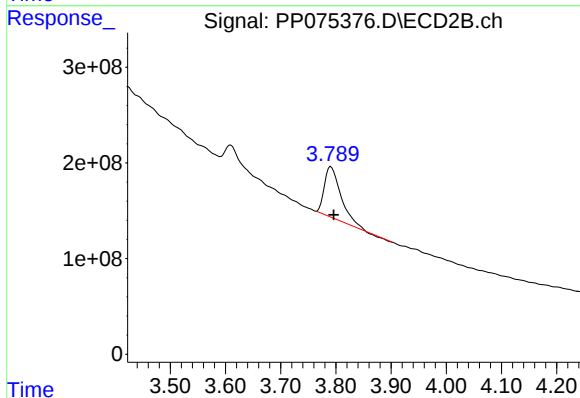


#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: -0.005 min
Response: 1036246361
Conc: 169.85 ng/ml

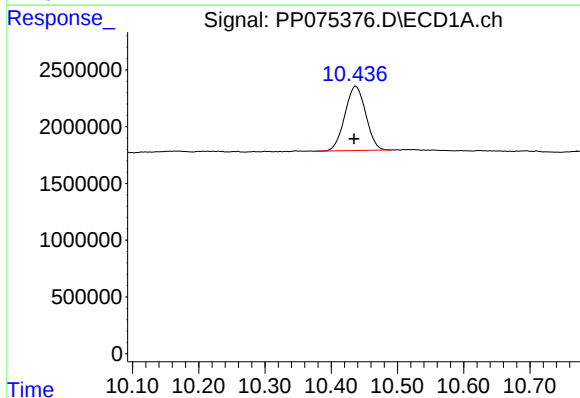

#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.003 min
Response: 12399599
Conc: 12.43 ng/ml

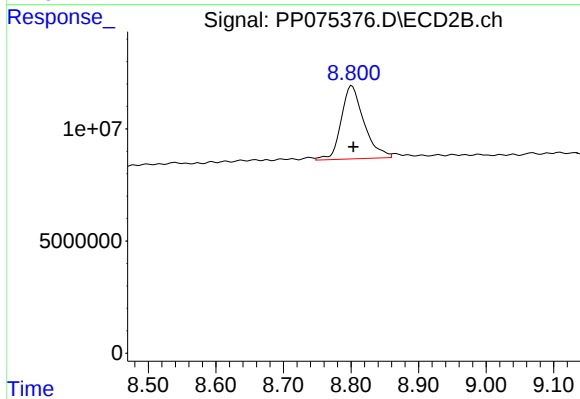

#2 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: -0.002 min
Response: 76146535
Conc: 12.62 ng/ml