

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
 Data File : PP075381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2025 02:43
 Operator : YP\AJ
 Sample : Q3198-04 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2308-0066-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2025
 Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 03:35:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 24 10:55:35 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.655	3.796	2528858	8072374	1.933m	1.323 #
2) SA Decachlor...	10.436	8.802	1672307	10345922	1.676m	1.715

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092625\
Data File : PP075381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2025 02:43
Operator : YP\AJ
Sample : Q3198-04 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2308-0066-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2025
Supervised By :mohammad ahmed 09/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 03:35:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092325.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 24 10:55:35 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

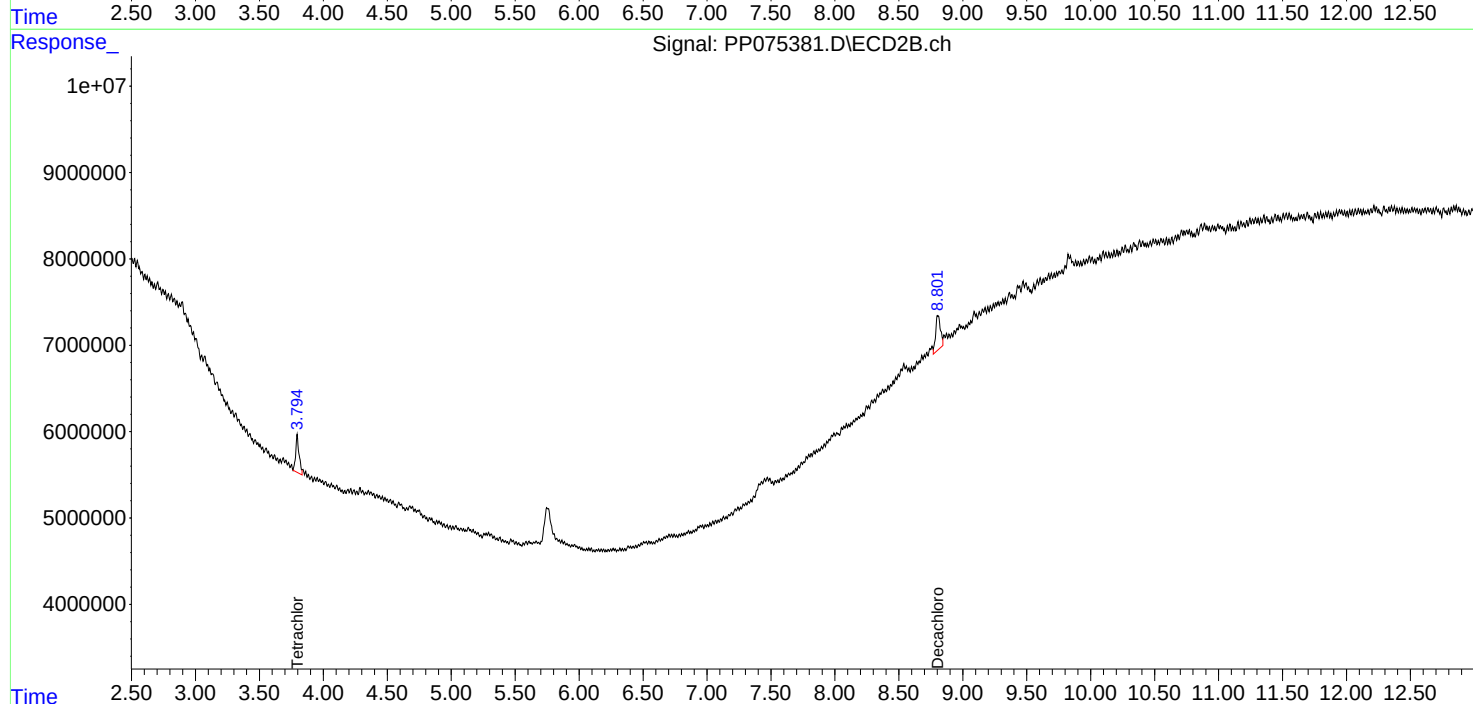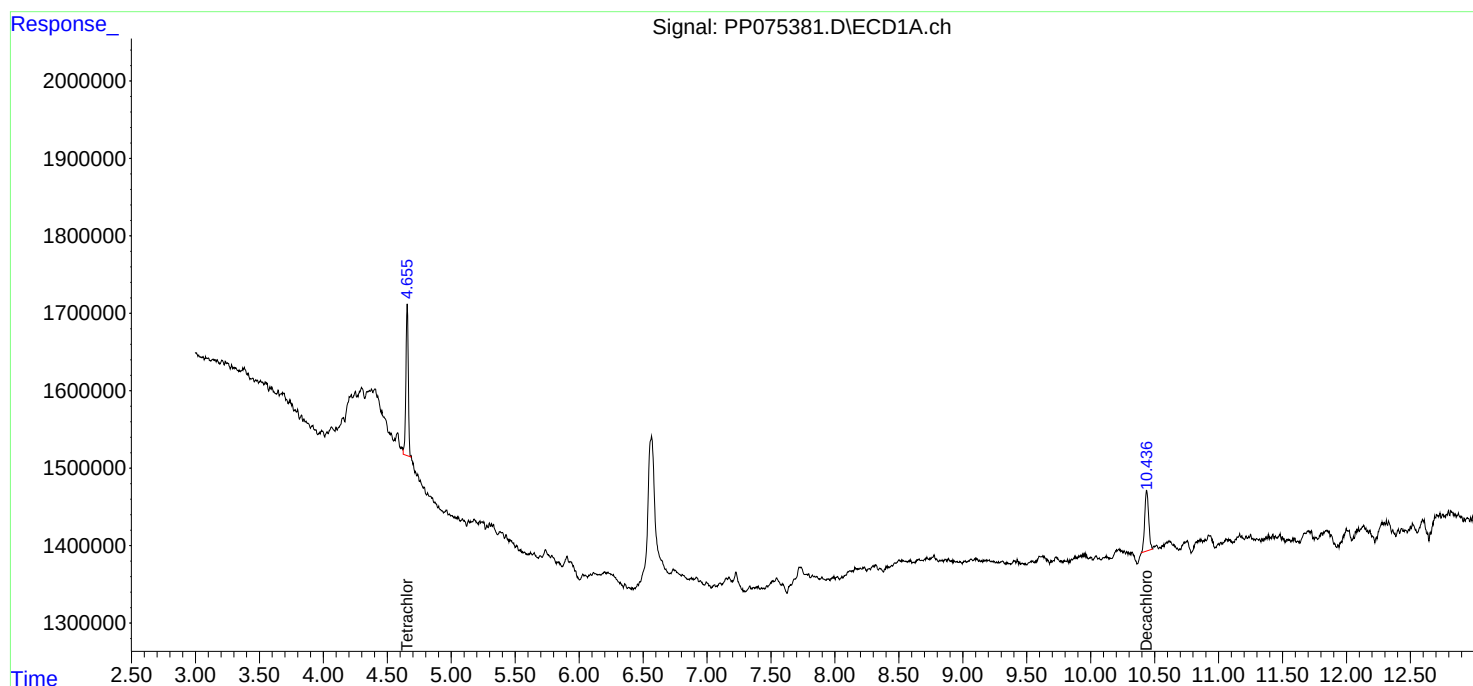

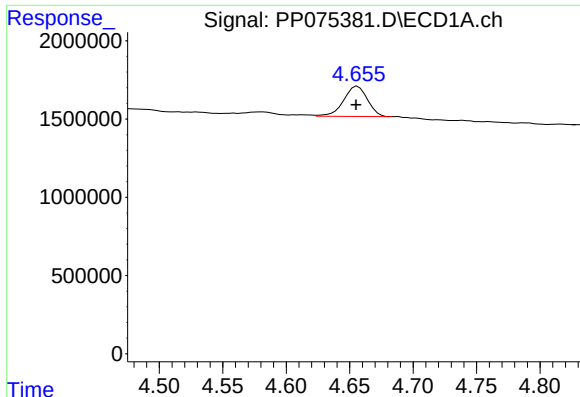


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 2528858
Conc: 1.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2308-0066-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2025
Supervised By :mohammad ahmed 09/30/2025

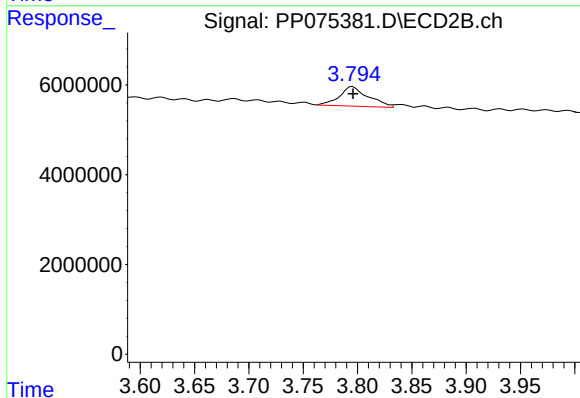


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: 0.000 min
Response: 8072374
Conc: 1.32 ng/ml

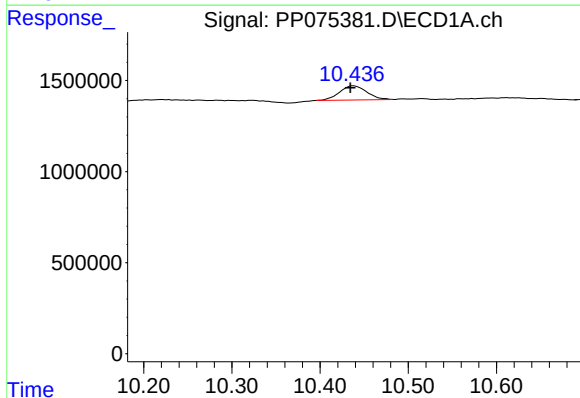

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.002 min
Response: 1672307
Conc: 1.68 ng/ml m

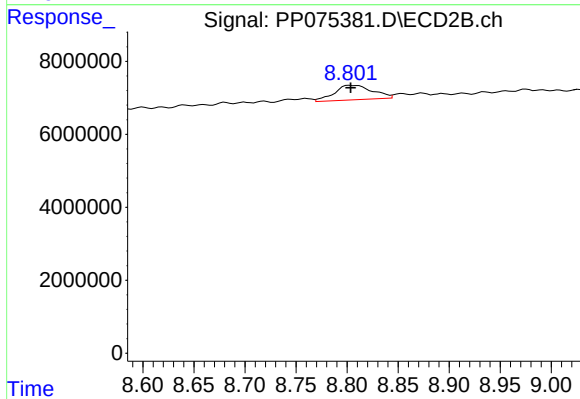

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 10345922
Conc: 1.72 ng/ml