

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092721\
 Data File : PP039552.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2021 17:01
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:26:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.907	3.997	738763	390785	23.336	23.983
2)	SA Decachlor...	10.930	9.337	505209	548873	23.288	25.117
Target Compounds							
24)	L5 AR-1248-4	7.178	0.000	1367	0	1.259	N.D. #
26)	L6 AR-1254-1	7.148	0.000	54875	0	50.274	N.D. #
28)	L6 AR-1254-3	7.769f	0.000	19122	0	11.492	N.D. #
29)	L6 AR-1254-4	8.056	0.000	4402	0	3.603	N.D. #
32)	L7 AR-1260-2	8.209f	0.000	10069	0	7.273	N.D. #
34)	L7 AR-1260-4	8.767f	0.000	2825	0	2.834	N.D. #
38)	L8 AR-1262-3	0.000	8.222f	0	40117	N.D.	39.470 #
41)	L9 AR-1268-1	0.000	8.222f	0	40117	N.D.	13.758 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092721\
Data File : PP039552.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2021 17:01
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:26:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

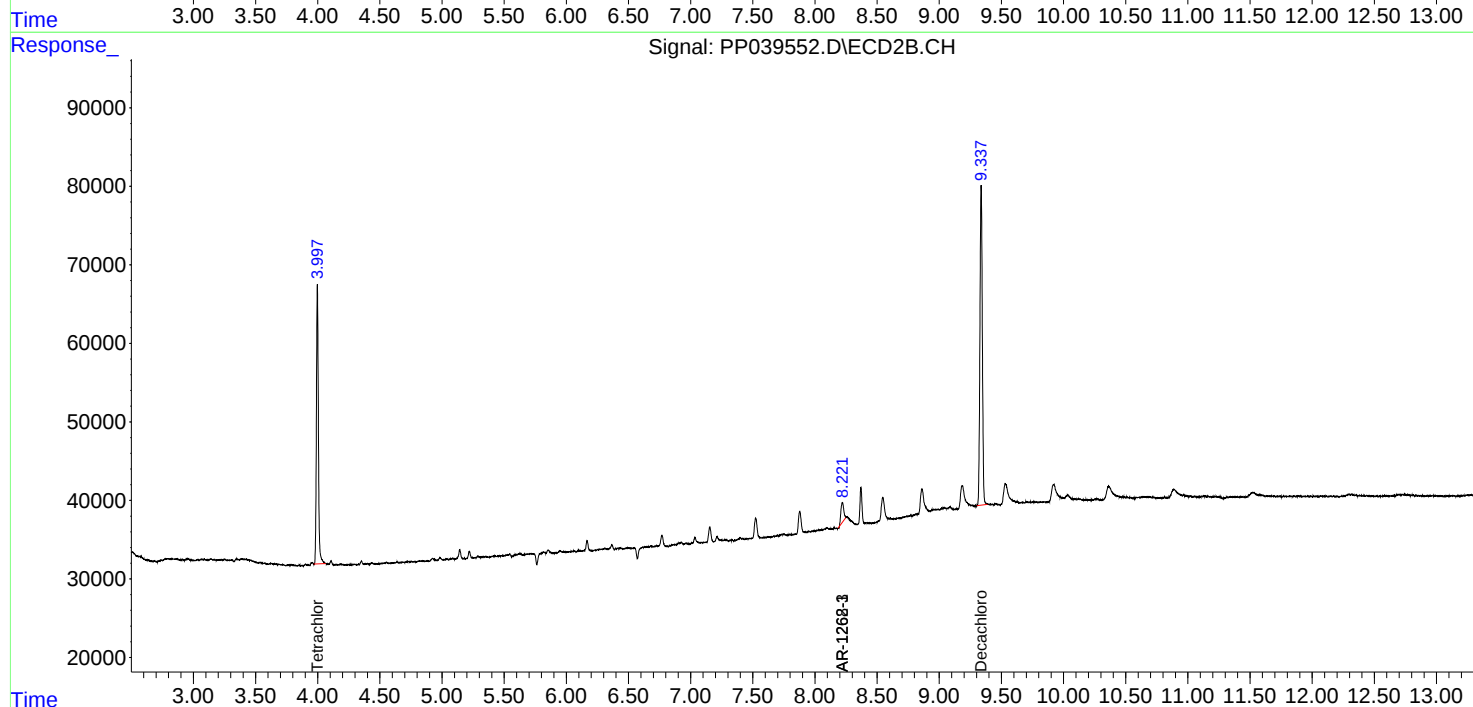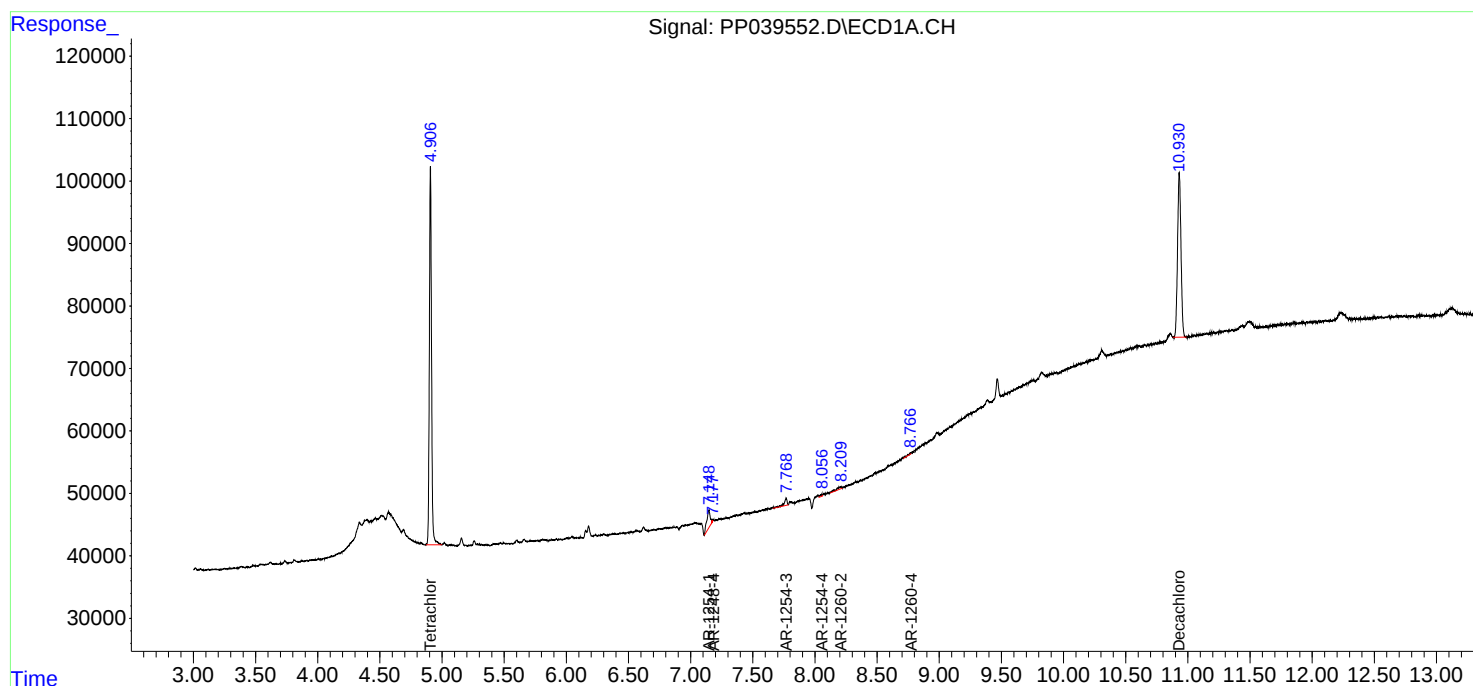


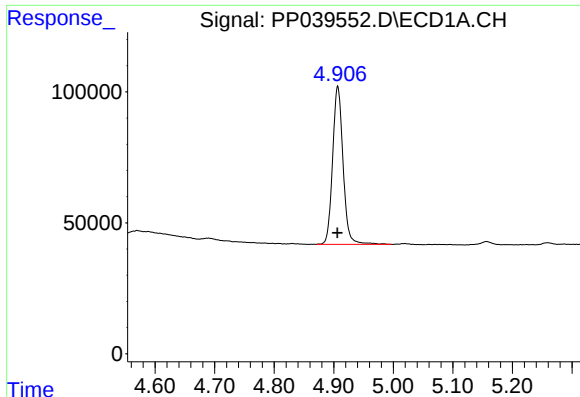

#1 Tetrachloro-m-xylene


R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 738763
Conc: 23.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

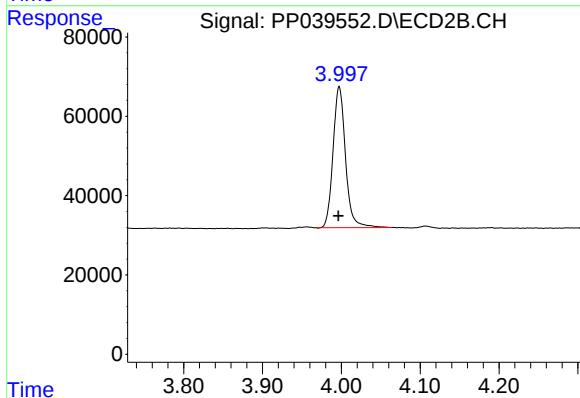


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: 0.001 min
Response: 390785
Conc: 23.98 ng/ml

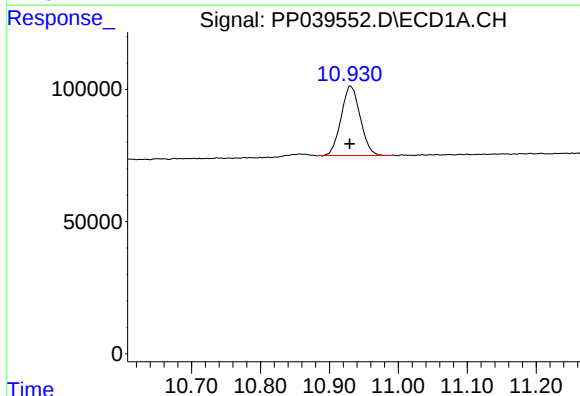


#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 505209
Conc: 23.29 ng/ml

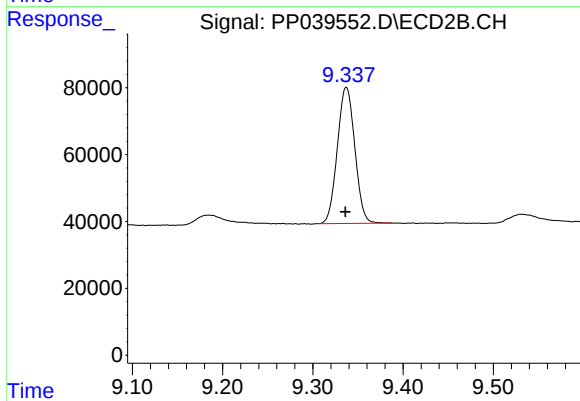

#2 Decachlorobiphenyl


R.T.: 9.337 min
Delta R.T.: 0.000 min
Response: 548873
Conc: 25.12 ng/ml

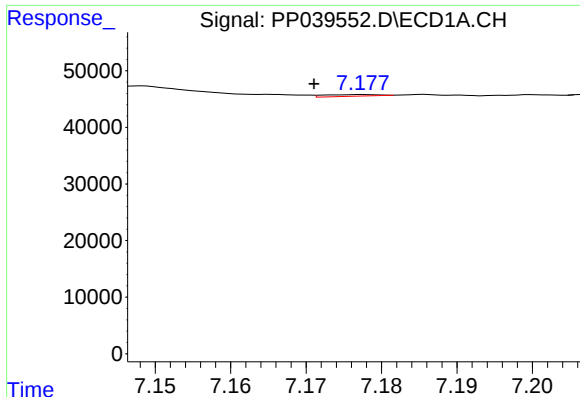

#24 AR-1248-4


R.T.: 7.178 min
Delta R.T.: 0.007 min
Response: 1367
Conc: 1.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

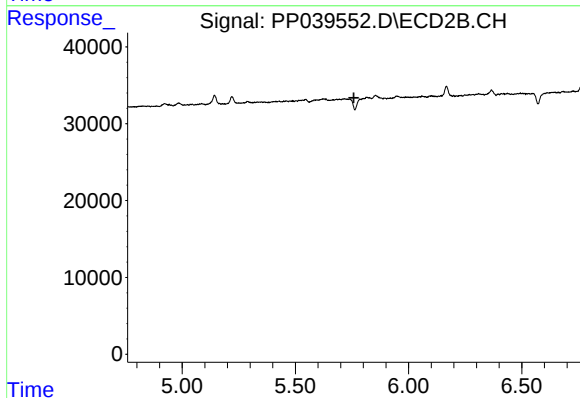


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.758 min
Response: 0
Conc: N.D.

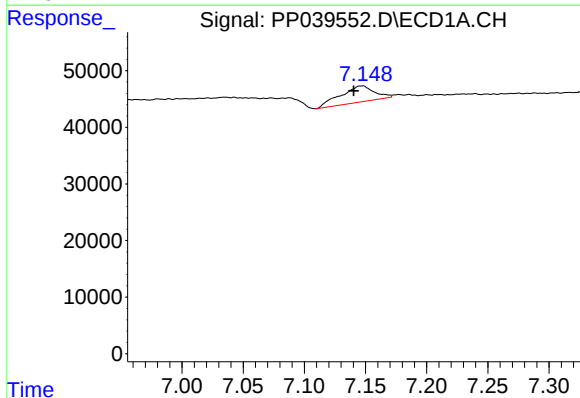


#26 AR-1254-1

R.T.: 7.148 min
Delta R.T.: 0.008 min
Response: 54875
Conc: 50.27 ng/ml

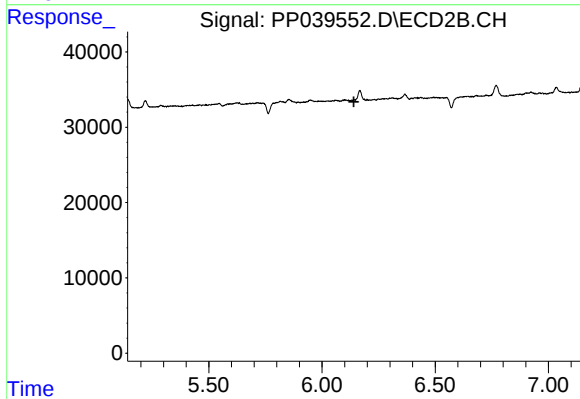

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

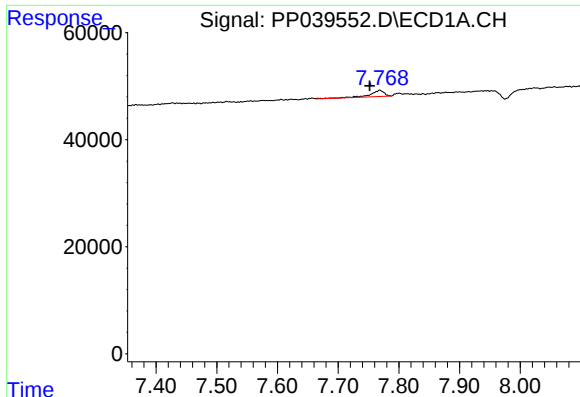

#28 AR-1254-3


R.T.: 7.769 min
Delta R.T.: 0.016 min
Response: 19122
Conc: 11.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

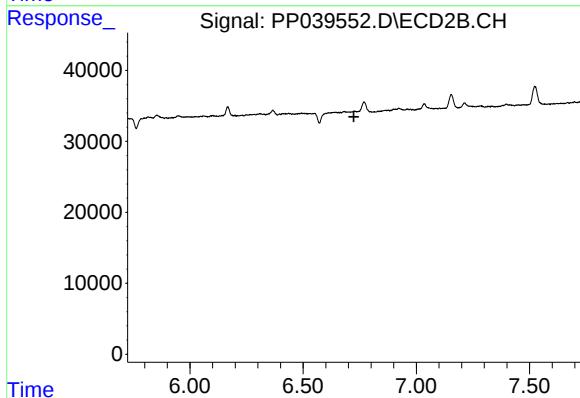


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

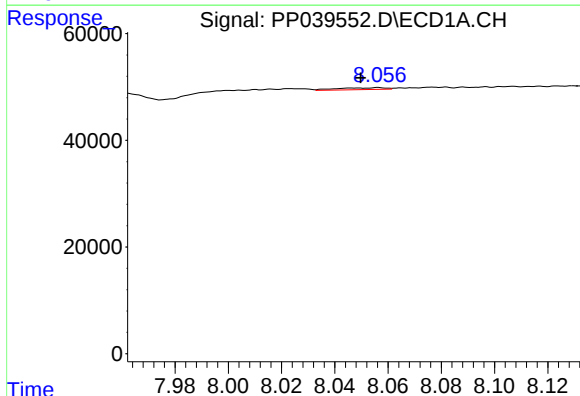


#29 AR-1254-4

R.T.: 8.056 min
Delta R.T.: 0.007 min
Response: 4402
Conc: 3.60 ng/ml

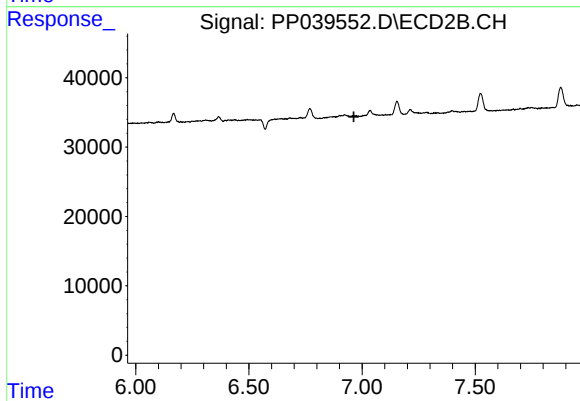

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

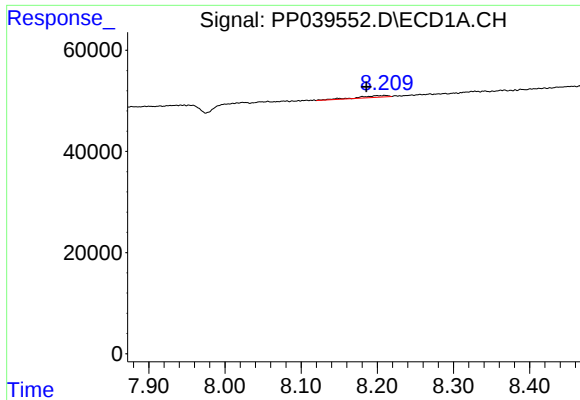

#32 AR-1260-2


R.T.: 8.209 min
Delta R.T.: 0.024 min
Response: 10069
Conc: 7.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

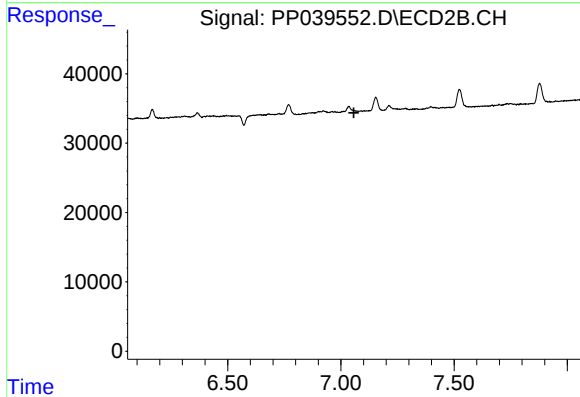


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

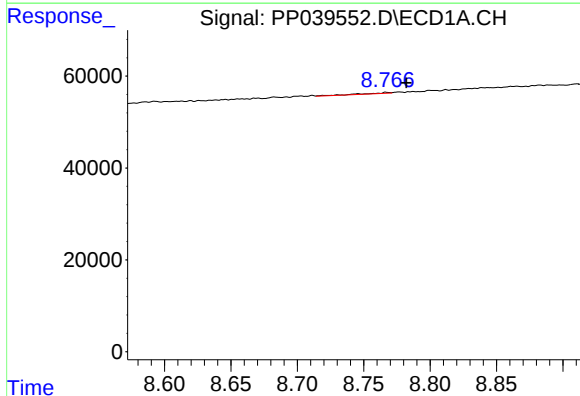


#34 AR-1260-4

R.T.: 8.767 min
Delta R.T.: -0.016 min
Response: 2825
Conc: 2.83 ng/ml

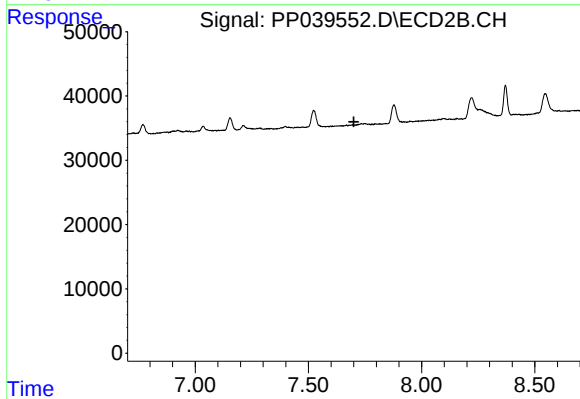

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

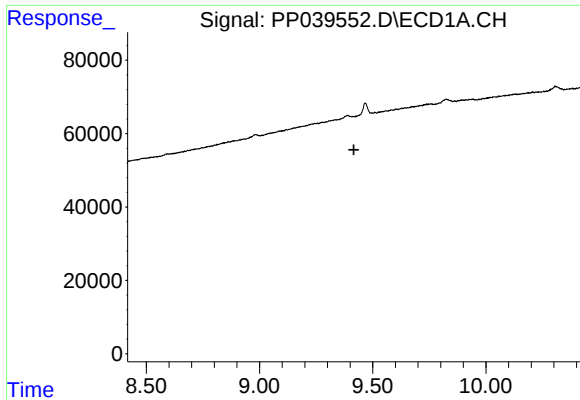

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

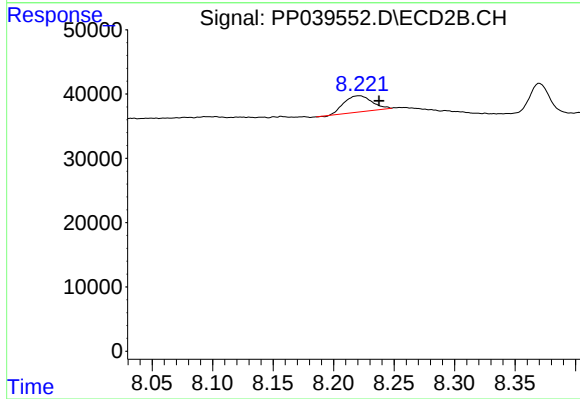


#38 AR-1262-3

R.T.: 8.222 min
Delta R.T.: -0.016 min
Response: 40117
Conc: 39.47 ng/ml

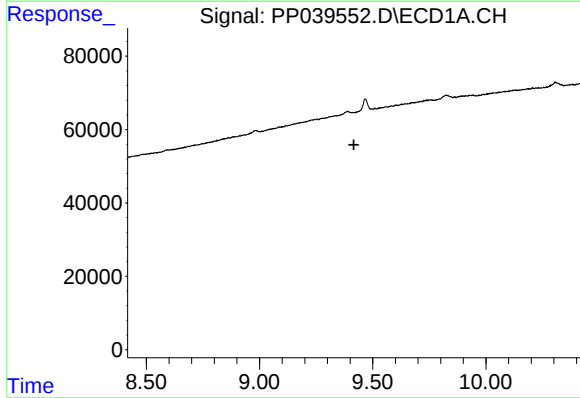

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

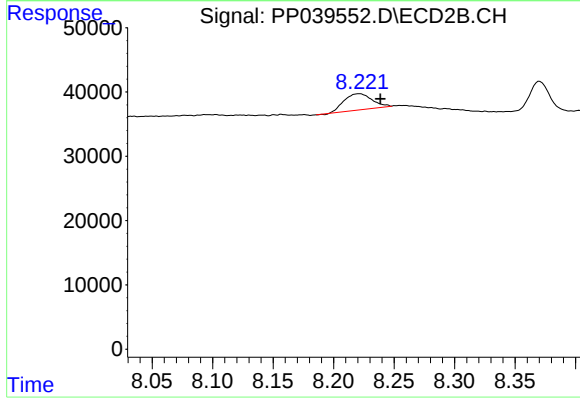

#41 AR-1268-1

R.T.: 8.222 min
Delta R.T.: -0.017 min
Response: 40117
Conc: 13.76 ng/ml