

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092721\
 Data File : PP039566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Sep 2021 21:24
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 01:35:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.907	3.998	744528	391399	23.518	24.021
2)	SA Decachlor...	10.931	9.337	511708	567828	23.588	25.985
Target Compounds							
20)	L4 AR-1242-5	0.000	6.168f	0	18447	N.D.	34.762 #
24)	L5 AR-1248-4	7.147f	0.000	59791	0	55.078	N.D. #
25)	L5 AR-1248-5	0.000	6.168f	0	18447	N.D.	26.170 #
26)	L6 AR-1254-1	7.147	6.168f	59791	18447	54.778	17.718 #
29)	L6 AR-1254-4	8.051	0.000	25370	0	20.769	N.D. #
34)	L7 AR-1260-4	8.783	0.000	4381	0	4.395	N.D. #
38)	L8 AR-1262-3	0.000	8.220f	0	22998	N.D.	22.627 #
41)	L9 AR-1268-1	0.000	8.220f	0	22998	N.D.	7.887 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092721\
Data File : PP039566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Sep 2021 21:24
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 01:35:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

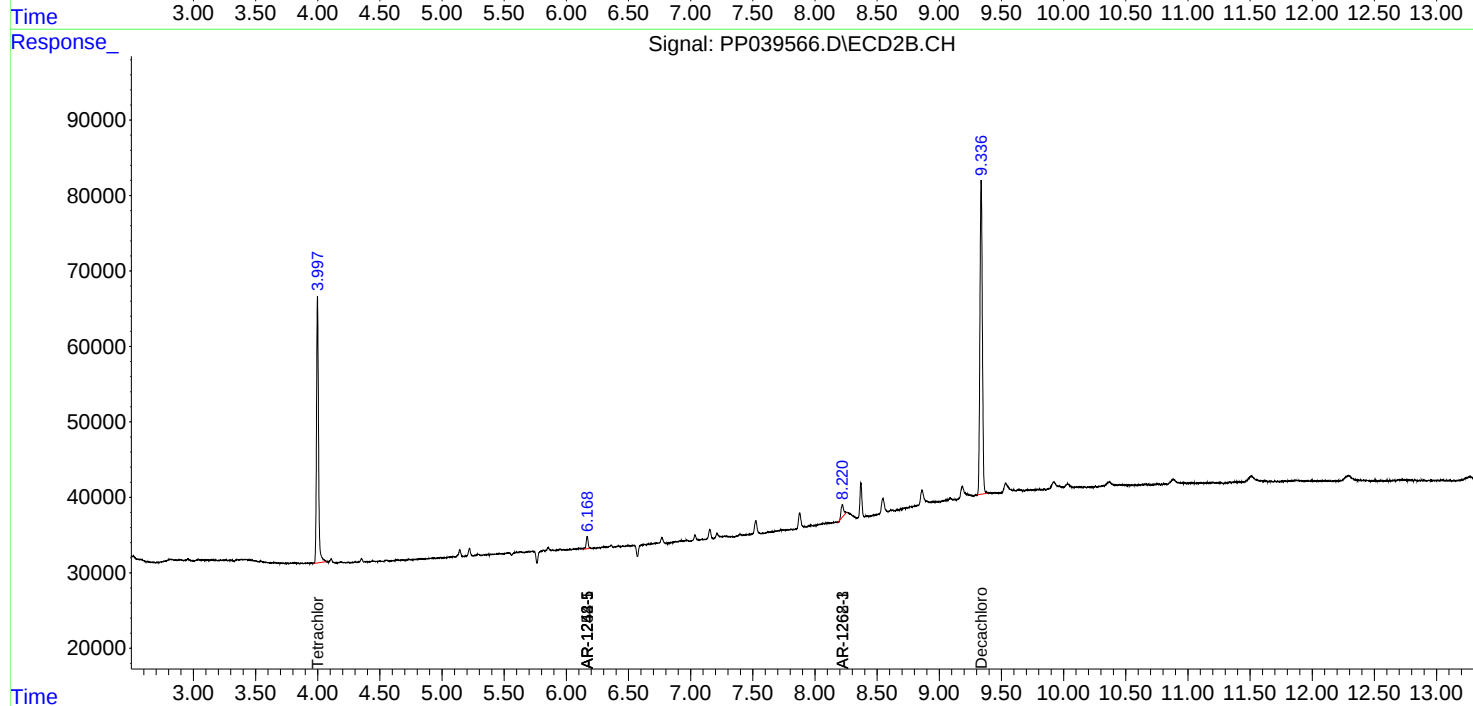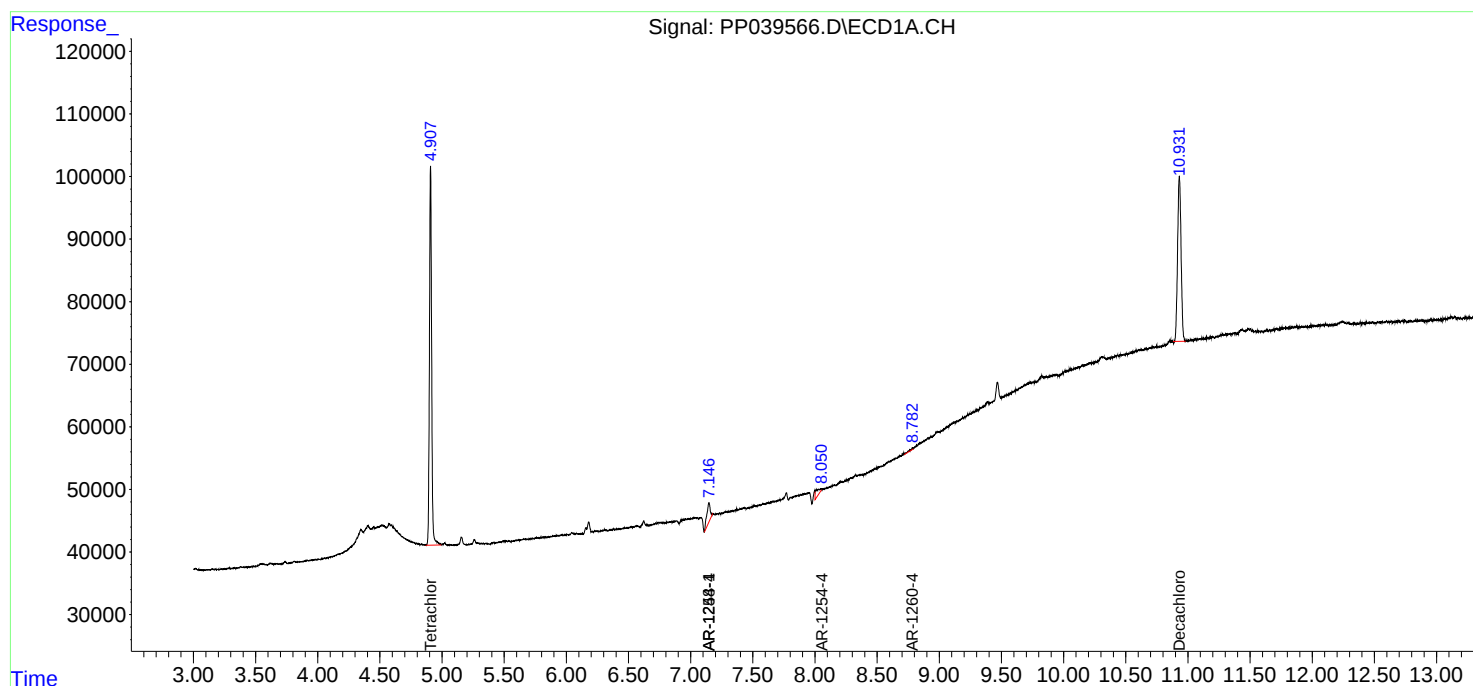


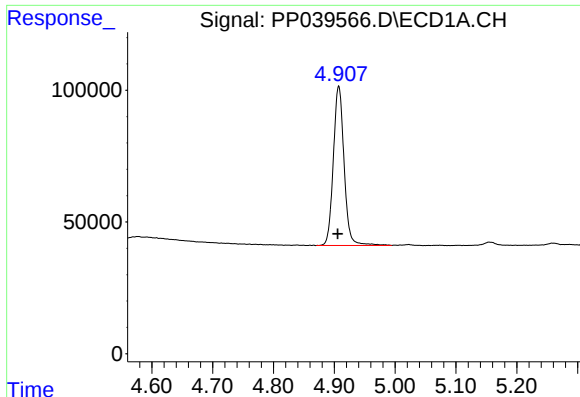

#1 Tetrachloro-m-xylene


R.T.: 4.907 min
Delta R.T.: 0.001 min
Response: 744528
Conc: 23.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

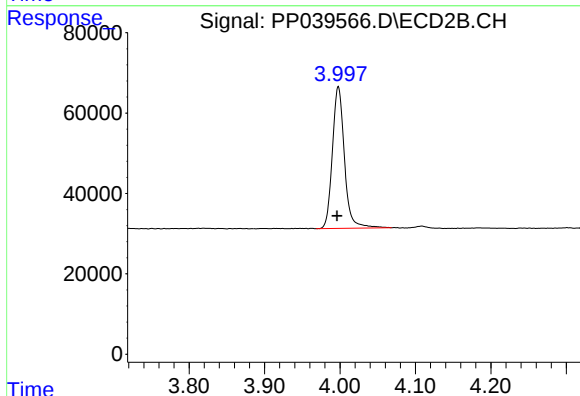


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: 0.002 min
Response: 391399
Conc: 24.02 ng/ml

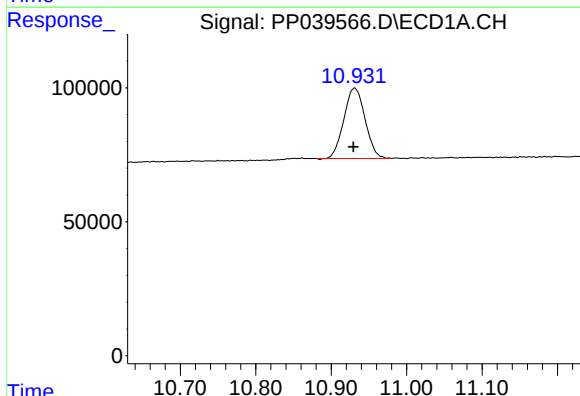


#2 Decachlorobiphenyl

R.T.: 10.931 min
Delta R.T.: 0.001 min
Response: 511708
Conc: 23.59 ng/ml

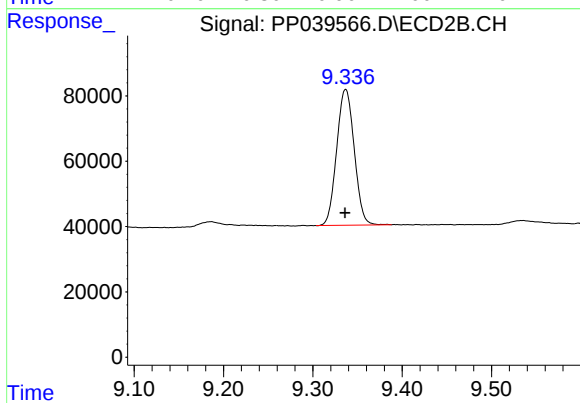

#2 Decachlorobiphenyl


R.T.: 9.337 min
Delta R.T.: 0.000 min
Response: 567828
Conc: 25.98 ng/ml

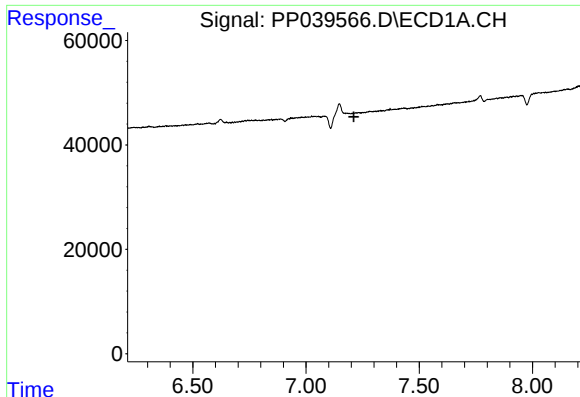

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

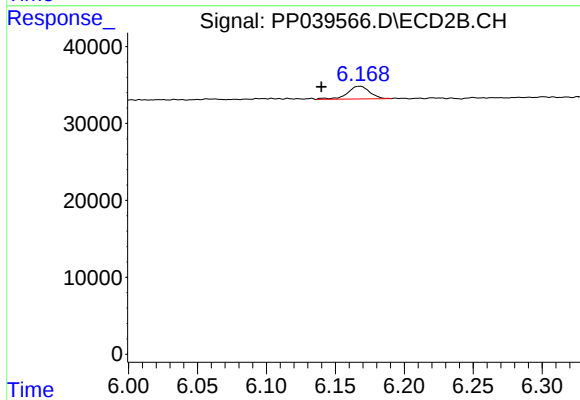


#20 AR-1242-5

R.T.: 6.168 min
Delta R.T.: 0.028 min
Response: 18447
Conc: 34.76 ng/ml

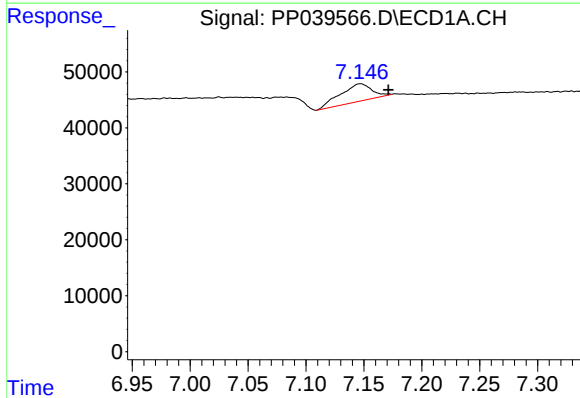


#24 AR-1248-4

R.T.: 7.147 min
Delta R.T.: -0.024 min
Response: 59791
Conc: 55.08 ng/ml

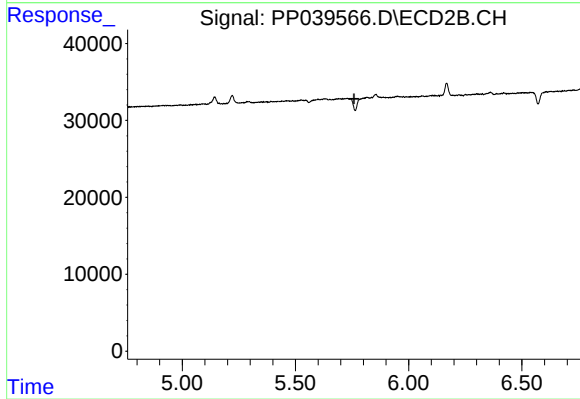

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.758 min
Response: 0
Conc: N.D.

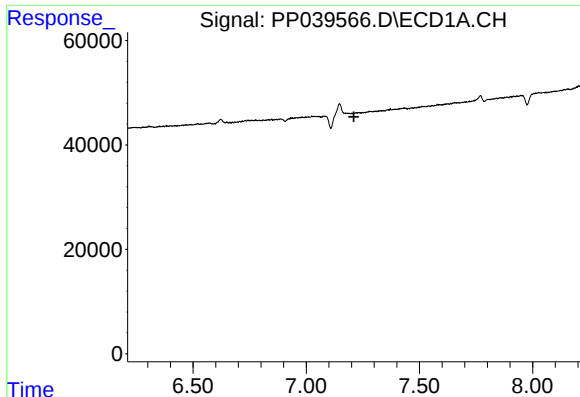

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

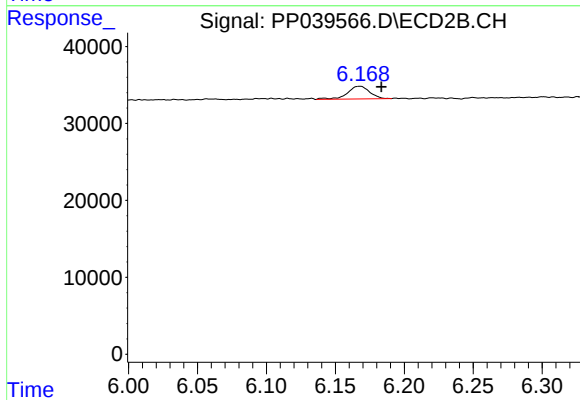


#25 AR-1248-5

R.T.: 6.168 min
Delta R.T.: -0.015 min
Response: 18447
Conc: 26.17 ng/ml

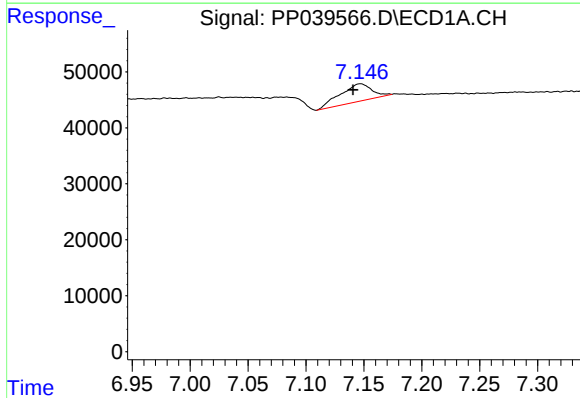


#26 AR-1254-1

R.T.: 7.147 min
Delta R.T.: 0.006 min
Response: 59791
Conc: 54.78 ng/ml

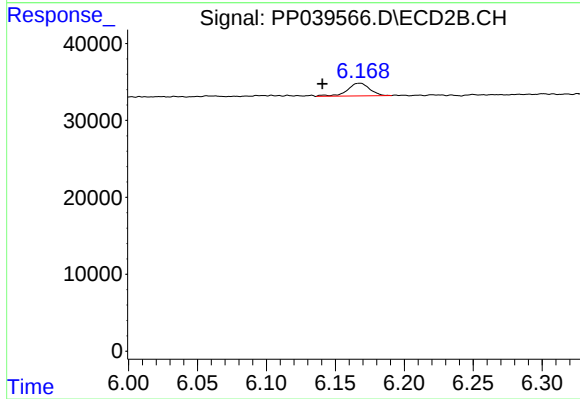

#26 AR-1254-1


R.T.: 6.168 min
Delta R.T.: 0.027 min
Response: 18447
Conc: 17.72 ng/ml

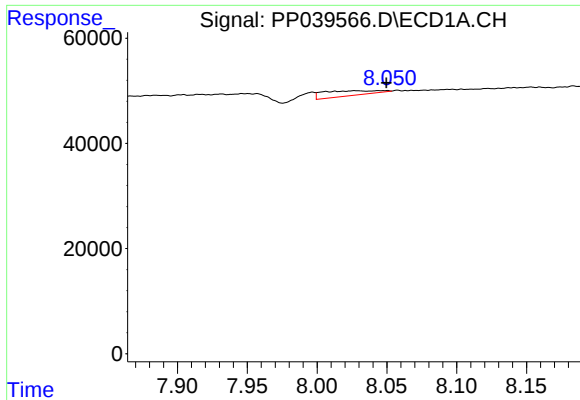

#29 AR-1254-4


R.T.: 8.051 min
Delta R.T.: 0.000 min
Response: 25370
Conc: 20.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

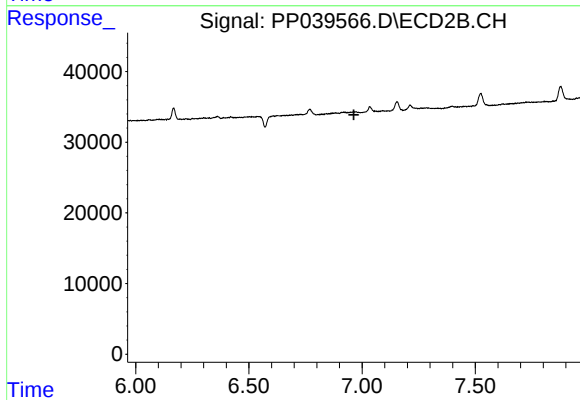


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.964 min
Response: 0
Conc: N.D.

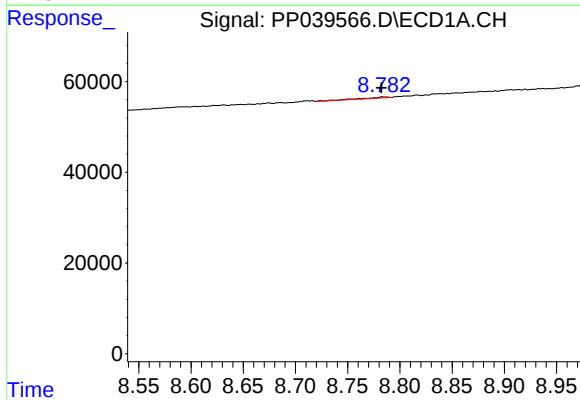


#34 AR-1260-4

R.T.: 8.783 min
Delta R.T.: 0.000 min
Response: 4381
Conc: 4.39 ng/ml

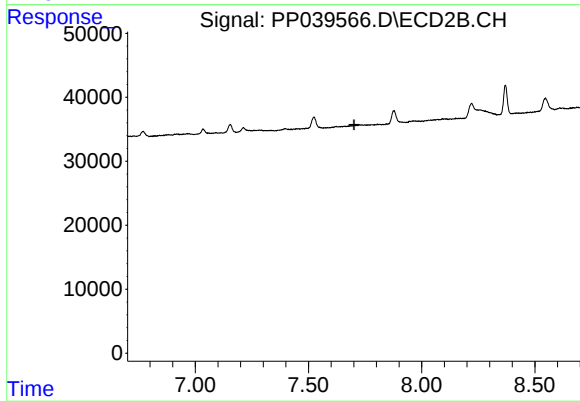

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.701 min
Response: 0
Conc: N.D.

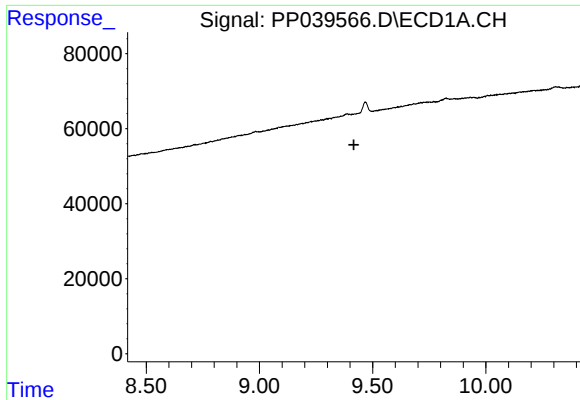

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

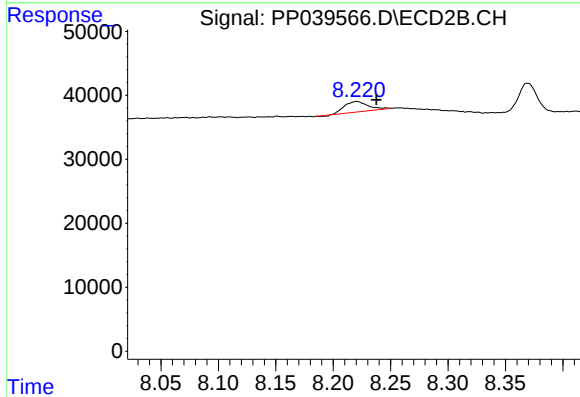


#38 AR-1262-3

R.T.: 8.220 min
Delta R.T.: -0.017 min
Response: 22998
Conc: 22.63 ng/ml

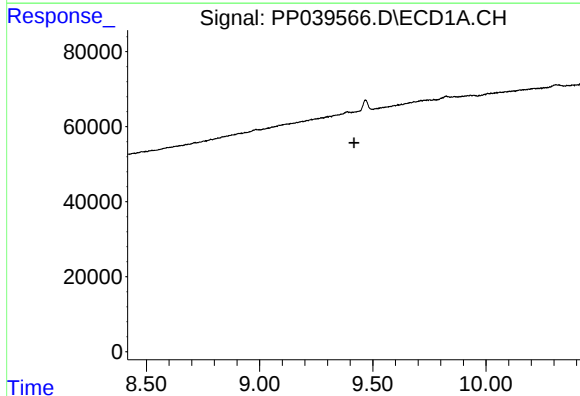

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

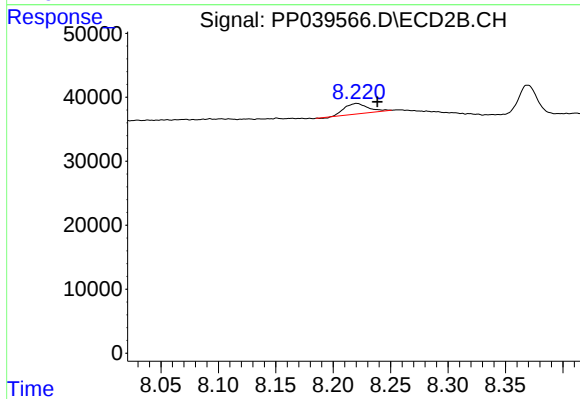

#41 AR-1268-1

R.T.: 8.220 min
Delta R.T.: -0.018 min
Response: 22998
Conc: 7.89 ng/ml