

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092723\
 Data File : PP060306.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Sep 2023 16:03
 Operator : YP\AJ
 Sample : 04615-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-40279

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/28/2023
 Supervised By :Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 27 16:46:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.532	3.685	38274481	24364408	17.091	16.368
2) SA Decachlor...	10.457	8.750	35027241	27376834	19.839	16.783
Target Compounds						
26) L6 AR-1254-1	6.611f	5.587	6233555	3534272	73.044	35.729 #
27) L6 AR-1254-2	6.811	5.741	3807001	817101	29.829	9.507m#
28) L6 AR-1254-3	7.177	6.150	4611042	2851246	34.691	19.893 #
29) L6 AR-1254-4	7.465	6.379	6868453	5122029	69.845	58.764
30) L6 AR-1254-5	7.888	6.800	11505582	10324990	106.196	81.479

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092723\
Data File : PP060306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Sep 2023 16:03
Operator : YP\AJ
Sample : 04615-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-40279


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 27 16:46:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

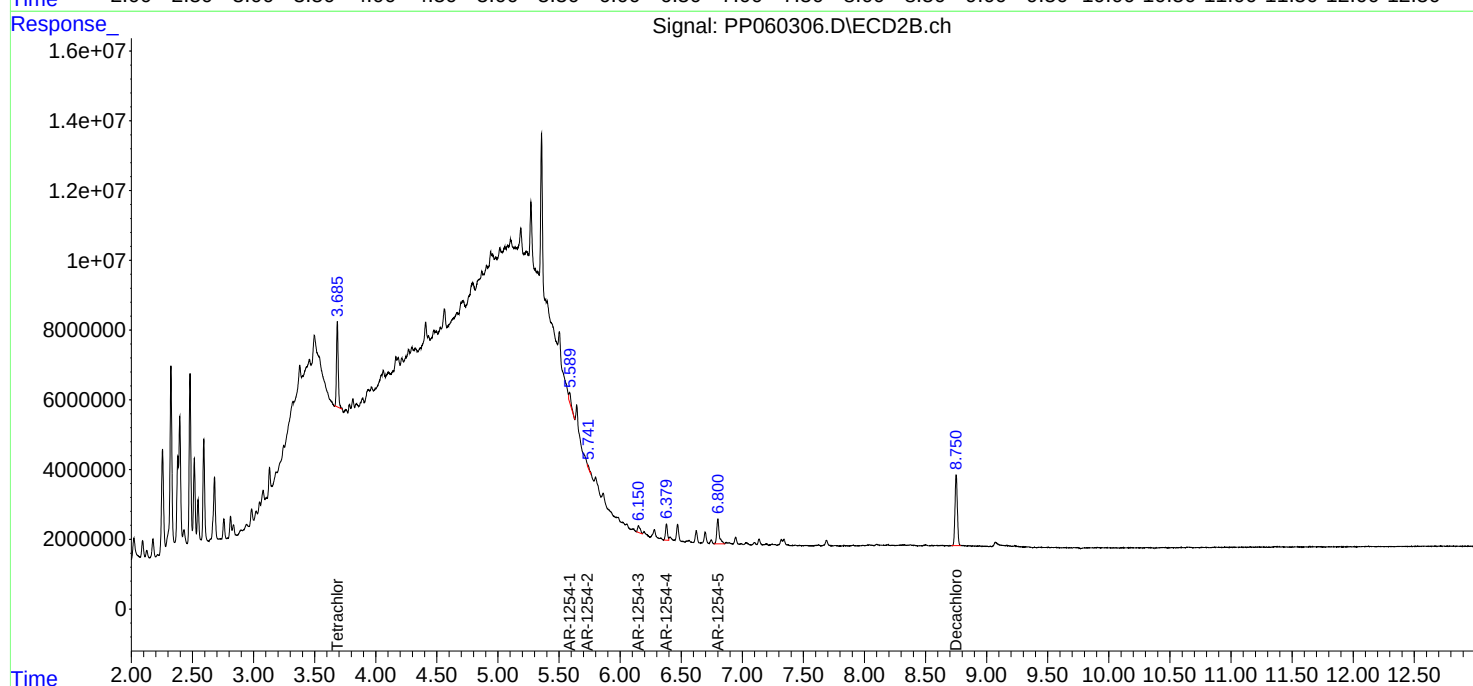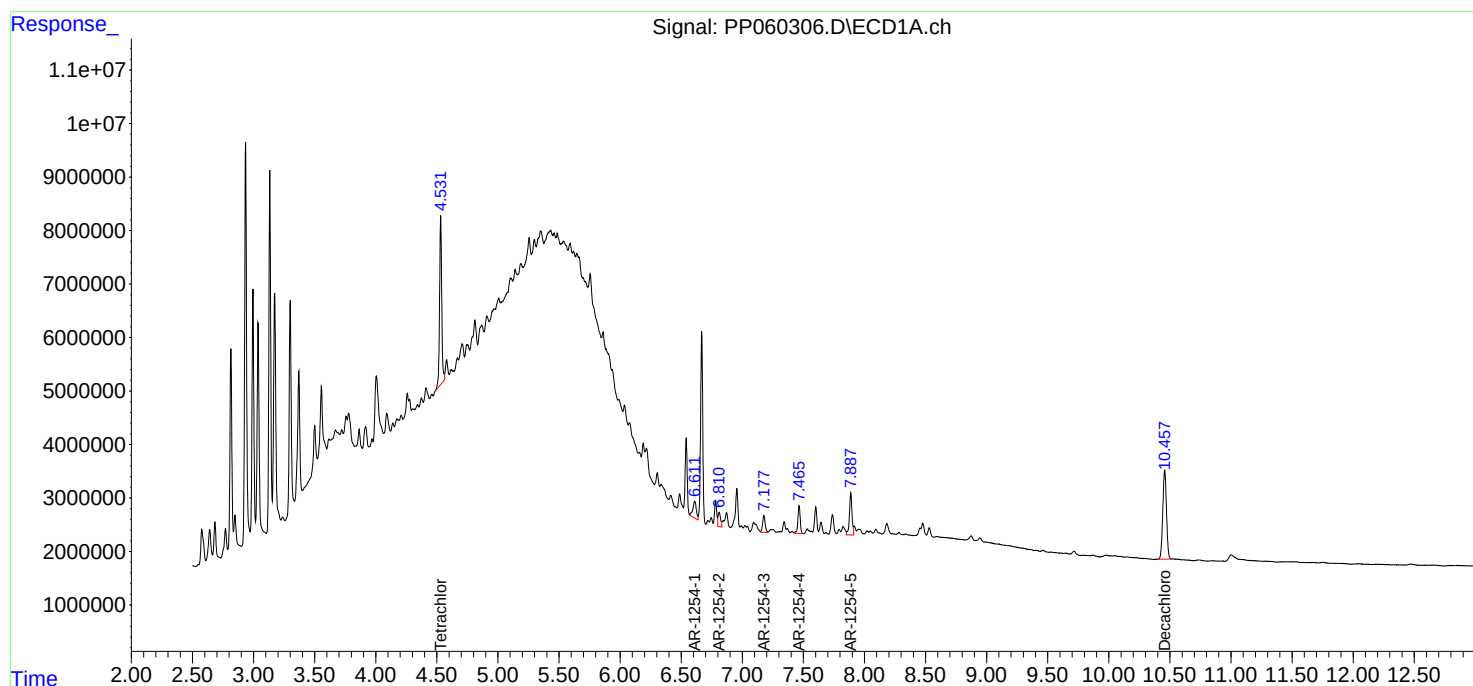

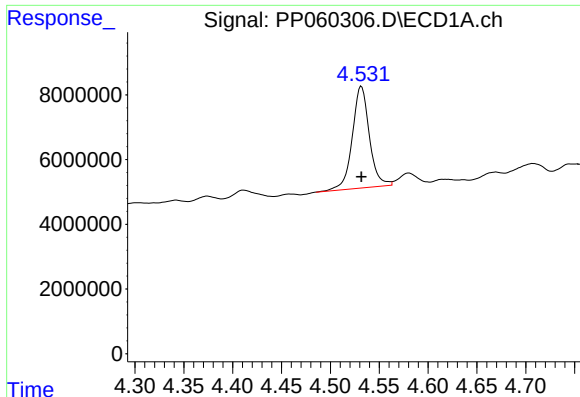


#1 Tetrachloro-m-xylene

R.T.: 4.532 min
Delta R.T.: 0.000 min
Response: 38274481
Conc: 17.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40279


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

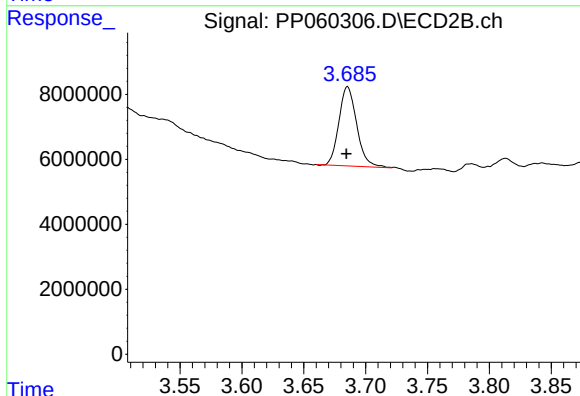


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 24364408
Conc: 16.37 ng/ml

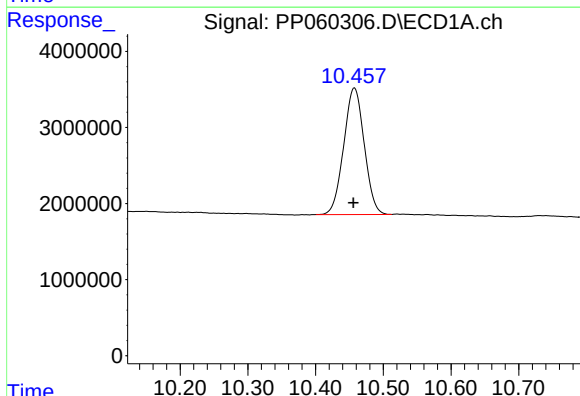


#2 Decachlorobiphenyl

R.T.: 10.457 min
Delta R.T.: 0.002 min
Response: 35027241
Conc: 19.84 ng/ml

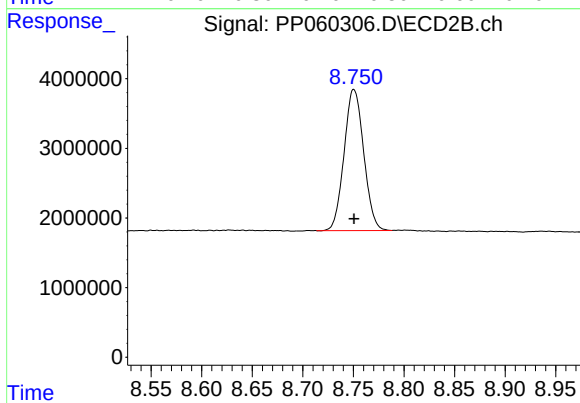

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: 0.000 min
Response: 27376834
Conc: 16.78 ng/ml

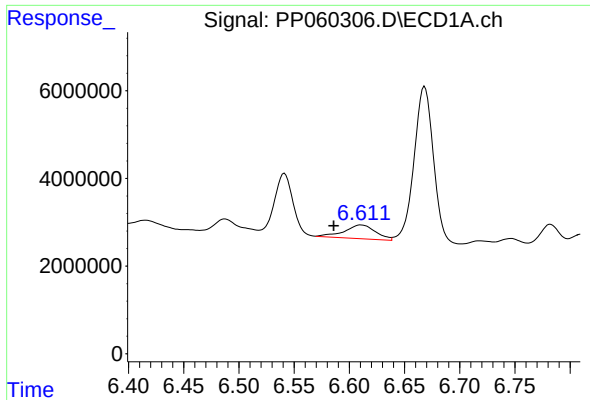


#26 AR-1254-1

R.T.: 6.611 min
Delta R.T.: 0.025 min
Response: 6233555
Conc: 73.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40279


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

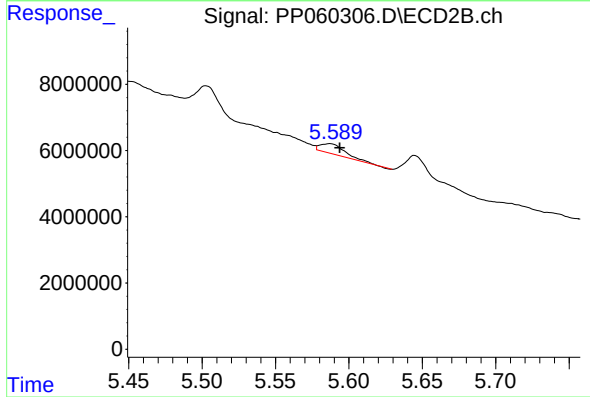


#26 AR-1254-1

R.T.: 5.587 min
Delta R.T.: -0.007 min
Response: 3534272
Conc: 35.73 ng/ml

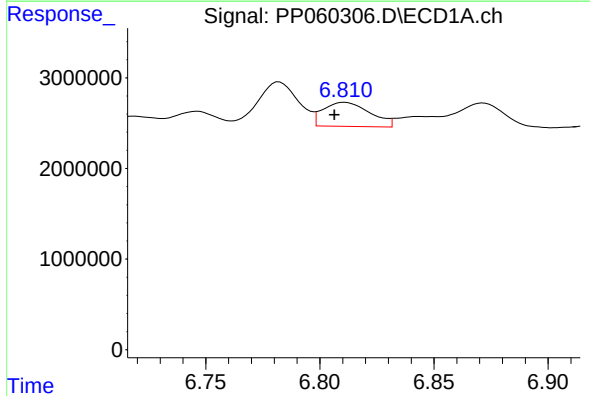


#27 AR-1254-2

R.T.: 6.811 min
Delta R.T.: 0.005 min
Response: 3807001
Conc: 29.83 ng/ml

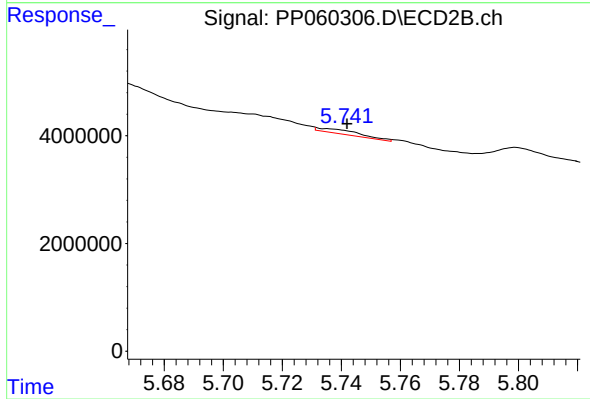

#27 AR-1254-2

R.T.: 5.741 min
Delta R.T.: -0.001 min
Response: 817101
Conc: 9.51 ng/ml m

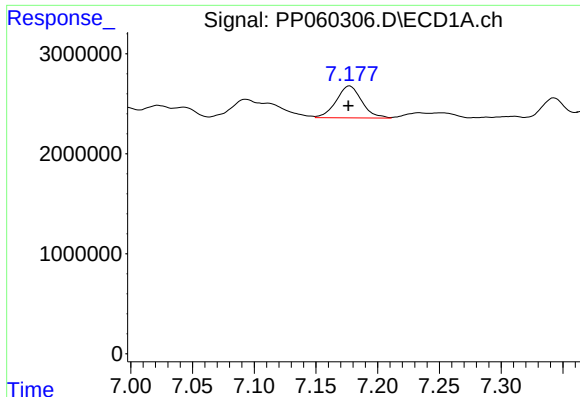


#28 AR-1254-3

R.T.: 7.177 min
Delta R.T.: 0.000 min
Response: 4611042
Conc: 34.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40279


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

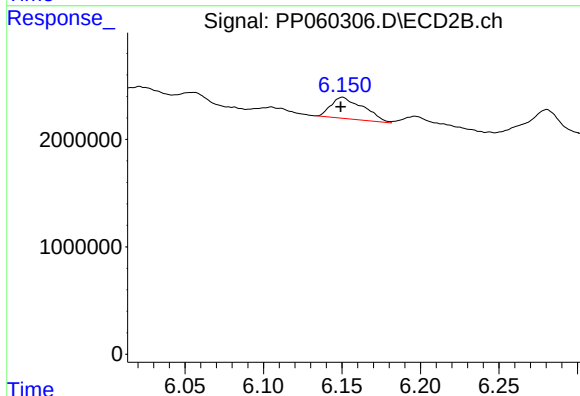


#28 AR-1254-3

R.T.: 6.150 min
Delta R.T.: 0.001 min
Response: 2851246
Conc: 19.89 ng/ml

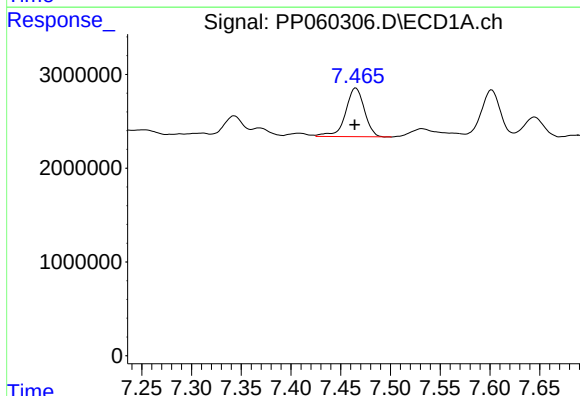


#29 AR-1254-4

R.T.: 7.465 min
Delta R.T.: 0.001 min
Response: 6868453
Conc: 69.84 ng/ml

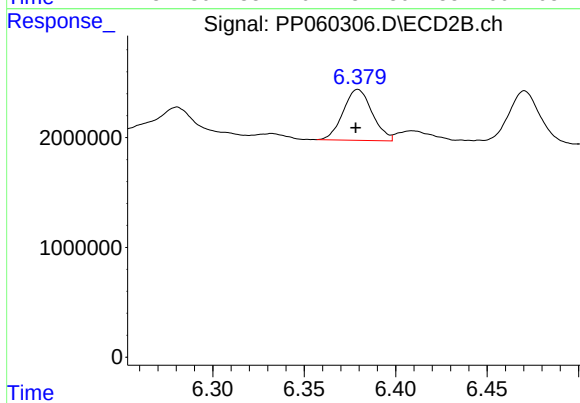

#29 AR-1254-4

R.T.: 6.379 min
Delta R.T.: 0.001 min
Response: 5122029
Conc: 58.76 ng/ml

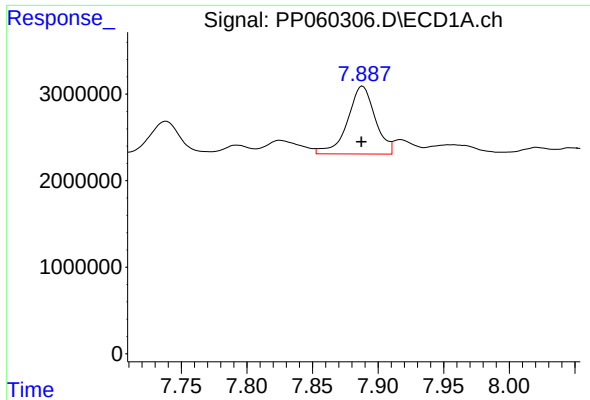


#30 AR-1254-5

R.T.: 7.888 min
Delta R.T.: 0.001 min
Response: 11505582
Conc: 106.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40279

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/28/2023
Supervised By :Ankita Jodhani 09/28/2023

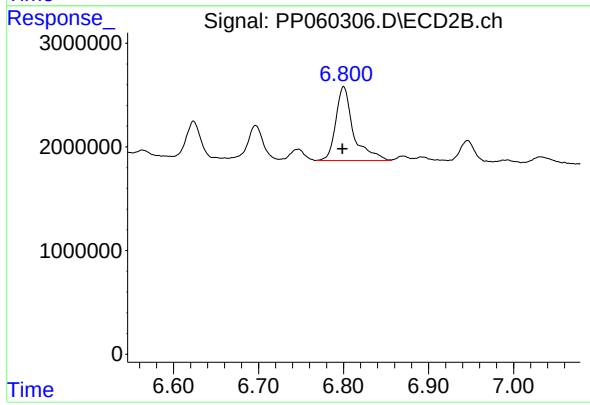

#30 AR-1254-5

R.T.: 6.800 min
Delta R.T.: 0.001 min
Response: 10324990
Conc: 81.48 ng/ml