

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092821\
 Data File : PP039572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2021 10:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 01:45:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.907	3.996	761183	415064	24.044	25.473
2)	SA Decachlor...	10.930	9.336	533996	594330	24.615	27.198
Target Compounds							
20)	L4 AR-1242-5	0.000	6.166f	0	27593	N.D.	51.998 #
24)	L5 AR-1248-4	7.147f	0.000	75973	0	69.984	N.D. #
25)	L5 AR-1248-5	0.000	6.166f	0	27593	N.D.	39.146 #
26)	L6 AR-1254-1	7.147	6.166f	75973	27593	69.603	26.503 #
32)	L7 AR-1260-2	8.200	7.033f	22966	10357	16.589	8.086 #
33)	L7 AR-1260-3	0.000	7.212	0	5257	N.D.	4.369 #
38)	L8 AR-1262-3	0.000	8.262f	0	57595	N.D.	56.667 #
41)	L9 AR-1268-1	0.000	8.262f	0	57595	N.D.	19.752 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092821\
Data File : PP039572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2021 10:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 01:45:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

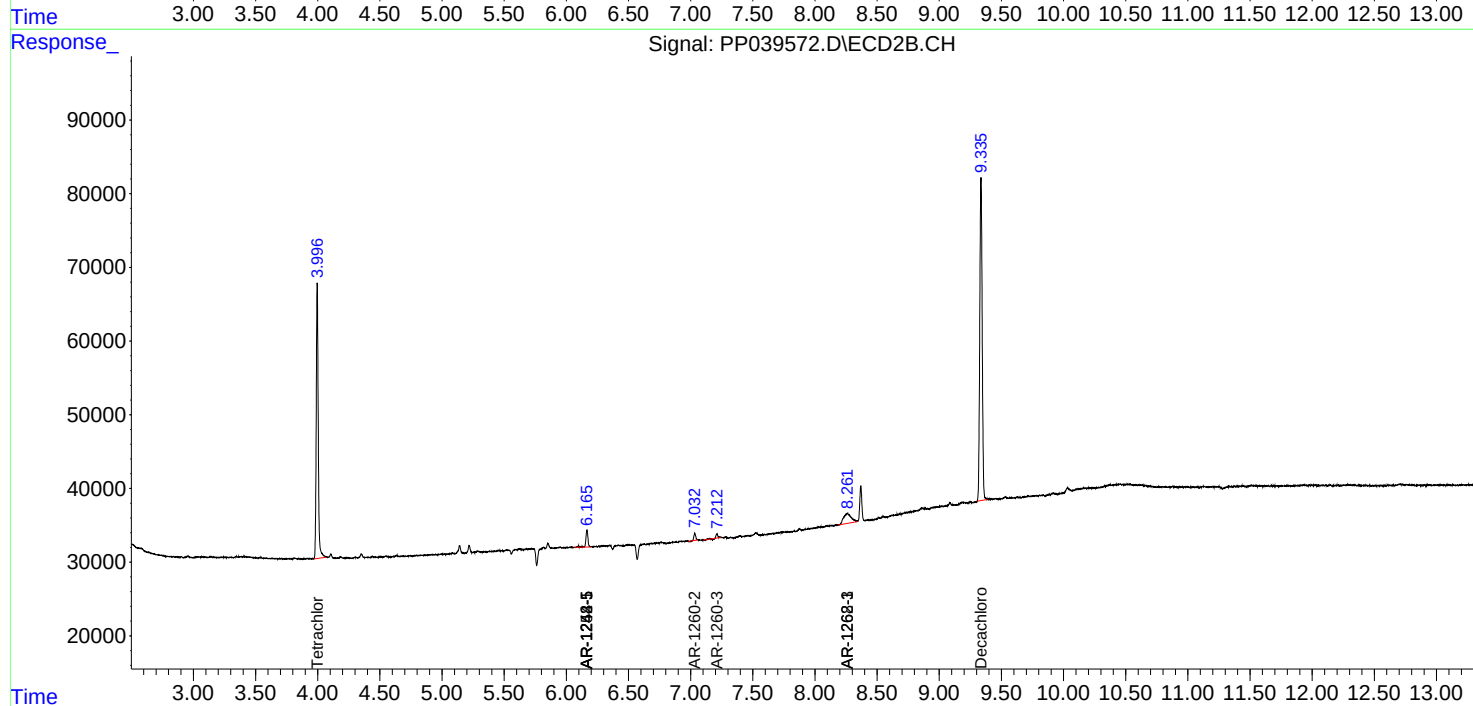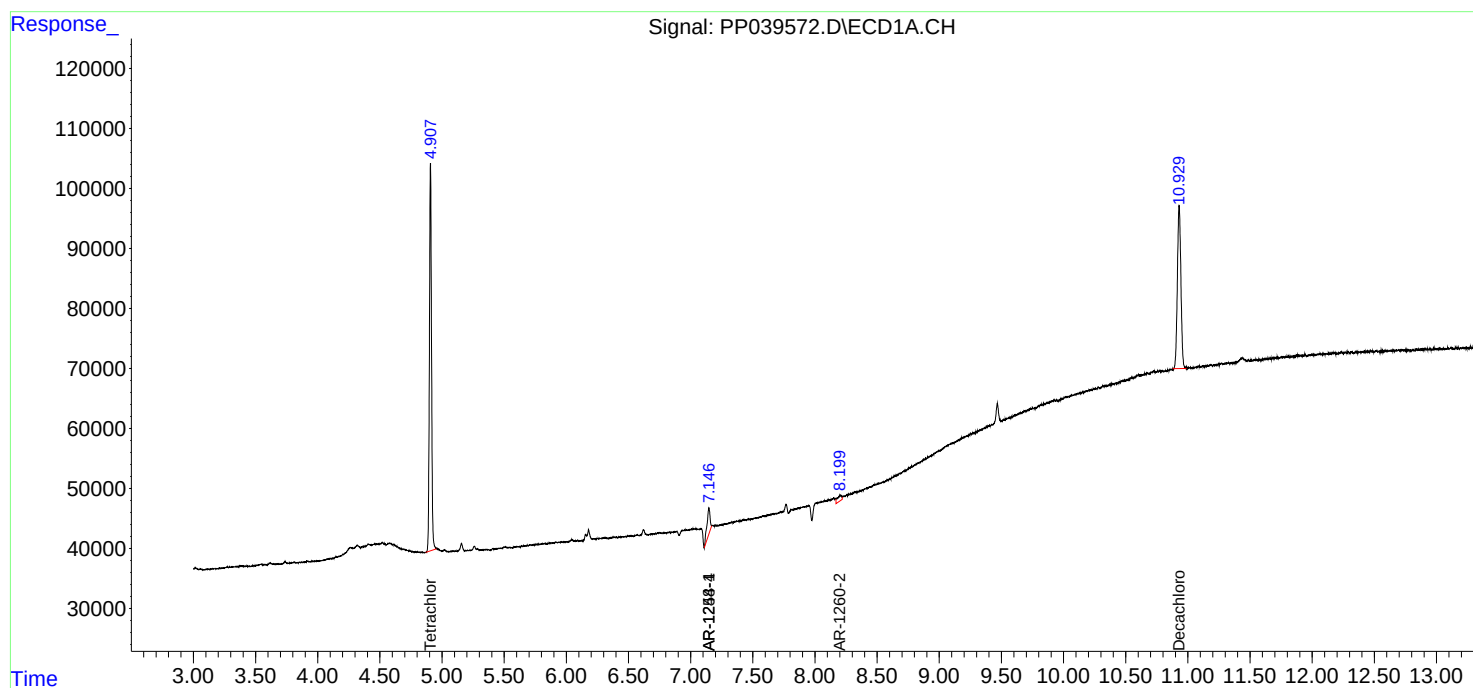


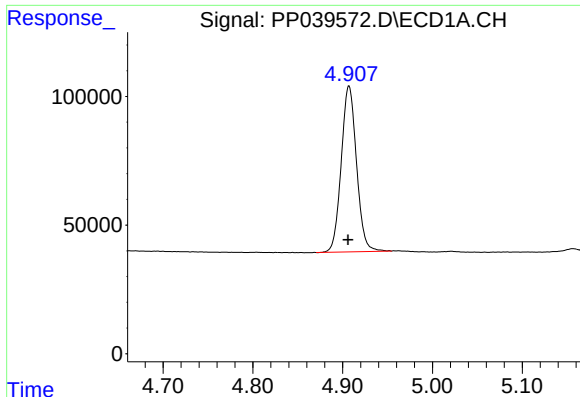

#1 Tetrachloro-m-xylene


R.T.: 4.907 min
Delta R.T.: 0.001 min
Response: 761183
Conc: 24.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

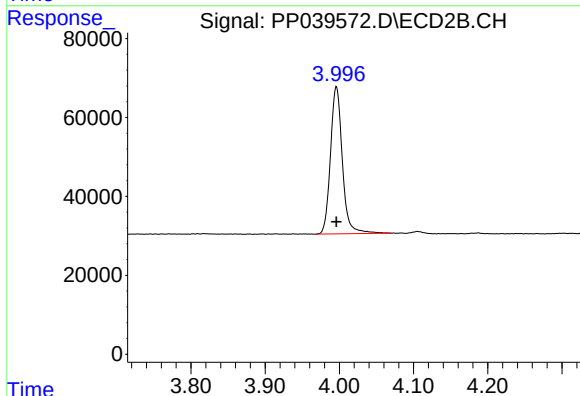


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 415064
Conc: 25.47 ng/ml

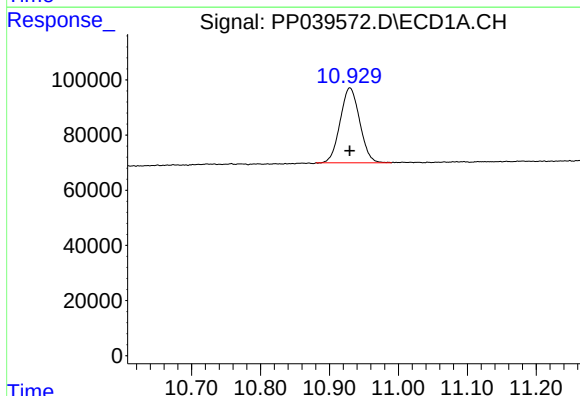


#2 Decachlorobiphenyl

R.T.: 10.930 min
Delta R.T.: 0.000 min
Response: 533996
Conc: 24.62 ng/ml

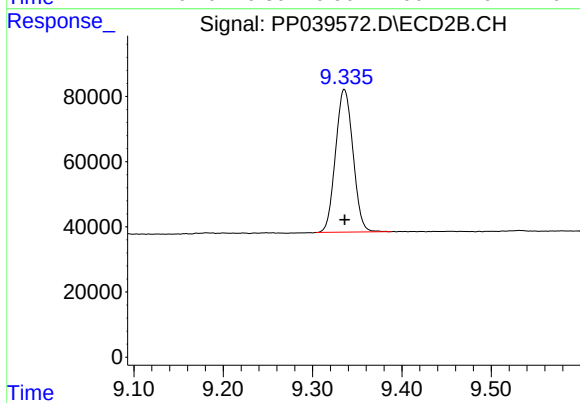

#2 Decachlorobiphenyl


R.T.: 9.336 min
Delta R.T.: 0.000 min
Response: 594330
Conc: 27.20 ng/ml

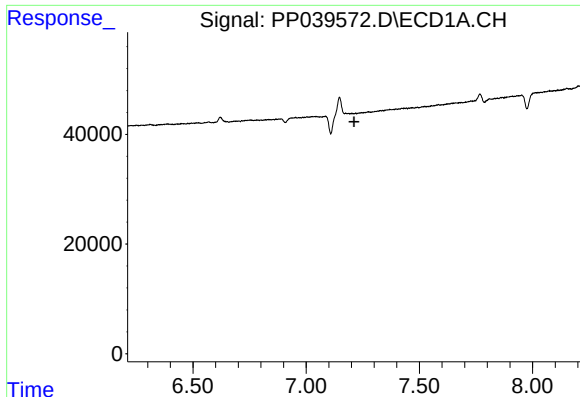

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

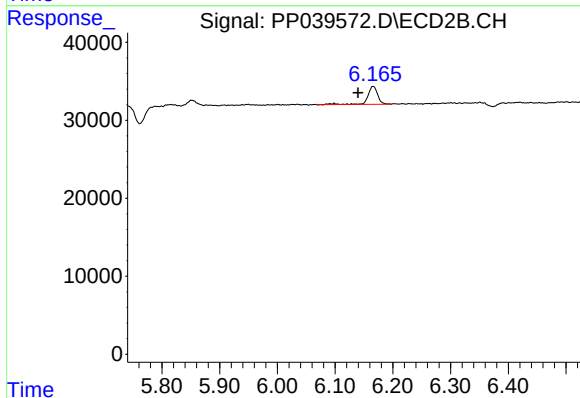


#20 AR-1242-5

R.T.: 6.166 min
Delta R.T.: 0.026 min
Response: 27593
Conc: 52.00 ng/ml

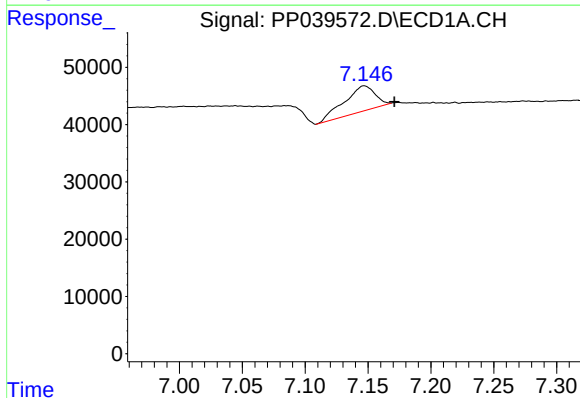


#24 AR-1248-4

R.T.: 7.147 min
Delta R.T.: -0.024 min
Response: 75973
Conc: 69.98 ng/ml

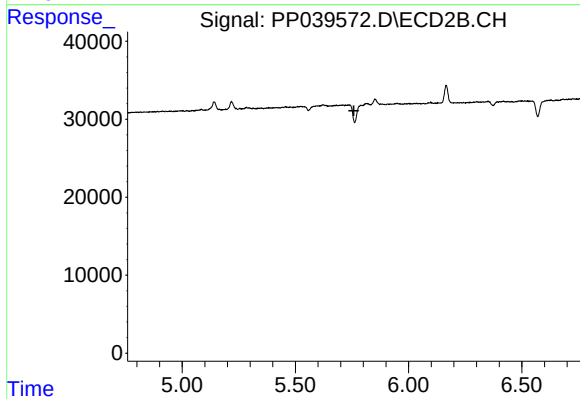

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.758 min
Response: 0
Conc: N.D.

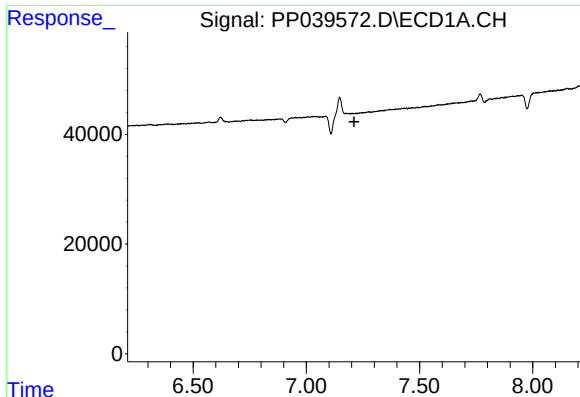

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

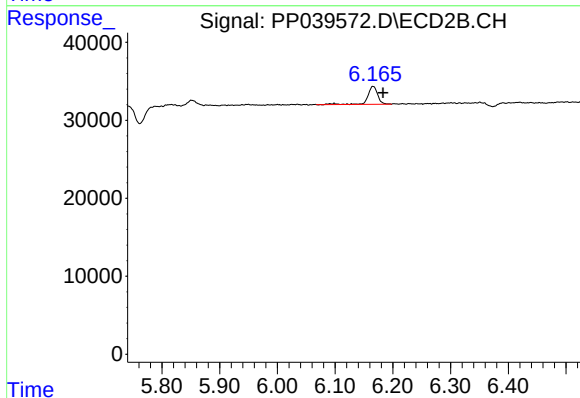


#25 AR-1248-5

R.T.: 6.166 min
Delta R.T.: -0.018 min
Response: 27593
Conc: 39.15 ng/ml

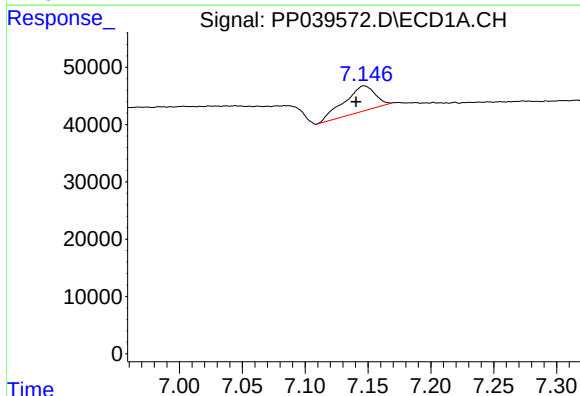


#26 AR-1254-1

R.T.: 7.147 min
Delta R.T.: 0.006 min
Response: 75973
Conc: 69.60 ng/ml

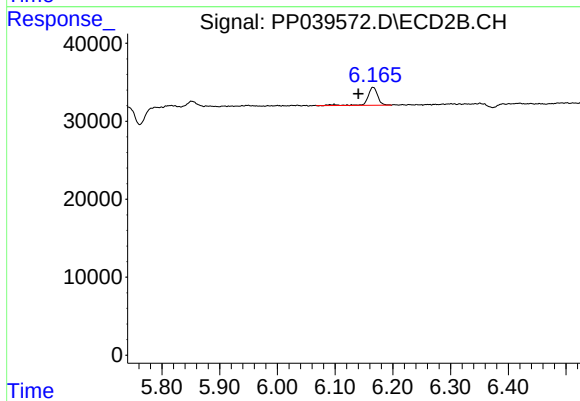

#26 AR-1254-1


R.T.: 6.166 min
Delta R.T.: 0.025 min
Response: 27593
Conc: 26.50 ng/ml

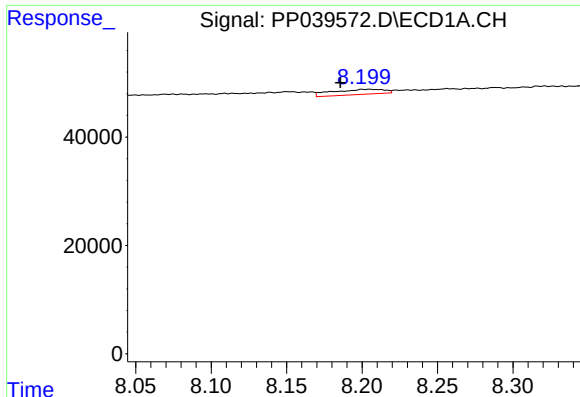

#32 AR-1260-2


R.T.: 8.200 min
Delta R.T.: 0.014 min
Response: 22966
Conc: 16.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

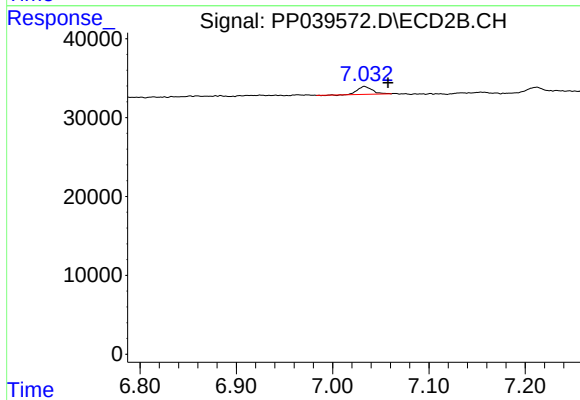


#32 AR-1260-2

R.T.: 7.033 min
Delta R.T.: -0.024 min
Response: 10357
Conc: 8.09 ng/ml

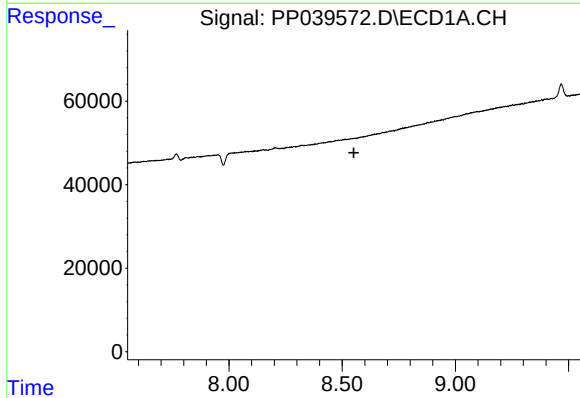


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.551 min
Response: 0
Conc: N.D.

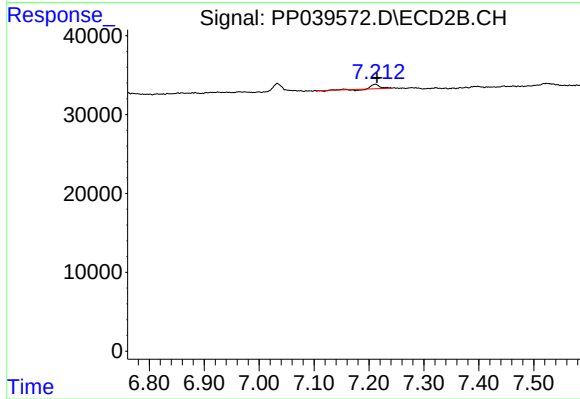

#33 AR-1260-3


R.T.: 7.212 min
Delta R.T.: -0.003 min
Response: 5257
Conc: 4.37 ng/ml

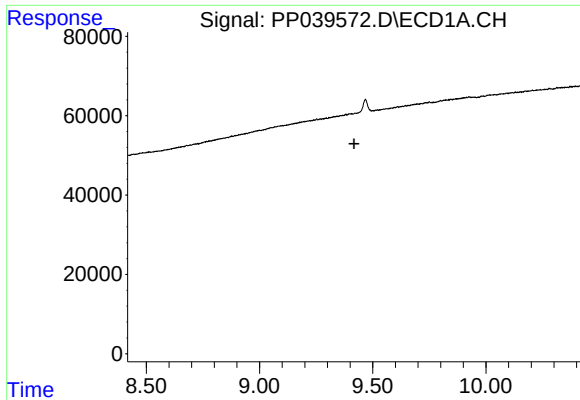

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

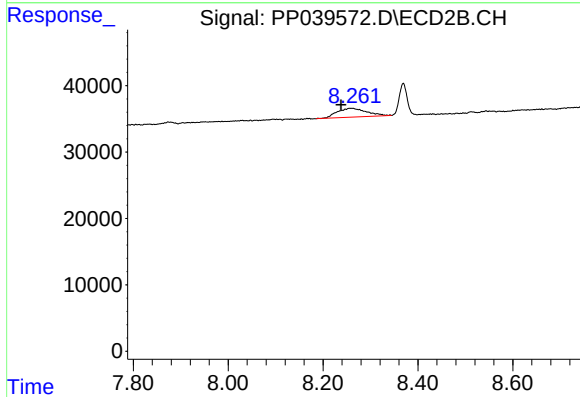


#38 AR-1262-3

R.T.: 8.262 min
Delta R.T.: 0.024 min
Response: 57595
Conc: 56.67 ng/ml

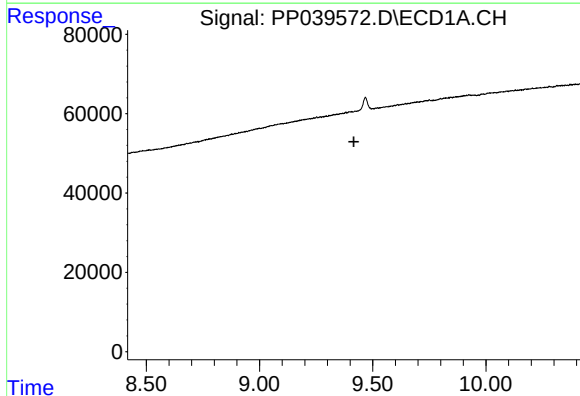

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.417 min
Response: 0
Conc: N.D.

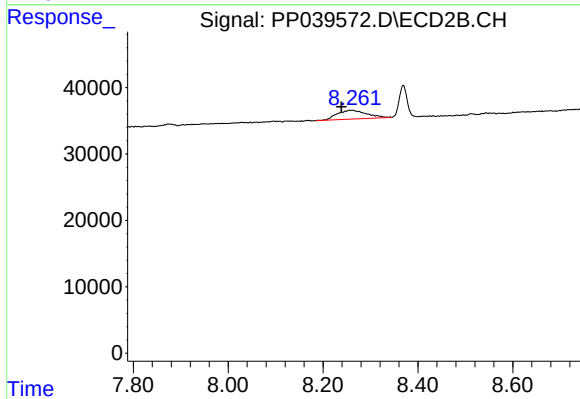

#41 AR-1268-1

R.T.: 8.262 min
Delta R.T.: 0.023 min
Response: 57595
Conc: 19.75 ng/ml