

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092821\
 Data File : PP039584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Sep 2021 17:27
 Operator : AJ\MA
 Sample : M3957-01 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HED760-2-(1-1)

Manual Integrations
 APPROVED

mohammad
 9/29/2021 4:01:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 29 02:11:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.905	3.996	30393	23672	0.960	1.453 #
2) SA Decachlor...	10.927	9.335	37213	38007	1.715	1.739m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092821\
Data File : PP039584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Sep 2021 17:27
Operator : AJ\MA
Sample : M3957-01 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HED760-2-(1-1)


Manual Integrations
APPROVED

mohammad
9/29/2021 4:01:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 29 02:11:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

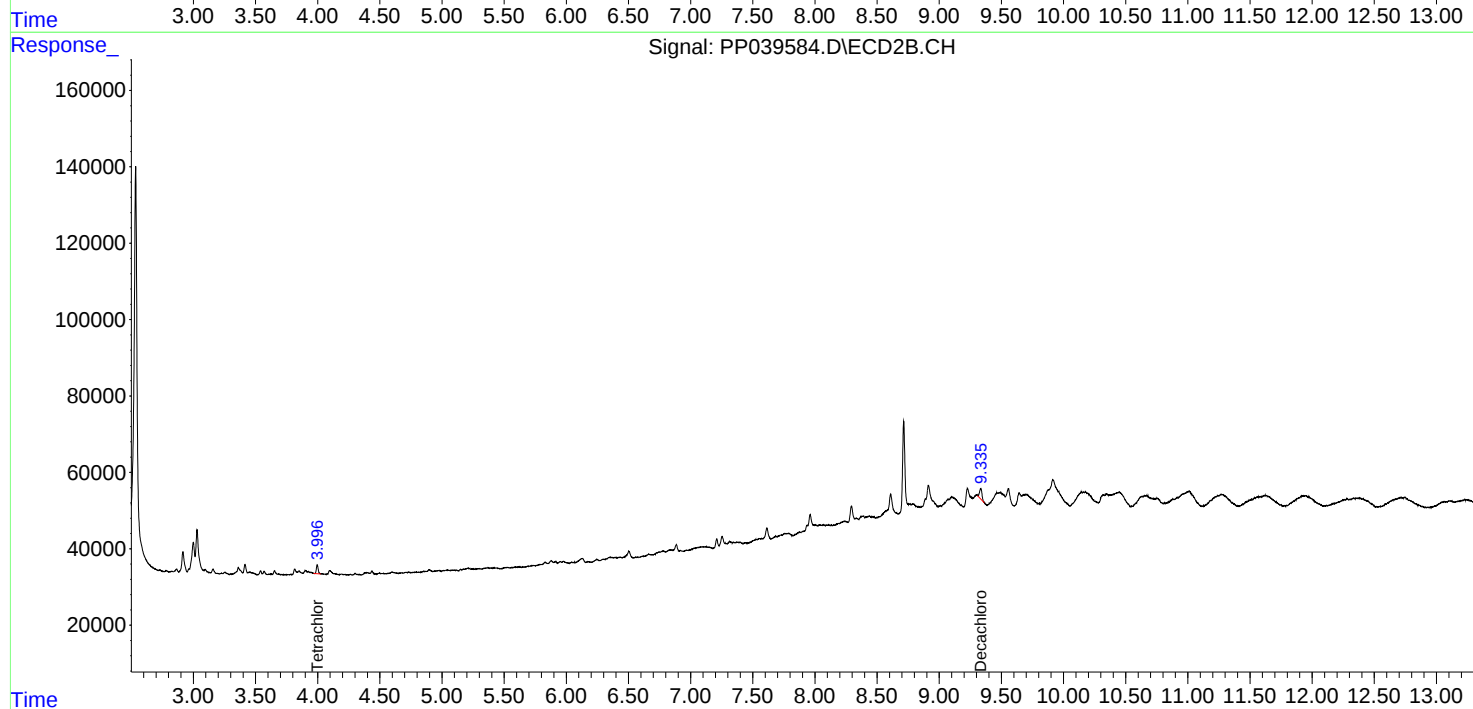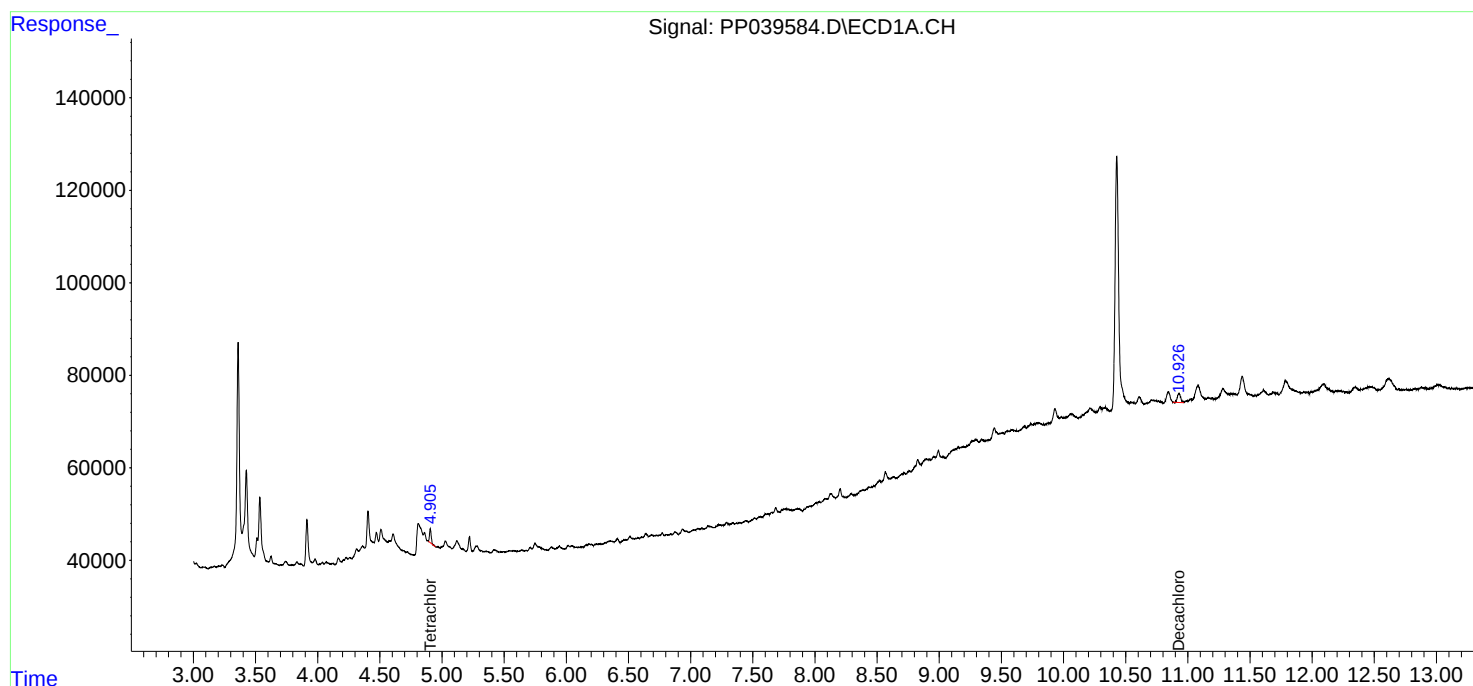

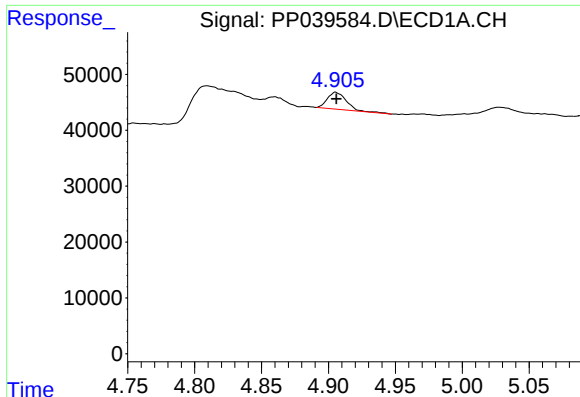


#1 Tetrachloro-m-xylene

R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 30393
Conc: 0.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
HED760-2-(1-1)


Manual Integrations
APPROVED

mohammad
9/29/2021 4:01:20 PM

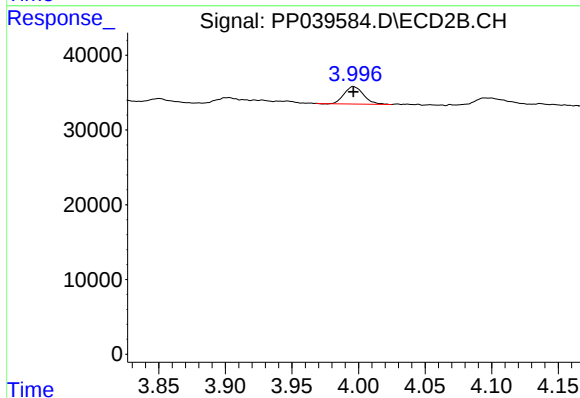


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 23672
Conc: 1.45 ng/ml

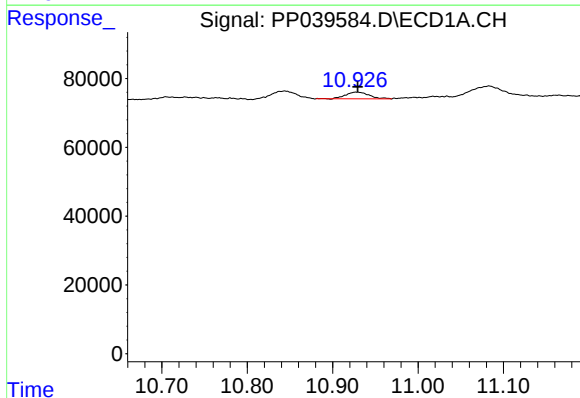

#2 Decachlorobiphenyl

R.T.: 10.927 min
Delta R.T.: -0.002 min
Response: 37213
Conc: 1.72 ng/ml

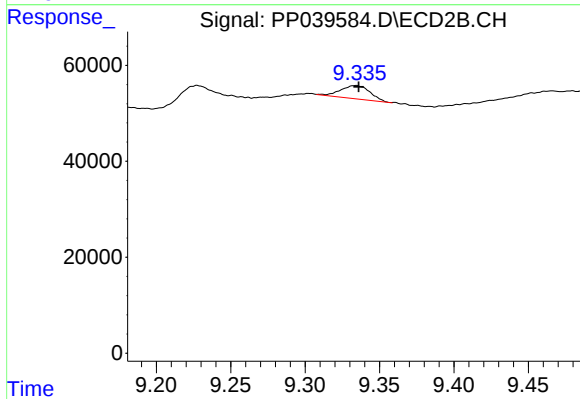

#2 Decachlorobiphenyl

R.T.: 9.335 min
Delta R.T.: -0.001 min
Response: 38007
Conc: 1.74 ng/ml m