

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092823\
 Data File : PP060336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 11:12
 Operator : YP\AJ
 Sample : 04615-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AUD-40284

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 12:19:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.531	3.684	46262201	30688736	20.657	20.617
2)	SA Decachlor...	10.453	8.747	41477237	32056389	23.493	19.652
Target Compounds							
26)	L6 AR-1254-1	6.585	5.592	4043522	3572556	47.381	36.116
27)	L6 AR-1254-2	6.798	5.741	3004533	2076014	23.542m	24.156
28)	L6 AR-1254-3	7.175	6.148	5821867	4163519	43.801	29.049 #
29)	L6 AR-1254-4	7.463	6.377	7901607	5428416	80.351	62.279
30)	L6 AR-1254-5	7.886	6.797	16083473	13157282	148.449	103.829 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092823\
Data File : PP060336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 11:12
Operator : YP\AJ
Sample : 04615-06
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AUD-40284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 12:19:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

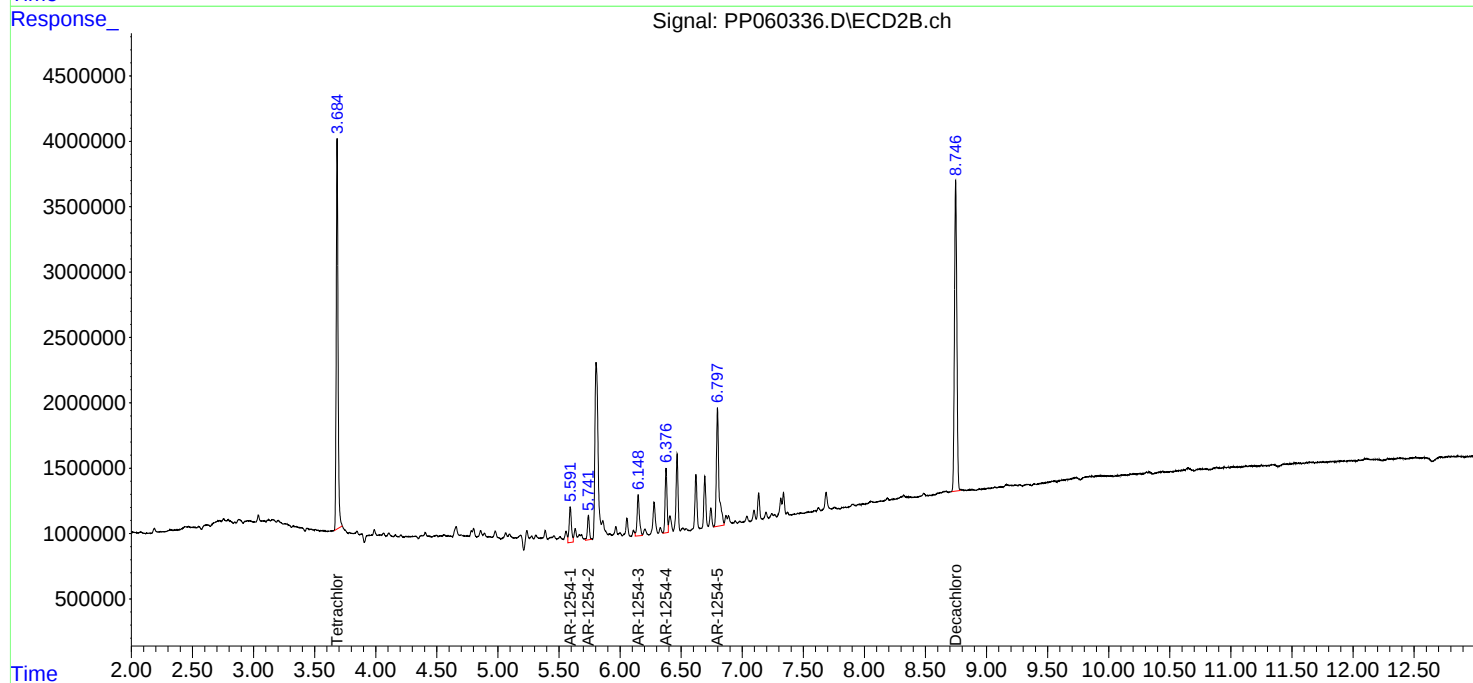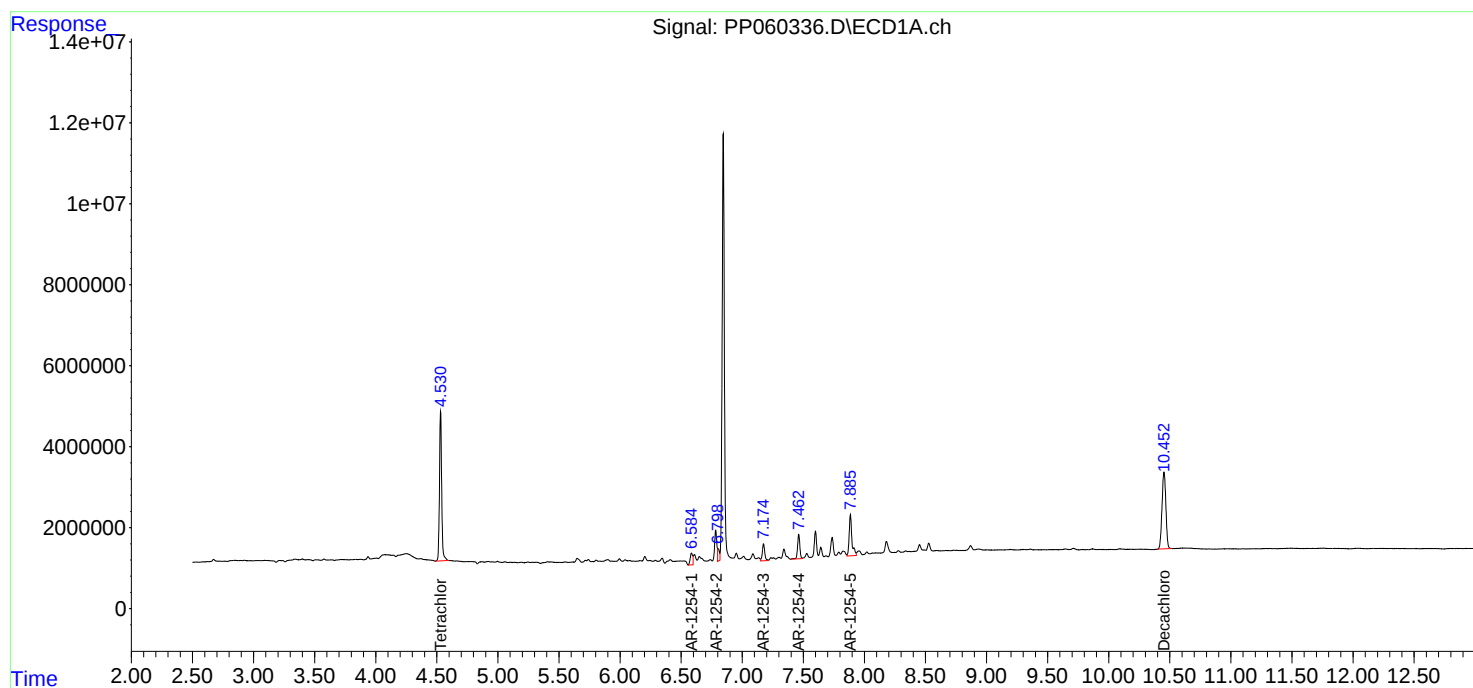

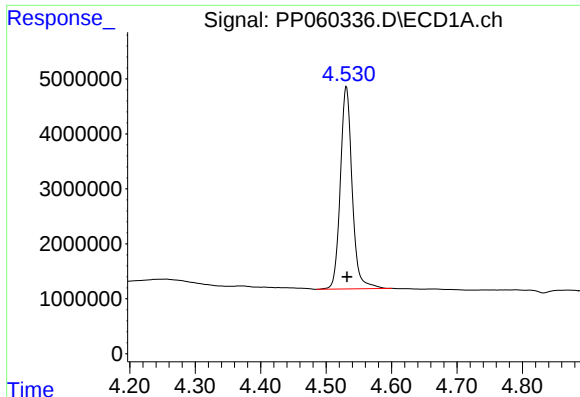


#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 46262201
Conc: 20.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

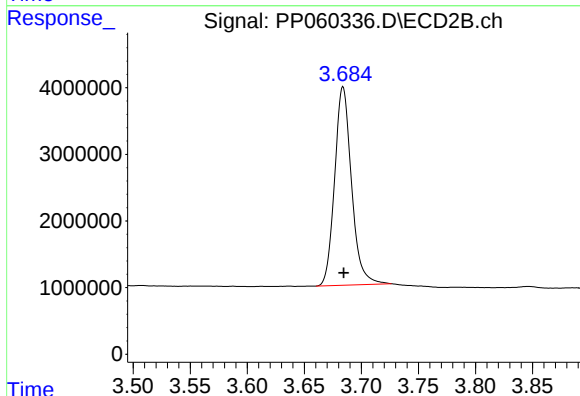


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.000 min
Response: 30688736
Conc: 20.62 ng/ml

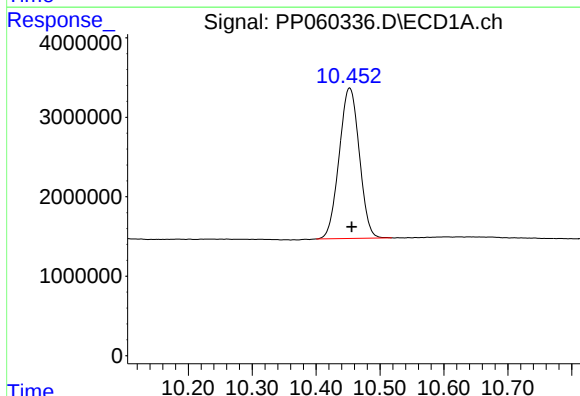


#2 Decachlorobiphenyl

R.T.: 10.453 min
Delta R.T.: -0.003 min
Response: 41477237
Conc: 23.49 ng/ml

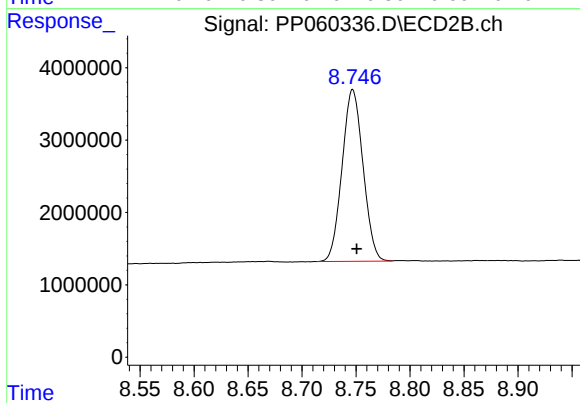

#2 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: -0.004 min
Response: 32056389
Conc: 19.65 ng/ml

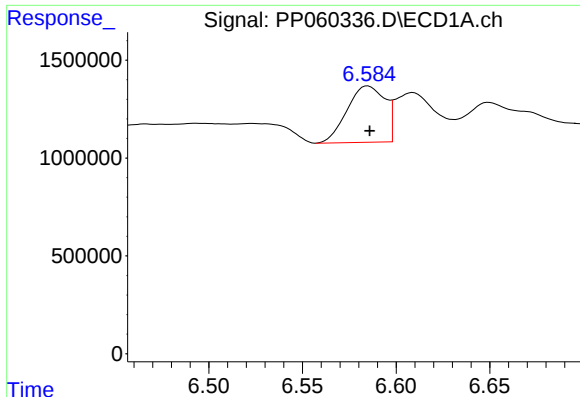


#26 AR-1254-1

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 4043522
Conc: 47.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

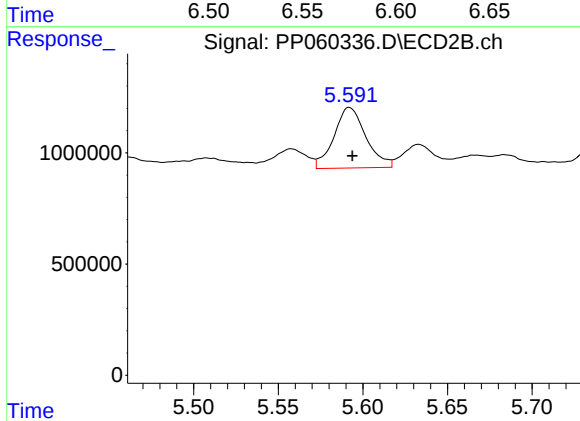


#26 AR-1254-1

R.T.: 5.592 min
Delta R.T.: -0.002 min
Response: 3572556
Conc: 36.12 ng/ml

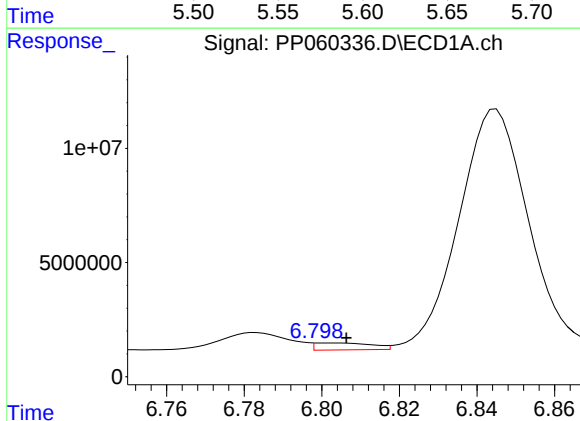


#27 AR-1254-2

R.T.: 6.798 min
Delta R.T.: -0.008 min
Response: 3004533
Conc: 23.54 ng/ml m

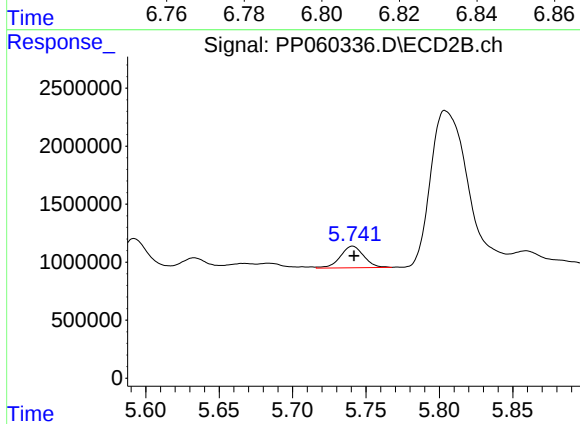

#27 AR-1254-2

R.T.: 5.741 min
Delta R.T.: 0.000 min
Response: 2076014
Conc: 24.16 ng/ml

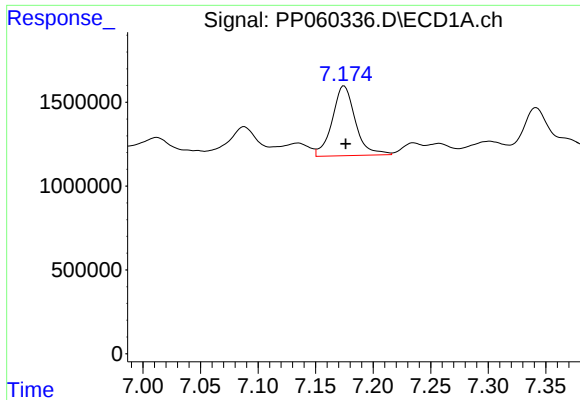


#28 AR-1254-3

R.T.: 7.175 min
Delta R.T.: -0.002 min
Response: 5821867
Conc: 43.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40284


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

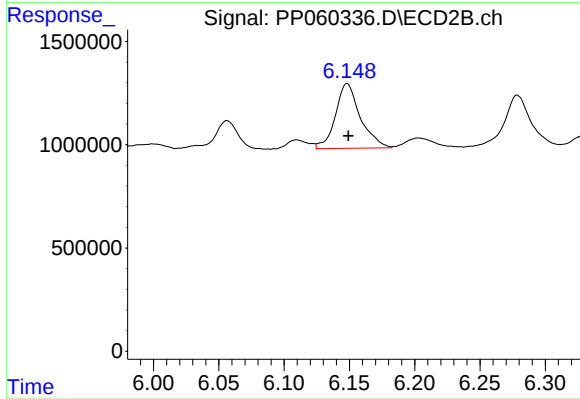


#28 AR-1254-3

R.T.: 6.148 min
Delta R.T.: 0.000 min
Response: 4163519
Conc: 29.05 ng/ml

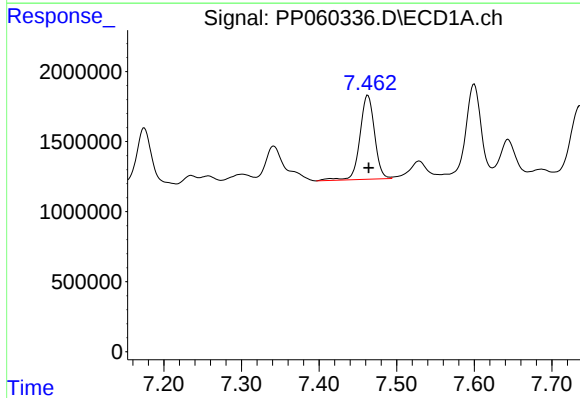


#29 AR-1254-4

R.T.: 7.463 min
Delta R.T.: -0.001 min
Response: 7901607
Conc: 80.35 ng/ml

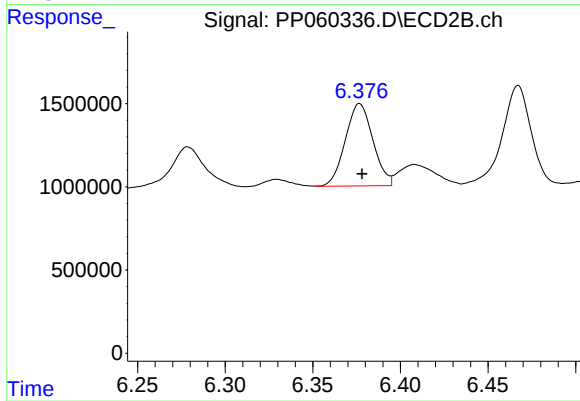

#29 AR-1254-4

R.T.: 6.377 min
Delta R.T.: -0.002 min
Response: 5428416
Conc: 62.28 ng/ml

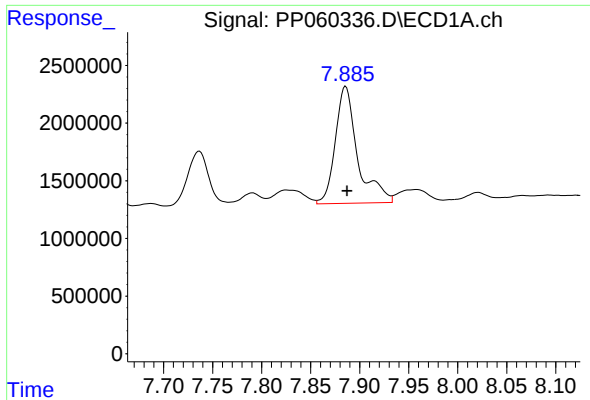


#30 AR-1254-5

R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 16083473
Conc: 148.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AUD-40284

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

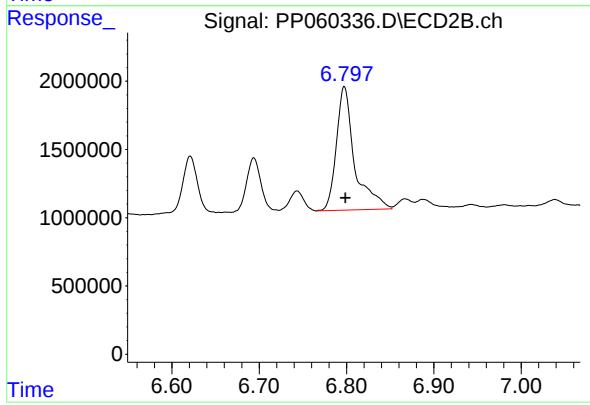

#30 AR-1254-5

R.T.: 6.797 min
Delta R.T.: -0.001 min
Response: 13157282
Conc: 103.83 ng/ml