

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092823\
 Data File : PP060352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Sep 2023 15:43
 Operator : YP\AJ
 Sample : 04642-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-01-09272023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/29/2023
 Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 28 17:03:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 27 11:30:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.531	3.685	34836698	25333231	15.556	17.019
2) SA Decachlor...	10.457	8.749	17903724	14890061	10.141	9.128

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092823\
Data File : PP060352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Sep 2023 15:43
Operator : YP\AJ
Sample : 04642-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAT-01-09272023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 28 17:03:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 27 11:30:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

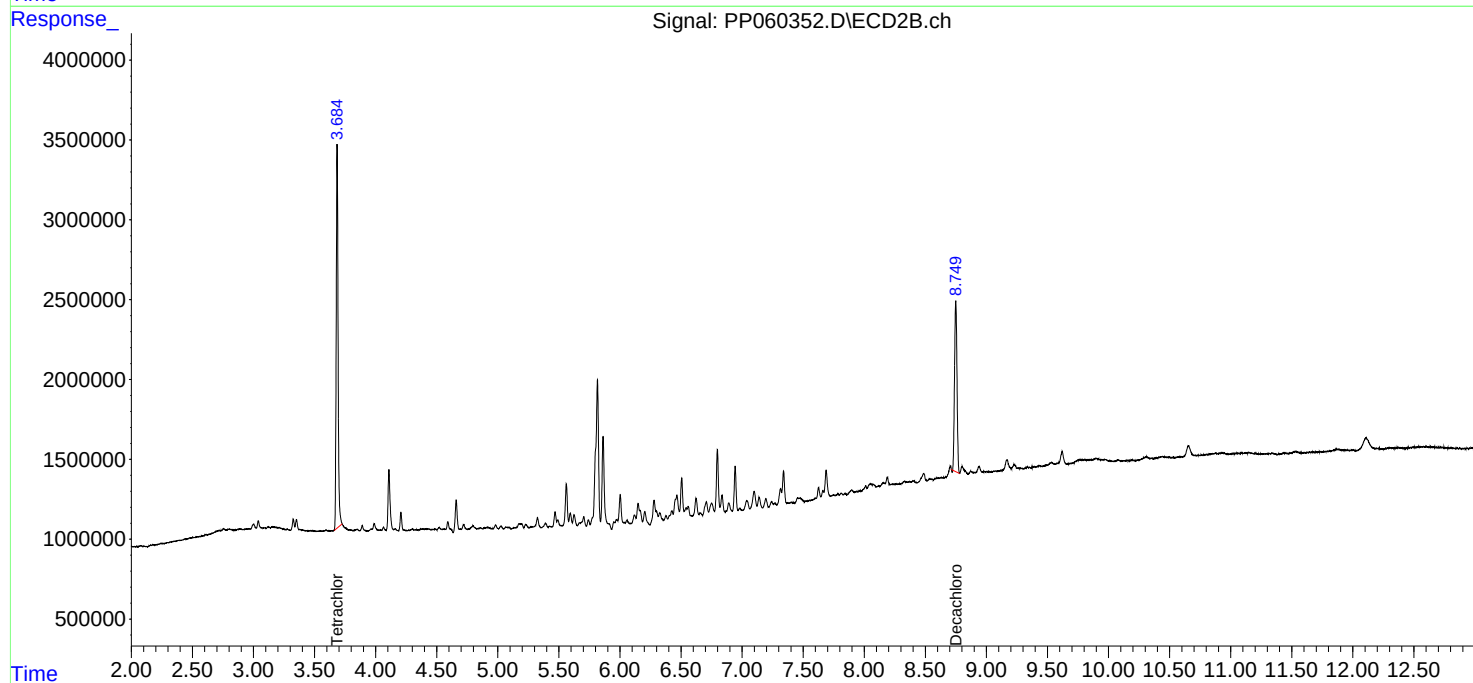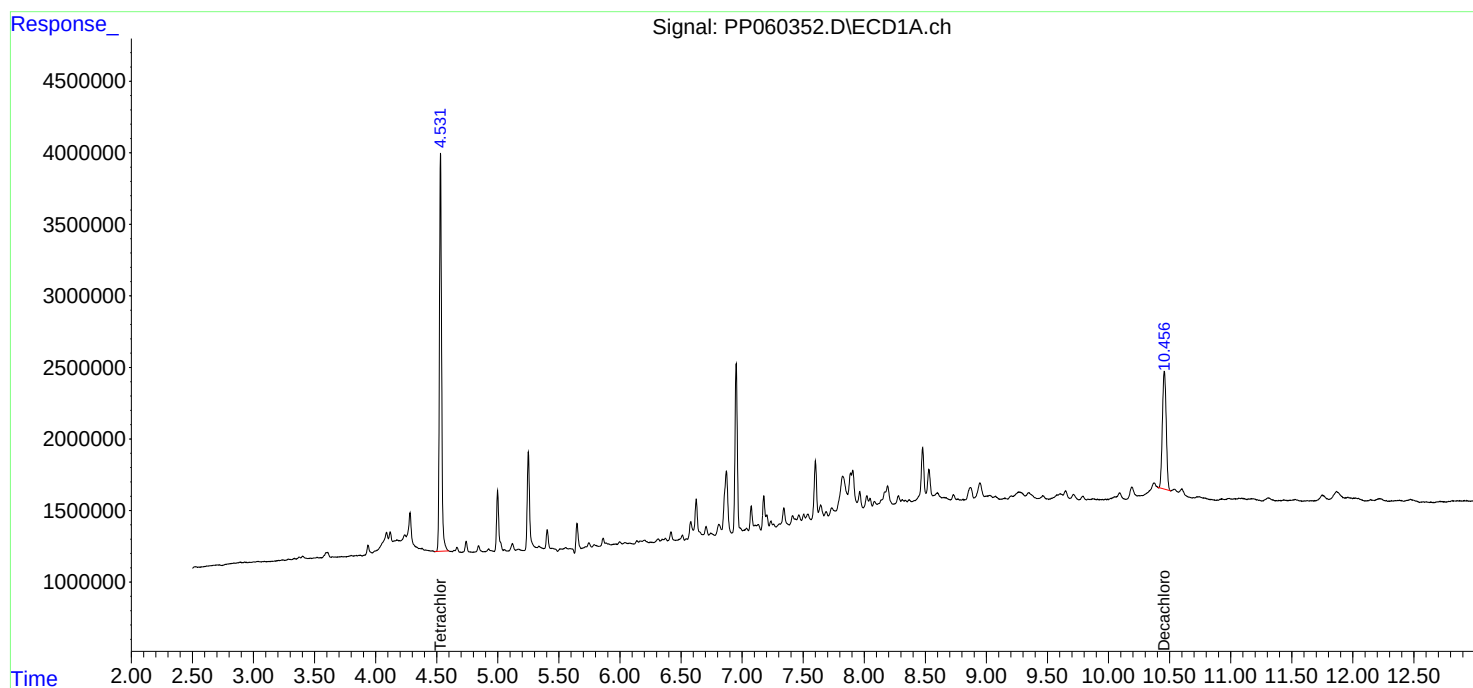

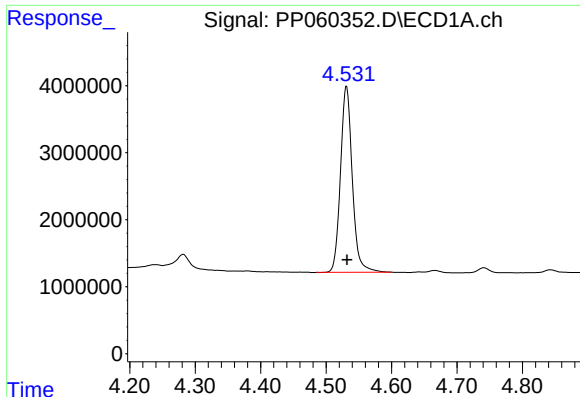


#1 Tetrachloro-m-xylene

R.T.: 4.531 min
Delta R.T.: 0.000 min
Response: 34836698
Conc: 15.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-01-09272023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/29/2023
Supervised By :Ankita Jodhani 09/29/2023

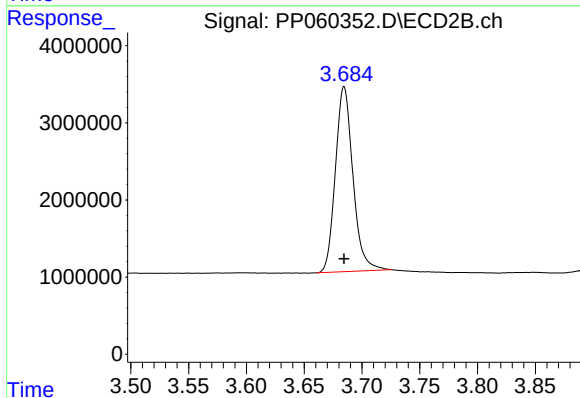


#1 Tetrachloro-m-xylene

R.T.: 3.685 min
Delta R.T.: 0.000 min
Response: 25333231
Conc: 17.02 ng/ml

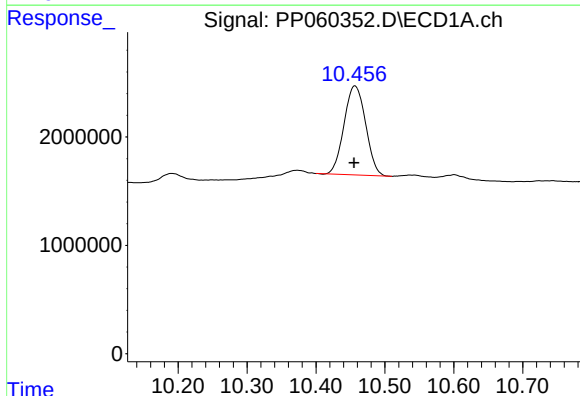

#2 Decachlorobiphenyl

R.T.: 10.457 min
Delta R.T.: 0.001 min
Response: 17903724
Conc: 10.14 ng/ml

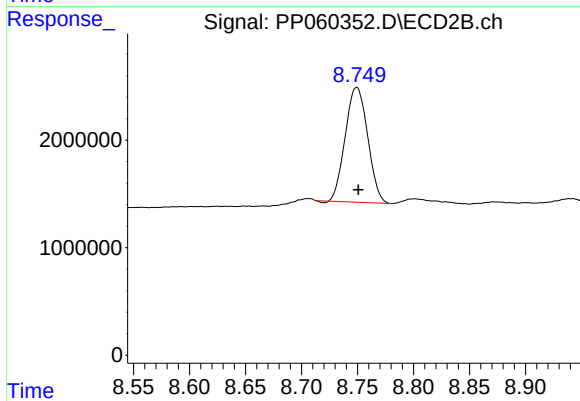

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.001 min
Response: 14890061
Conc: 9.13 ng/ml