

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039607.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2021 14:47
 Operator : AJ\MA
 Sample : M3975-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 03:02:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.908	3.998	715628	422449	22.605	25.926
2)	SA Decachlor...	10.933	9.334	467649	465609	21.557	21.307
Target Compounds							
30)	L6 AR-1254-5	8.507f	7.395	3633	14909	2.863	10.592 #
32)	L7 AR-1260-2	8.185	0.000	32646	0	23.581	N.D. #
36)	L8 AR-1262-1	0.000	7.395	0	14909	N.D.	21.148 #
39)	L8 AR-1262-4	9.502	0.000	53057	0	88.702	N.D. #
40)	L8 AR-1262-5	0.000	8.809	0	5725	N.D.	6.288 #
42)	L9 AR-1268-2	9.502	0.000	53057	0	20.598	N.D. #
44)	L9 AR-1268-4	0.000	8.809	0	5725	N.D.	5.562 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039607.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2021 14:47
Operator : AJ\MA
Sample : M3975-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 03:02:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

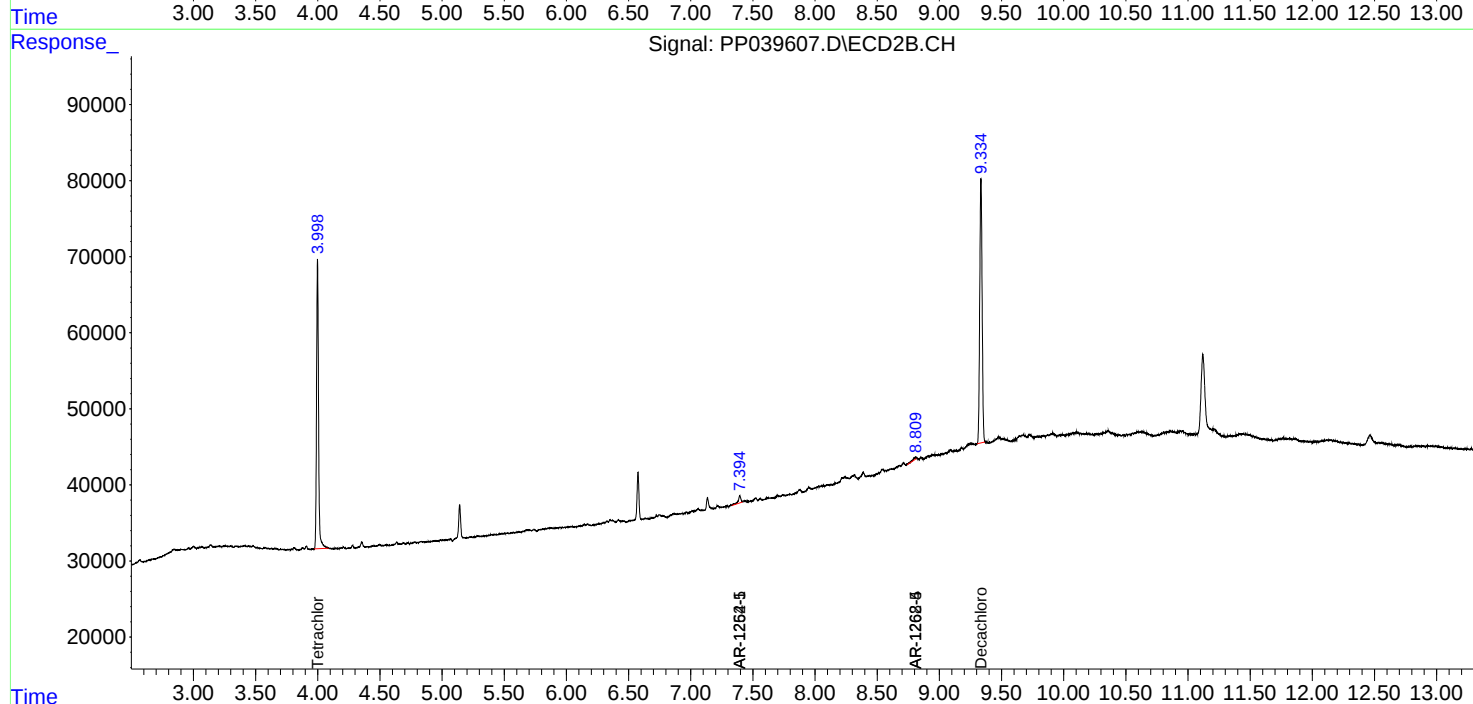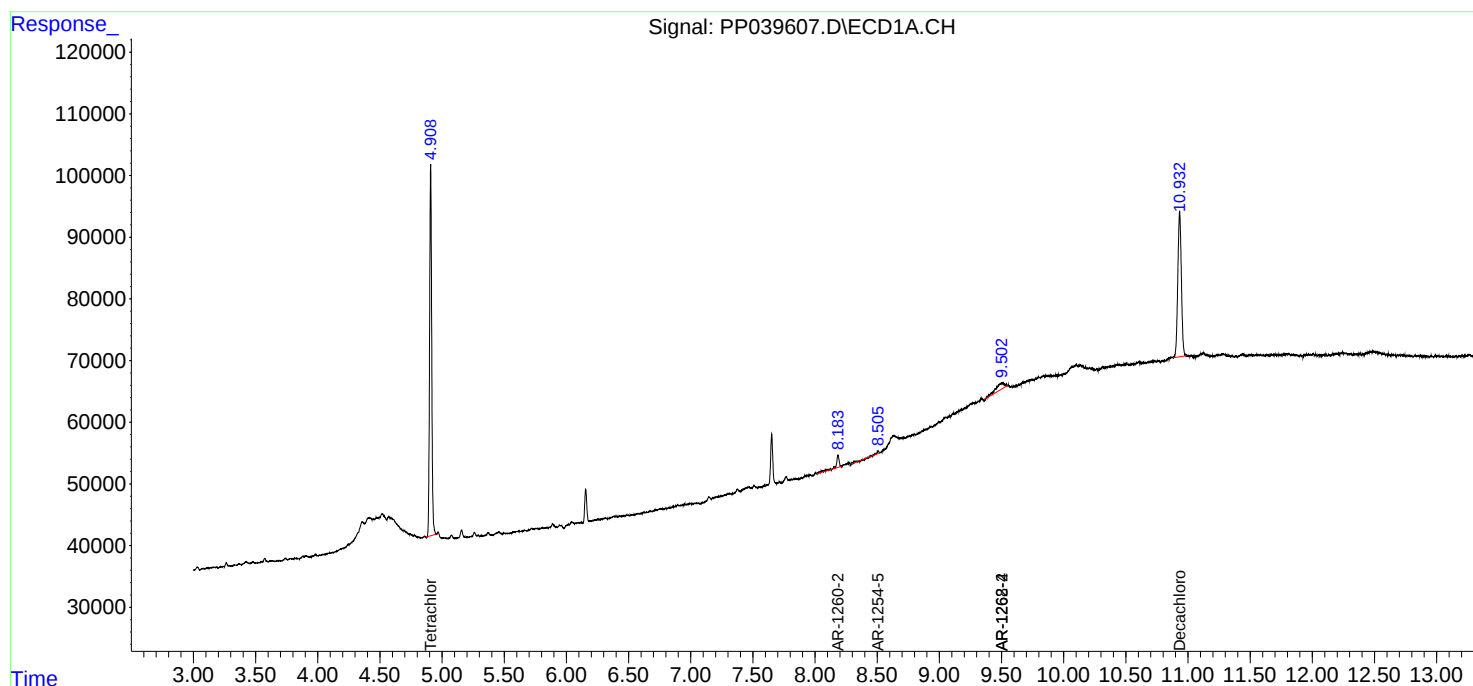


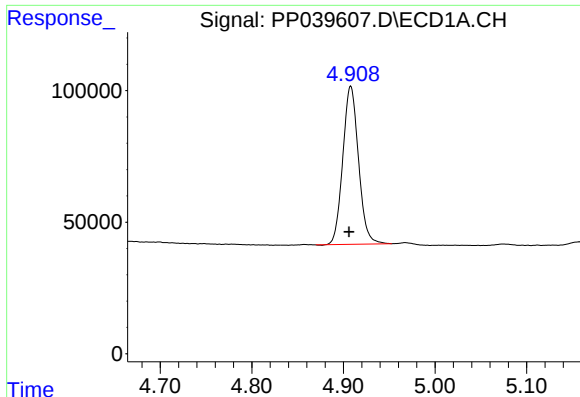

#1 Tetrachloro-m-xylene


R.T.: 4.908 min
Delta R.T.: 0.002 min
Response: 715628
Conc: 22.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

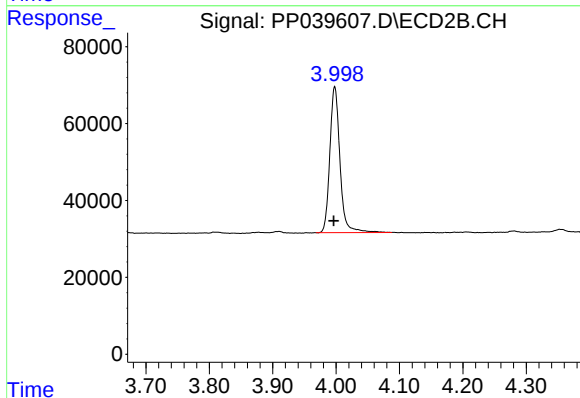


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: 0.002 min
Response: 422449
Conc: 25.93 ng/ml

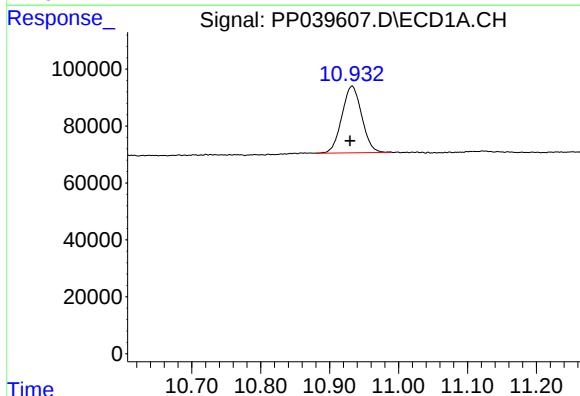


#2 Decachlorobiphenyl

R.T.: 10.933 min
Delta R.T.: 0.003 min
Response: 467649
Conc: 21.56 ng/ml

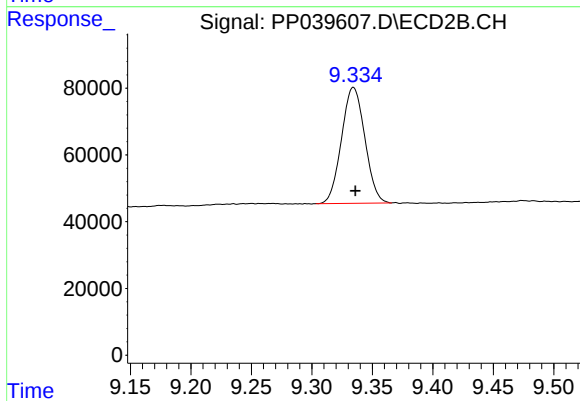

#2 Decachlorobiphenyl


R.T.: 9.334 min
Delta R.T.: -0.002 min
Response: 465609
Conc: 21.31 ng/ml

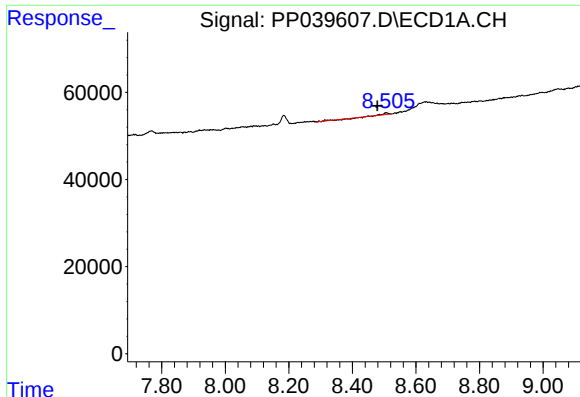

#30 AR-1254-5


R.T.: 8.507 min
Delta R.T.: 0.028 min
Response: 3633
Conc: 2.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

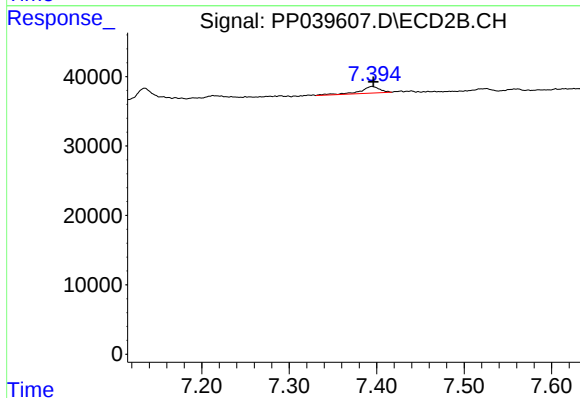


#30 AR-1254-5

R.T.: 7.395 min
Delta R.T.: -0.001 min
Response: 14909
Conc: 10.59 ng/ml

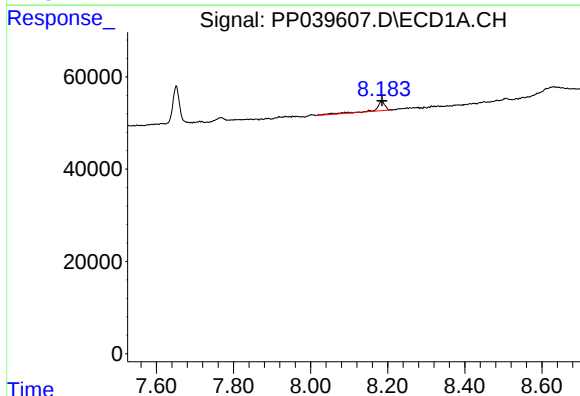


#32 AR-1260-2

R.T.: 8.185 min
Delta R.T.: -0.001 min
Response: 32646
Conc: 23.58 ng/ml

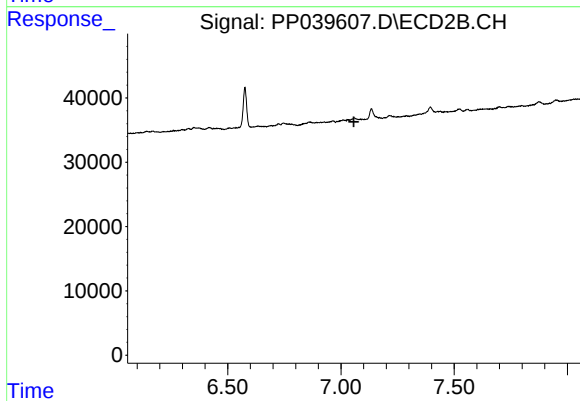

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.057 min
Response: 0
Conc: N.D.

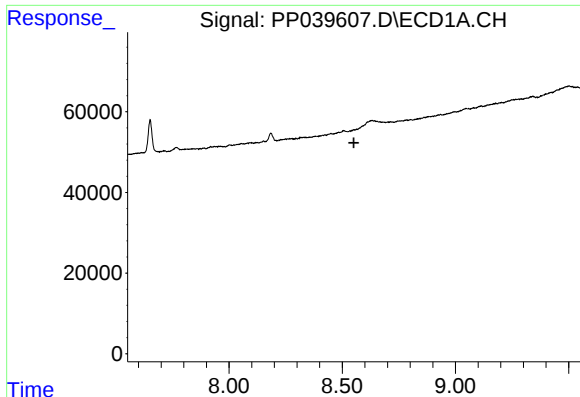

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

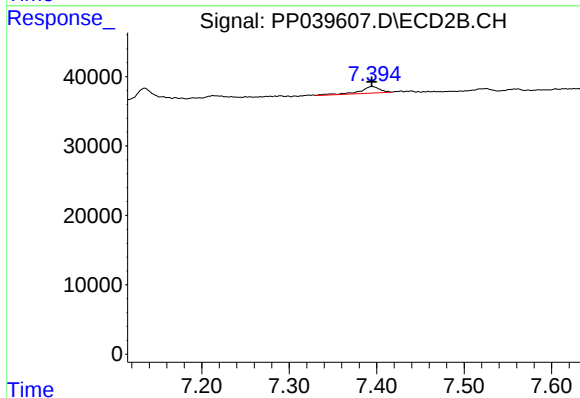


#36 AR-1262-1

R.T.: 7.395 min
Delta R.T.: 0.000 min
Response: 14909
Conc: 21.15 ng/ml

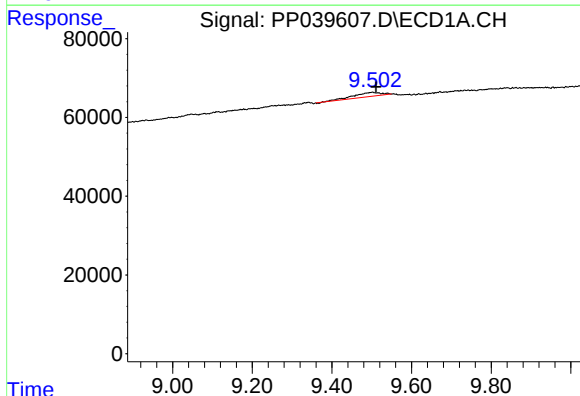


#39 AR-1262-4

R.T.: 9.502 min
Delta R.T.: -0.009 min
Response: 53057
Conc: 88.70 ng/ml

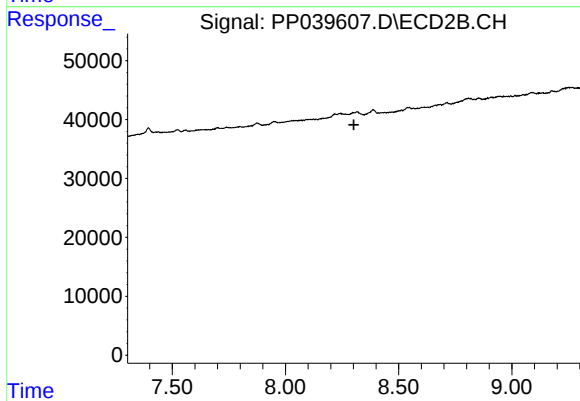

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.302 min
Response: 0
Conc: N.D.

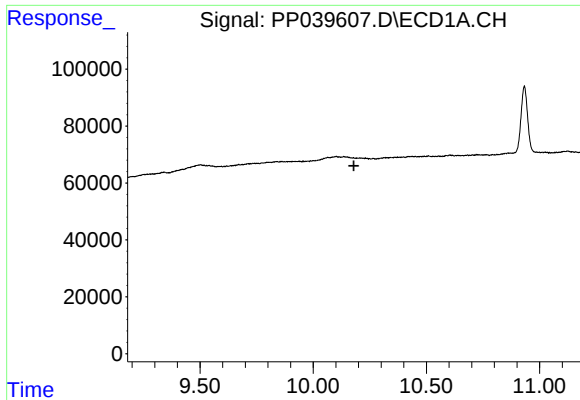

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

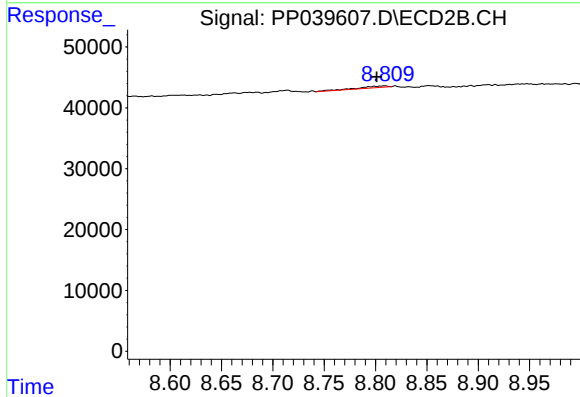


#40 AR-1262-5

R.T.: 8.809 min
Delta R.T.: 0.008 min
Response: 5725
Conc: 6.29 ng/ml

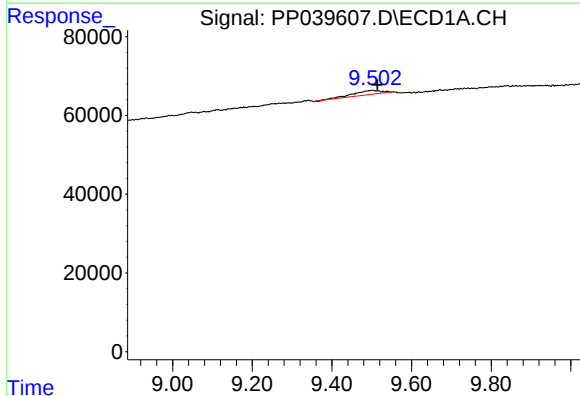


#42 AR-1268-2

R.T.: 9.502 min
Delta R.T.: -0.012 min
Response: 53057
Conc: 20.60 ng/ml

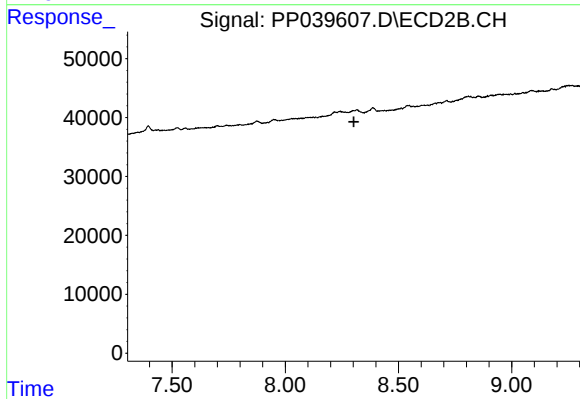

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.303 min
Response: 0
Conc: N.D.

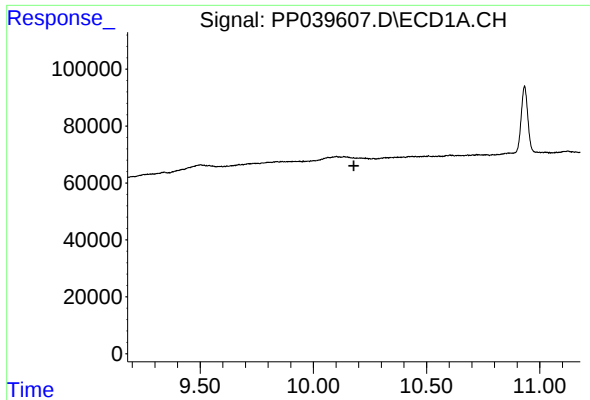

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 10.179 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

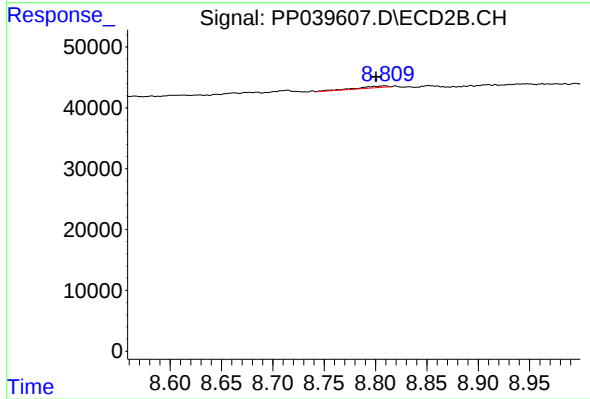

#44 AR-1268-4

R.T.: 8.809 min
Delta R.T.: 0.009 min
Response: 5725
Conc: 5.56 ng/ml