

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039646.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 3:37
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 04:16:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.904	3.994	682085	398440	21.546	24.453
2)	SA Decachlor...	10.928	9.330	503834	534239	23.225	24.448
Target Compounds							
20)	L4 AR-1242-5	0.000	6.163f	0	18646	N.D.	35.137 #
24)	L5 AR-1248-4	7.145f	0.000	79988	0	73.683	N.D. #
25)	L5 AR-1248-5	0.000	6.163f	0	18646	N.D.	26.452 #
26)	L6 AR-1254-1	7.145	6.163f	79988	18646	73.282	17.909 #
28)	L6 AR-1254-3	7.766	0.000	46767	0	28.107	N.D. #
32)	L7 AR-1260-2	0.000	7.030f	0	33751	N.D.	26.352 #
33)	L7 AR-1260-3	0.000	7.208	0	13157	N.D.	10.936 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039646.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 3:37
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 04:16:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

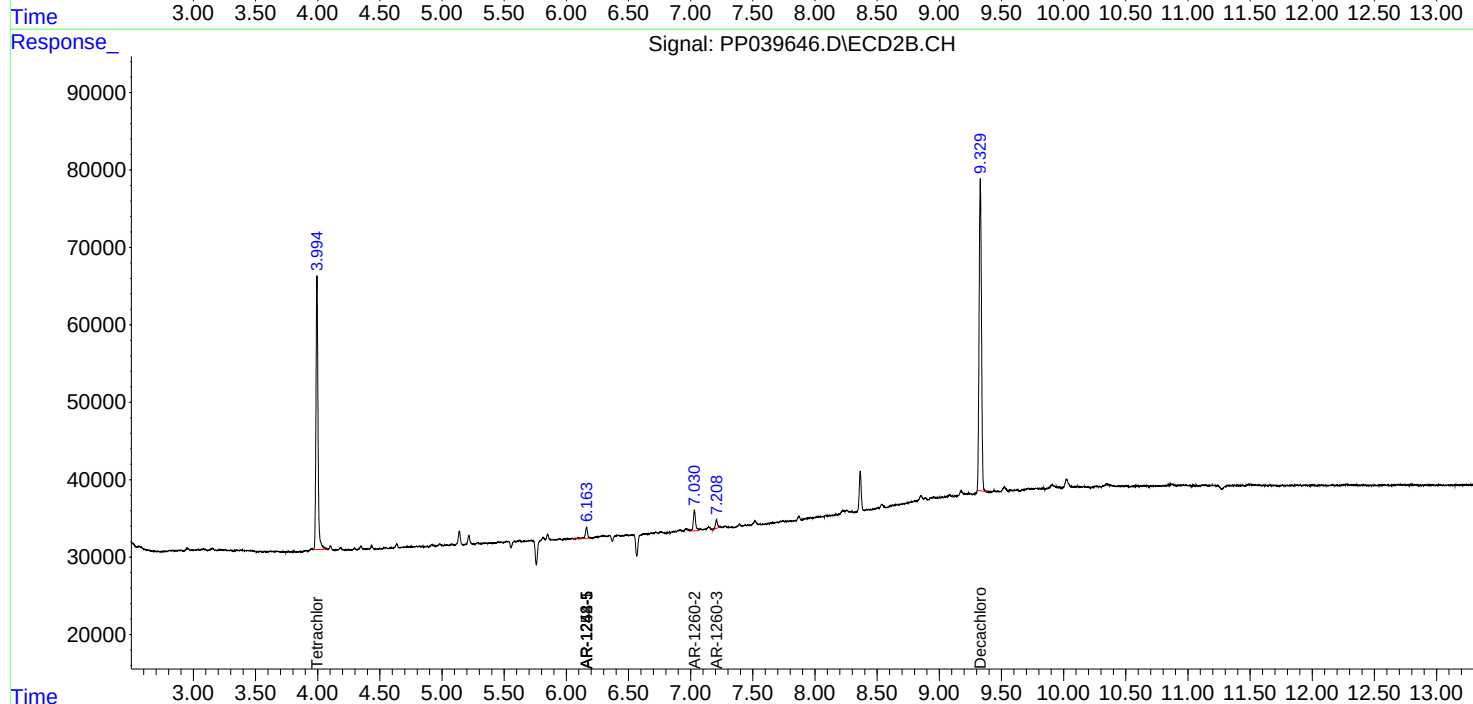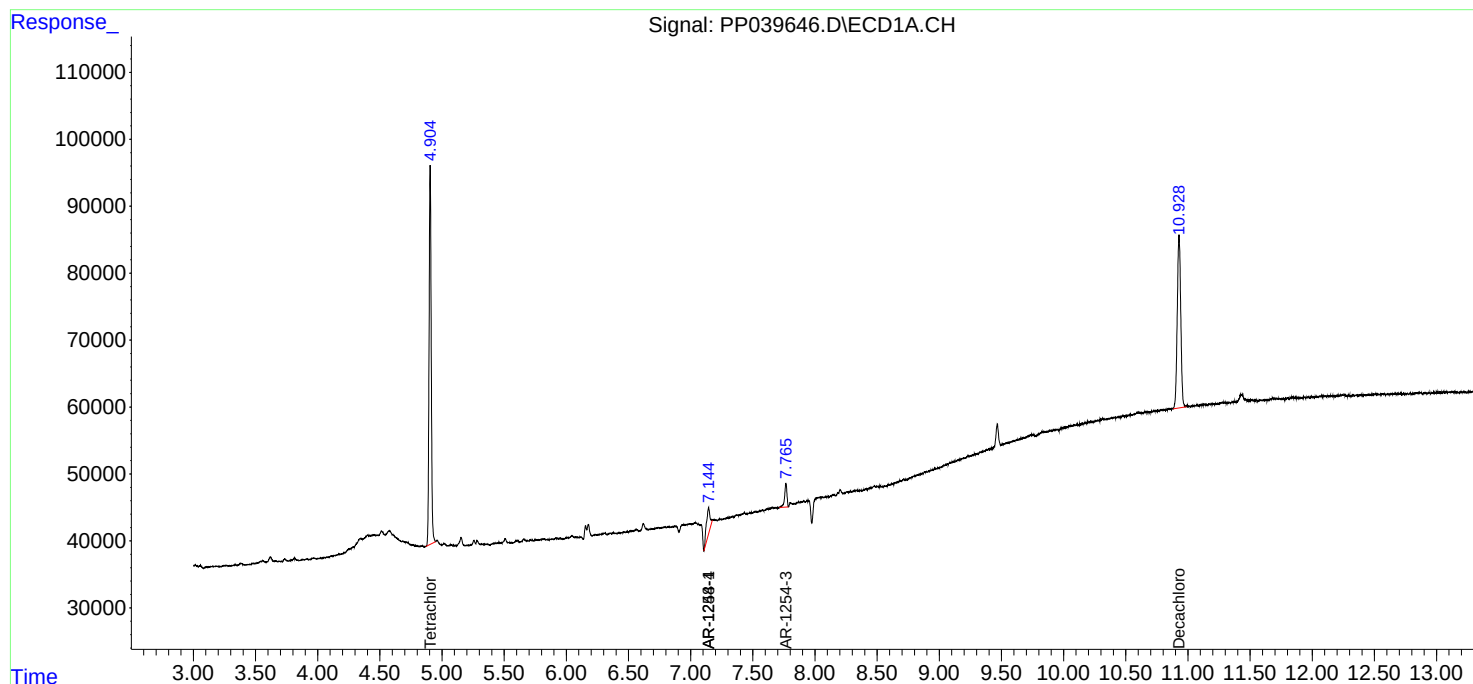


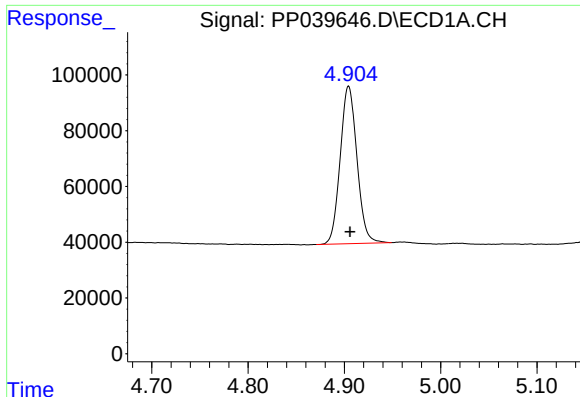

#1 Tetrachloro-m-xylene


R.T.: 4.904 min
Delta R.T.: -0.002 min
Response: 682085
Conc: 21.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

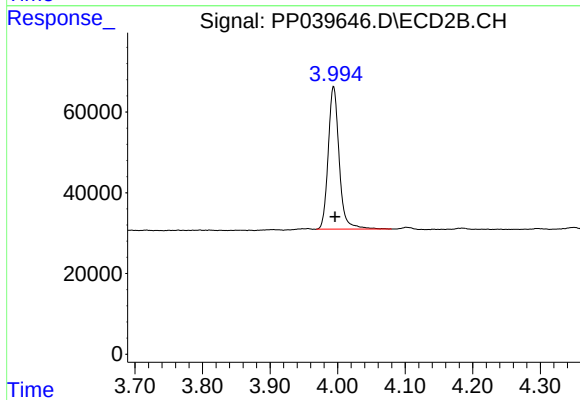


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 398440
Conc: 24.45 ng/ml

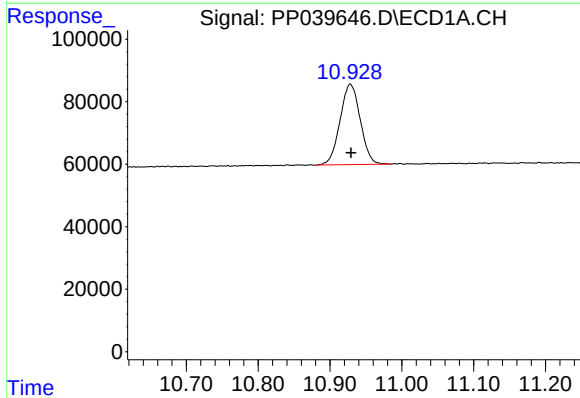


#2 Decachlorobiphenyl

R.T.: 10.928 min
Delta R.T.: -0.001 min
Response: 503834
Conc: 23.22 ng/ml

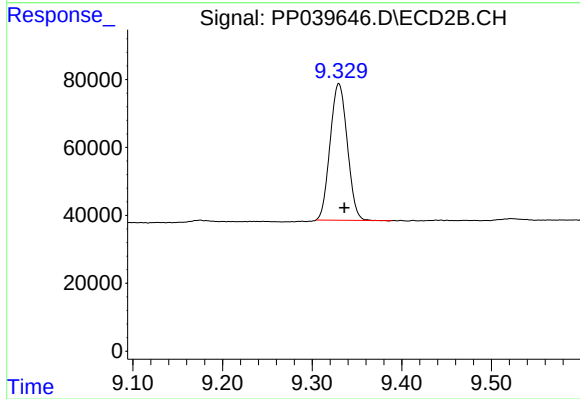

#2 Decachlorobiphenyl


R.T.: 9.330 min
Delta R.T.: -0.006 min
Response: 534239
Conc: 24.45 ng/ml

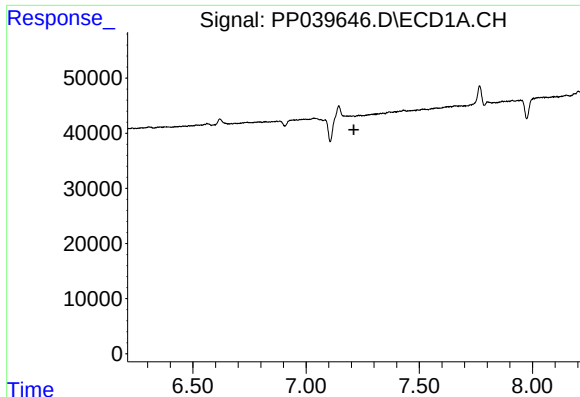

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

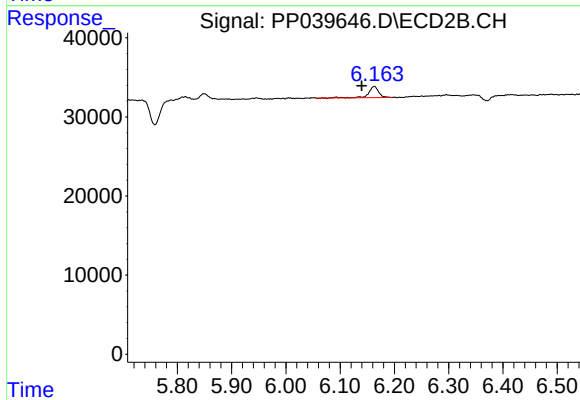


#20 AR-1242-5

R.T.: 6.163 min
Delta R.T.: 0.023 min
Response: 18646
Conc: 35.14 ng/ml

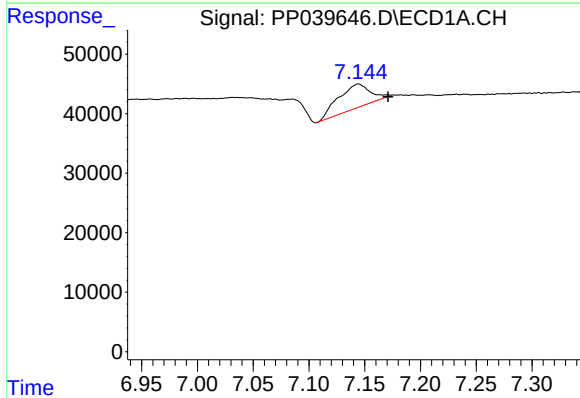


#24 AR-1248-4

R.T.: 7.145 min
Delta R.T.: -0.026 min
Response: 79988
Conc: 73.68 ng/ml

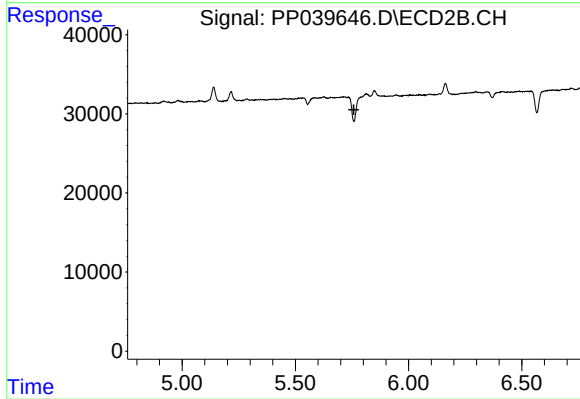

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.758 min
Response: 0
Conc: N.D.

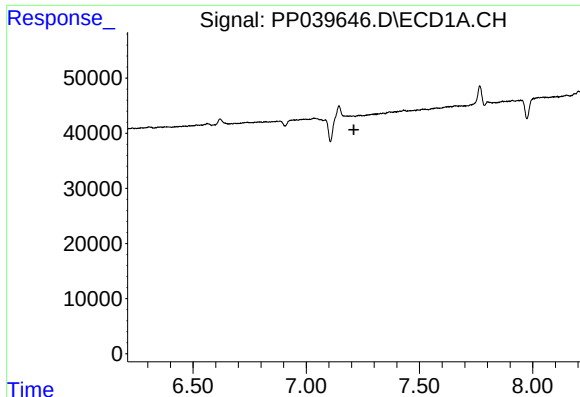

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

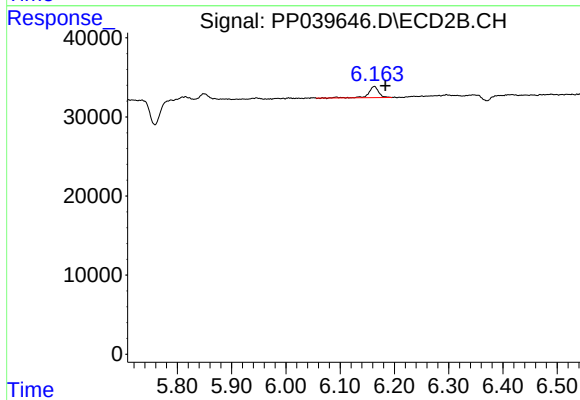


#25 AR-1248-5

R.T.: 6.163 min
Delta R.T.: -0.020 min
Response: 18646
Conc: 26.45 ng/ml

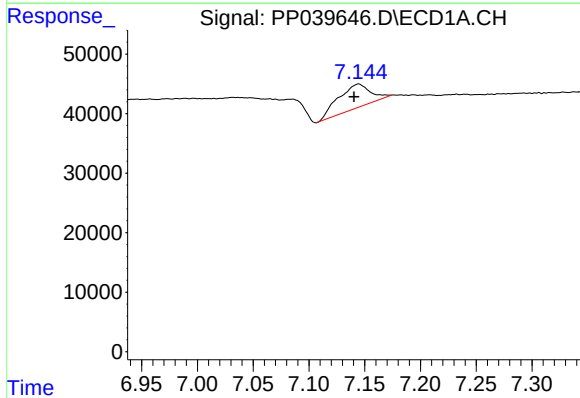


#26 AR-1254-1

R.T.: 7.145 min
Delta R.T.: 0.004 min
Response: 79988
Conc: 73.28 ng/ml

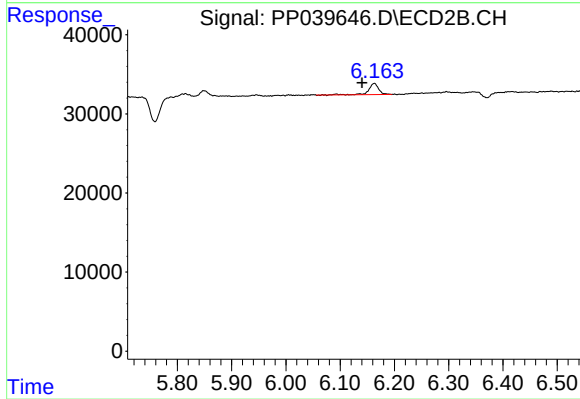

#26 AR-1254-1


R.T.: 6.163 min
Delta R.T.: 0.022 min
Response: 18646
Conc: 17.91 ng/ml

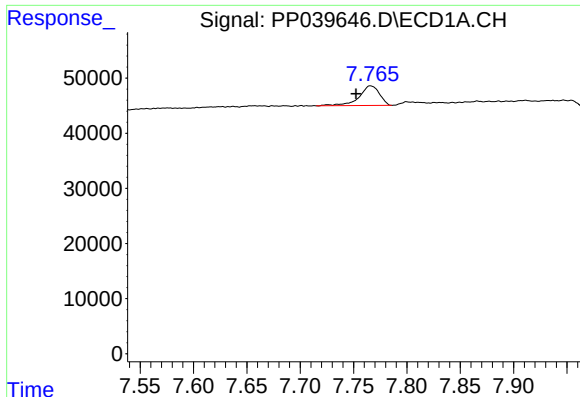

#28 AR-1254-3


R.T.: 7.766 min
Delta R.T.: 0.013 min
Response: 46767
Conc: 28.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

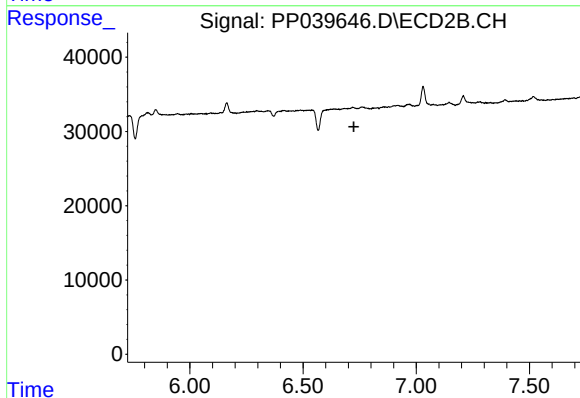


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.724 min
Response: 0
Conc: N.D.

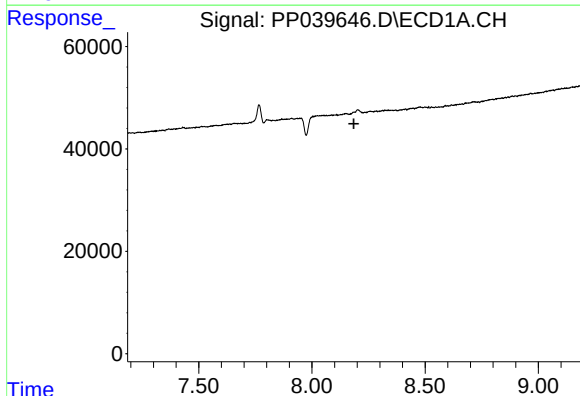


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.186 min
Response: 0
Conc: N.D.

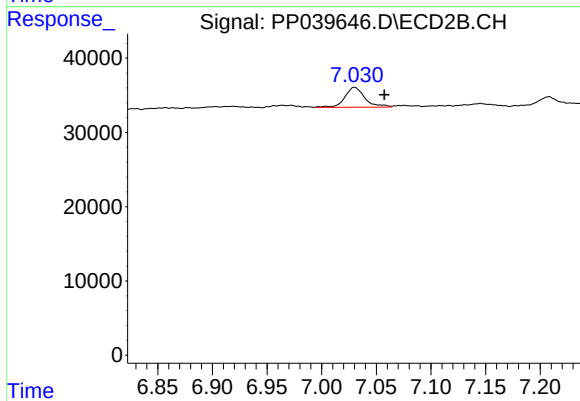

#32 AR-1260-2


R.T.: 7.030 min
Delta R.T.: -0.027 min
Response: 33751
Conc: 26.35 ng/ml

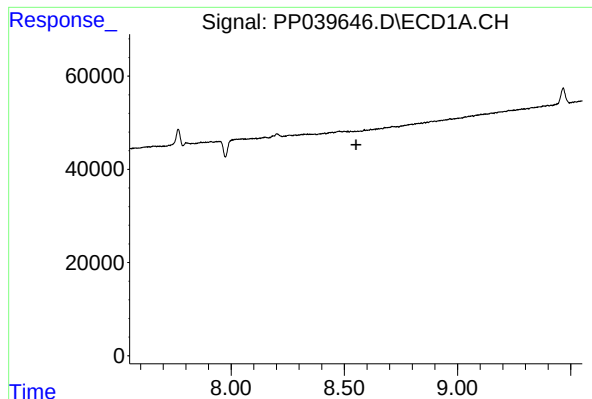

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

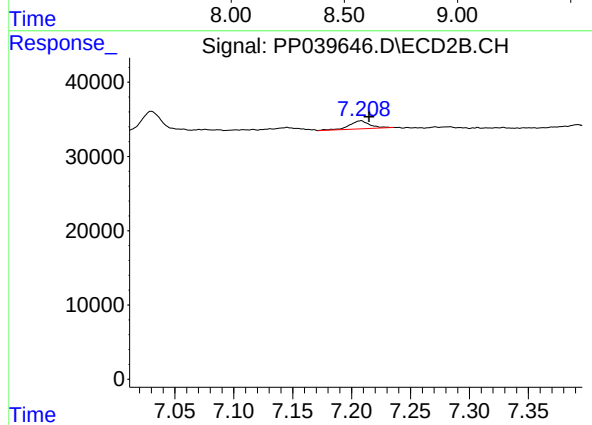

#33 AR-1260-3

R.T.: 7.208 min
Delta R.T.: -0.007 min
Response: 13157
Conc: 10.94 ng/ml