

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039620.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2021 18:25
 Operator : AJ\MA
 Sample : M3971-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RP-COMP-3

Manual Integrations
 APPROVED

mohammad
 9/30/2021 9:30:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 03:25:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.906	3.996	768727	405772	24.283	24.903
2) SA Decachlor...	10.929	9.332	475004	493887	21.896	22.601
Target Compounds						
31) L7 AR-1260-1	7.918	6.858	59066	29702	48.065	27.581m#
32) L7 AR-1260-2	8.183	7.059	54688	48153	39.502	37.597
33) L7 AR-1260-3	8.551	7.214	29855	29204	36.095	24.275 #
34) L7 AR-1260-4	8.780	7.698	29249	28105	29.338	30.177
35) L7 AR-1260-5	9.105	7.945	52234	77576	27.564	36.167 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039620.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2021 18:25
Operator : AJ\MA
Sample : M3971-07
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleID :
RP-COMP-3


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 03:25:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

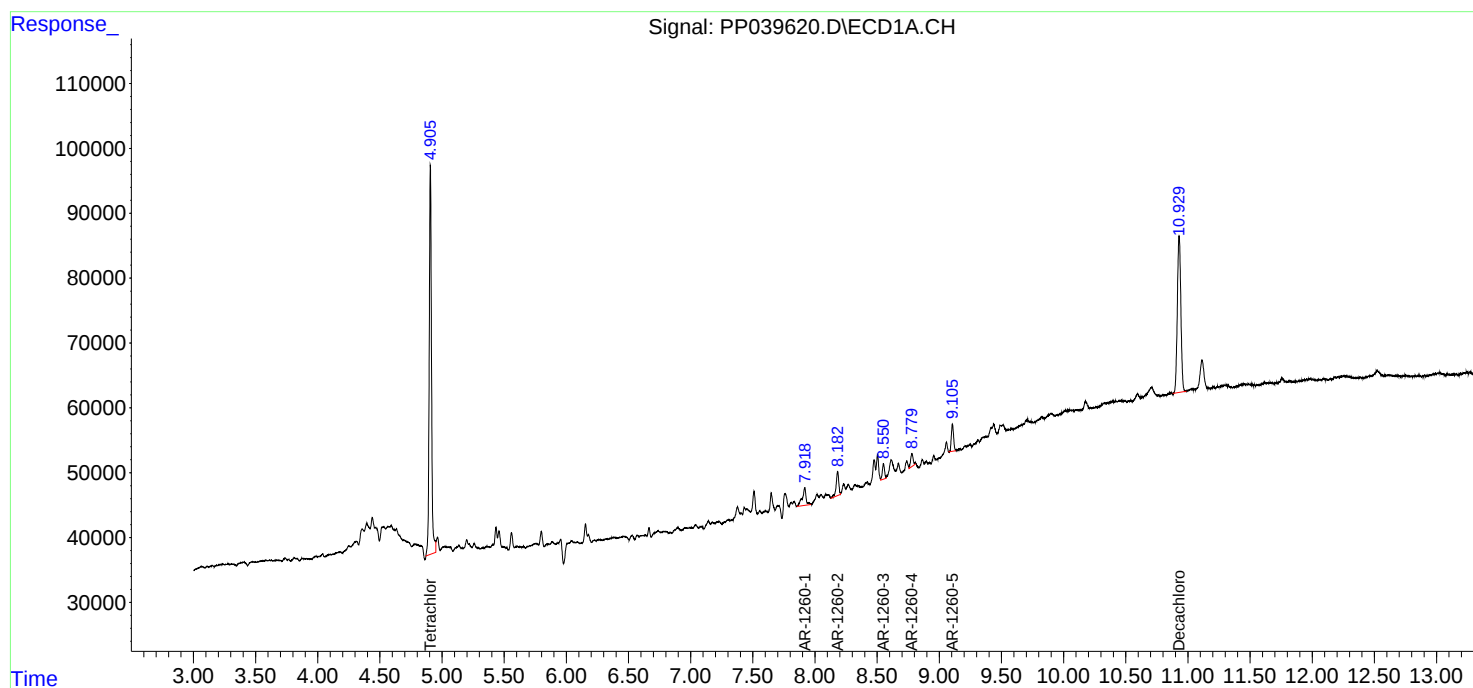

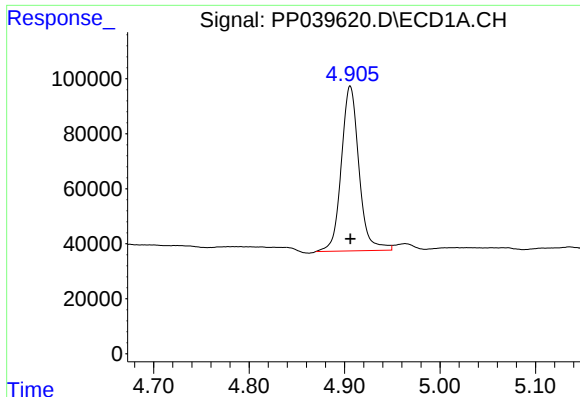


#1 Tetrachloro-m-xylene

R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 768727
Conc: 24.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
RP-COMP-3


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:47 AM

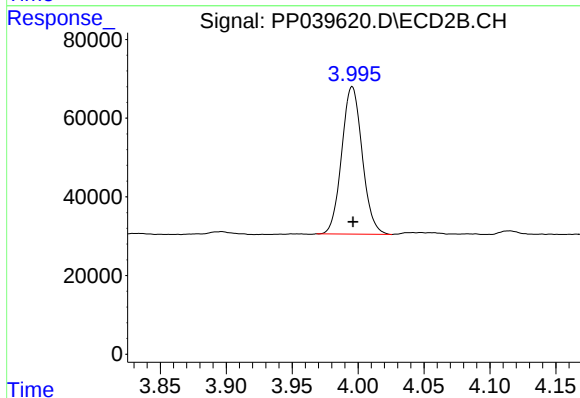


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 405772
Conc: 24.90 ng/ml

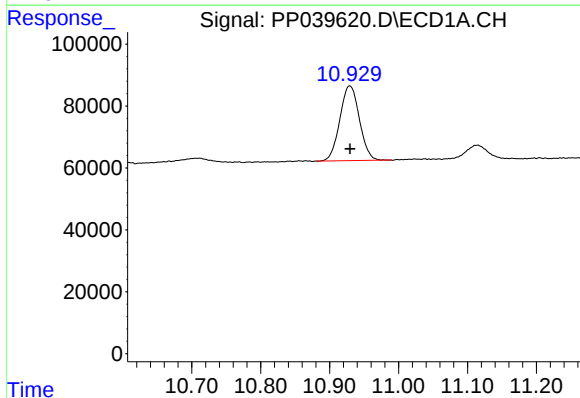


#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: 0.000 min
Response: 475004
Conc: 21.90 ng/ml

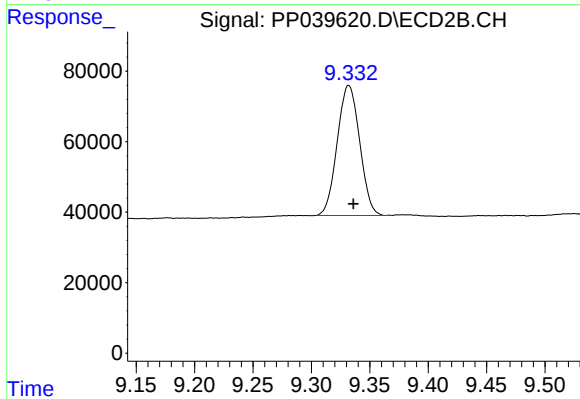

#2 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: -0.004 min
Response: 493887
Conc: 22.60 ng/ml

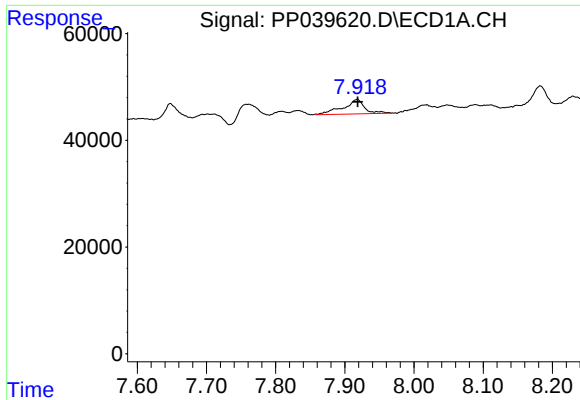


#31 AR-1260-1

R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 59066
Conc: 48.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
RP-COMP-3


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:47 AM

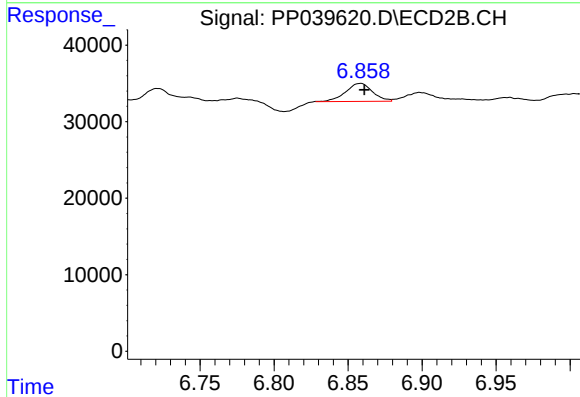


#31 AR-1260-1

R.T.: 6.858 min
Delta R.T.: -0.003 min
Response: 29702
Conc: 27.58 ng/ml m

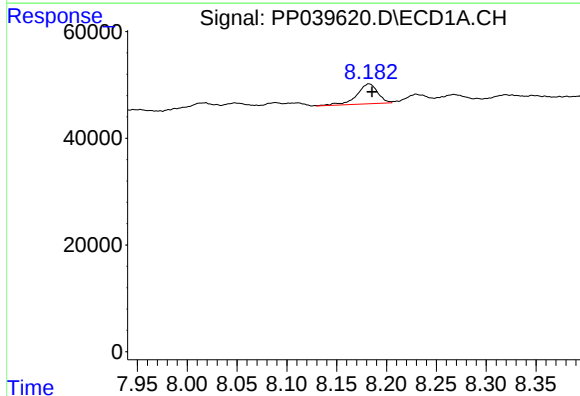


#32 AR-1260-2

R.T.: 8.183 min
Delta R.T.: -0.003 min
Response: 54688
Conc: 39.50 ng/ml

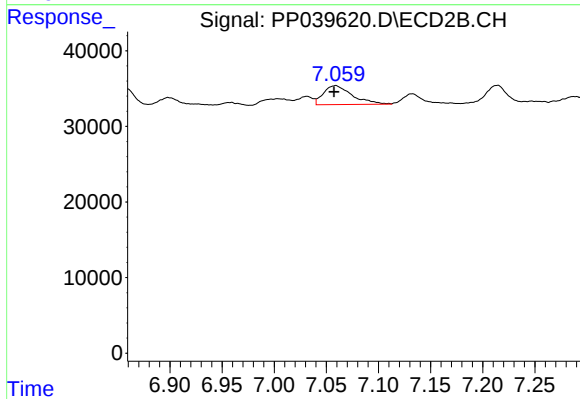

#32 AR-1260-2

R.T.: 7.059 min
Delta R.T.: 0.001 min
Response: 48153
Conc: 37.60 ng/ml

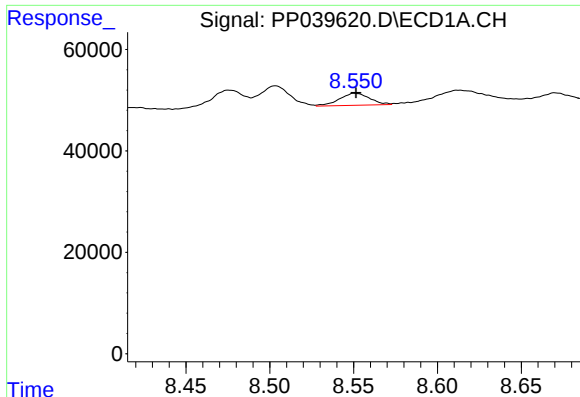


#33 AR-1260-3

R.T.: 8.551 min
Delta R.T.: 0.000 min
Response: 29855
Conc: 36.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
RP-COMP-3


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:47 AM

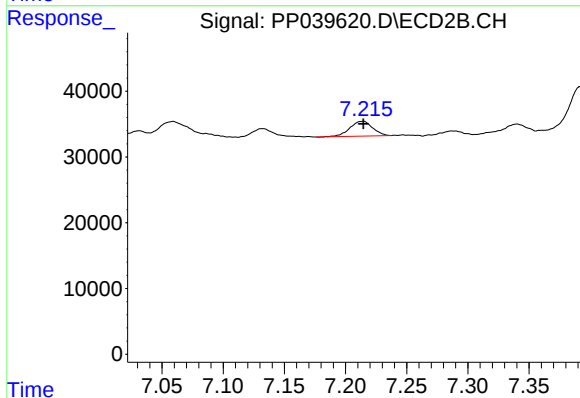


#33 AR-1260-3

R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 29204
Conc: 24.28 ng/ml

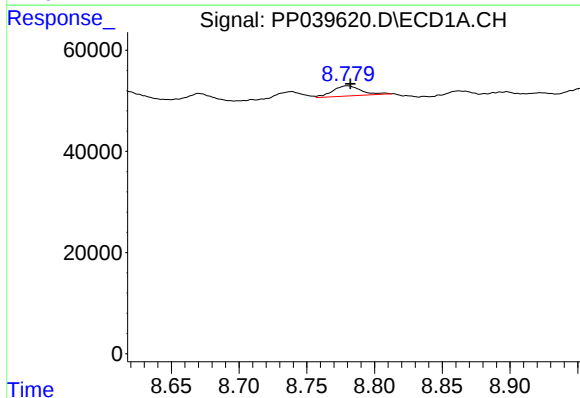


#34 AR-1260-4

R.T.: 8.780 min
Delta R.T.: -0.002 min
Response: 29249
Conc: 29.34 ng/ml

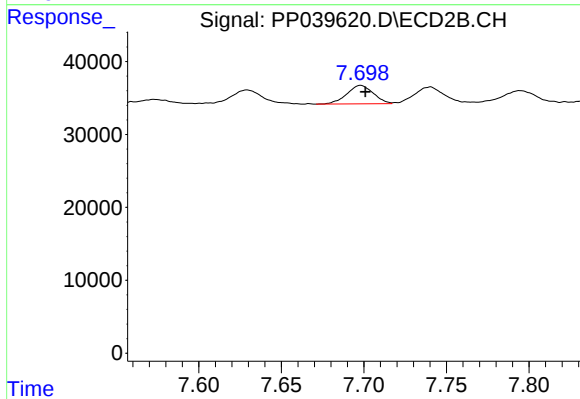

#34 AR-1260-4

R.T.: 7.698 min
Delta R.T.: -0.003 min
Response: 28105
Conc: 30.18 ng/ml

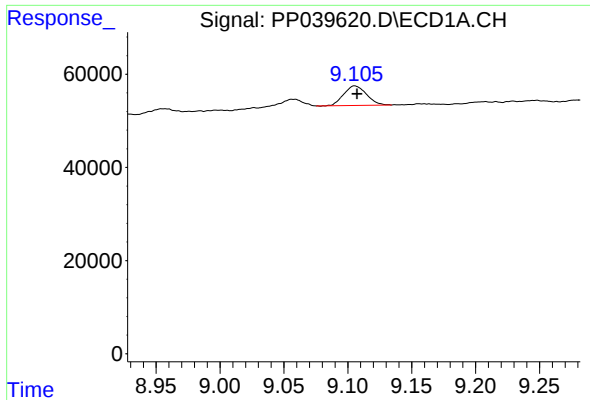


#35 AR-1260-5

R.T.: 9.105 min
Delta R.T.: -0.002 min
Response: 52234
Conc: 27.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
RP-COMP-3

Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:47 AM

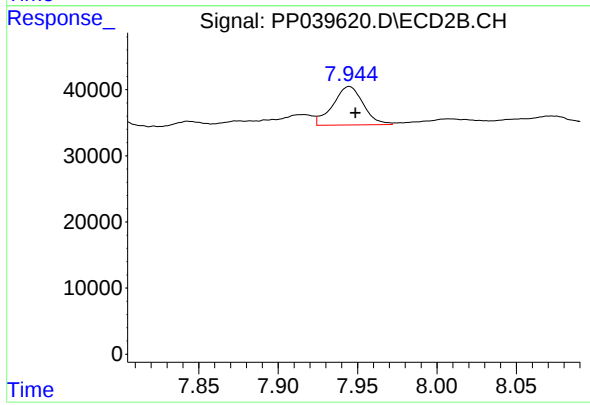

#35 AR-1260-5

R.T.: 7.945 min
Delta R.T.: -0.004 min
Response: 77576
Conc: 36.17 ng/ml