

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039621.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Sep 2021 18:42
 Operator : AJ\MA
 Sample : M3971-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KEARNY-COMP

Manual Integrations
 APPROVED

mohammad
 9/30/2021 9:30:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 03:26:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.906	3.996	734855	401038	23.213	24.612
2)	SA Decachlor...	10.929	9.331	502854	540501	23.179m	24.734m
Target Compounds							
26)	L6 AR-1254-1	7.140	6.139	131291	96575	120.284	92.760
27)	L6 AR-1254-2	7.371	6.297	238458	86953	147.628	90.227 #
28)	L6 AR-1254-3	7.754	6.721	348677	216133	209.559	143.672 #
29)	L6 AR-1254-4	8.047	6.959	90278	54491	73.906	56.588m
30)	L6 AR-1254-5	8.476	7.393	234285	353558	184.651	251.189 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039621.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Sep 2021 18:42
Operator : AJ\MA
Sample : M3971-10
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
KEARNY-COMP


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 03:26:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

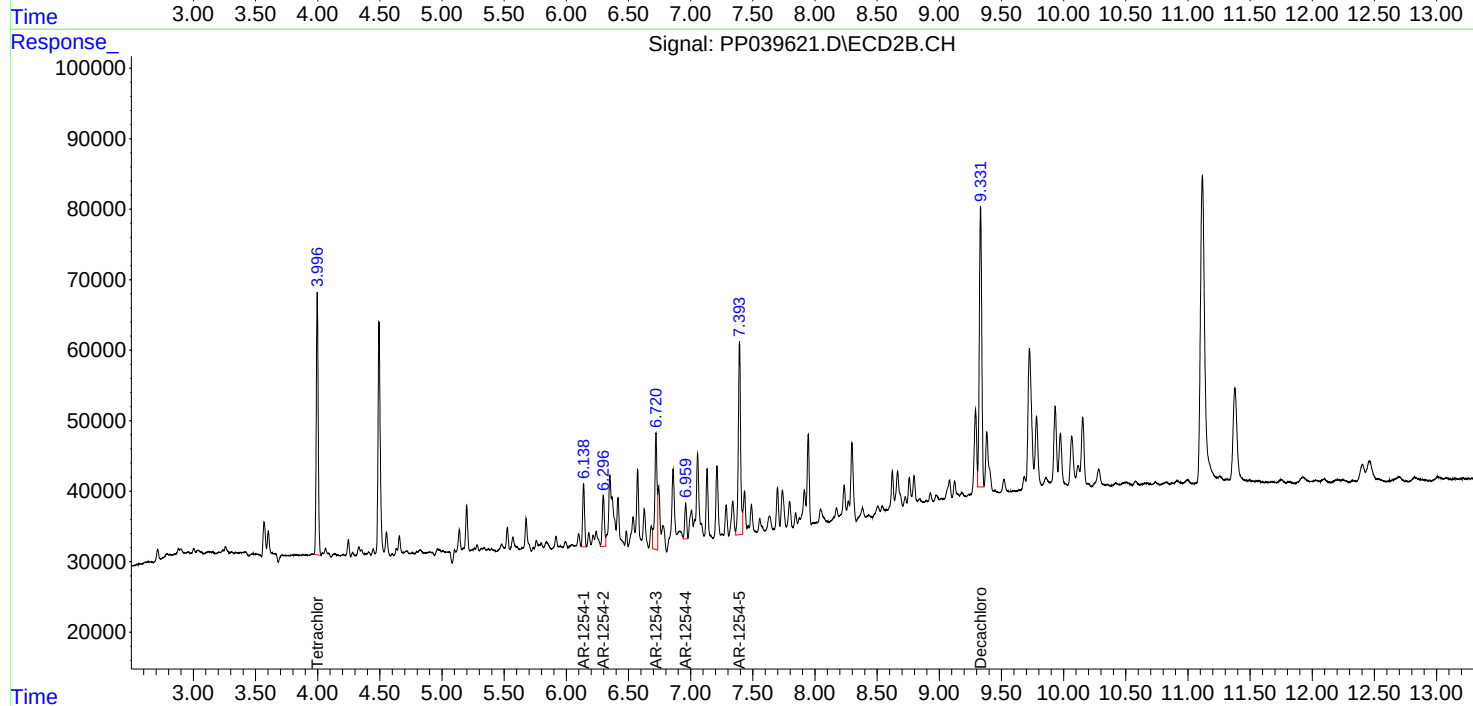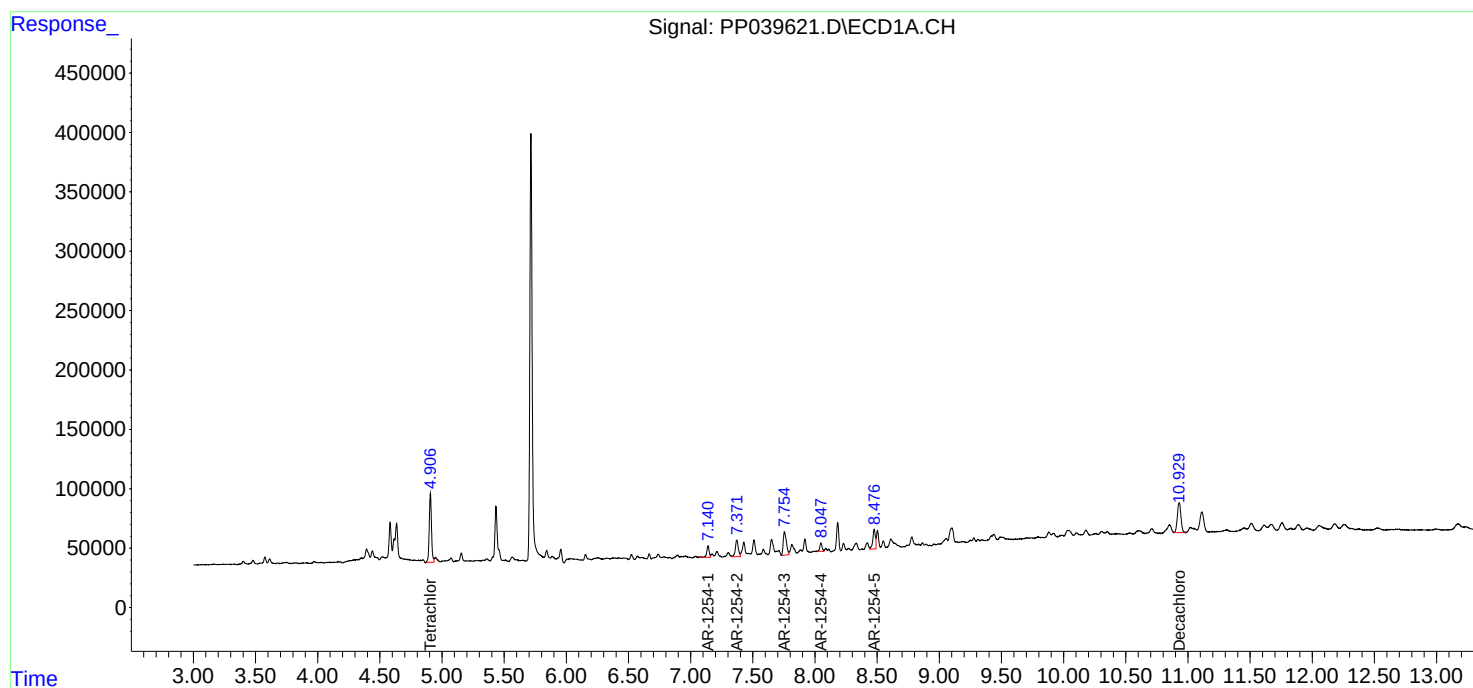

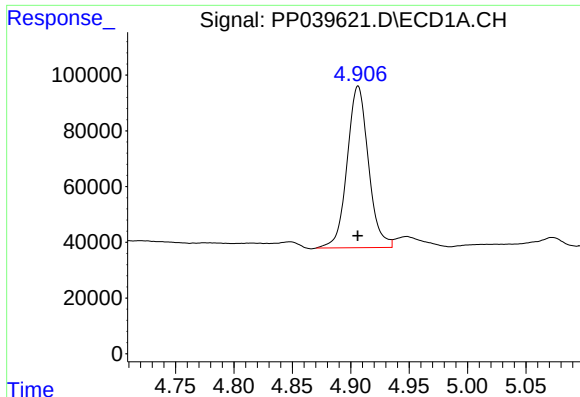


#1 Tetrachloro-m-xylene

R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 734855
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
KEARNY-COMP


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:50 AM

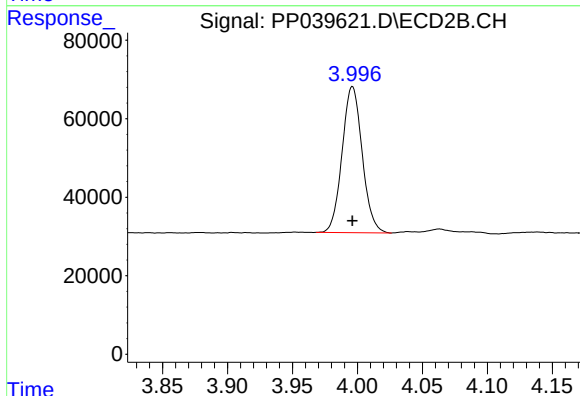


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 401038
Conc: 24.61 ng/ml

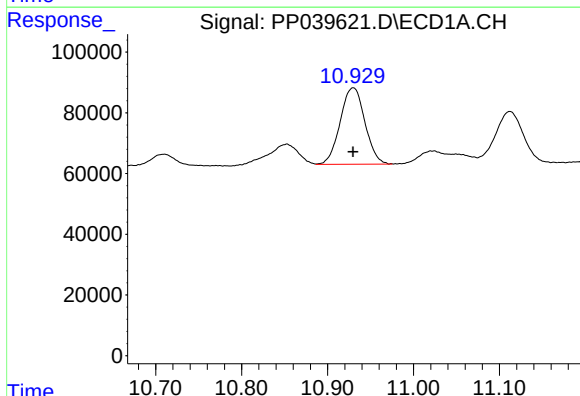


#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: 0.000 min
Response: 502854
Conc: 23.18 ng/ml m

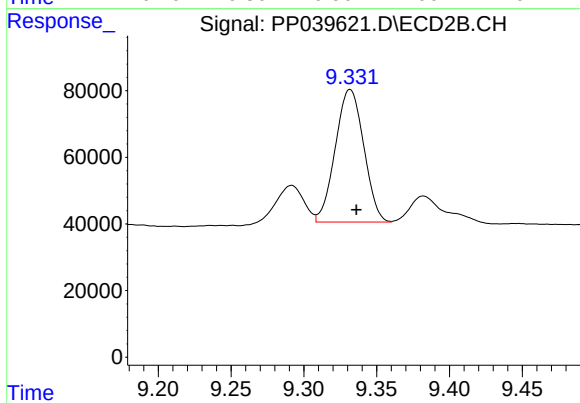

#2 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: -0.005 min
Response: 540501
Conc: 24.73 ng/ml m

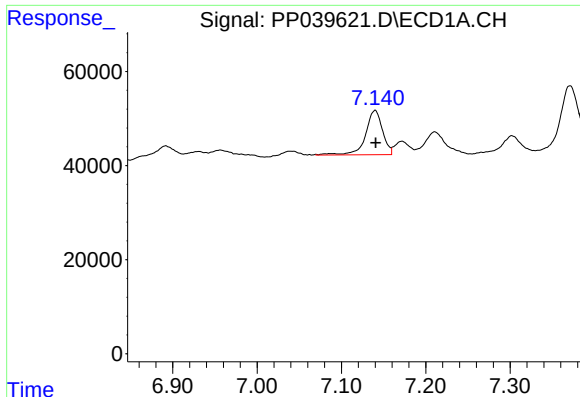


#26 AR-1254-1

R.T.: 7.140 min
Delta R.T.: 0.000 min
Response: 131291
Conc: 120.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
KEARNY-COMP


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:50 AM

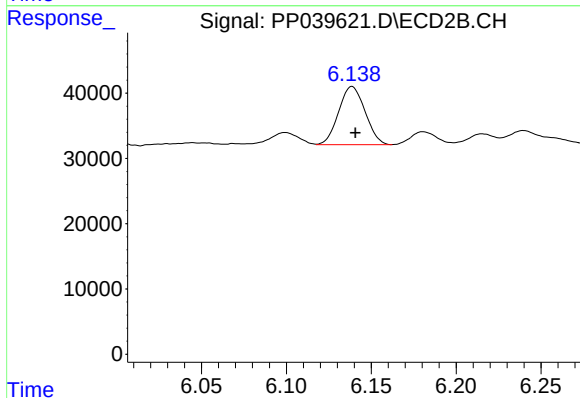


#26 AR-1254-1

R.T.: 6.139 min
Delta R.T.: -0.002 min
Response: 96575
Conc: 92.76 ng/ml

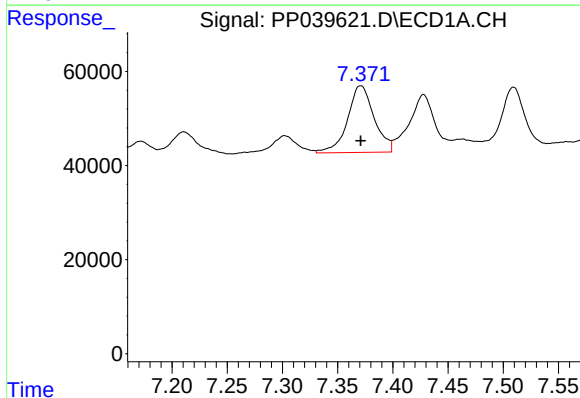


#27 AR-1254-2

R.T.: 7.371 min
Delta R.T.: 0.000 min
Response: 238458
Conc: 147.63 ng/ml

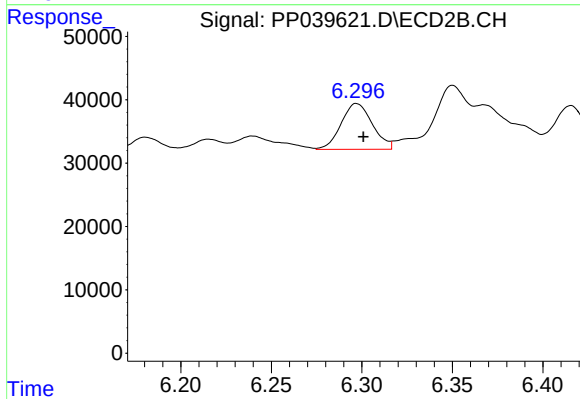

#27 AR-1254-2

R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 86953
Conc: 90.23 ng/ml

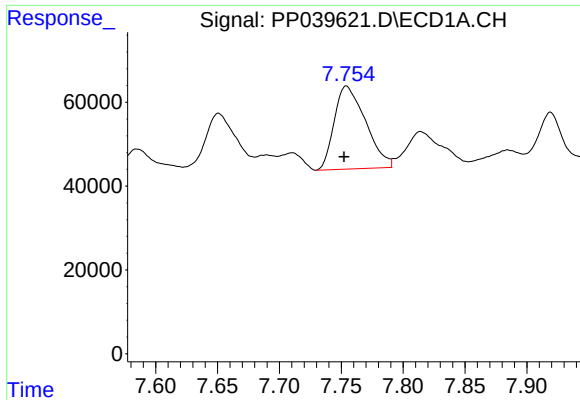


#28 AR-1254-3

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 348677
Conc: 209.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
KEARNY-COMP


Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:50 AM

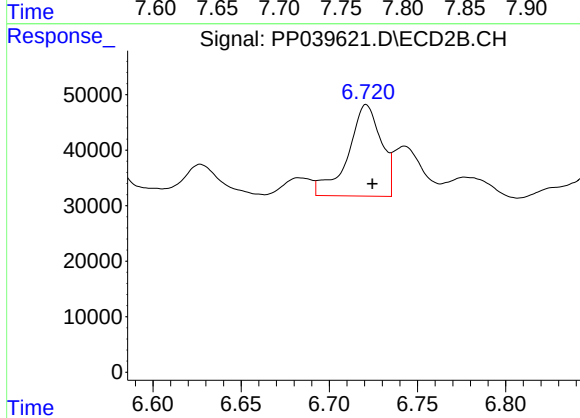


#28 AR-1254-3

R.T.: 6.721 min
Delta R.T.: -0.003 min
Response: 216133
Conc: 143.67 ng/ml

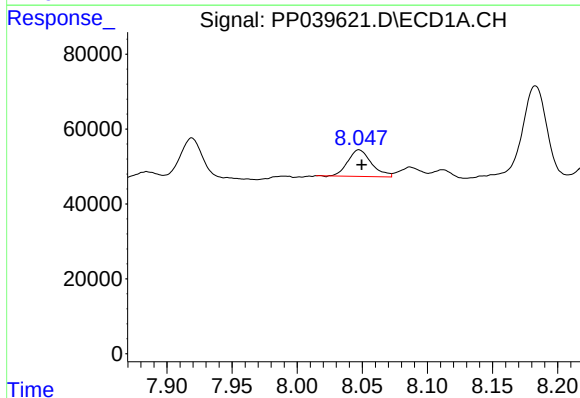


#29 AR-1254-4

R.T.: 8.047 min
Delta R.T.: -0.002 min
Response: 90278
Conc: 73.91 ng/ml

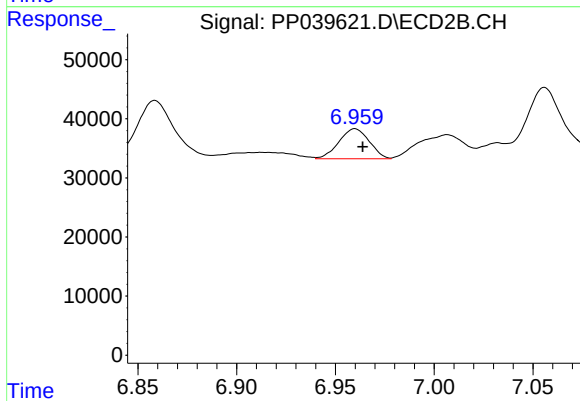

#29 AR-1254-4

R.T.: 6.959 min
Delta R.T.: -0.004 min
Response: 54491
Conc: 56.59 ng/ml m

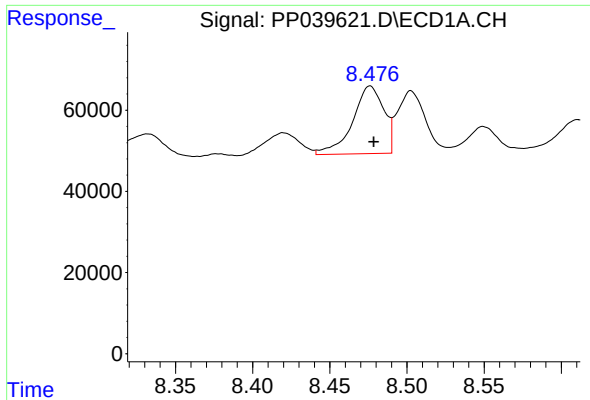


#30 AR-1254-5

R.T.: 8.476 min
Delta R.T.: -0.002 min
Response: 234285
Conc: 184.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
KEARNY-COMP

Manual Integrations
APPROVED

mohammad
9/30/2021 9:30:50 AM

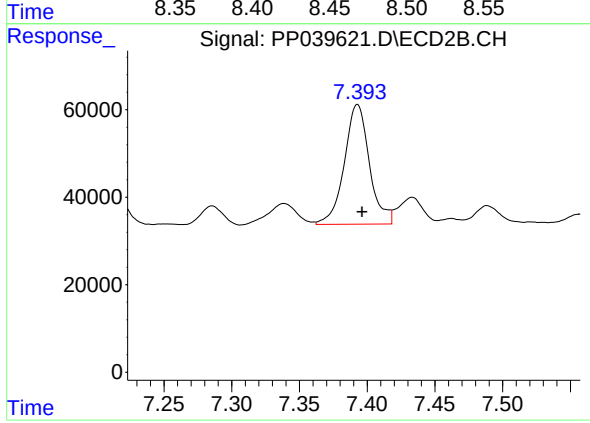

#30 AR-1254-5

R.T.: 7.393 min
Delta R.T.: -0.003 min
Response: 353558
Conc: 251.19 ng/ml