

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
 Data File : PP039639.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Sep 2021 00:42
 Operator : AJ\MA
 Sample : M3976-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MW-14-20210928-2-3-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 30 03:58:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Sep 25 01:28:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.905	3.995	712967	407331	22.521	24.998
2)	SA Decachlor...	10.929	9.331	445592	467038	20.540	21.372

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP092921\
Data File : PP039639.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Sep 2021 00:42
Operator : AJ\MA
Sample : M3976-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MW-14-20210928-2-3-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 30 03:58:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP092421.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Sep 25 01:28:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

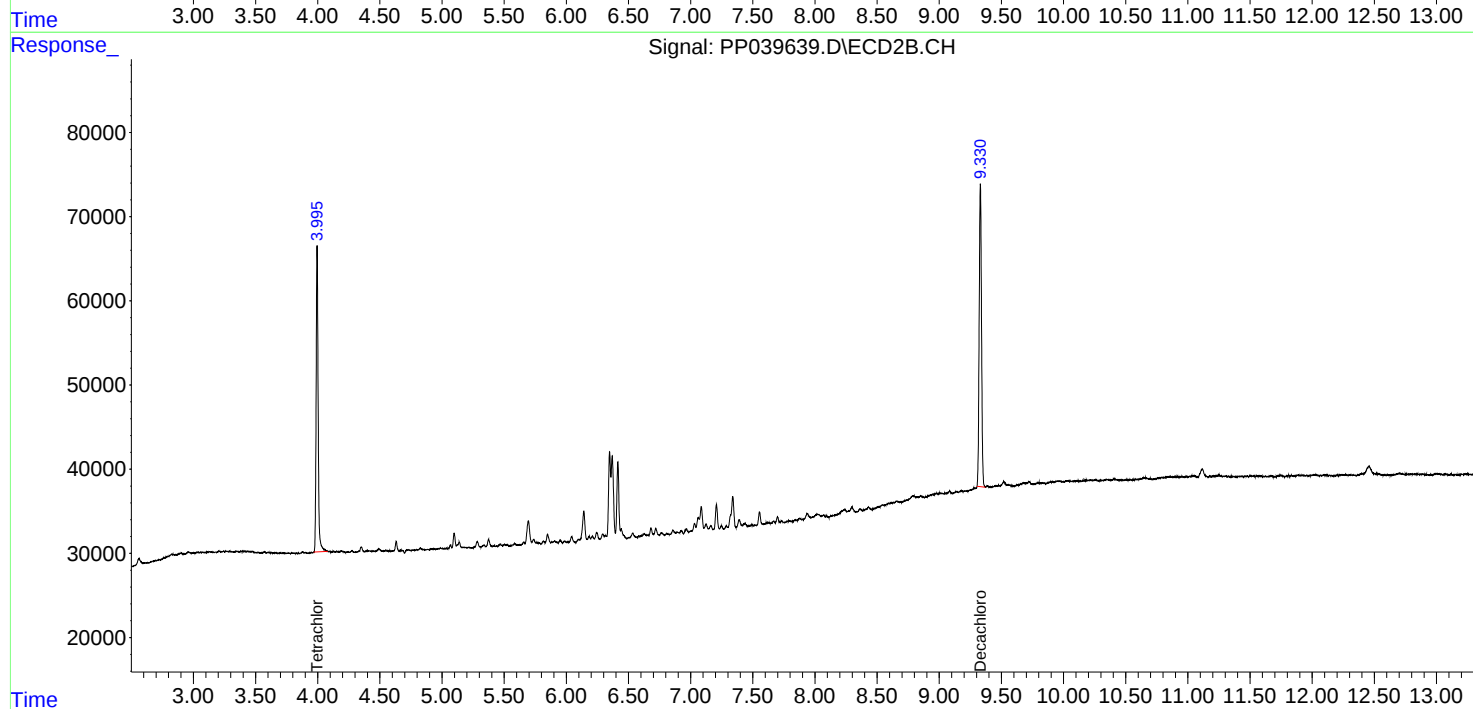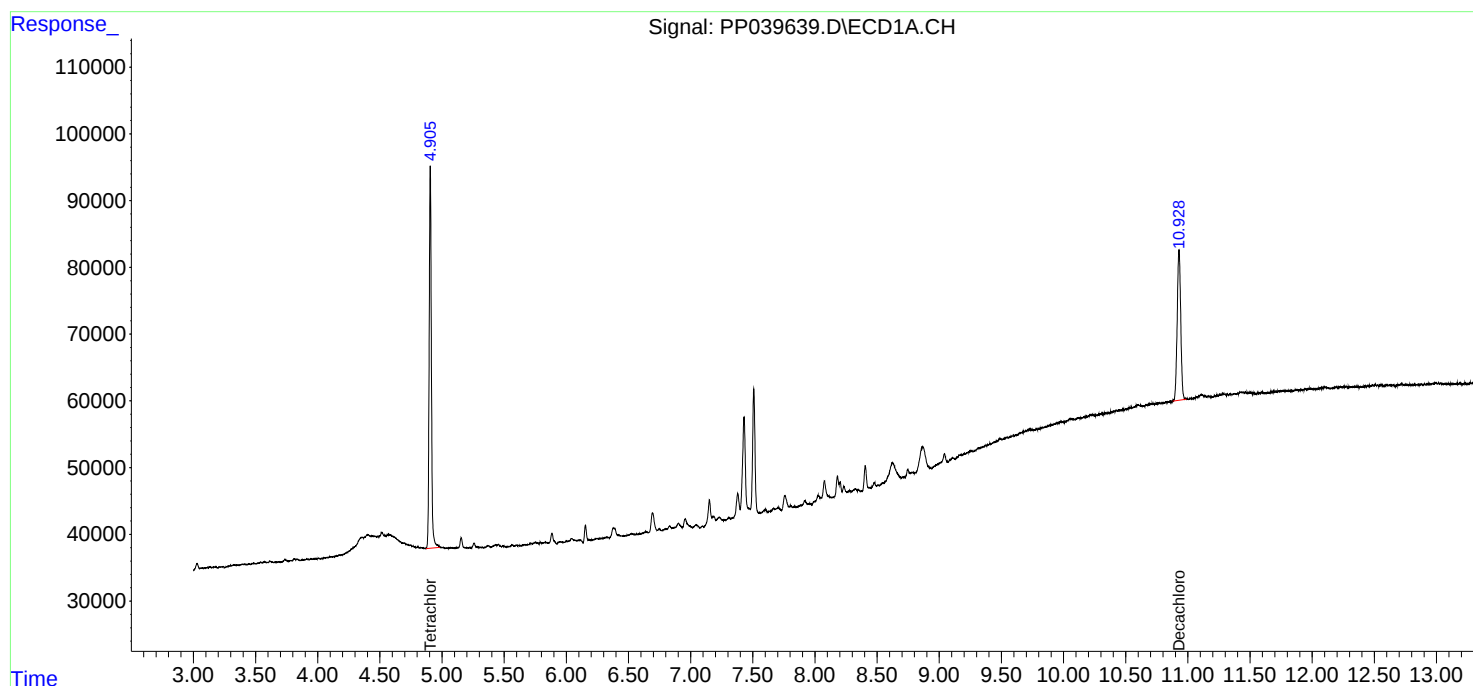


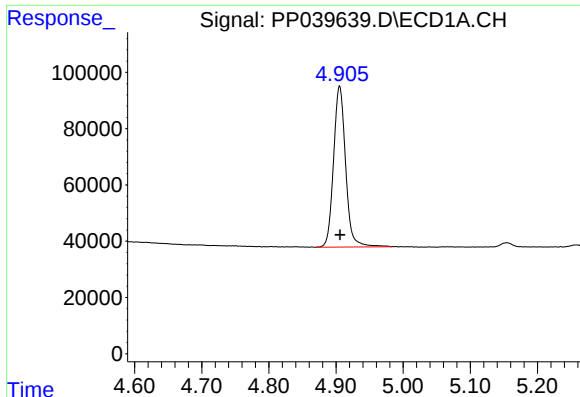

#1 Tetrachloro-m-xylene


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 712967
Conc: 22.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MW-14-20210928-2-3-WC

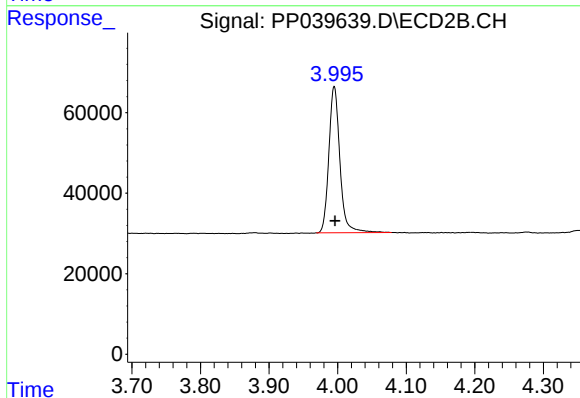


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.001 min
Response: 407331
Conc: 25.00 ng/ml

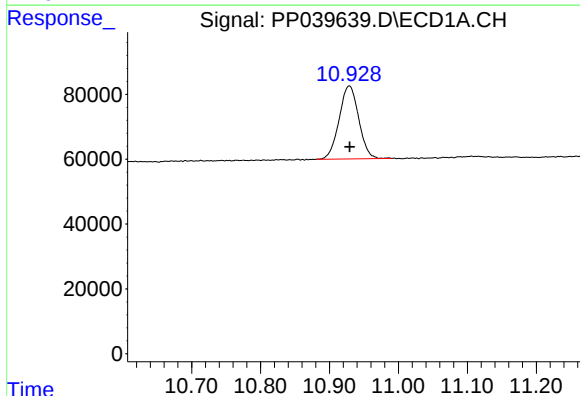

#2 Decachlorobiphenyl

R.T.: 10.929 min
Delta R.T.: 0.000 min
Response: 445592
Conc: 20.54 ng/ml

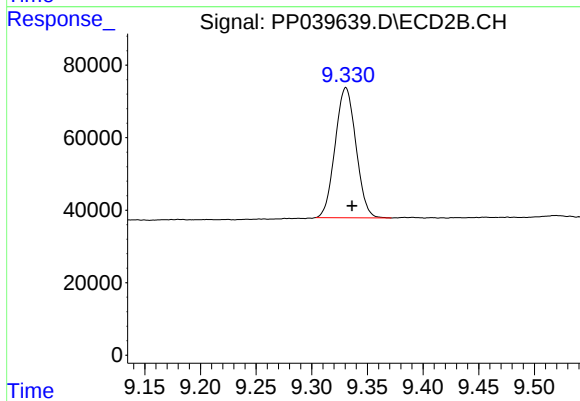

#2 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: -0.005 min
Response: 467038
Conc: 21.37 ng/ml